Device-to-Dashboard Operations Handbook

Contents

1.Vital Sign Measurement Guide 1

1.1 Measuring Vitals Using Dr Trust Pulse Oximeter 2

1.2. Measuring Vitals Using Dr Odin Pulse Oximeter 3

1.3. Measuring Vitals Using VinCense Remote Health Monitoring and Alerting System 5

2. VinCense Portal Navigation & Data Analysis Guide 11

2.1. Portal Login 12

2.2 Home Dashboard Overview 13

2.3 Patient Detailed Profile 16

2.4 Trend Analysis Section 19

2.5 Readings History Table 20

2.6 Doctor Notes Module 22

2.7 Health Screening Report Generation 24

2.8 My Account - Settings Module 25

2.9 Data Flow and Synchronization 29

3. Communitiful x VinCense Dashboard Navigation & Data Analysis Guide 30

3.1 Introduction 30

3.2 Landing Page 31

3.3 Main Dashboard Layout 32

3.4 Overview Section 35

3.5 Analytics Modules 36

3.6 Health Profile Modal 45

3.7 Video Gallery 46

3.8. FAQ & Help Panel 46

3.9. Add Vitals 47

3.10. Sync Vitals 48

3.11. Theme Toggle 49

3.12. Data Filtering Logic 50

3.13. Intended Usage 51

3.14. Overview 52

Xinthe
Excellence Forever...

1.Vital Sign Measurement Guide

Devices Covered:

- Dr Trust Pulse Oximeter
- Dr Odin Pulse Oximeter
- VinCense Remote Health Monitoring and Alerting System

1.1 Measuring Vitals Using Dr Trust Pulse Oximeter

Parameters Measured:

- Pulse Rate (PR)
- Oxygen Saturation (SpO_2)
- Respiratory Rate (RR)

Fig: Dr Trust Pulse Oxi-Meter

1.1.1 Preparation

1. Ensure the device batteries are properly installed.
2. Clean the finger clip sensor with an alcohol swab.
3. Ensure the subject:
    a. Is seated comfortably
    b. Has warm hands (cold fingers may affect readings)
    c. Has no nail polish or artificial nails

1.1.2 Procedure

1. Open the clip of the pulse oximeter.
2. Insert the subject's index finger fully into the device.
3. Press the **Power Button**.
4. Ask the subject to remain still.
5. Wait 10–20 seconds until readings stabilize.
6. Note the displayed:
    a. **SpO_2 (%)**
    b. **Pulse Rate (Beats per Minute - BPM)**
    c. **Respiratory Rate (Breaths Per Minute – BPM)**

1.1.3 After Measurement

1. Remove the finger.
2. Device will automatically turn off after a few seconds.
3. Record the values manually in the reporting system.

1.2. Measuring Vitals Using Dr Odin Pulse Oximeter

Parameters Measured:

- Pulse Rate (PR)
- Oxygen Saturation (SpO_2)
- Respiratory Rate (RR)

Fig: Dr Odin Pulse Oxi-Meter

1.2.1 Preparation

1. Check battery level.
2. Ensure subject is seated and relaxed.
3. Remove nail polish/artificial nails if present.

1.2.2 Procedure

1. Insert subject's index finger into the oximeter.
2. Press the **Power Button**.
3. Keep the hand steady.
4. Wait 10–20 seconds for stable readings.
5. Record:
    a. **SpO_2 (%)**
    b. **Pulse Rate (BPM)**
    c. **Respiratory Rate (if available)**

1.2.3 After Measurement

1. Remove the finger.
2. Device powers off automatically.
3. Record readings as required.

1.3. Measuring Vitals Using VinCense Remote Health Monitoring and Alerting System

Parameters Measured:

- Pulse Rate
- SpO_2
- Respiratory Rate
- Skin Temperature

Fig: VinCense Remote Health Monitoring and Alerting System

1.3.1 System Components

- VinCense Wearable Device
- Mobile Application
- Bluetooth Connectivity
- Cloud-based VinCense Portal Dashboard

1.3.2 Login Procedure (Mobile App)

1. Open the VinCense Mobile Application.

2. Enter:
    a. **Code**
    b. **Username**
    c. **Password**

3. Tap **Login**.

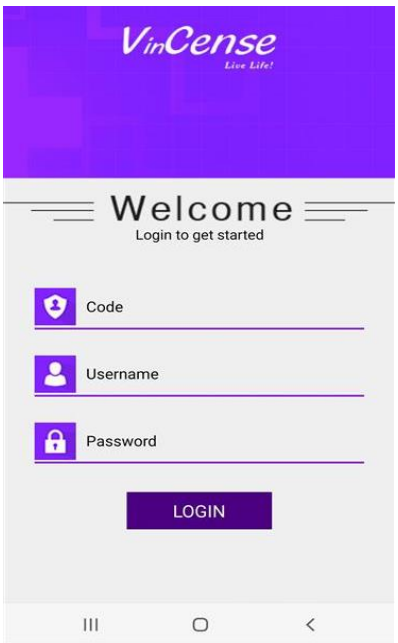

Fig: Login Using User Credentials

1.3.3 Device Configuration (Bluetooth Pairing)

1. Open the **Menu**.
2. Select **Config**.
3. Tap on **Scan**. (Parallelly make sure the VinCense Device is turned on with probe connected and charged)
4. The mobile app searches for nearby wearables.
5. Once the wearable appears:
    a. Tap on the device name.
    b. Unlock Icon is displayed referring to the device - **Connected**.
6. Confirm successful connection.

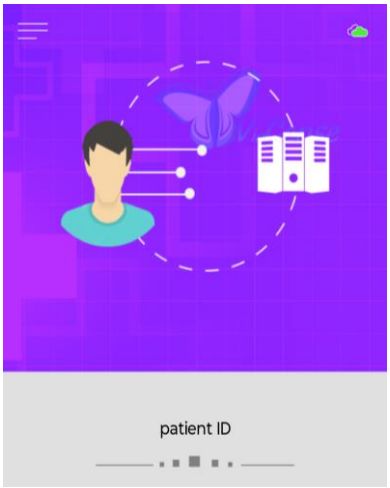

Step 1: Open the Menu

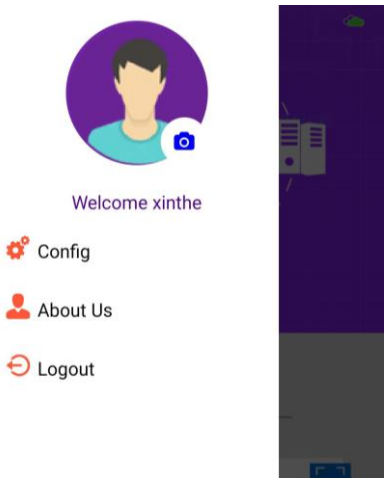

Step 2: Select Config

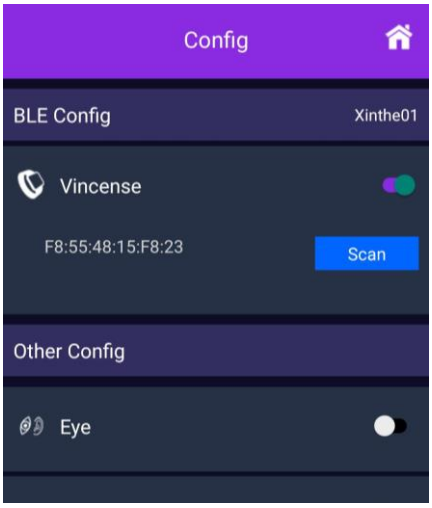

Step 3: Tap on Scan

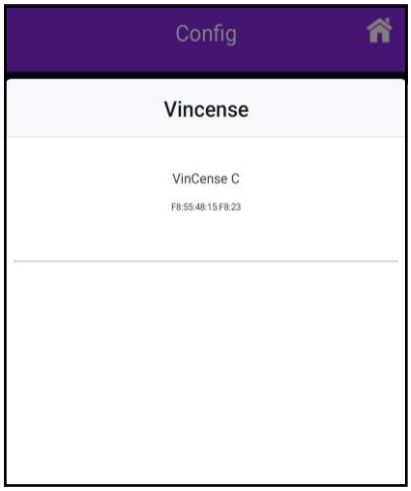

Step 4 & 5a: Tap on the device name

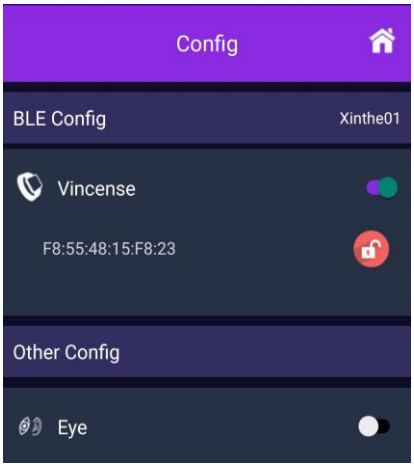

Step 5b: Unlock Icon is displayed referring to the device - **Connected**

1.3.4 Registering or Selecting Subject

1. Go back to the **Home Page**.

If Subject is New:

- Assign a **Unique Subject ID**.
- Enter all required demographic and personal details.
- Click **DONE**.

If Subject is Already Registered:

- Enter the **Subject ID**.
- Click the arrow button.
- Verify details displayed.
- Click **DONE**.

The Vitals Display Page will now open.

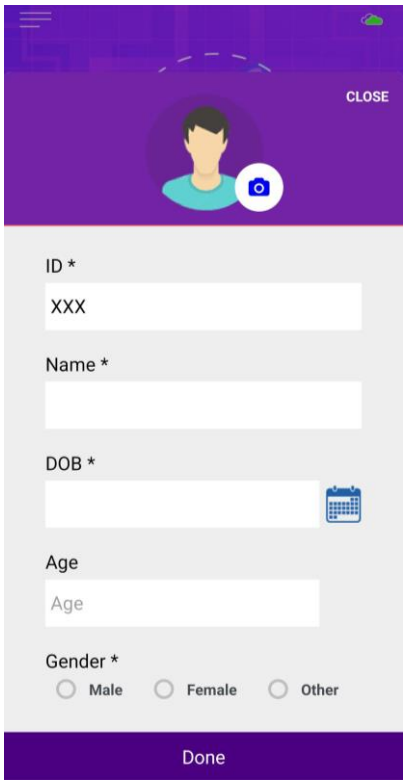

Fig: If Subject is New

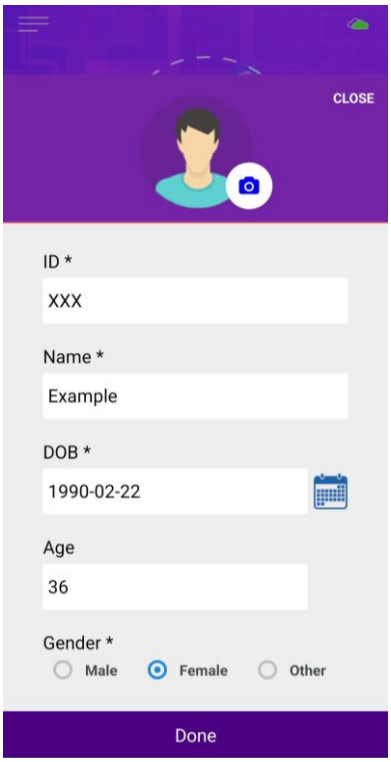

Fig: If the Subject is Already Registered

1.3.5 Confirming Device Readiness

1. On the top-right corner of the screen, observe the **connection icon**.
2. Wait until:
    a. A **Green Tick Mark** appears.
    b. The device emits a **beep sound**.

This indicates the system is connected and ready.

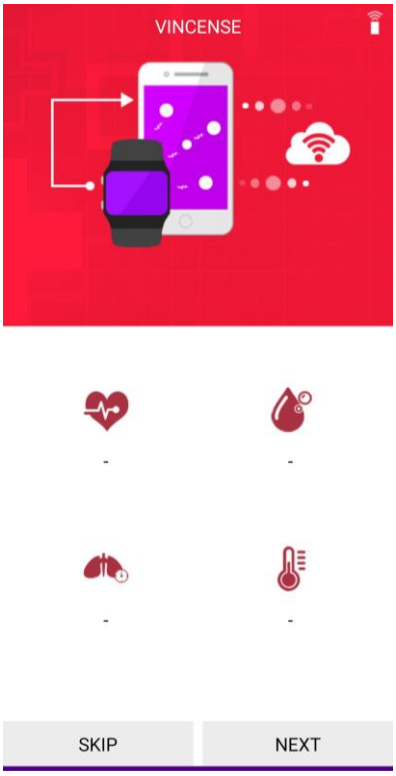

Fig: Before Green Tick Mark

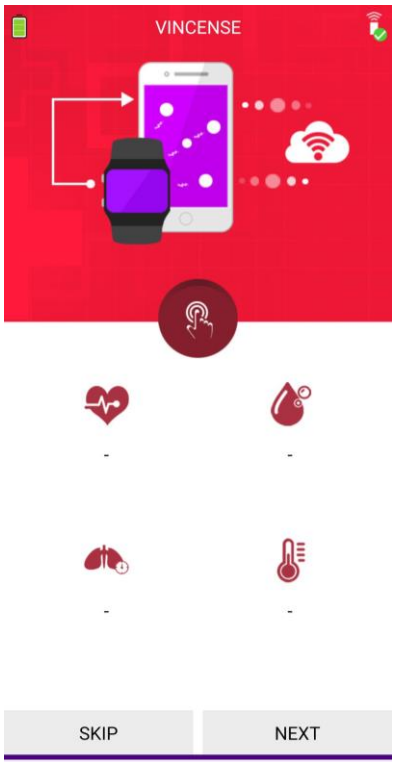

Fig: After Green Tick Mark

1.3.6 Capturing Vitals

1. An **Orange Icon** appears at the centre of the screen.
2. Tap the Orange Icon to start measurement.
3. A **double beep** is heard.
4. The device captures vitals for **20–30 seconds**.
5. After completion, a **long beep** is heard.
6. Captured vitals are displayed on the mobile interface.

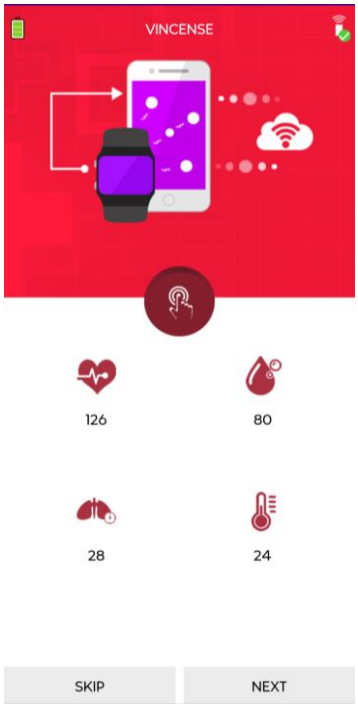

Fig: Vitals Displayed in the VinCense App

1.3.7 Viewing and Submitting Results

1. Click **Next**.
2. Click **OK**.
3. The system displays:
    a. Pulse Rate
    b. SpO_2
    c. Respiratory Rate
    d. Skin Temperature
    e. COVID Risk Report:
        i. No COVID Risk
        ii. Mild COVID Risk
        iii. Moderate COVID Risk
        iv. High COVID Risk
4. Click **Submit**.

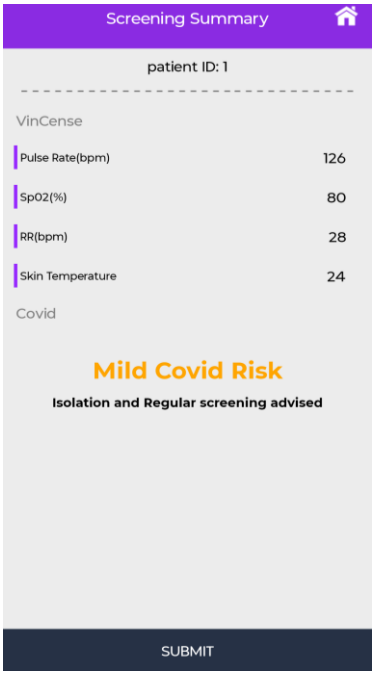

Fig: Vitals and Overall Covid Risk Analysis Shown in the VinCense App

1.3.8 Data Synchronization

Upon clicking **Submit**:

- Data is automatically synced to the VinCense Cloud.
- Values are updated in the respective **VinCense Portal Dashboard**.
- Alerts (if applicable) are generated in the monitoring system.

2. VinCense Portal Navigation & Data Analysis Guide

Platform: VinCense Portal

2.1. Portal Login

Step 1: Access the Portal

- Open a web browser.
- Enter the VinCense Portal URL.
- The Login Page appears.

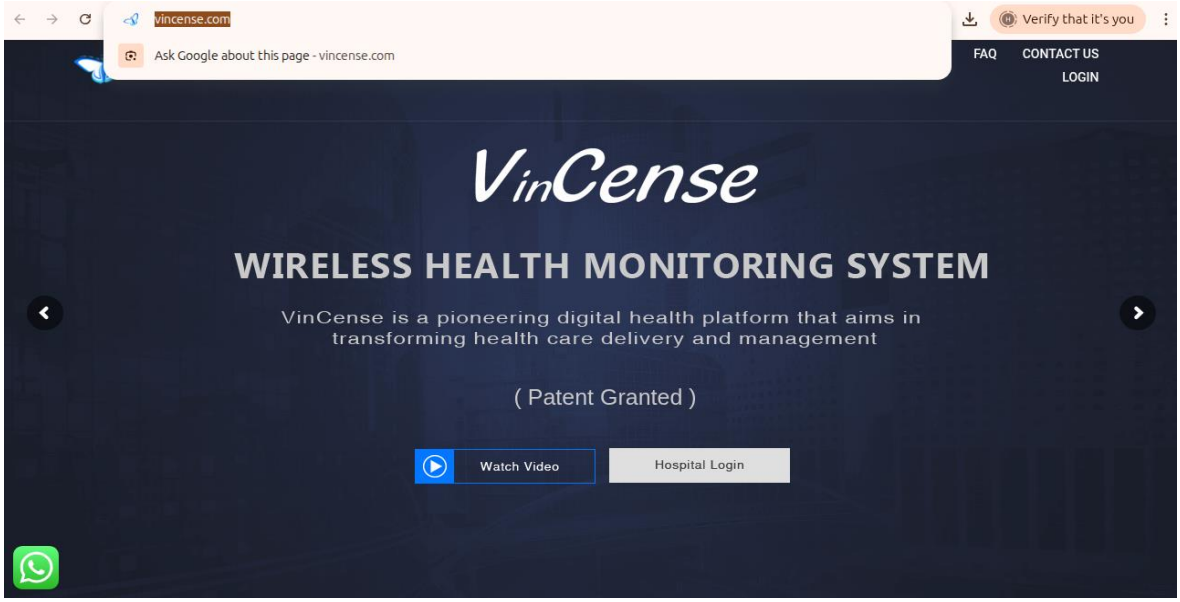

Fig: VinCense Website

Step 2: Enter Credentials

- Enter:
  - Code
  - Username
  - Password
- Click **Login**.

Xinthe
Excellence Forever...

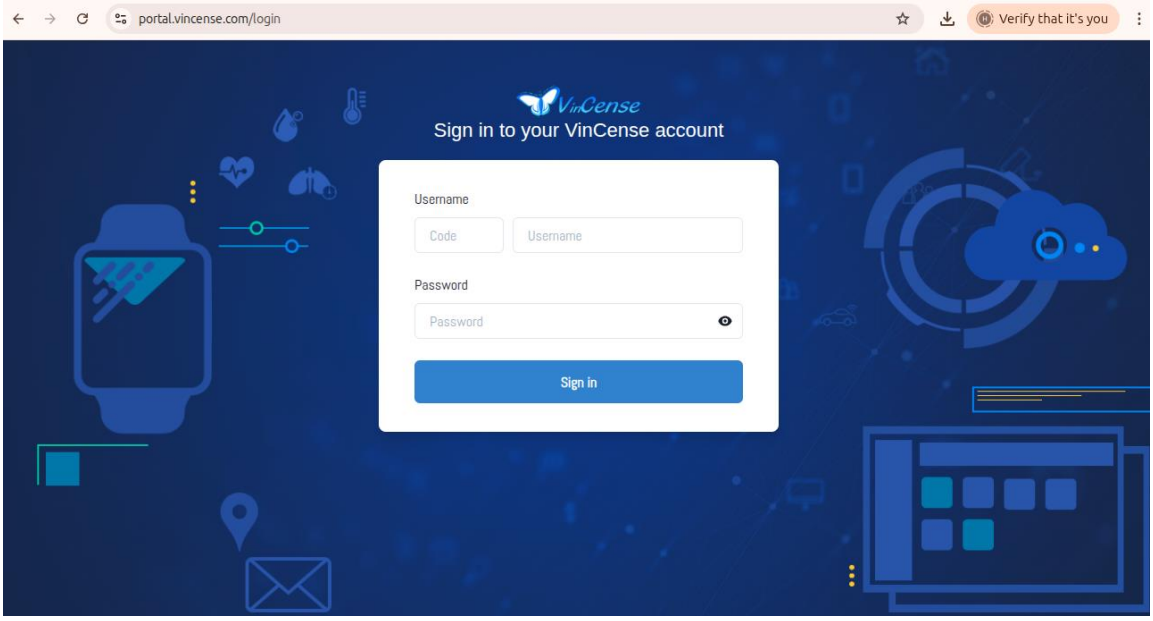

Fig: VinCense Portal Login Page

If credentials are correct, the system redirects to the **Dashboard Home Page**.

2.2 Home Dashboard Overview

2.2.1 Filters Panel

Located on the left side of the screen.

Available Filters:

- Date Range
- Age (0–120 slider)
- Age Groups (18–29 Yrs, 30–44 Yrs, 45+ Yrs)
- Gender
- View Readings by Patient
    - All Readings
    - Last Reading

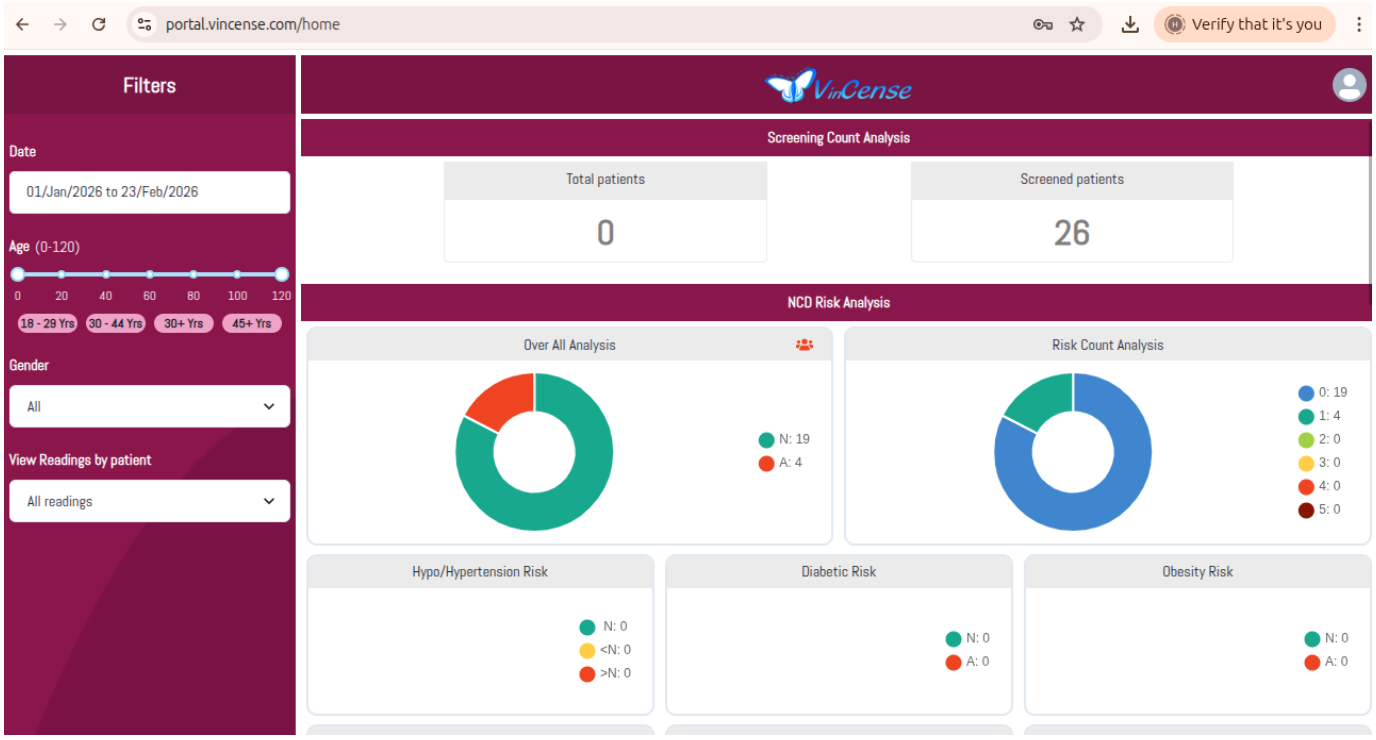

Fig: VinCense Portal Dashboard Overview Page with Default features

Procedure:

Step 1: Select the required Date Range.

Step 2: Adjust Age slider if required.

Step 3: Select Gender.

Step 4: Choose View Readings option.

The dashboard refreshes automatically based on selected filters.

Xinthe
Excellence Forever...

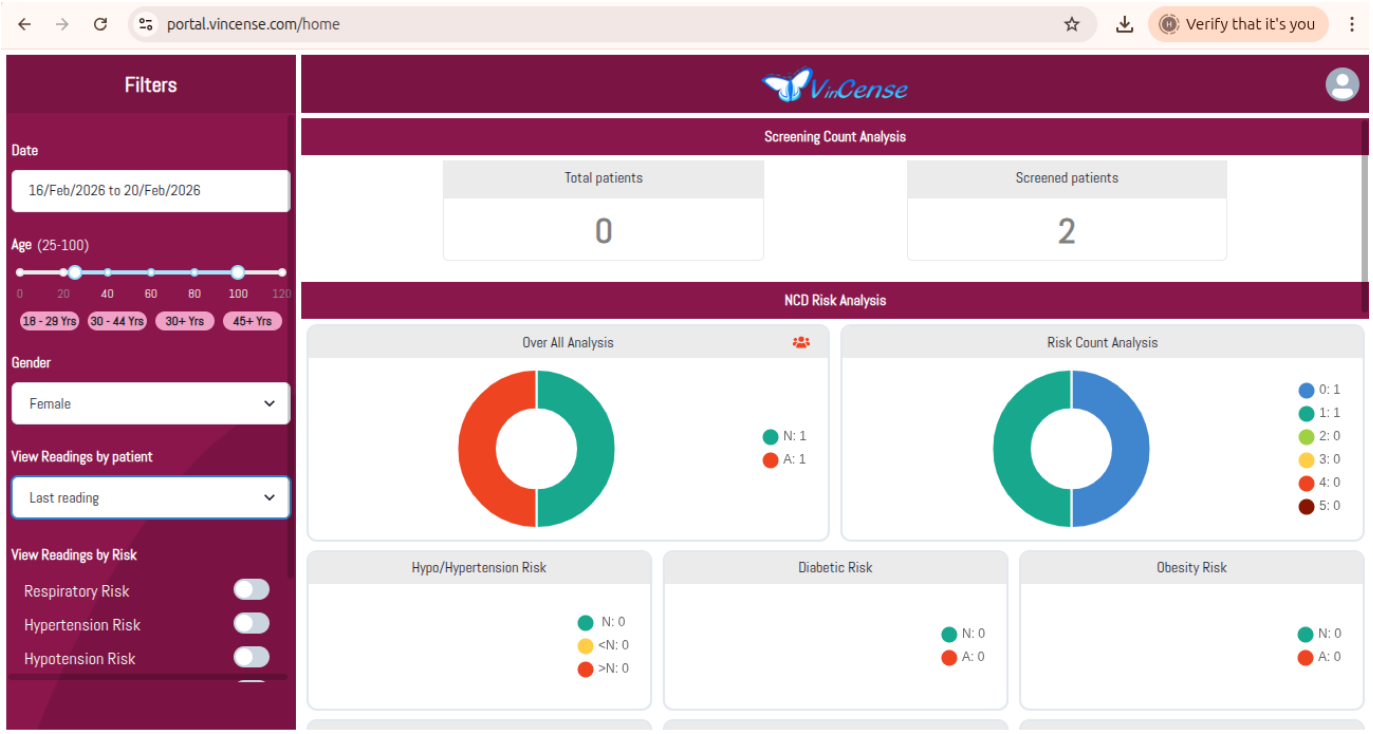

Fig: VinCense Portal Dashboard Overview Page with Features Selected

2.2.2 Patients Overview Grid

Displays:

- Patient Name
- Patient ID
- Total Patients Count (displayed at top)

Steps:

- ➢ Use the Search bar (top right) to locate a patient by Name or ID.
- ➢ Click on a patient card to open the detailed profile.

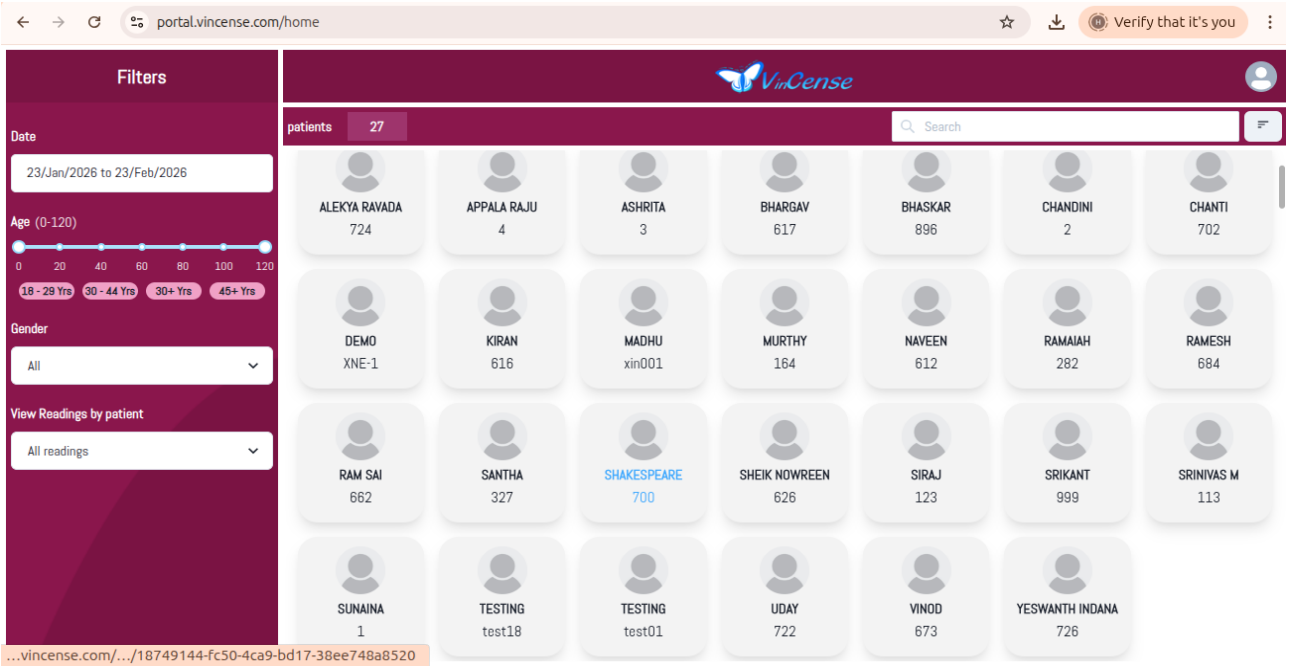

Fig: Overall Patient Overview Grid

2.3 Patient Detailed Profile

Upon selecting a patient, the Patient Detail Page opens.

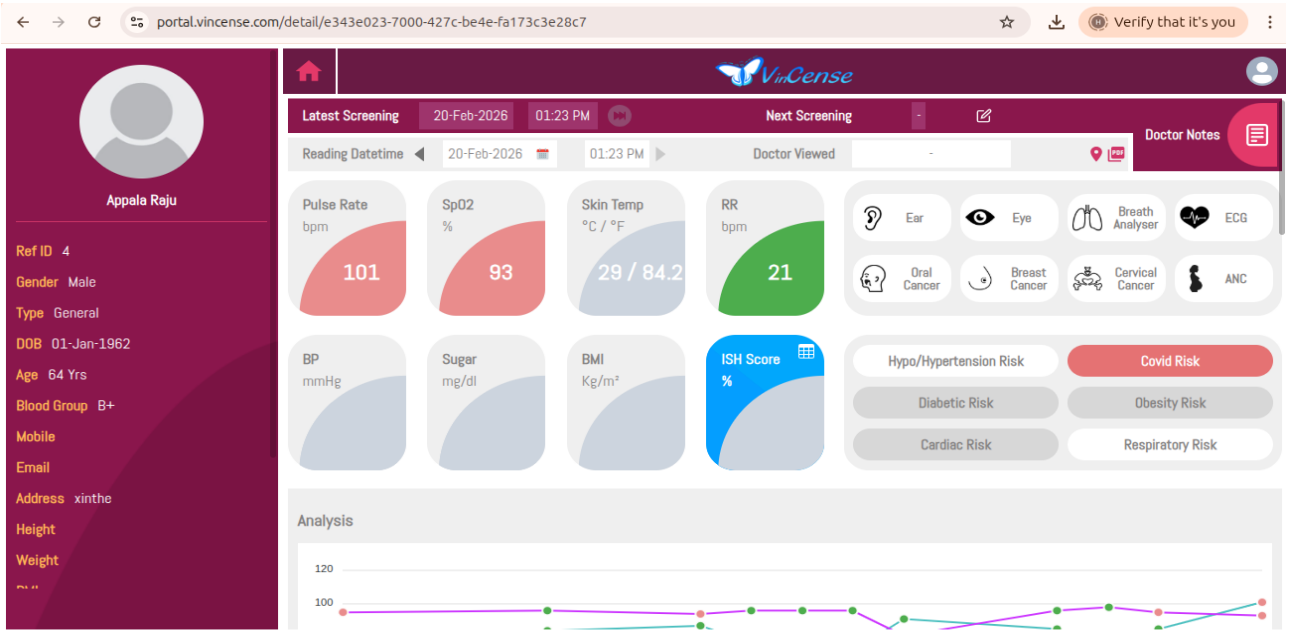

Fig: Individual Profile of Patient Details

2.3.1 Patient Information Panel

Xinthe
Excellence Forever...

Located on the left side.

Displays:

- Ref ID
- Gender
- Type
- Date of Birth
- Age
- Blood Group
- Mobile Number
- Email
- Address
- Height
- Weight

This section provides complete demographic information.

2.3.2 Latest Screening Section

Displays:

- Latest Screening Date
- Screening Time
- Next Screening
- Doctor Viewed Status

This indicates the most recent screening session and review status.

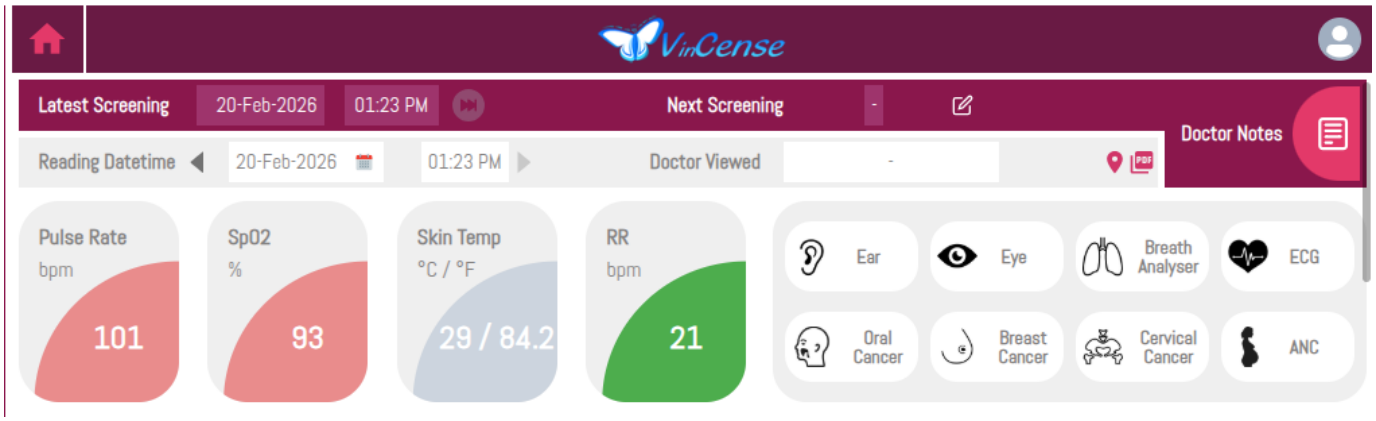

Fig: Shows the Analytics of the Latest Reading captured

2.3.3 Vital Parameters Display

The following vitals are shown in graphical tile format:

- Pulse Rate (bpm)
- SpO_2 (%)
- Skin Temperature (°C / °F)
- Respiratory Rate (RR)
- BP (if available) - Currently not being captured
- Sugar (if available) - Currently not being captured
- BMI - Currently not being captured
- ISH Score (%) - Currently not being captured

These tiles provide quick visual assessment of patient condition.

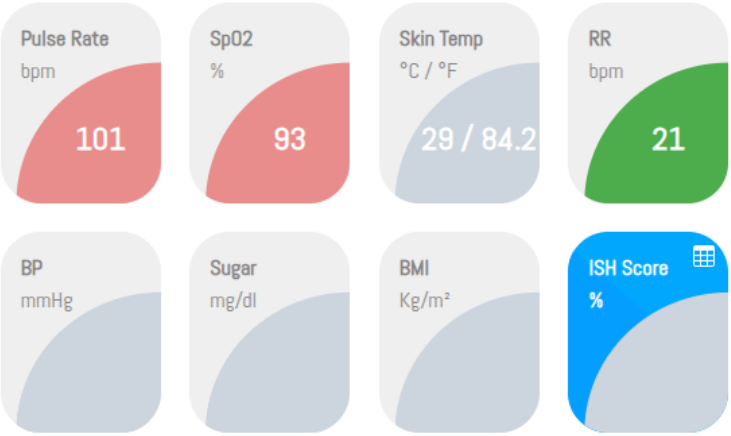

Fig: All Vitals Parameters Available

2.3.4 Risk Assessment Panel

Displays calculated risk categories:

- Hypo/Hypertension Risk
- COVID Risk
- Diabetic Risk
- Obesity Risk
- Cardiac Risk
- Respiratory Risk

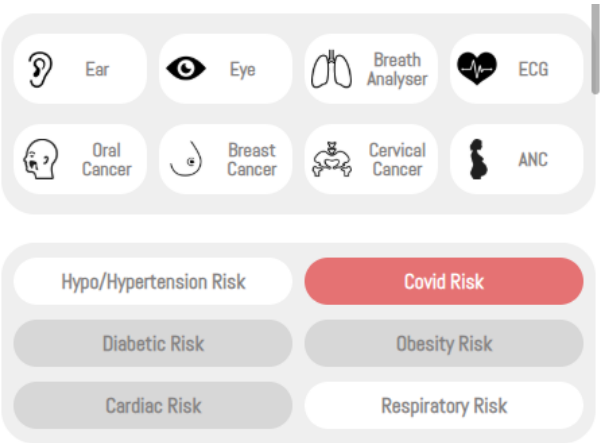

Fig: Various Kinds of Risks Calculated

These are derived from captured vital parameters and screening logic.

2.4 Trend Analysis Section

The Analysis section displays graphical trends over time.

Parameters Included:

- Pulse Rate
- Skin Temperature
- SpO_2
- Respiratory Rate
- Systolic

- Diastolic
- Random Sugar
- Fasting Sugar
- PP Sugar
- BMI

Procedure to Analyse:

Step 1: Hover over any data point to view exact Date and Time.

Step 2: Observe upward or downward trends.

Step 3: Identify abnormal spikes or repeated deviations.

Step 4: Compare trends across multiple days.

Step 5: Use the Date Filter (Left Side Bar) to change analysis range.

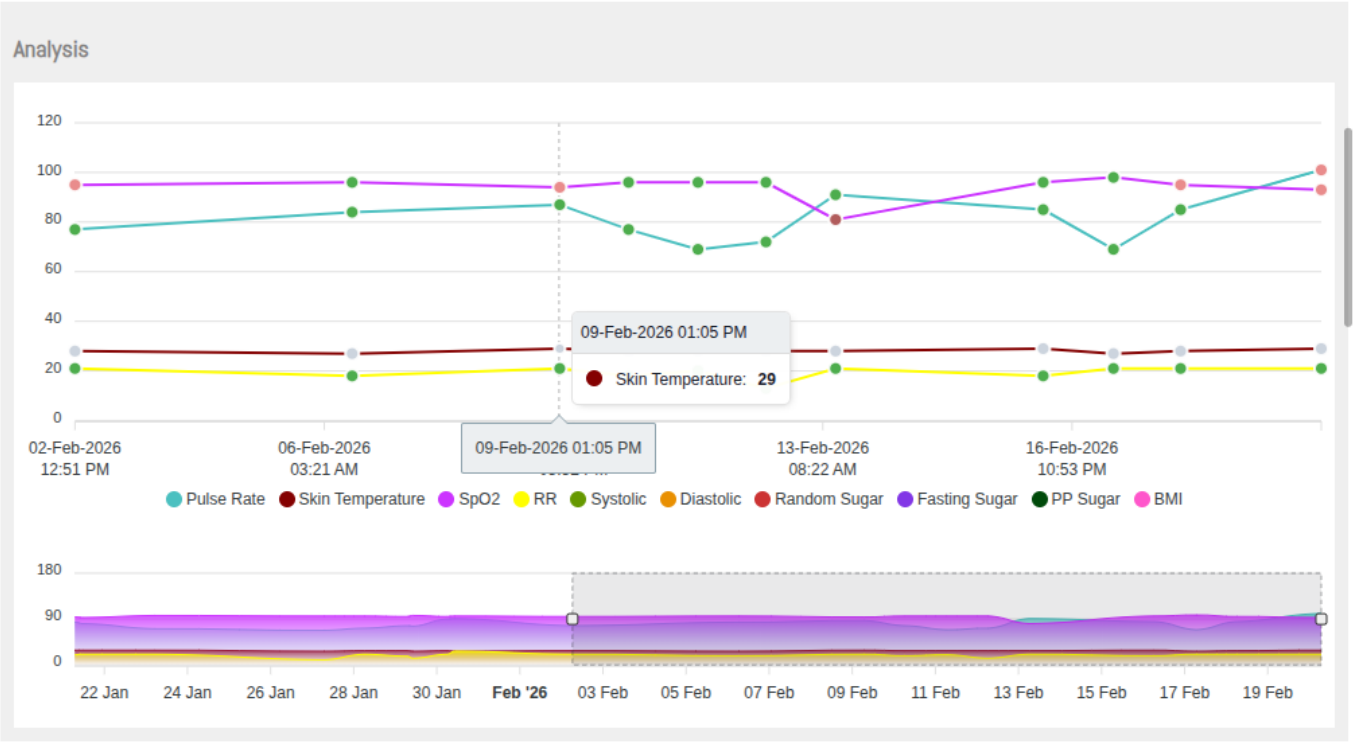

Fig: Trend Analysis of an Individual Patient

2.5 Readings History Table

Located below the trend graph.

Columns Include:

- Date/Time
- Pulse Rate
- Skin Temperature
- SpO_2
- Respiratory Rate
- BP
- Sugar
- BMI
- ISH Score
- PDF Download Icon

Procedure:

Step 1: Scroll to view historical data.

Step 2: Use date filter to narrow range.

Step 3: Click Export icon to Download or Email Readings Excel

Step 4: Click PDF icon to generate screening report.

Readings 20 | 21/Jan/2026 to 20/Feb/2026

Date/Time	Pulse Rate	Skin Temp	SpO2	RR	BP	Sugar	BMI	ISH Score
20-Feb-2026 01:23 PM	101	29 / 84.2	93	21	/			
18-Feb-2026 12:34 PM	85	28 / 82.4	95	21	/			
17-Feb-2026 01:15 PM	69	27 / 80.6	98	21	/			
16-Feb-2026 12:52 PM	85	29 / 84.2	96	18	/			
13-Feb-2026 12:50 PM	91	28 / 82.4	81	21	/			
12-Feb-2026 12:40 PM	72	28 / 82.4	96	13	/			
11-Feb-2026 01:04 PM	69	28 / 82.4	96	20	/			
10-Feb-2026 12:58 PM	77	28 / 82.4	96	18	/			

Fig: Readings History of an Individual Patient

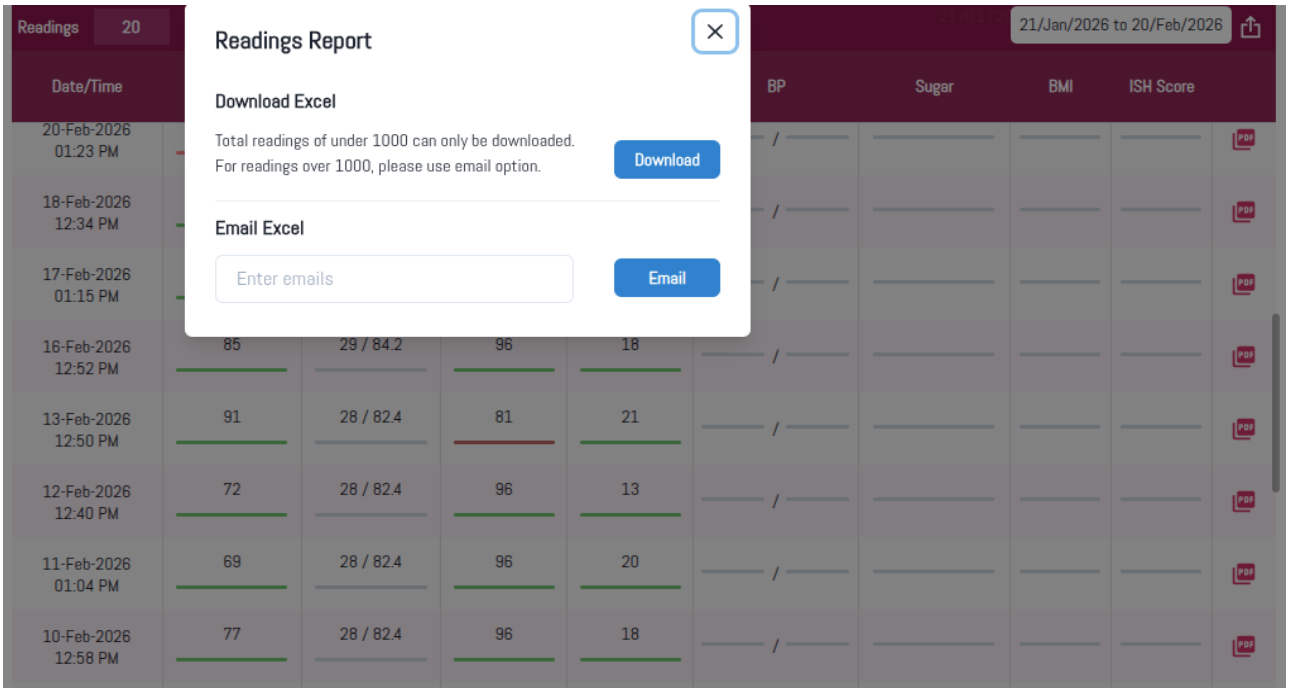

Fig: User can Download or E-mail the Excel Consisting of all the Historical Data

Xinthe
Excellence Forever...

2.6 Doctor Notes Module

Accessible via **Doctor Notes** button.

Procedure:

Step 1: Click Doctor Notes.

Step 2: A side panel opens.

Step 3: Enter clinical remarks or observations.

Step 4: Save notes.

Step 5: Close panel using "X".

This section is used for documentation and follow-up planning.

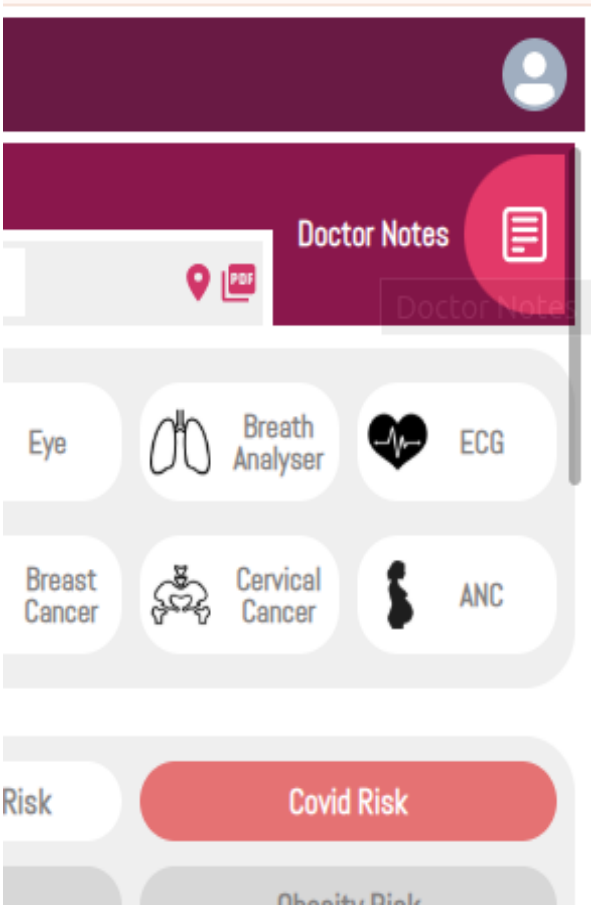

Fig: Doctor's Notes Feature to the Top right corner on the Patient Information Panel

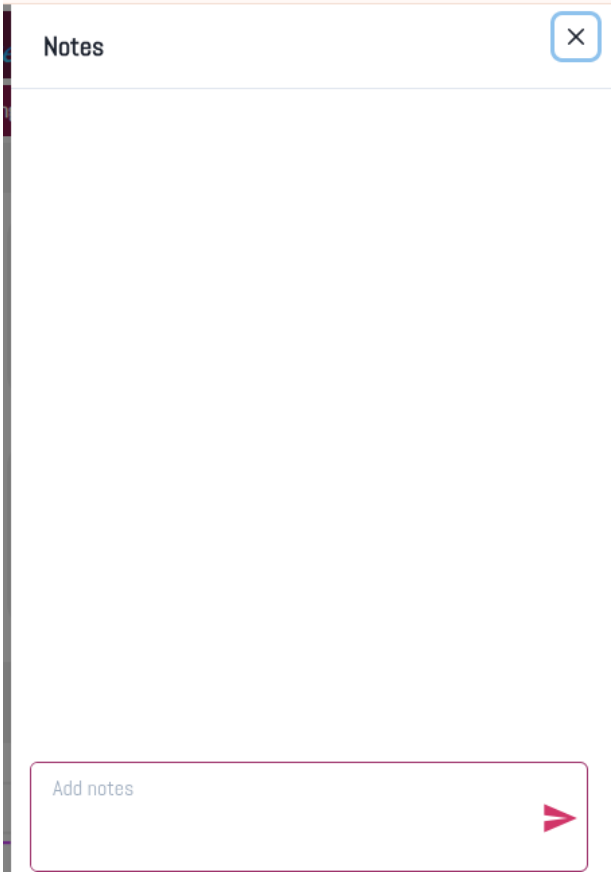

Fig: Doctor's Notes Section

Xinthe
Excellence Forever...

2.7 Health Screening Report Generation

Upon clicking the PDF icon, the Health Screening Report window opens.

Procedure to Download:

Step 1: Click Download icon.

Step 2: The file is saved as a PDF document.

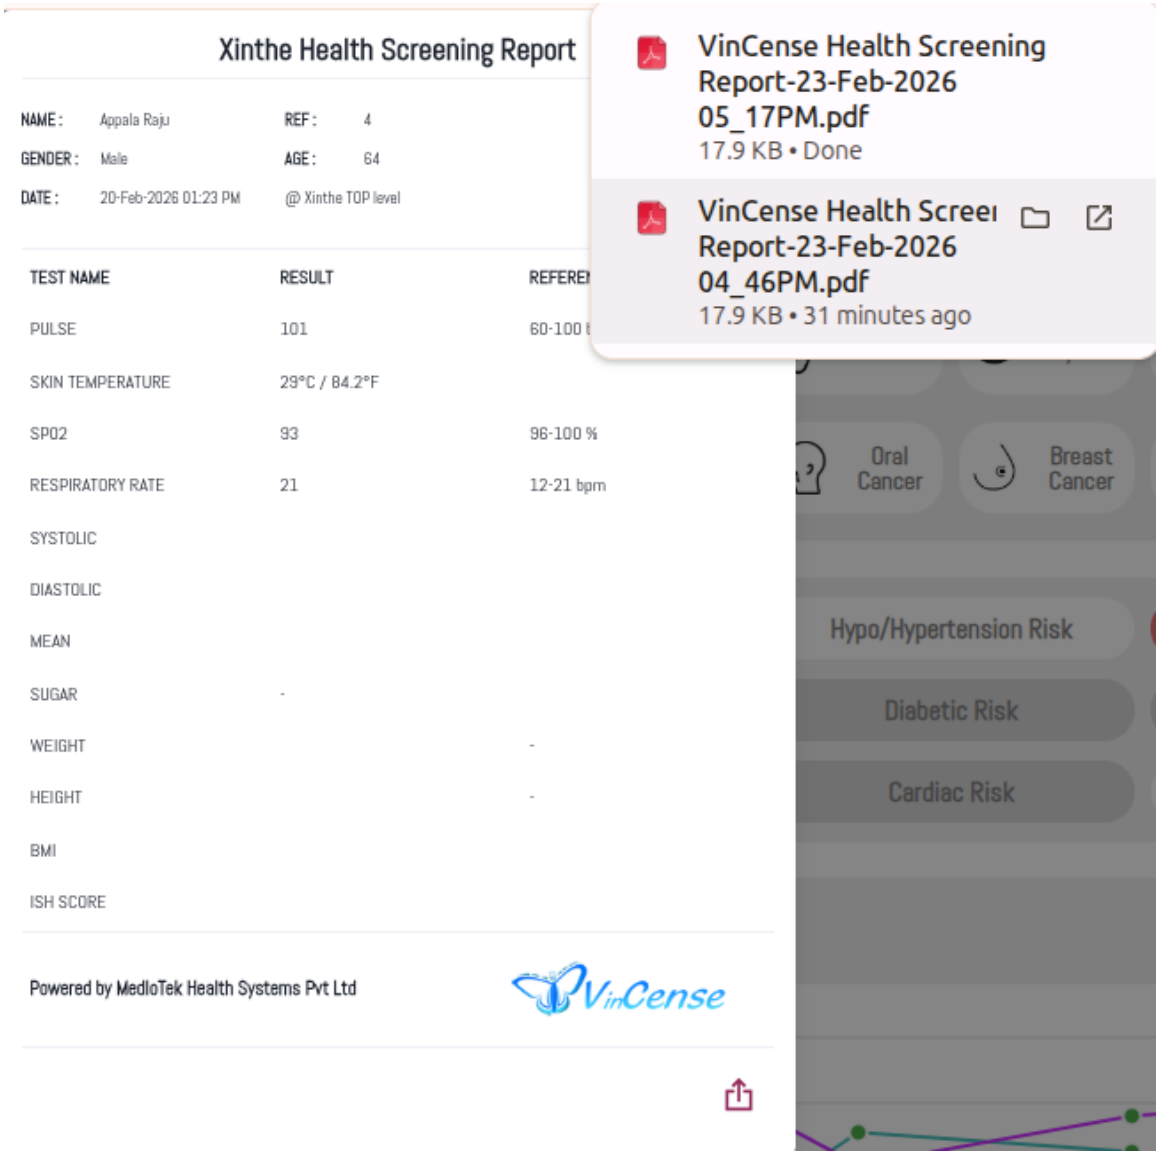

Fig: Patient's Health Screening Report

The report includes:

- Patient Name
- Ref ID
- Gender
- Age
- Date & Time of Screening
- Test Name
- Result
- Reference Range

Parameters Included:

- Pulse
- Skin Temperature
- SpO_2
- Respiratory Rate
- Systolic
- Diastolic
- Sugar
- Weight
- Height
- BMI
- ISH Score

2.8 My Account - Settings Module

Accessible via left-side menu → **Settings**

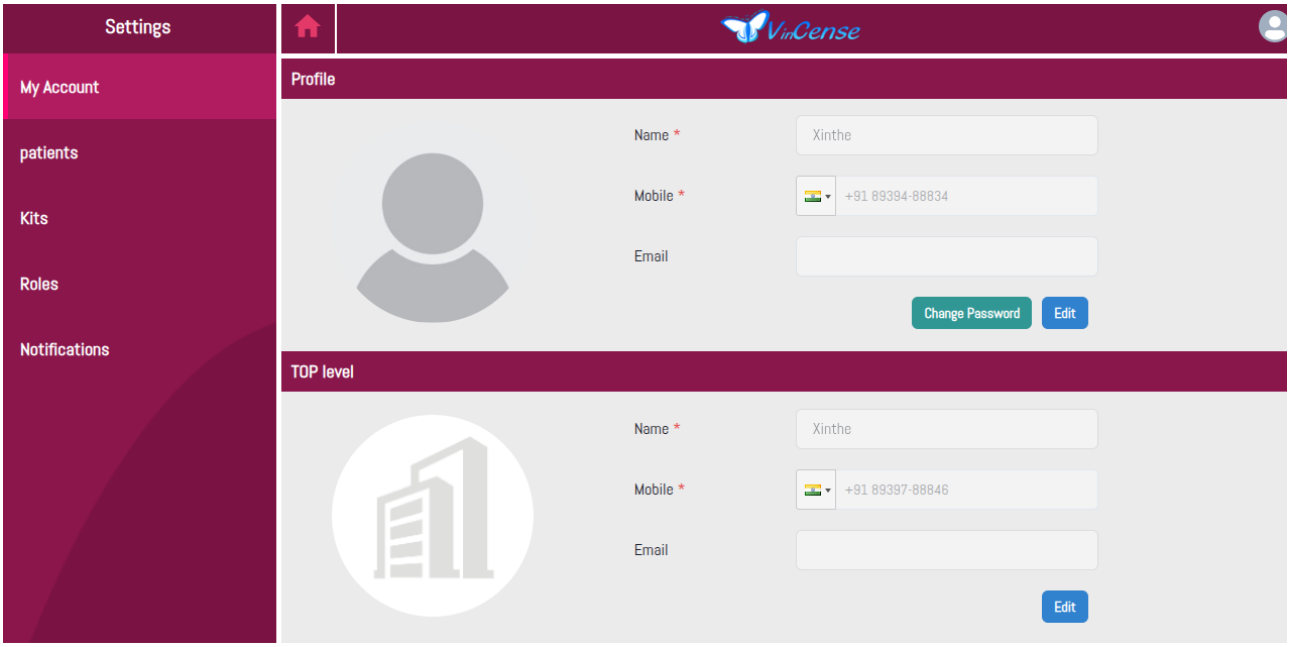

Fig: User Account Section

2.8.1 Patients Management

Displays all registered patients in card format.

Options Available:

- View Patient
- Assign Kit
- Edit Patient Details

Filters Available:

- Search
- Status (Active/Inactive)

Used for patient record management.

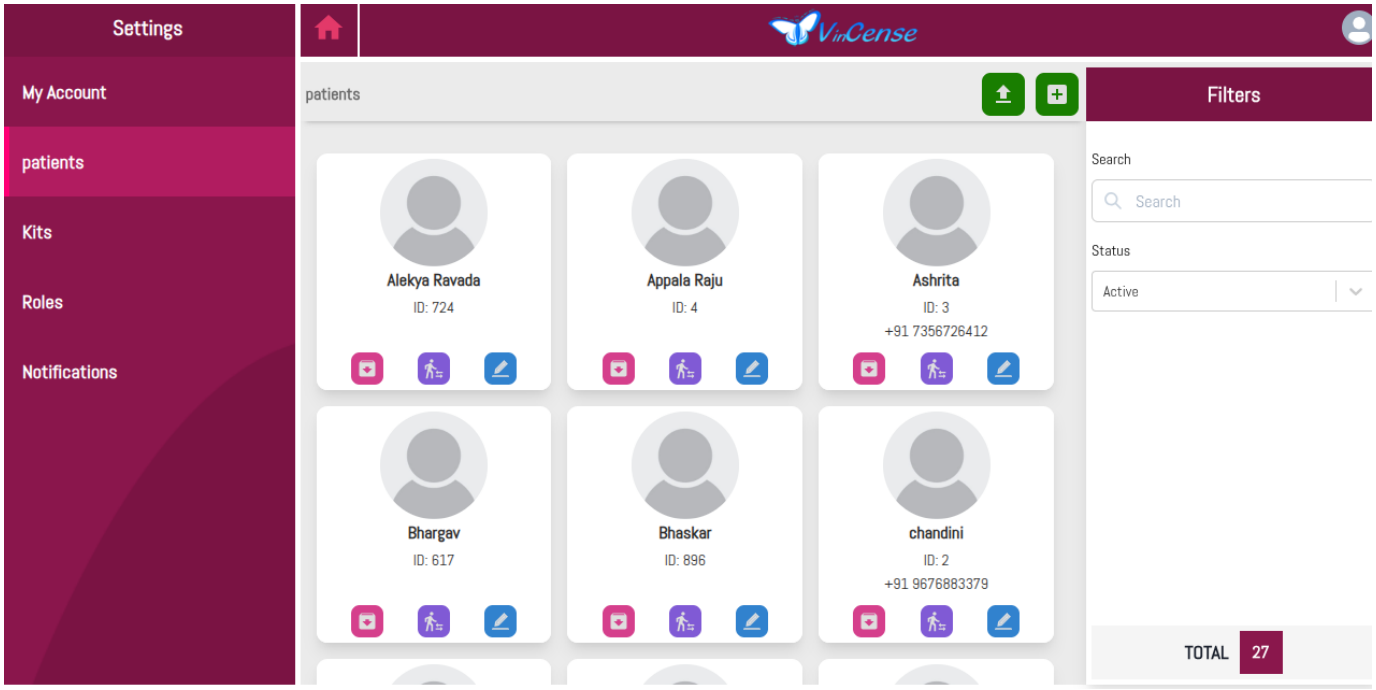

Fig: Patient Record Management Section

2.8.2 Kits Management

Displays available VinCense wearable kits.

Information Shown:

- Kit Name
- MAC Address
- Assigned Operator
- Valid Till Date
- Status

Filters Available:

- Search
- Operator

- Validity

Used to monitor device assignment and expiry.

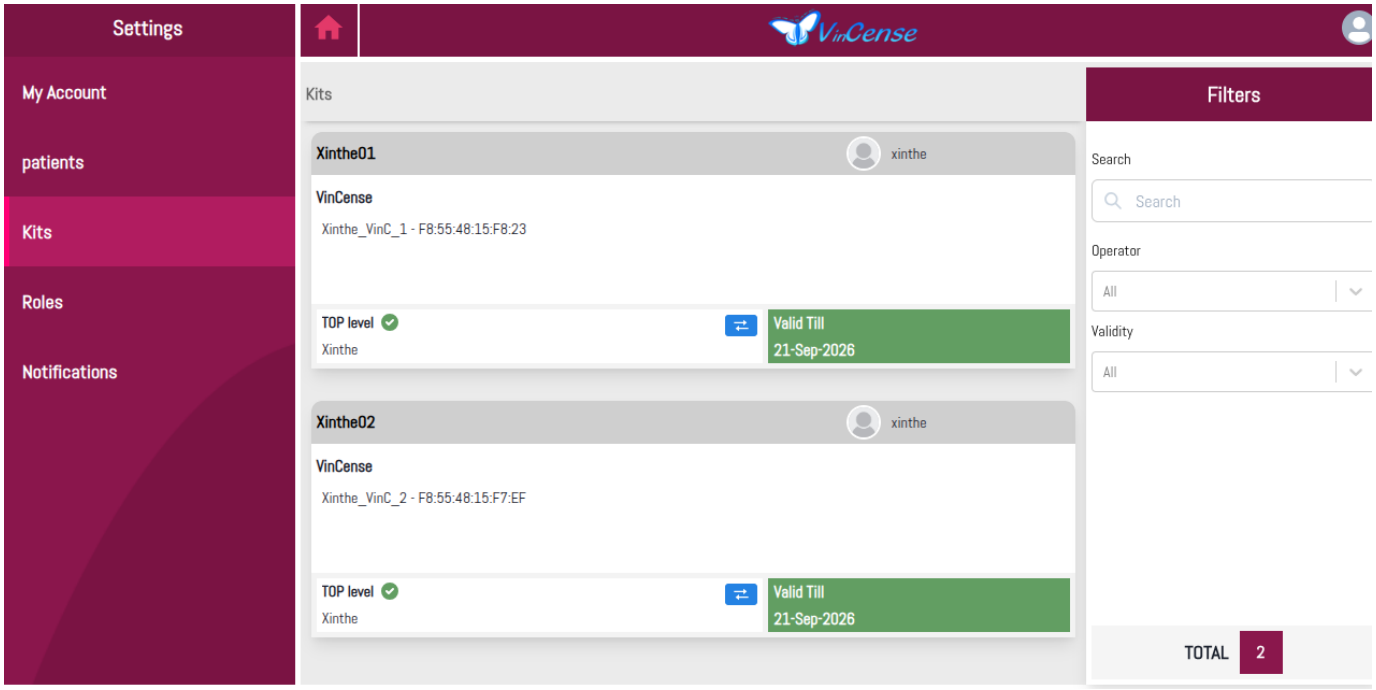

Fig: Multiple Kits Management Section

2.8.3 Notifications Configuration

Displays automated alert settings.

Notification Types:

- Daily Abnormal Screening Notification
- Hourly Abnormal Screening Notification
- Daily Next Screening Notification

Procedure:

Add Email IDs.

Edit notification schedule.

Save configuration.

System sends alerts based on abnormal screening events.

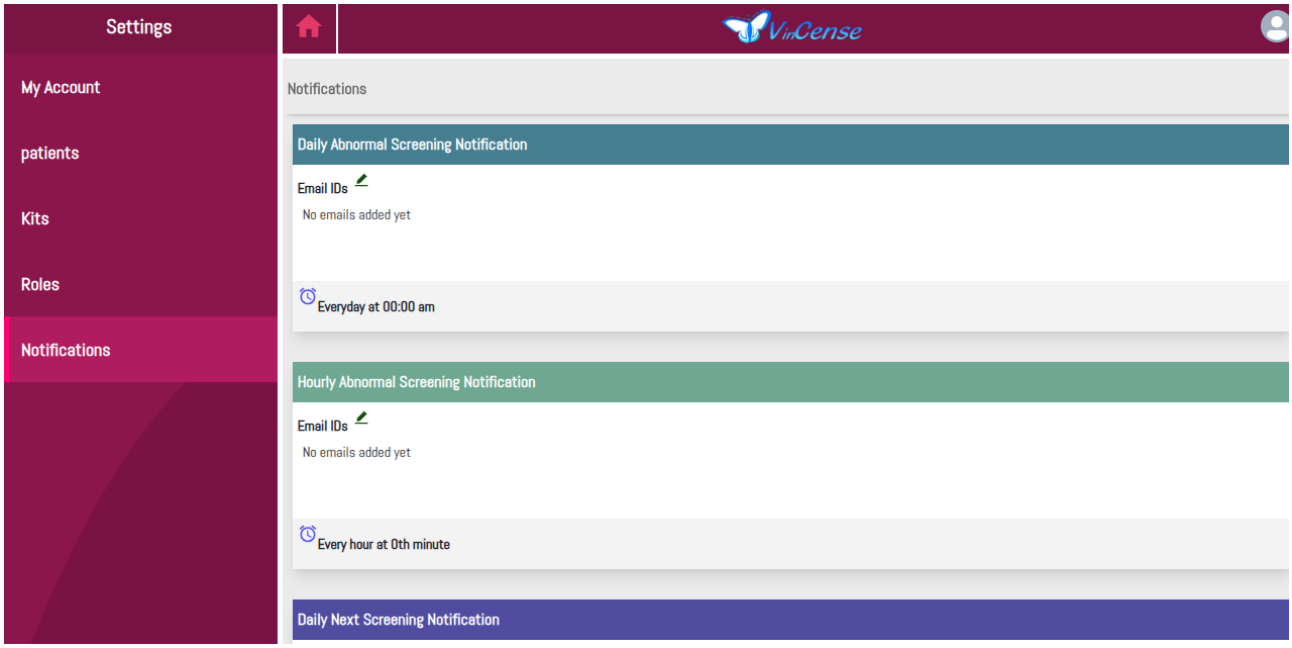

Fig: Notifications Section

2.9 Data Flow and Synchronization

After vitals are captured via the VinCense Mobile App and submitted:

- Data is transmitted via Bluetooth to the mobile application.
- The mobile application uploads data to the VinCense Cloud.
- The VinCense Portal Dashboard updates in real time.
- Alerts are triggered if abnormal values are detected.

2.9.1 Interpretation Guidelines:

Parameter	Normal Range
SpO_2	95–100%
Pulse	60–100 BPM
Respiratory Rate	12–20 breaths/min
Skin Temperature	~36–37.5°C

Red/Orange highlights indicate abnormal values.

2.9.2 Logout Procedure

1. Click Profile icon (top right).
2. Select **Logout**.
3. Ensure session is properly closed.

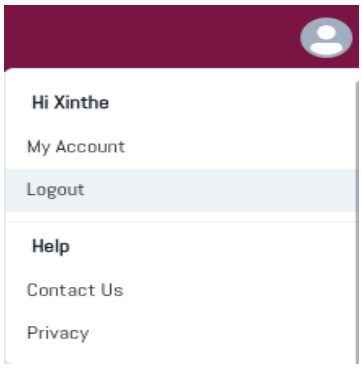

Fig: Logout Option

3. Communitiful x VinCense Dashboard Navigation & Data Analysis Guide

3.1 Introduction

The **Communitiful x VinCense Dashboard** is a comprehensive medical analytics platform designed to:

- Analyse physiological vitals (Pulse, SpO_2, Respiratory Rate, Skin Temperature)
- Compare readings across multiple devices (VinCense, Dr Trust, Dr Odin)
- Perform demographic-based analytics (Gender, Age Group, Circumstance)
- Provide subject-level health insights
- Support research validation and performance benchmarking

This dashboard enables both high-level overview and deep analytical exploration.

3.2 Landing Page

When the dashboard is opened:

- A **full-screen landing page** is displayed.
- It contains:
  - Overview description of the dashboard
  - Purpose of the study
  - Photo gallery
  - Testimonials
  - Navigation guide
- Click **"Start Navigating Dashboard"** to enter the main interface.

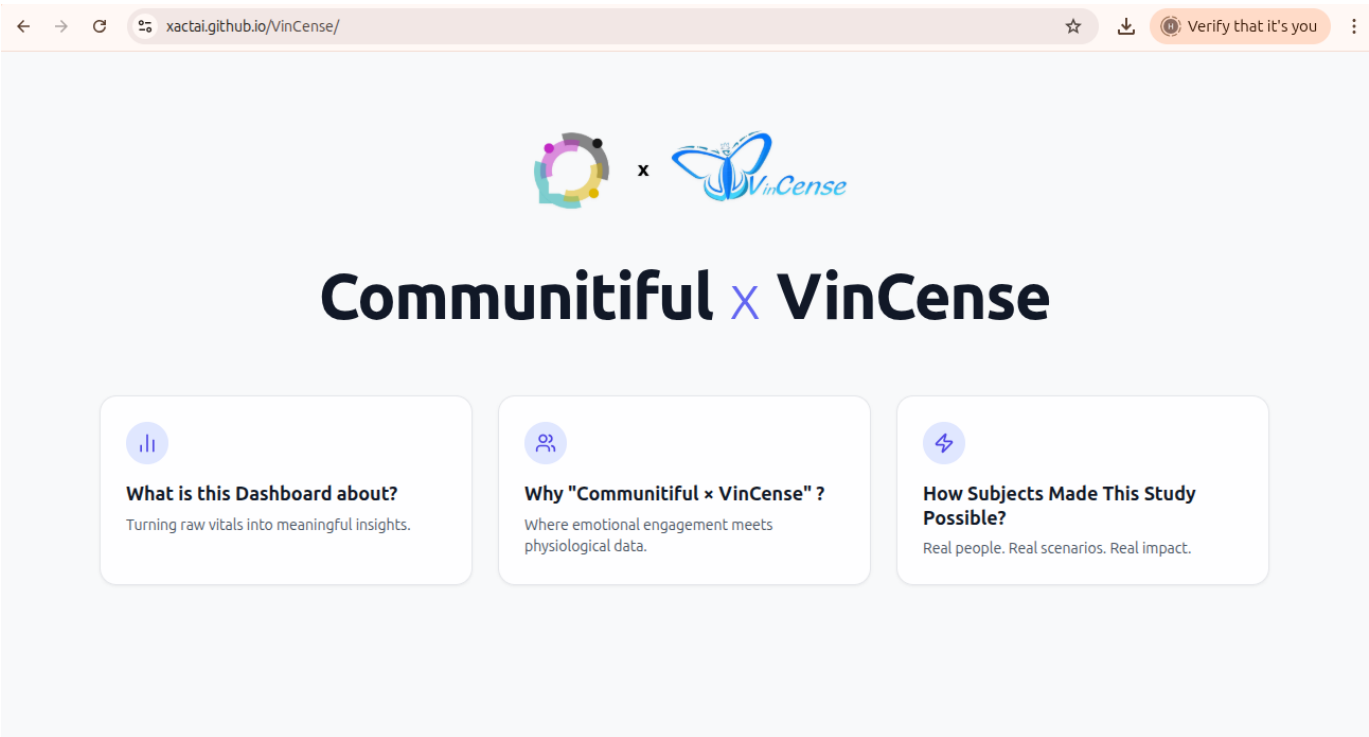

Fig: Communitiful x VinCense Landing Page

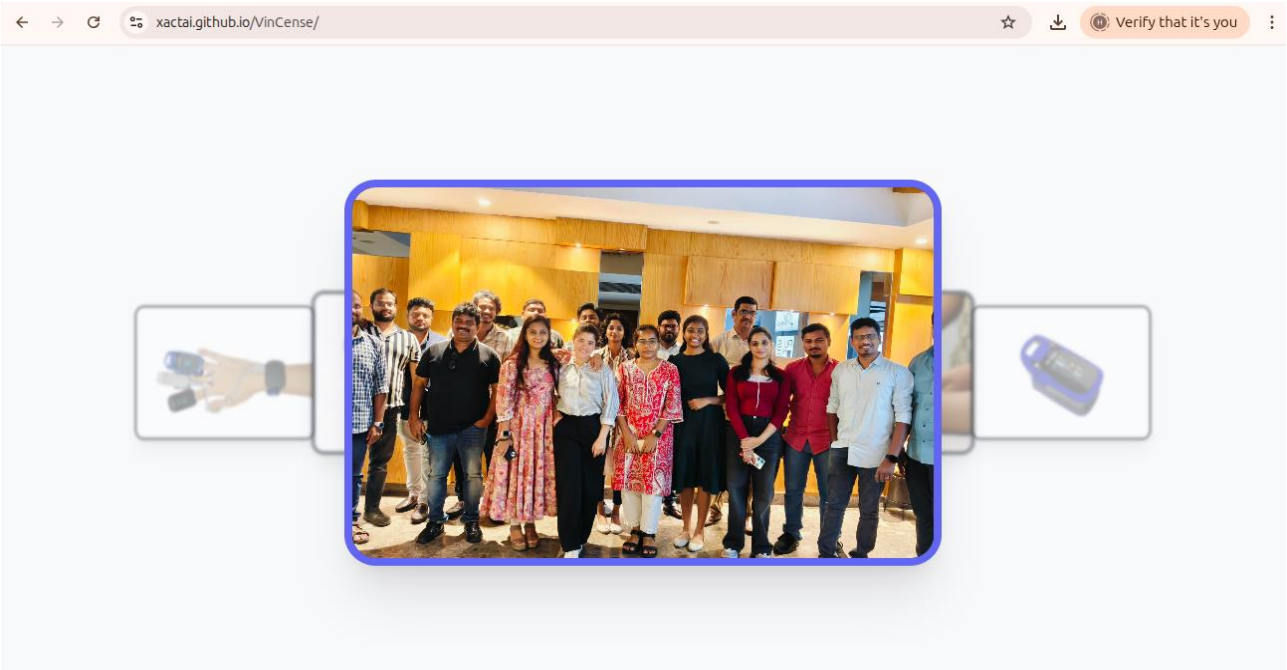

Fig: Communitiful x VinCense Landing Page – Photo Gallery

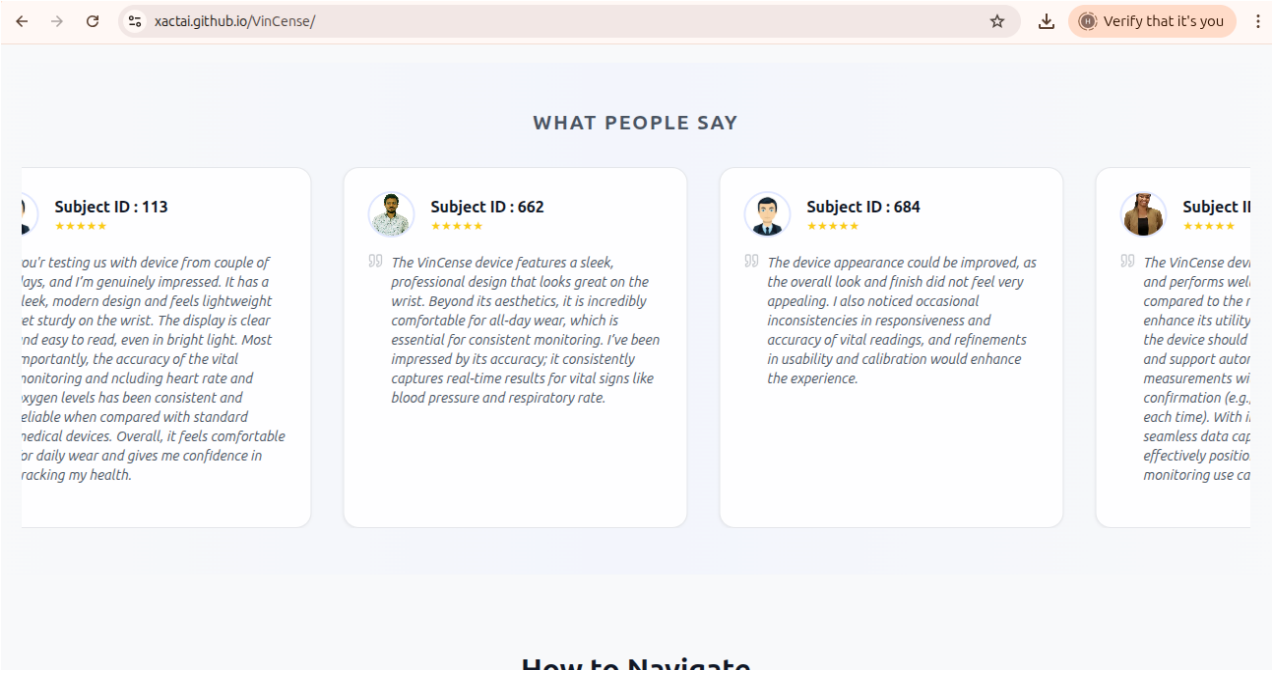

Fig: Communitiful x VinCense Landing Page – Testimonials

3.3 Main Dashboard Layout

After entering:

3.3.1. Sidebar (Left Panel)

Contains:

- **Subject Name Dropdown**
    - Select individual subject or "All Subjects"
- **Date / Range Selector**
    - Choose specific date or date range
- **Sync Vitals Log**
    - Fetch and update latest readings
- **Your Health Profile**
    - Opens personalized health modal
- **Video Gallery**
    - Displays masked subject recordings
- **FAQ**
    - Opens interactive help panel

Xinthe
Excellence Forever...

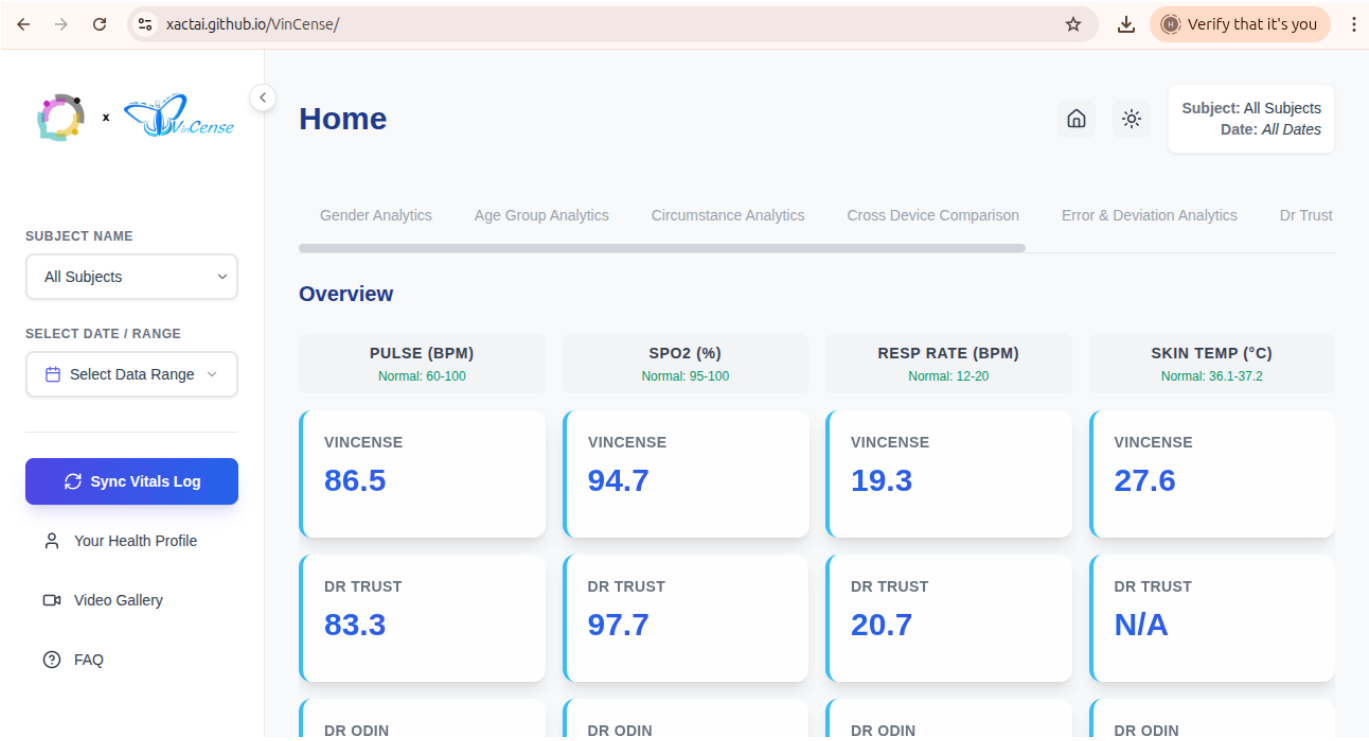

Fig: Fig: Communitiful x VinCense – Side Bar

3.3.2 Top Navigation Tabs

- Gender Analytics
- Age Group Analytics
- Circumstance Analytics
- Cross Device Comparison
- Error & Deviation Analytics
- Dr Trust vs Dr Odin
- VinCense Accuracy Overview
- Data Source

Each tab dynamically updates content based on subject/date filters.

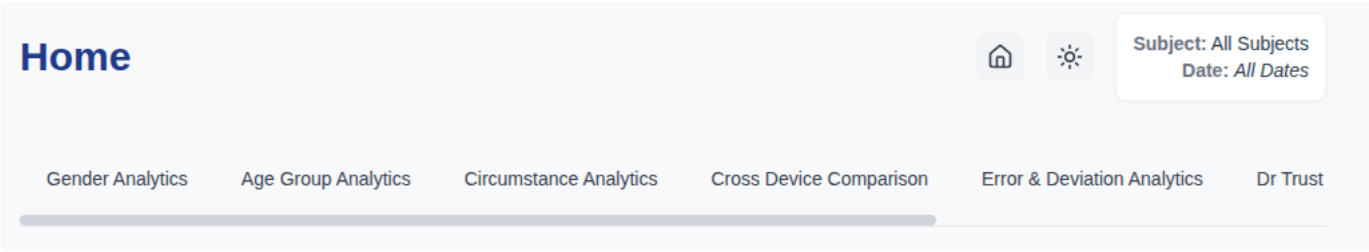

Fig: Communitiful x VinCense – Top Navigation Tabs

3.4 Overview Section

Displays:

- Average vital readings for:
  - VinCense
  - Dr Trust
  - Dr Odin
- Normal reference ranges (IMA/WMA)
- Device performance comparison summary

Purpose:

Quickly assess device accuracy and vital distribution.

Xinthe
Excellence Forever...

Fig: Communitiful x VinCense – Overview Section

3.5 Analytics Modules

3.5.1 Gender Analytics

Includes:

- **Gendered Distribution (Normal Range)**
- **AM vs PM Shift (Diurnal Delta)**
- **Stability Index (CV Over Time)**
- **Zone Analysis (Normal, Warning, Alert)**

All the above charts are implemented for:

- Pulse Rate (bpm)
- SpO_2 (%)
- Respiratory Rate (bpm)
- Skin Temperature (°C)

Purpose:

Identify physiological trends and device bias across genders.

Xinthe
Excellence Forever...

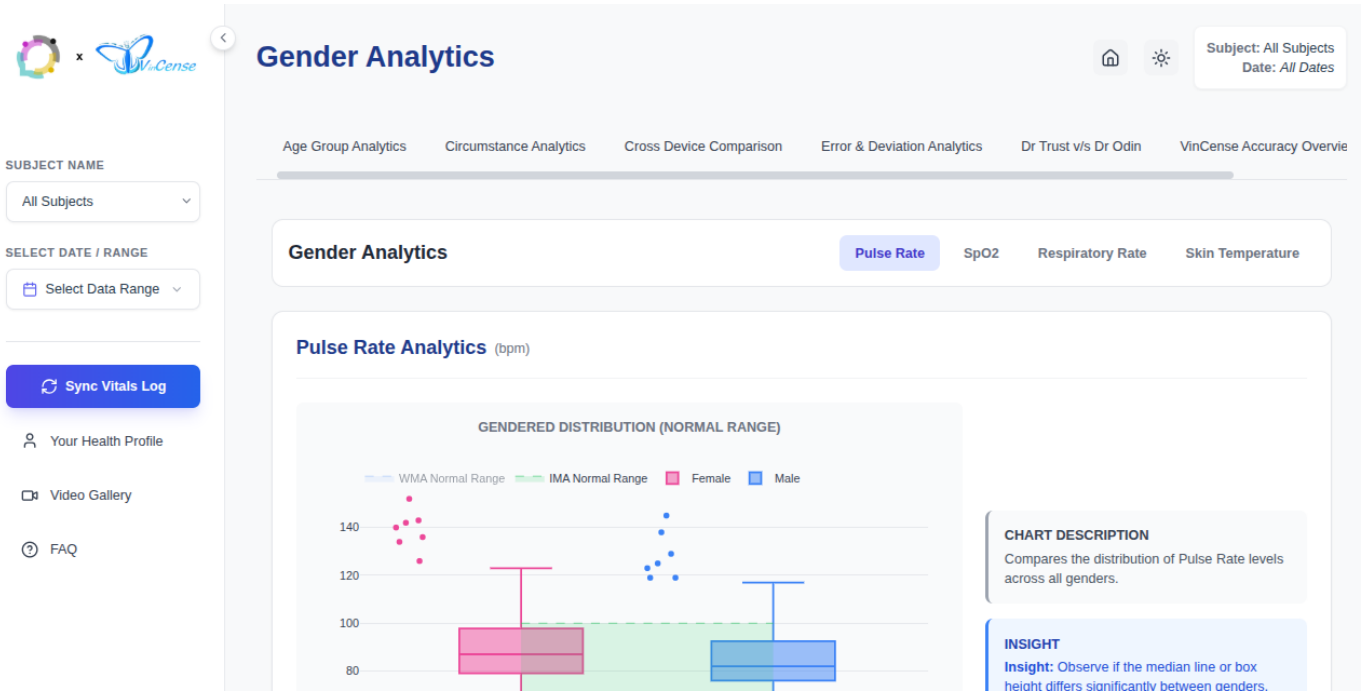

Fig: Communitiful x VinCense – Gender Analytics Tab

3.5.2 Age Group Analytics (18–25, 26–50, 51+)

Includes:

- **Vital Age Radar (Selection vs 30yo / 26–50 Benchmark)**

  (Radar Chart – compares selected group averages against benchmark)
- **Age vs Pulse Rate (Decay Trend)**

  (Scatter Plot with Linear Regression Trend Line)
- **Risk Matrix (Pulse vs Respiratory Rate)**

  (Quadrant Chart – physiological stress zoning)
- **Biological Clock (AM vs PM Intensity)**

  (Polar Area Chart – diurnal rhythm comparison)
- **Subject Stability Heatmap (Daily Pulse CV)**

  (Heatmap – variability across subjects and dates)

These charts collectively analyze age-based physiological trends, stability, stress zoning, and circadian patterns across the dataset.

Purpose:

Validate device reliability across demographic bands.

Xinthe
Excellence Forever...

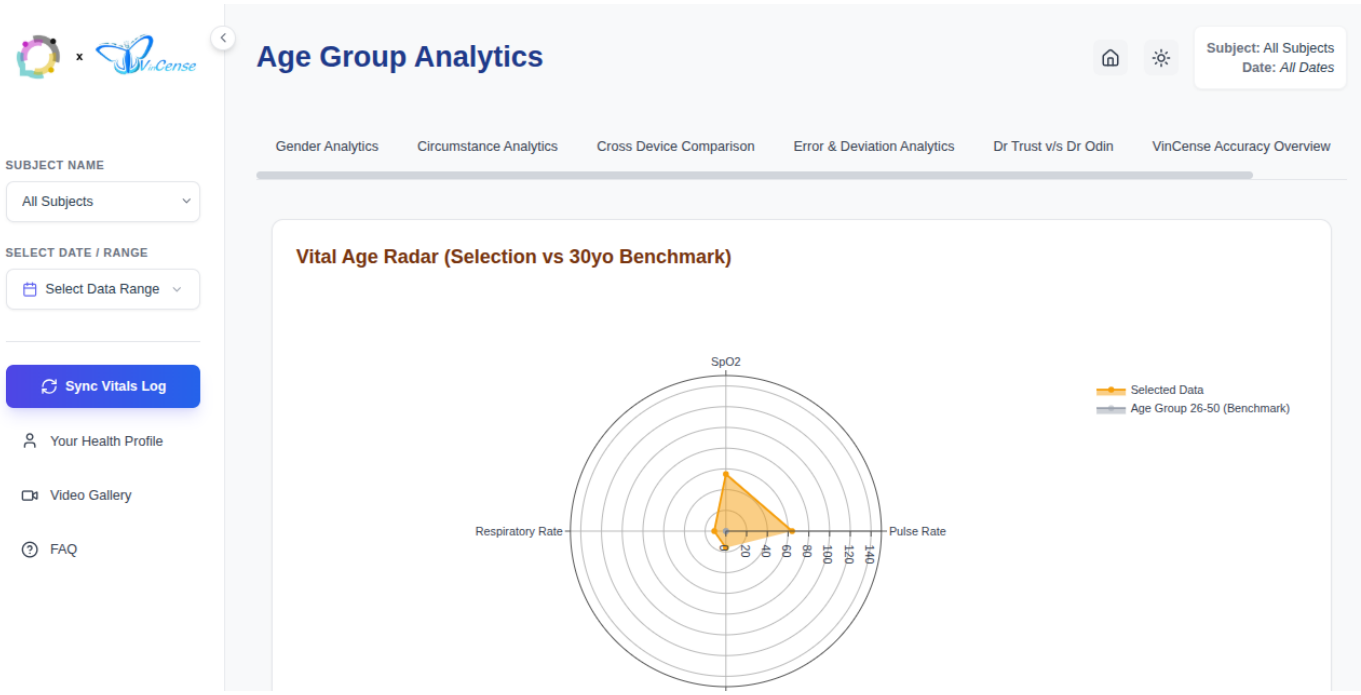

Fig: Communitiful x VinCense – Age Group Analytics Tab

3.5.3 Circumstance Analytics

Conditions include:

- At Desk
- Post Walk
- Standing
- In a Meeting
- Post Meeting
- Before Lunch
- Start of the Day
- Post Lunch
- Before Leaving Office
- Under the AC
- Before Meeting
- Post Coffee
- Post Breakfast
- Post Tea Break
- Post Climbing Stairs
- Feeling Tensed
- Post Brisk Walk
- Relaxed

Vitals Covered:

- Pulse Rate (bpm)
- SpO_2 (%)
- Respiratory Rate (bpm)
- Skin Temperature (°C)

Charts Included:

- Mean Readings by Circumstance
- VinCense Distribution

Purpose:

Validate physiological realism across circumstances, assess device sensitivity under dynamic conditions, and detect motion artifacts or instability during activity-based measurements.

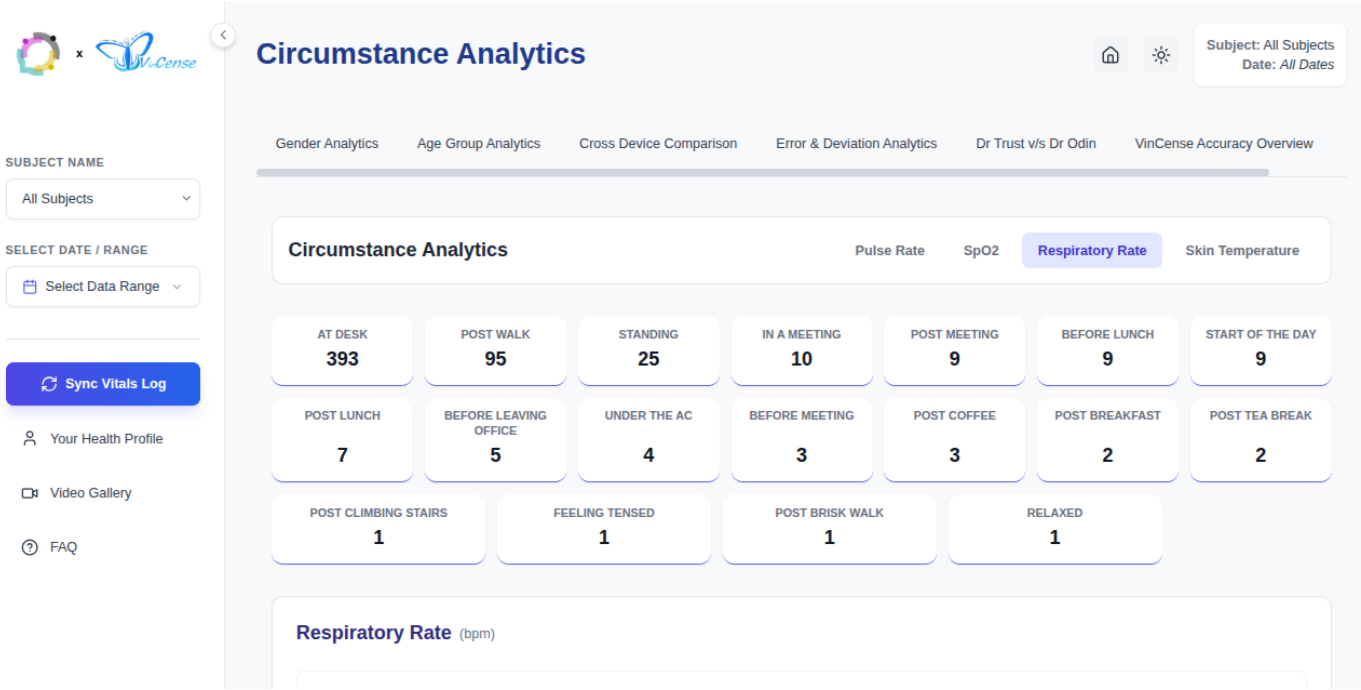

Fig: Communitiful x VinCense – Circumstance Analytics Tab

Xinthe
Excellence Forever...

3.5.4 Cross Device Comparison

Includes:

- Comparative Trend
- Identity plot (VinCense vs Dr Trust)
- Identity plot (VinCense vs Dr Odin)
- Identity plot (Dr Trust vs Dr Odin)

Purpose:

Evaluate accuracy and agreement between devices.

All the above charts are implemented for:

- Pulse Rate (bpm)
- SpO_2 (%)
- Respiratory Rate (bpm)
- Skin Temperature (°C)

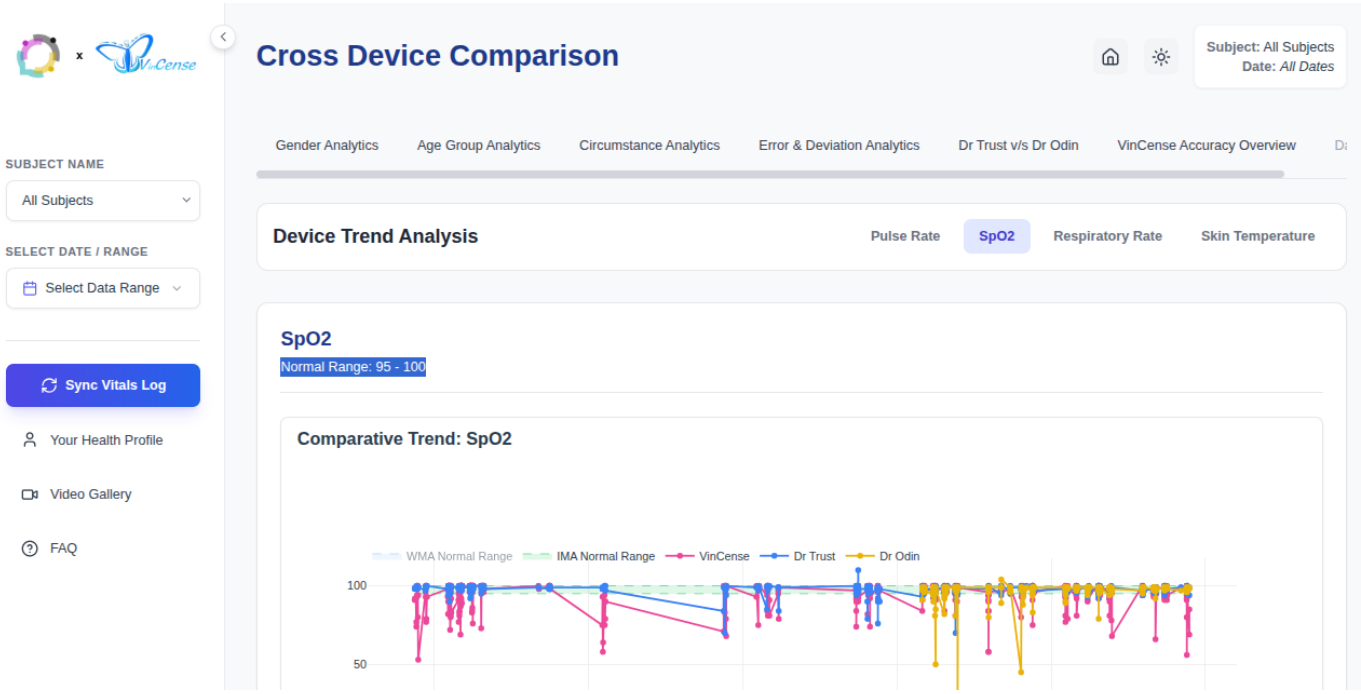

Fig: Communitiful x VinCense – Cross Device Comparison Tab

Xinthe
Excellence Forever...

3.5.5 Error & Deviation Analytics

Vitals Covered:

- Pulse Rate (bpm)
- SpO_2 (%)
- Respiratory Rate (bpm)
- Skin Temperature (°C)

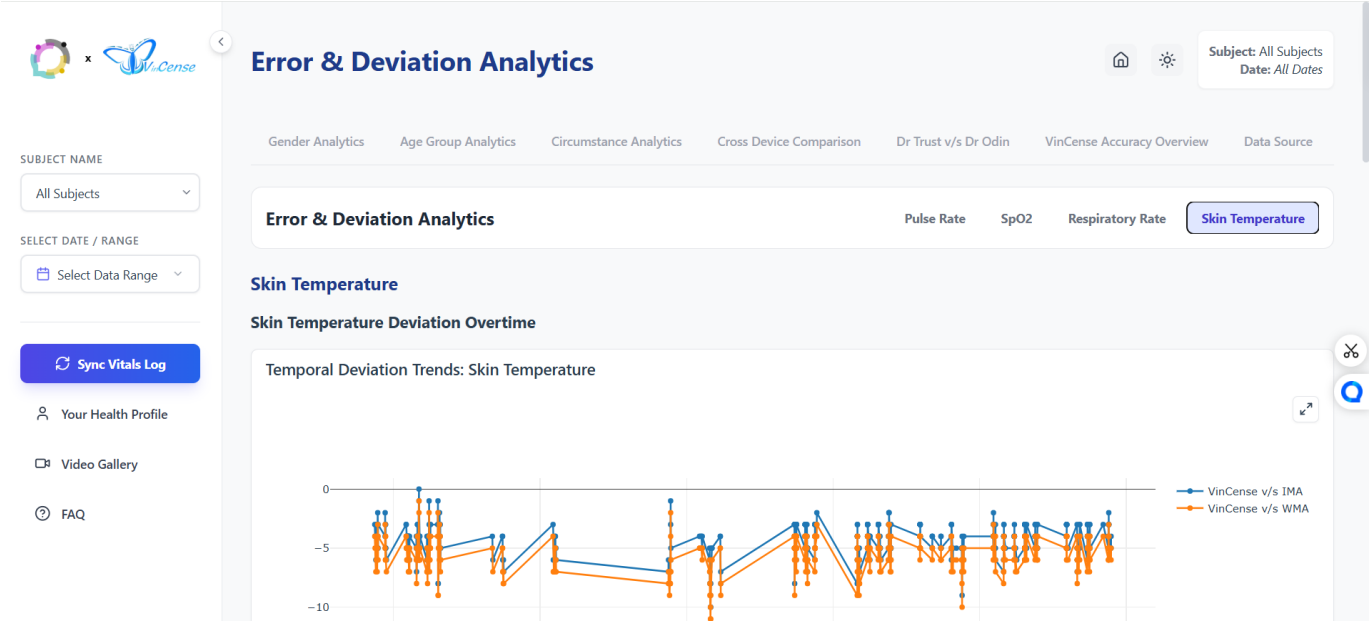

Fig: Communitiful x VinCense - Error & Deviation Analytics Tab

Charts Included:

- Deviation Over Time (Temporal Deviation Trends)
- Bland–Altman: VinCense v/s Dr Odin
- Bland–Altman: VinCense v/s Dr Trust
- Bland–Altman: Dr Trust v/s Dr Odin
- Deviation Distribution (Error Spread Across Devices)
- Summary Statistics (Aggregate Performance Metrics)

Purpose:

Quantify device accuracy, detect systematic bias, evaluate consistency under varying conditions, and identify potential calibration needs or performance risks across all vital parameters.

3.5.6 Dr Trust v/s Dr Odin Analysis

Vitals Covered:

- Pulse Rate (bpm)
- SpO_2 (%)
- Respiratory Rate (bpm)

Fig: Communitiful x VinCense – Dr Trust v/s Dr Odin Analysis Tab

Charts Included:

- Brand Correlation (Scatter Plot with Identity Line)
- Bland–Altman Analysis
- Discrepancy Distribution (Error Magnitude Histogram)
- Reliability (±2% Agreement)
- Average Absolute Deviation by Circumstance (Heatmap)
- Mean Absolute Error (MAE Summary Metric)

Purpose:

Evaluate cross-device consistency, detect calibration bias, quantify clinical interchangeability, and identify activity-based instability or motion-induced disagreement between reference devices.

3.5.7 VinCense Accuracy Overview

Vitals Covered:

- Pulse Rate (bpm)
- SpO_2 (%)
- Respiratory Rate (bpm)
- Skin Temperature (°C)

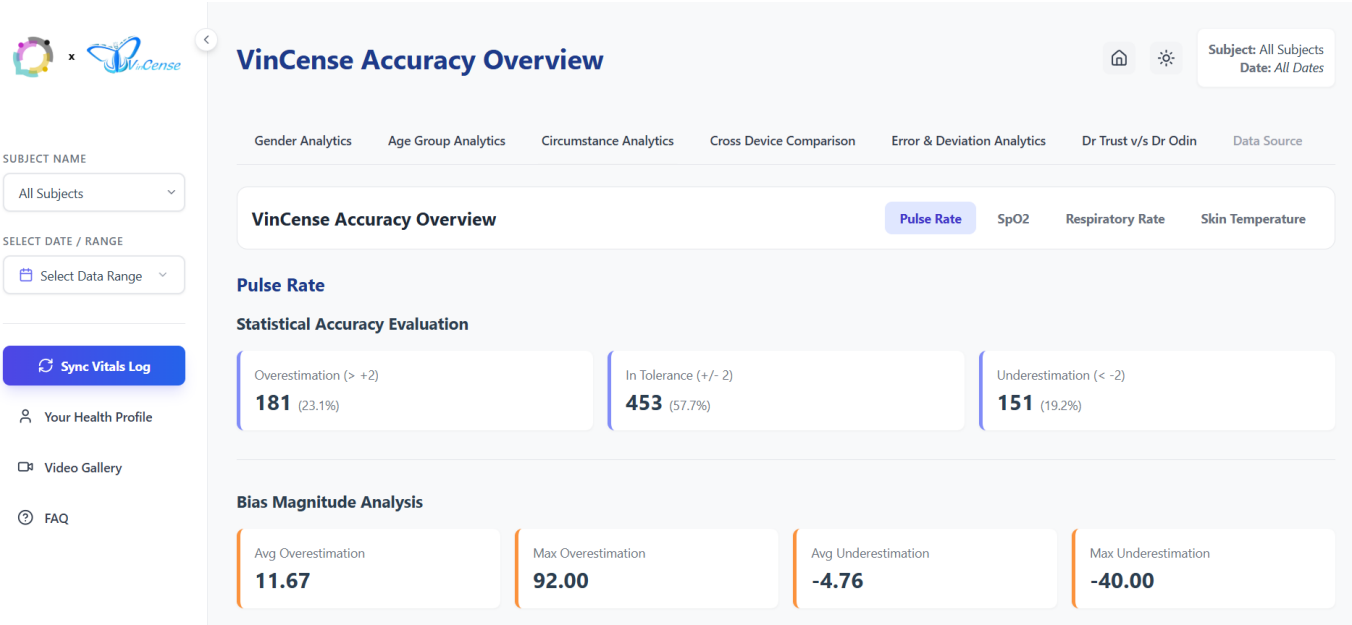

Fig: Communitiful x VinCense – VinCense Accuracy Overview Tab

Charts & Metrics Included:

- Statistical Accuracy Evaluation (Overestimation / In-Tolerance / Underestimation)
- Bias Magnitude Analysis (Avg & Max Over/Under Estimation)
- Deviation Profile vs Reference Devices
- Short-Term Stability (Rolling Standard Deviation)
- Drift Analysis Regression (Accuracy Drift Over Time)
- Anomalous Jump Detection (> Threshold)
- Mean Error by Observational Context (Activity-Based Heatmap)

Purpose:

Assess overall device accuracy, detect systematic bias and calibration offset, monitor stability and drift over time, identify anomalous behavior, and evaluate performance degradation under different real-world activity conditions.

3.5.8 Data Source

Key Features:

- Displays complete raw and consolidated data exactly as present in the Excel sheet.
- Automatically reflects the most recent entries at the top (latest date/time first).
- Allows filtering by Subject and Date for focused data inspection.
- Supports structured viewing of Pulse, SpO_2, Respiratory Rate, and Skin Temperature across devices.
- Provides multiple download options for external use and reporting.

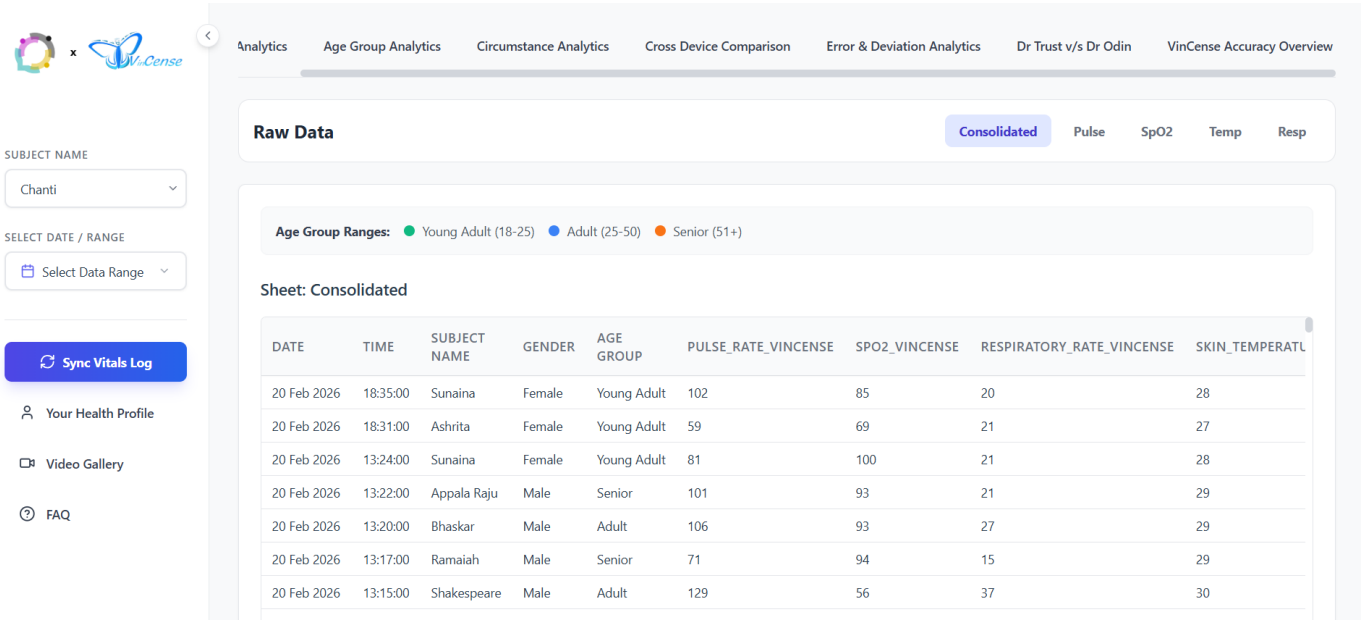

DATE	TIME	SUBJECT NAME	GENDER	AGE GROUP	PULSE_RATE_VINCENSE	SPO2_VINCENSE	RESPIRATORY_RATE_VINCENSE	SKIN_TEMPERATU
20 Feb 2026	18:35:00	Sunaina	Female	Young Adult	102	85	20	28
20 Feb 2026	18:31:00	Ashrita	Female	Young Adult	59	69	21	27
20 Feb 2026	13:24:00	Sunaina	Female	Young Adult	81	100	21	28
20 Feb 2026	13:22:00	Appala Raju	Male	Senior	101	93	21	29
20 Feb 2026	13:20:00	Bhaskar	Male	Adult	106	93	27	29
20 Feb 2026	13:17:00	Ramaiah	Male	Senior	71	94	15	29
20 Feb 2026	13:15:00	Shakespeare	Male	Adult	129	56	37	30

Fig: Communitiful x VinCense – Data Source Tab (All Sheets being Accesible)

Export Options Available:

- Download as CSV
- Download as Excel
- Download as PDF
- Download as Word

Purpose:

Ensure full data transparency, enable auditability of analytics, and allow users to export the dataset in multiple formats for research, validation, or documentation purposes.

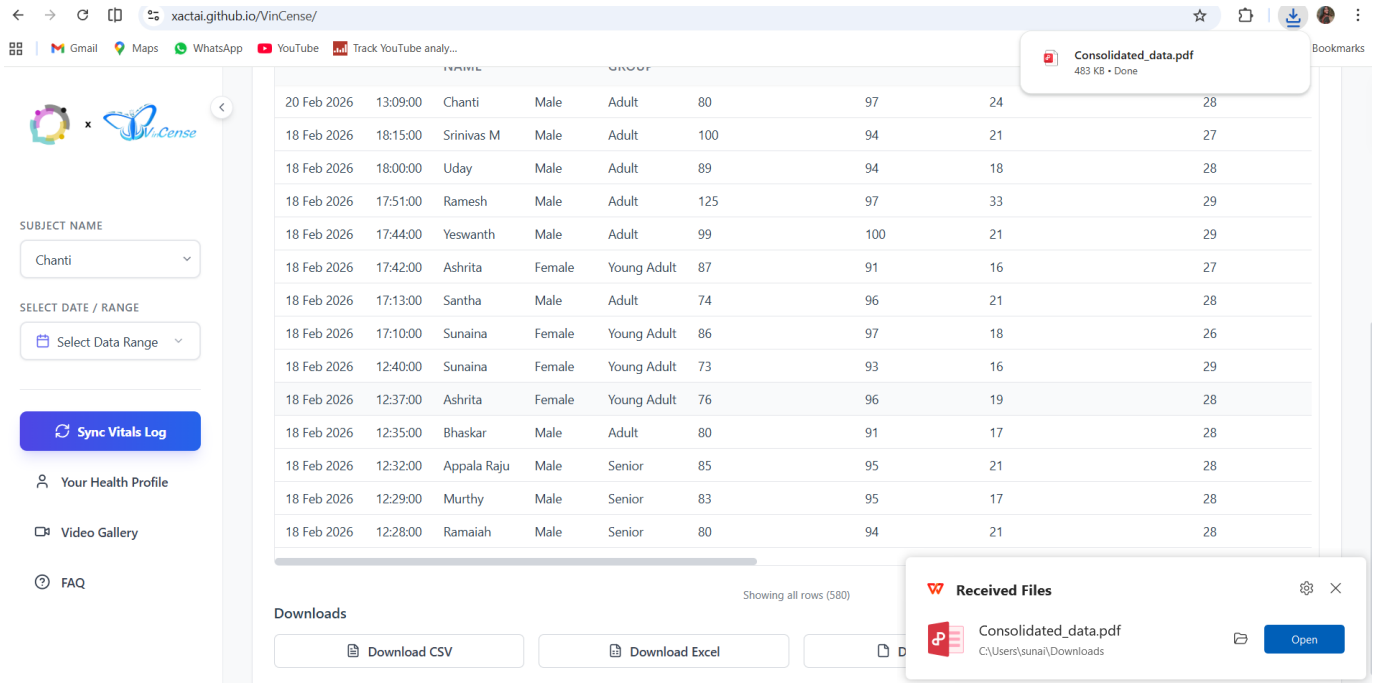

20 Feb 2026	13:09:00	Chanti	Male	Adult	80	97	24	28
18 Feb 2026	18:15:00	Srinivas M	Male	Adult	100	94	21	27
18 Feb 2026	18:00:00	Uday	Male	Adult	89	94	18	28
18 Feb 2026	17:51:00	Ramesh	Male	Adult	125	97	33	29
18 Feb 2026	17:44:00	Yeswanth	Male	Adult	99	100	21	29
18 Feb 2026	17:42:00	Ashrita	Female	Young Adult	87	91	16	27
18 Feb 2026	17:13:00	Santha	Male	Adult	74	96	21	28
18 Feb 2026	17:10:00	Sunaina	Female	Young Adult	86	97	18	26
18 Feb 2026	12:40:00	Sunaina	Female	Young Adult	73	93	16	29
18 Feb 2026	12:37:00	Ashrita	Female	Young Adult	76	96	19	28
18 Feb 2026	12:35:00	Bhaskar	Male	Adult	80	91	17	28
18 Feb 2026	12:32:00	Appala Raju	Male	Senior	85	95	21	28
18 Feb 2026	12:29:00	Murthy	Male	Senior	83	95	17	28
18 Feb 2026	12:28:00	Ramaiah	Male	Senior	80	94	21	28

Fig: Communitiful x VinCense – Data Source Tab – Can be Easily Downloaded in Required Format

3.6 Health Profile Modal

Access via **"Your Health Profile"**

Features:

- Average vitals for selected subject
- Status classification:
  - All Good
  - Slight Variation
  - Keep an Eye On
  - Needs Prompt Review
- Dynamic health tips
- Avoidance suggestions
- Color-coded severity indicators

Purpose:

Provide subject-specific observational health summary.

Xinthe
Excellence Forever...

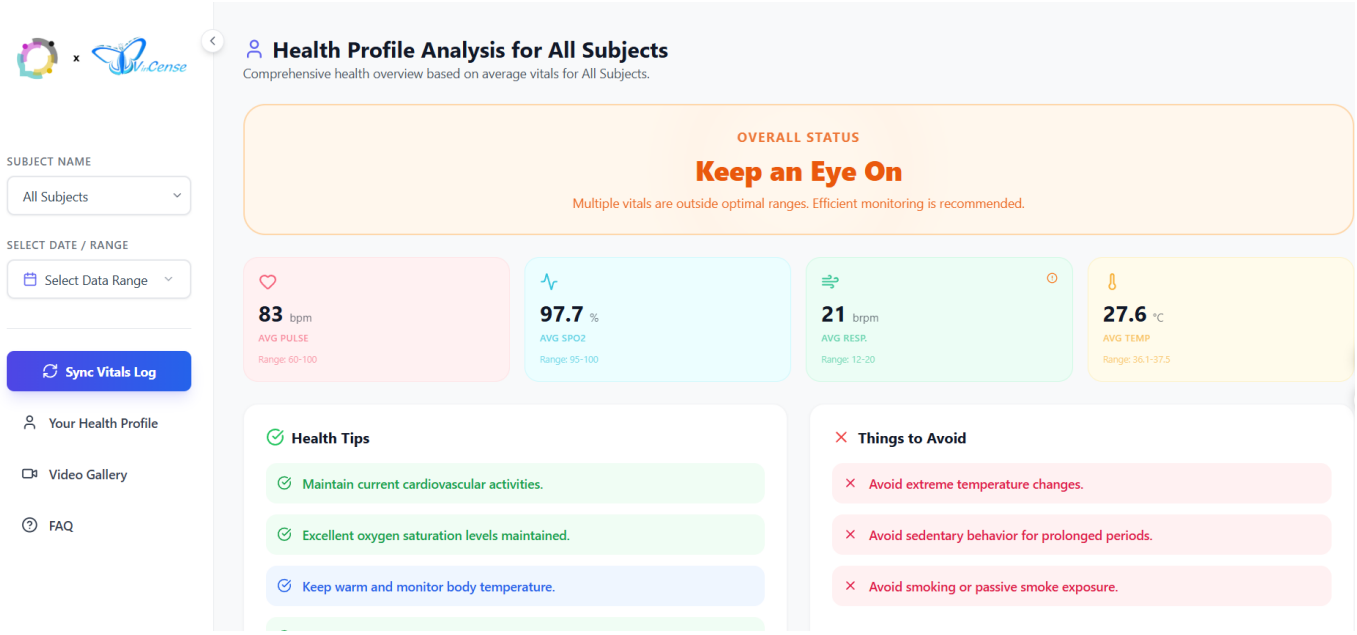

Fig: Communitiful x VinCense – Health Profile Section

3.7 Video Gallery

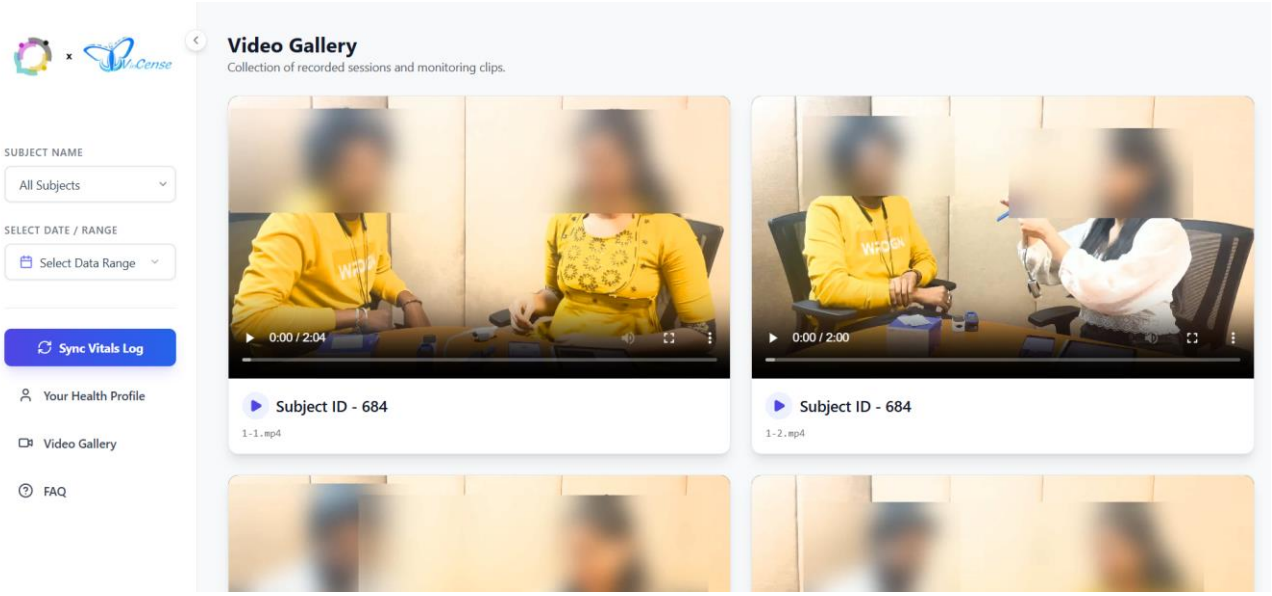

Fig: Communitiful x VinCense – Video Gallery Section – With Masked Videos

- Displays masked subject recordings
- Supports playback
- Designed for research transparency and validation
- Maintains privacy compliance

Xinthe
Excellence Forever...

3.8. FAQ & Help Panel

Interactive side panel includes:

- Device & Measurement
- About VinCense
- Data & Analytics
- Subjects & Participation
- Environment & Conditions.

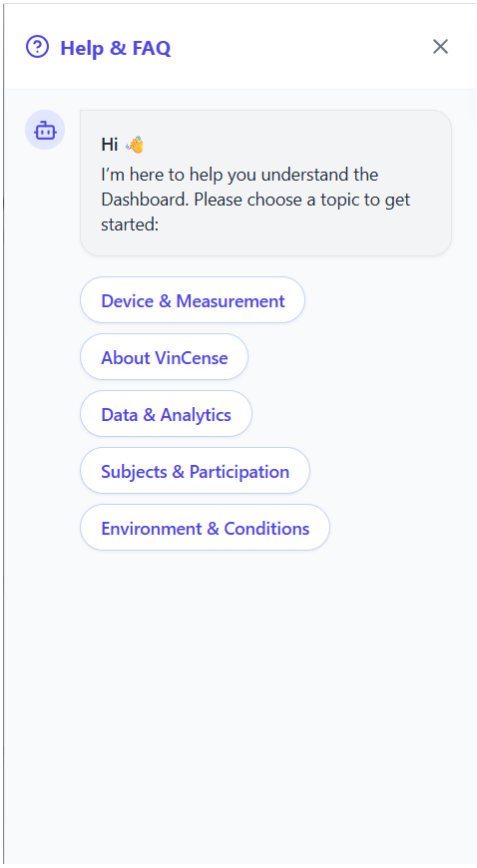

Fig: Communitiful x VinCense – FAQ Section

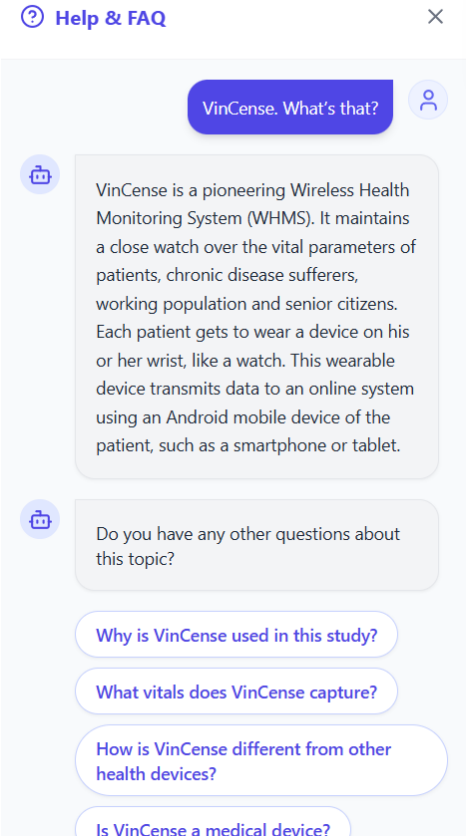

Fig: Communitiful x VinCense – FAQ & Answer

Purpose:

Educate users and explain analytics interpretation

3.9. Add Vitals

- Opens external data entry sheet
- Allows manual entry of vitals
- Updates dashboard upon synchronization

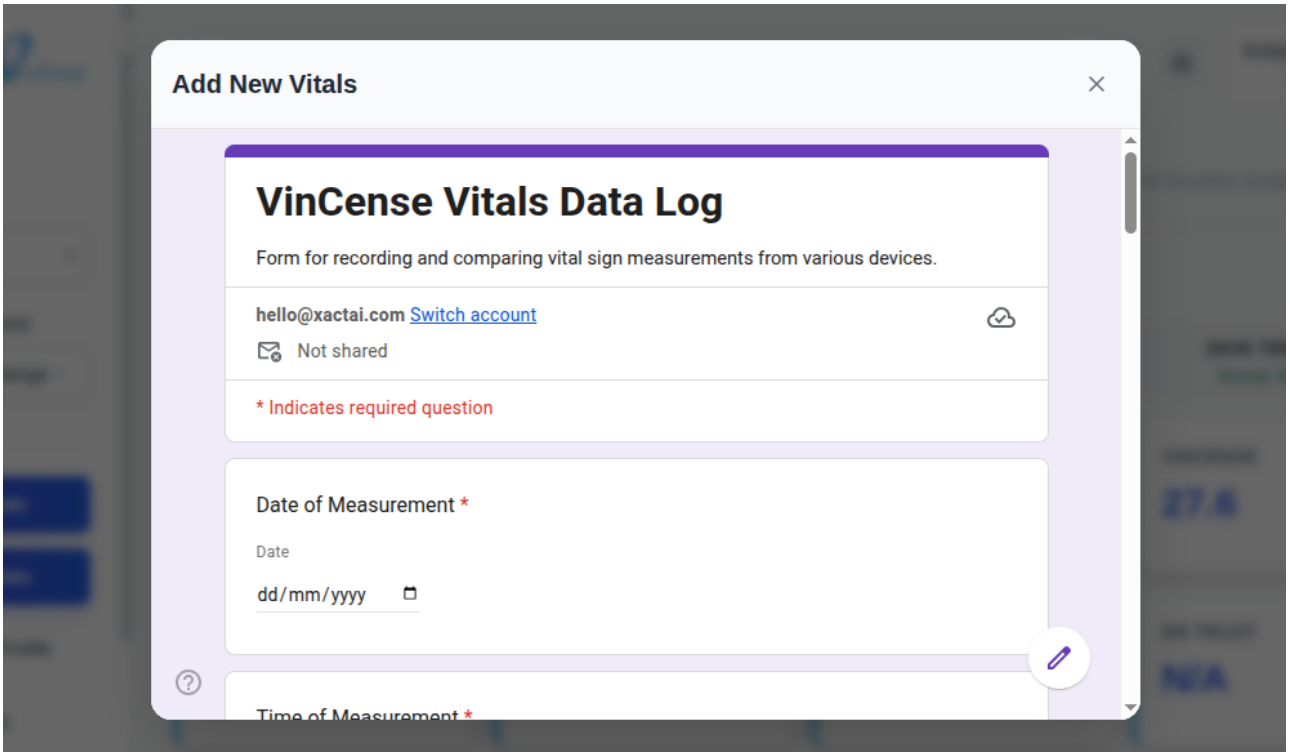

Fig: Communitiful x VinCense – Google Form being accesed in the Dashboard

3.10. Sync Vitals

- Fetches latest data
- Displays success confirmation
- Updates all analytics automatically

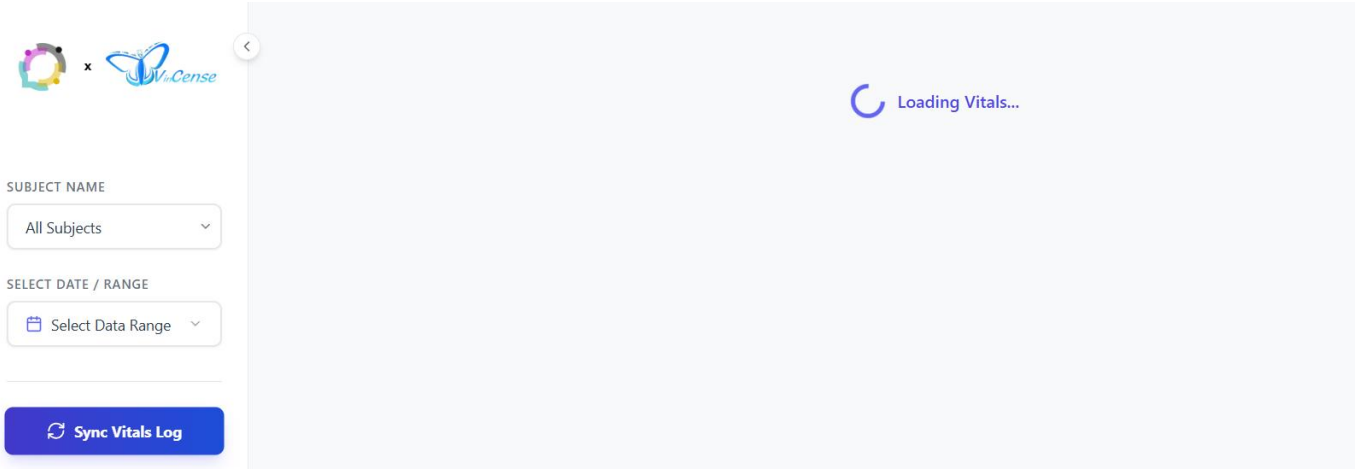

Fig: Communitiful x VinCense – Vitals Being Synced into the Dashboard

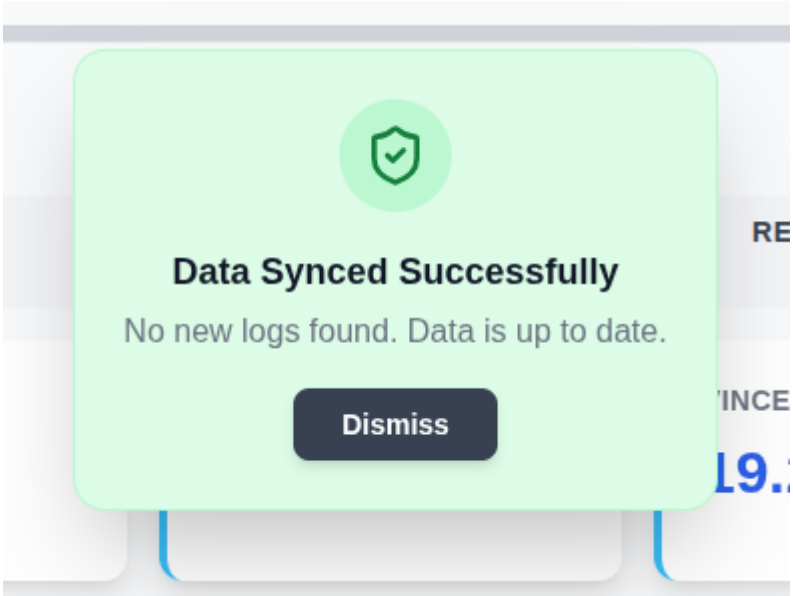

Fig: Communitiful x VinCense – Pop up Confirming Successful Syncing of Vitals

3.11. Theme Toggle

- Switch between Light and Dark mode
- Maintains readability and professional aesthetic

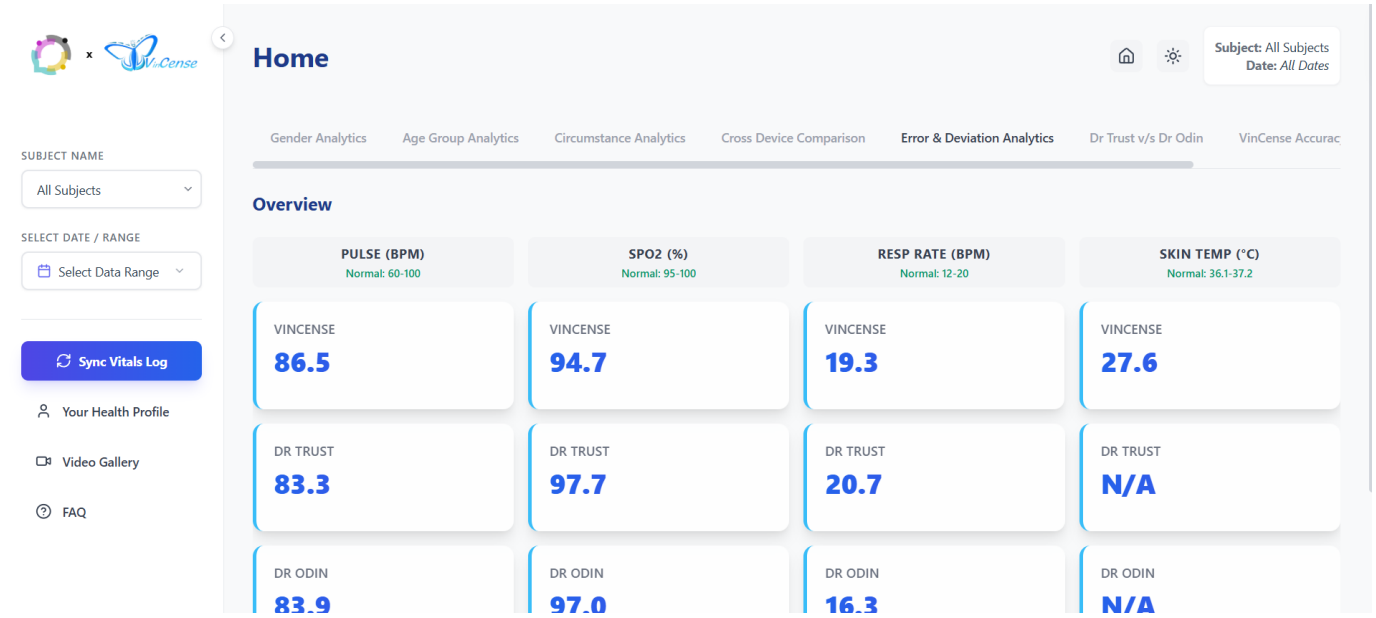

Fig: Communitiful x VinCense – Light Theme

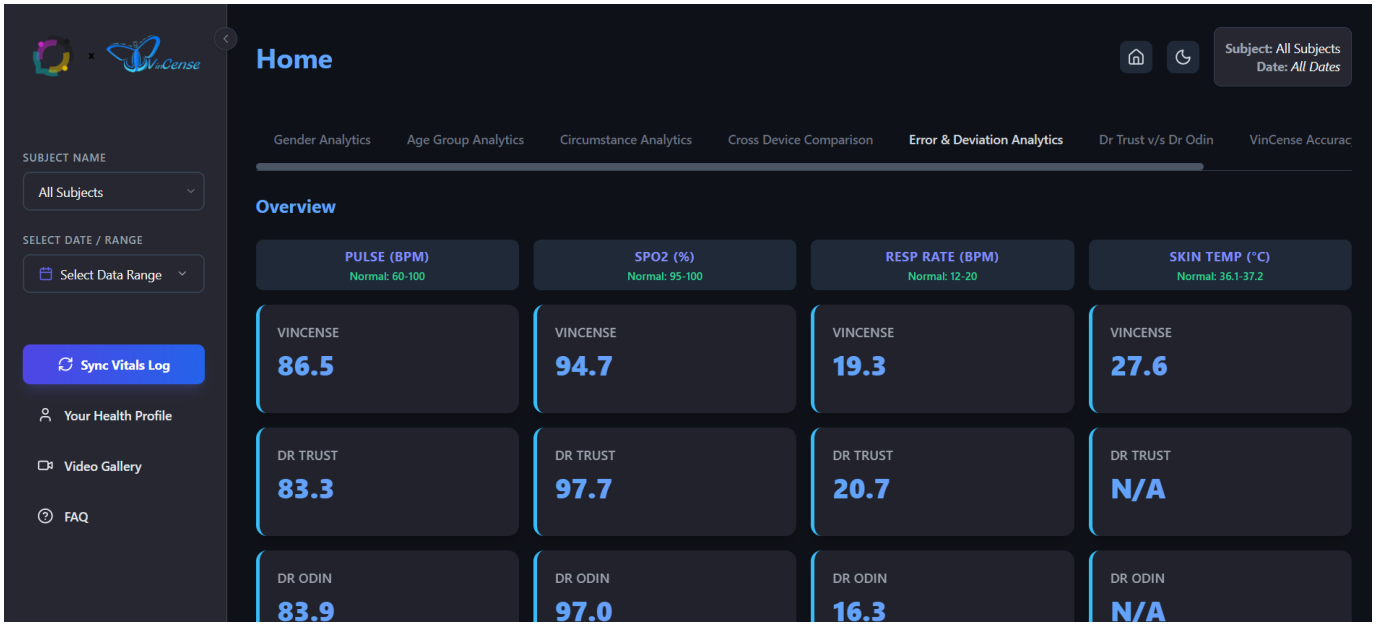

Fig: Communitiful x VinCense – Dark Theme

Xinthe
Excellence Forever...

3.12. Data Filtering Logic

All analytics dynamically respond to:

- Selected subject
- Date range
- Tab selection

Ensures contextual and precise analysis.

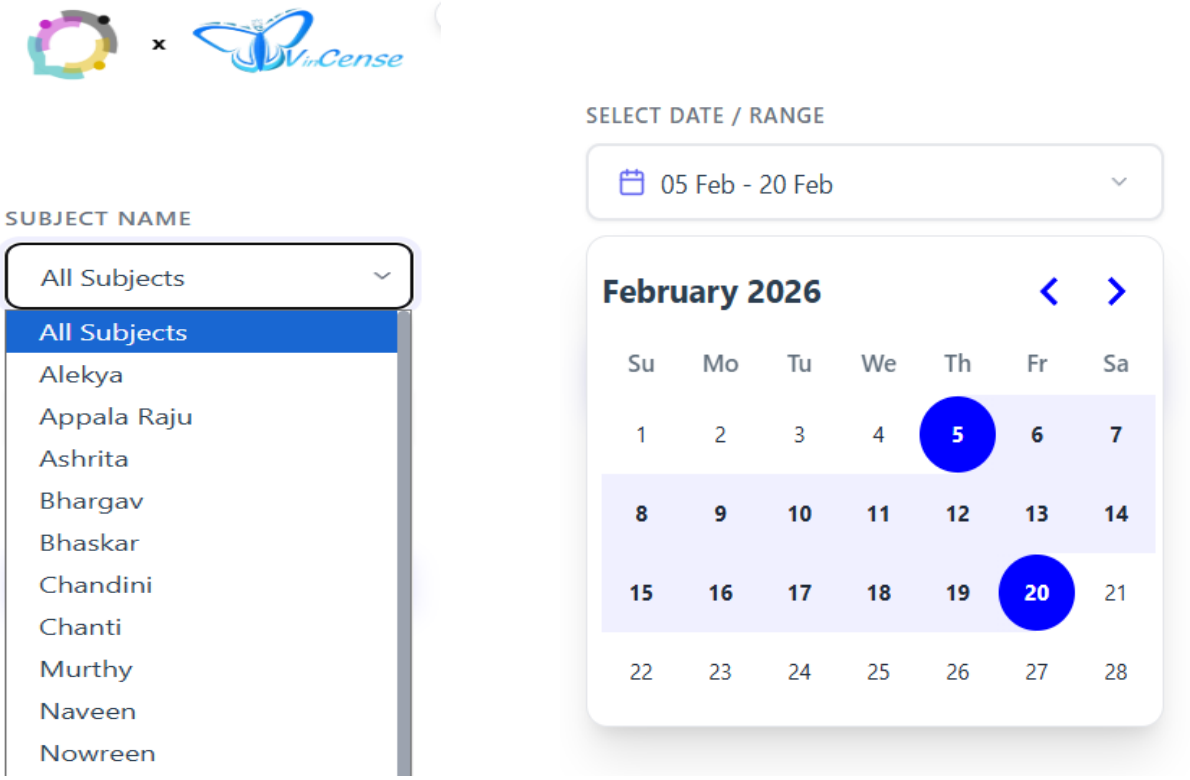

Fig: Communitiful x VinCense – Subject Selection Dropdown & Date Selection Calender

3.13. Intended Usage

This dashboard is designed for:

- Research validation
- Device benchmarking
- Demographic trend analysis
- Clinical observational study
- Continuous monitoring exploration

3.14. Overview

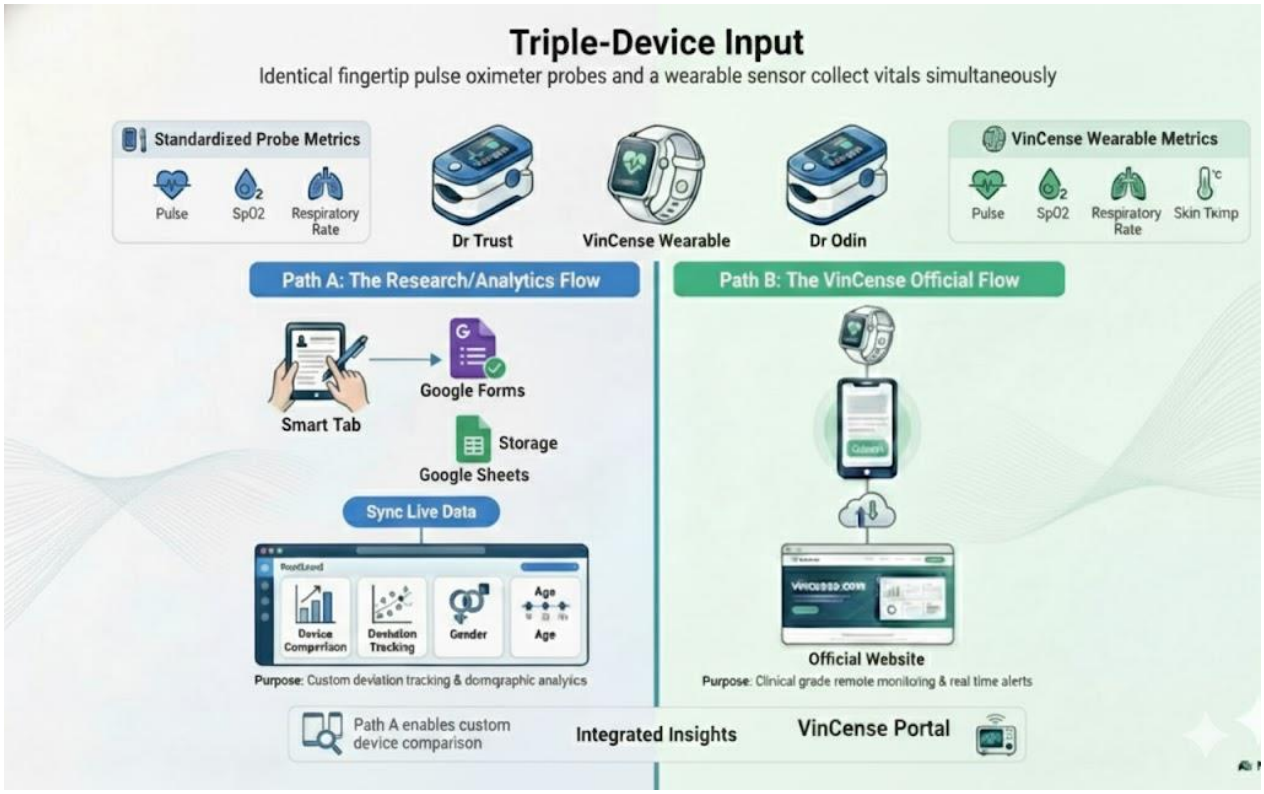

Fig: Overall Flow of Communitiful x VinCense