




Certificate of Hydrophone Calibration

Hydrophone:	Onda HNR-1000 S/N: 1837
Cable/Adaptor:	NONE
External Amplifier:	NONE
Electrical Loading:	OpenCircuit
Temperature:	23.5 deg C
Calibration Completed:	19-May-2017
Data File Name:	HNR1000-1837_XXXXXX-XXXX-XX_XX_20170519.txt

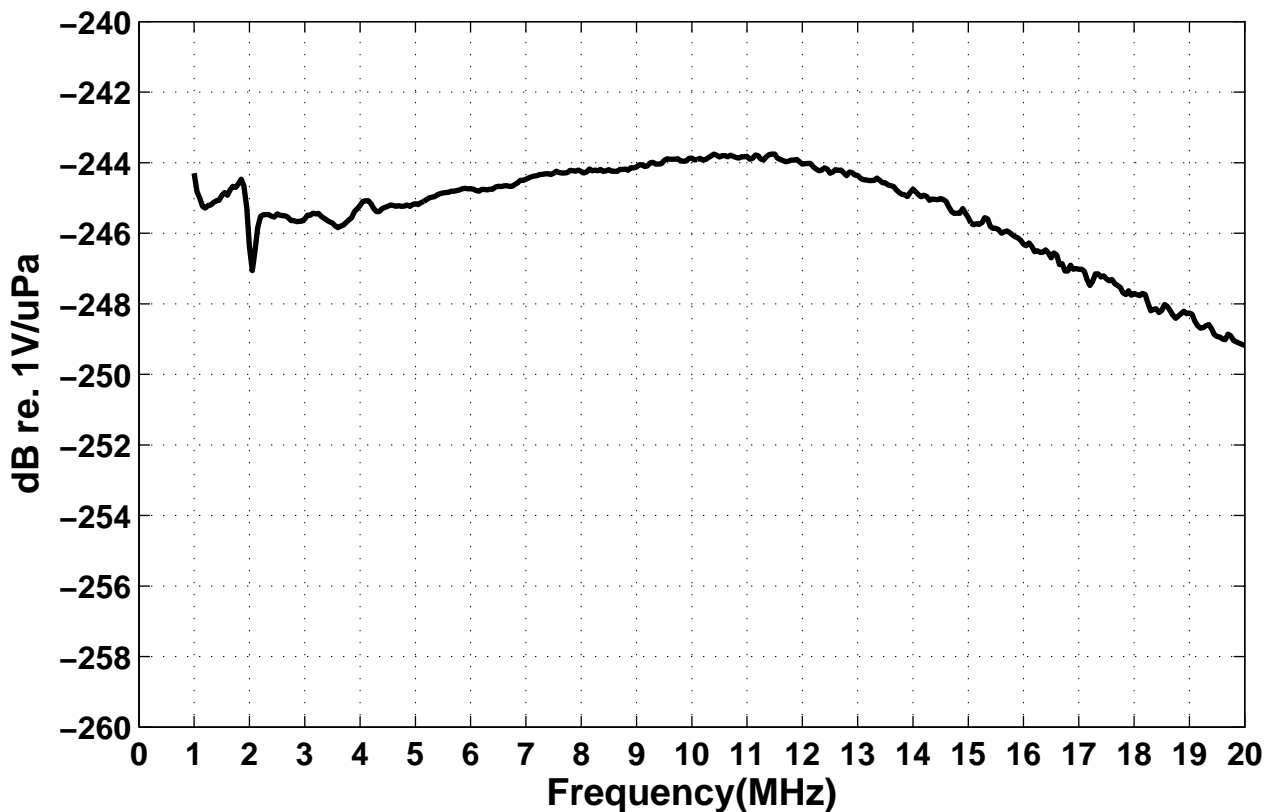

Calibration Method: Stepped single frequency comparison to Reference Standard

Measurement Uncertainty: 1-15 MHz: 1 dB; 15-20 MHz: 1.5 dB

Signature:  Date: 19-May-2017

1290 Hammerwood Avenue, Sunnyvale, CA 94089 T: (408) 745-0383 F: (408) 745-0956
www.ondacorp.com