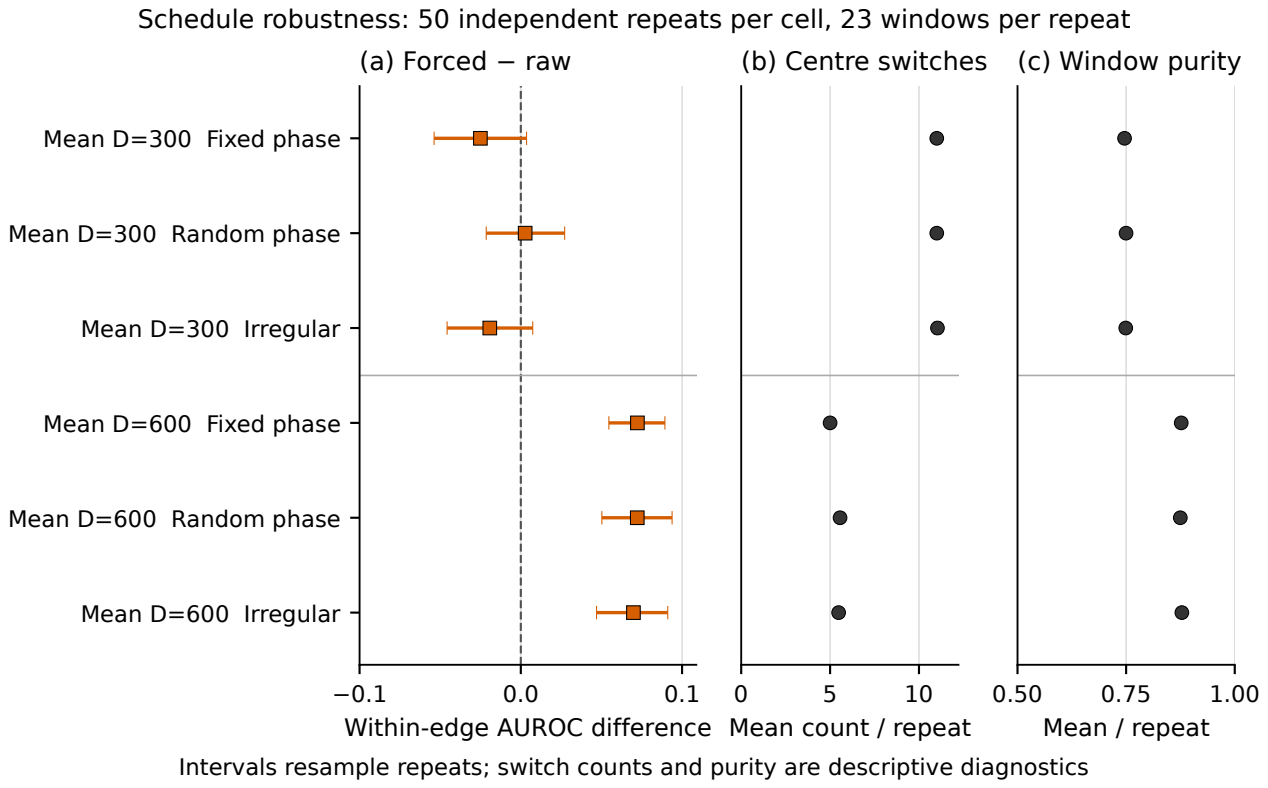
Schedule robustness: 50 independent repeats per cell, 23 windows per repeat
(a) Forced − raw
(b) Centre switches
(c) Window purity
Mean D=300 Fixed phase
Mean D=300 Random phase
Mean D=300 Irregular
Mean D=600 Fixed phase
Mean D=600 Random phase
Mean D=600 Irregular
−0.1
0.0
0.1
0
5
10
0.50
0.75
1.00
Within-edge AUROC difference
Mean count / repeat
Mean / repeat
Intervals resample repeats; switch counts and purity are descriptive diagnostics