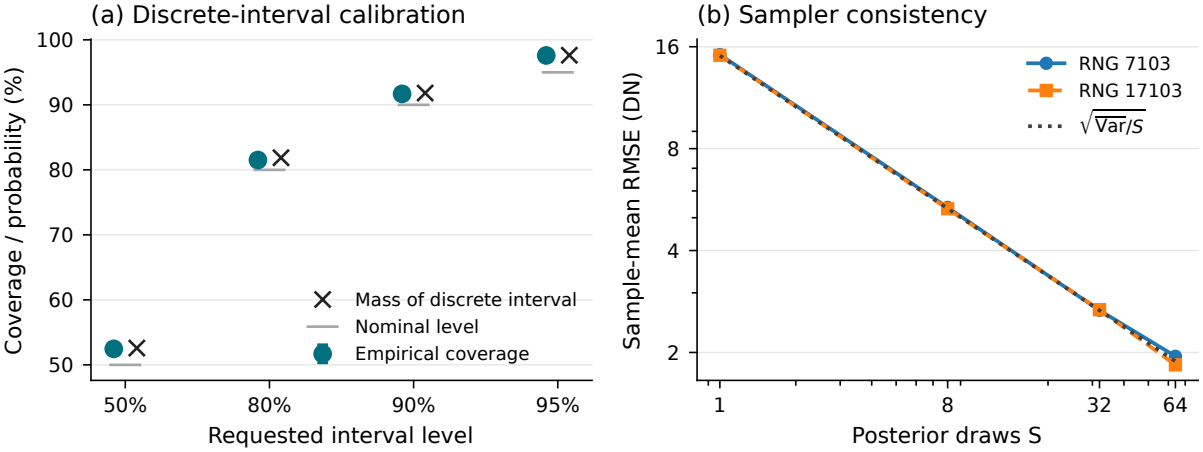
(a) Discrete-interval calibration
Coverage / probability (%)
100
90
80
70
60
50
50%
80%
90%
95%
Requested interval level
Mass of discrete interval
Nominal level
Empirical coverage
(b) Sampler consistency
Sample-mean RMSE (DN)
16
8
4
2
1
8
32
64
Posterior draws S
RNG 7103
RNG 17103
$\sqrt{\mathrm{Var}/S}$