

## Research Article

# A Detailed Research on Human Health Monitoring System Based on Internet of Things

Lei Ru <sup>1</sup>, Bin Zhang <sup>2</sup>, Jing Duan <sup>3</sup>, Guo Ru <sup>4</sup>, Ashutosh Sharma <sup>5</sup>, Gaurav Dhiman,<sup>6</sup>  
Gurjot Singh Gaba <sup>7</sup>, Emad Sami Jaha,<sup>8</sup> and Mehedi Masud <sup>9</sup>

<sup>1</sup>College of Physical Education, Fuyang Normal University, Fuyang 236041, China

<sup>2</sup>Anhui University of Chinese Medicine, Hefei 230012, China

<sup>3</sup>Middle School Affiliated to Fuyang Normal University, Fuyang 236037, China

<sup>4</sup>Graduate School, Beijing Sport University, Beijing 100084, China

<sup>5</sup>Institute of Computer Technology and Information Security, Southern Federal University, Russia

<sup>6</sup>Government Bikram College of Commerce, Punjab, India

<sup>7</sup>School of Electronics and Electrical Engineering, Lovely Professional University, Punjab 144411, India

<sup>8</sup>Department of Computer Science, Faculty of Computing and Information Technology, King Abdulaziz University, Jeddah 21589, Saudi Arabia

<sup>9</sup>Department of Computer Science, College of Computers and Information Technology, Taif University, P. O. Box 11099, Taif 21944, Saudi Arabia

Correspondence should be addressed to Bin Zhang; [binzhang231@outlook.com](mailto:binzhang231@outlook.com) and Mehedi Masud; [mmasud@tu.edu.sa](mailto:mmasud@tu.edu.sa)

Received 25 February 2021; Revised 7 April 2021; Accepted 3 May 2021; Published 15 May 2021

Academic Editor: Deepak Gupta

Copyright © 2021 Lei Ru et al. This is an open access article distributed under the Creative Commons Attribution License, which permits unrestricted use, distribution, and reproduction in any medium, provided the original work is properly cited.

The technological advent in smart sensing devices and the Internet has provided practical solutions in various sectors of networking, public and private sector industries, and government organizations worldwide. This study intends to combine the Internet of Things (IoT) technology with health monitoring to make it personalized and timely through allowing the interconnection between the devices. This work is aimed at exploring various wearable health monitoring modules that people wear to monitor heart rate, blood pressure, pulse, body temperature, and physiological information. The information is acquired using the wireless sensor to create a health monitoring system. The data is integrated using the Internet of Things for processing, connecting, and computing to achieve real-time monitoring. The temperature of three people measured by the temperature thermometer is 36.4, 36.7, and 36.5 (°C), respectively, and the average acquired by the monitoring system of the three people is 36.5, 36.4, and 36.5 (°C), respectively, indicating that the system demonstrated relatively accurate and stable testability. The user's ECG is displayed clearly and conveniently using the ECG acquisition system. The pulse rate of the three people tested by the system is 78, 78, and 79 (times/min), respectively, similar to the medical pulse meter results. The physiological information acquired using the semantic recognition, matching system, and character matching system is relatively accurate. It concludes that the human health monitoring system based on the Internet of Things can provide people with daily health management, instrumental in heightening health service quality and level.

## 1. Introduction

In 2017, the *Report on the Status of Chinese Residents' Nutrition and Chronic Diseases* issued by the Ministry of Health pointed out that the mortality rate of chronic diseases, represented by cardiovascular diseases and diabetes, is about 85.5% each year, and chronic diseases account for about

75% of all diseases in China [1]. Internet healthcare focuses on chronic high-risk diseases and subhealthy groups due to many subhealthy groups, together with the long course, complex etiology, and high treatment costs of chronic diseases. It follows that human health monitoring based on the Internet of Things (IoT) is popularized. As a result of the rapidly expanded aging population in China and the improvement

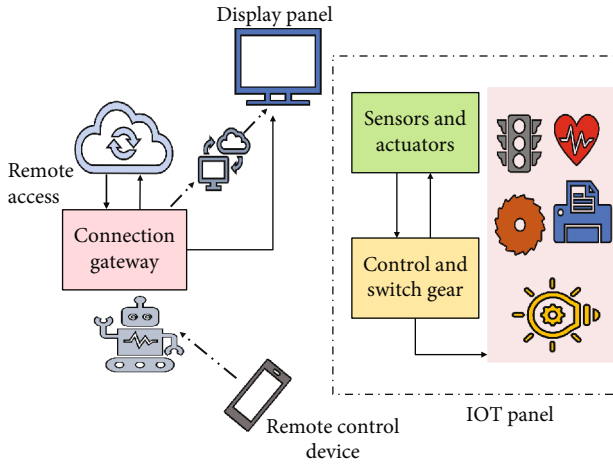


FIGURE 1: IoT architecture.

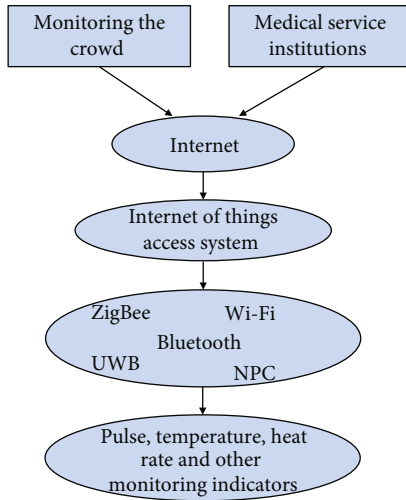


FIGURE 2: The framework of health monitoring and medical information system based on the Internet of Things.

of living standards, the subhealthy population increases with chronic diseases. Creating efficient, convenient, safe, and reliable healthcare conditions and services is a basic need for Chinese people. It is highly urgent to develop a health monitoring system to achieve remote real-time health monitoring [2–4].

IoT technology uses smart sensing devices and the Internet to provide an effective solution to the challenges faced by the networks, public and private sector industries, and government organizations worldwide [5]. The IoT innovations have emerged a new paradigm in using smart systems and intelligent devices to analyze data for various applications [6–10]. A basic IoT structure with generalized architecture is presented in Figure 1.

The various applications [11–15] in which IOT can comprise security and surveillance, automation of agriculture, healthcare, traffic management, the emergence of smart cities, etc. [16–19]. At present, there has not been a unified concept of the Internet of Things. Li Hang defines the Internet of

Things as a kind of Internet that is based on various information sensors, radio frequency identification technology, global positioning system, infrared sensors, light, heat, electricity, machinery, chemistry, biology, location, and other information of a target [20]. Health monitoring is the continuous collection of individual health-related physiological parameters and related influence factors through a certain monitoring system. That follows the process, analysis, and summarization of data to generate health-related information spread to the corresponding individuals or groups, guiding disease prevention and control, promoting health management, and accelerating health conditions.

At present, there is a variety of studies on human health monitoring systems based on the Internet of Things worldwide. The development of human health monitoring systems based on the Internet of Things in foreign countries is earlier than that in China. Significant progress has been made in remote consultation and remote monitoring of blood pressure, blood glucose values, and some medical data (long-distance transmission). Rezaeibagha and Mu [21] designed an Agent system that can monitor vital signs such as blood pressure, pulse, respiratory rate, and body temperature, which was connected to wireless sensors. Agnisarman et al. [22] have designed a remote video medical diagnosis system, which used the Internet of Things technology to facilitate the doctor's medical diagnosis process, with multifunctional modes such as online consultation and video dialogue. Mugica et al. [23] designed an ECG monitor matched with the Android system's intelligent terminal to realize remote monitoring. Tamilselvi et al. [24] proposed a health monitoring system that can assess patients' primary symptoms like their oxygen level, body temperature, and eye movement using the IoT platform. Acharya et al. [25] developed a kit for healthcare monitoring using the IoT platform to assess the parameters like a heartbeat, ECG, temperature, and respiration using various intelligent sensors. The major limitation of this system is that data visualization is ineffective due to the lack of interface. A pulse rate detection system was presented by Banerjee et al. [26] using a noninvasive method. This method uses a real-time monitoring platform for interactive IoT applications. Gregoski et al. [27] presented a smartphone-based technique for heart rate monitoring using mobile and camera interaction. Oresko et al. [28] developed a smartphone interactive tool for identifying cardiovascular diseases to monitor the level of heart rate during the progression of time. Trivedi et al. [29] developed a mobile-based method for monitoring analog data for surveillance applications. The Arduino platform is used for digital conversion, and Bluetooth transmission is required to transmit physical quantities to the device. Kumar et al. [30] suggested a safety device incorporating the IoT platform at three separate layers: control, device, and transport layer. The information is uploaded on the cloud platform using Wi-Fi and Ethernet. Desai et al. [31] proposed a wireless sensor network-based approach to track smart homes and heartbeat monitoring using the Spartan3 and FPGA interface.

IoT's evolution has increased nowadays with smart devices' tremendous ability to share information between them [32]. The reliance on IoT on various applications has

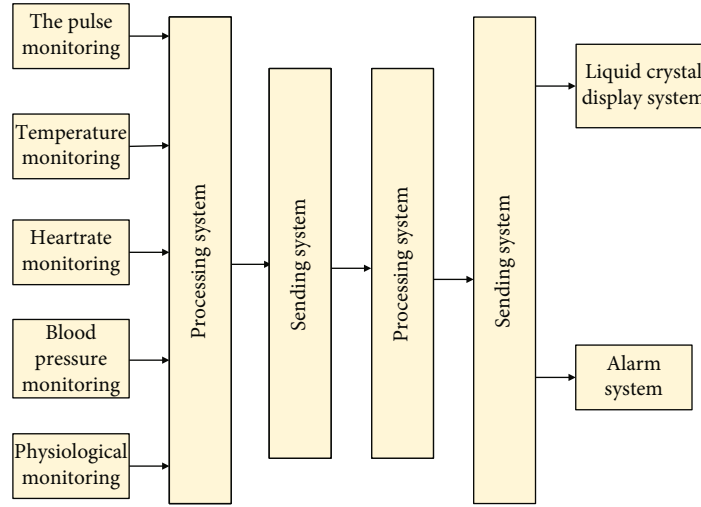


FIGURE 3: The framework of the human health monitoring terminal system.

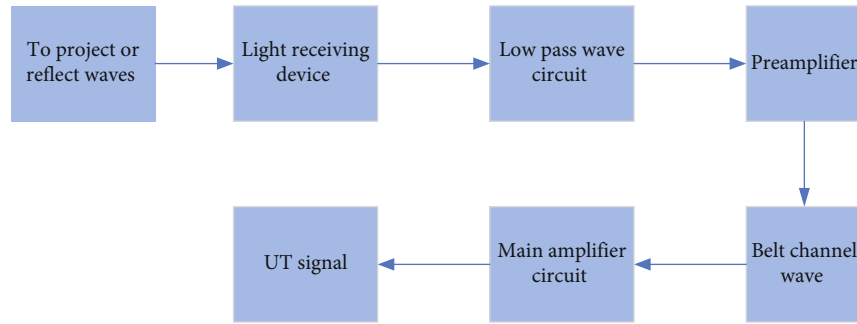


FIGURE 4: The pulse acquisition module diagram.

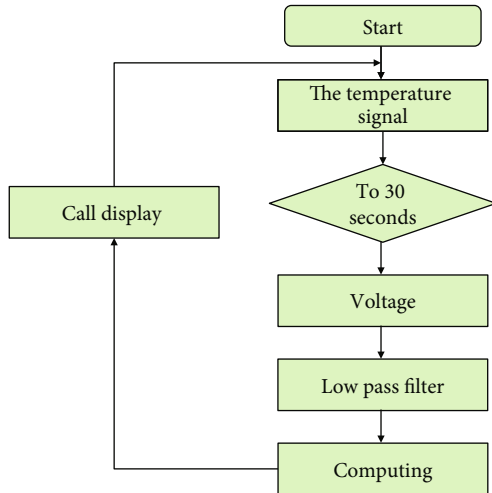


FIGURE 5: The structure diagram of the body temperature collection module.

widened its importance in the healthcare sector for remote monitoring of patients' criticality levels [33, 34]. This technological advent has come across various domains of safety, health, and human wellbeing [35, 36]. IoT is advantageous in computation, processing, and storage utilizing cloud-based solutions [35–37]. It is also beneficial in processing

and storing the geographical data on the cloud platform, which can be shared between the devices for various applications [38, 39]. The current human health monitoring system based on the Internet of Things has some limitations, such as increasing users and uploaded databases, no guarantee for users, poor real-time performance, and low data utilization. A human health monitoring system based on the Internet of Things is designed in this work. The system can uninterruptedly and accurately monitor the human body's heart rate, blood pressure, pulse, body temperature, physiological information, and other vital sign parameters. This work uses wireless sensors to retain the information for health monitoring. The data is integrated using the Internet of Things for processing, connecting, and computing to achieve real-time monitoring. The proposed system demonstrated relatively accurate and stable test ability improving deficiencies in the existing health monitoring platform [40, 41]. This article contributes in daily health management using the human health monitoring system based on the Internet of Things which is instrumental in heightening health service quality and level.

This article is organized as follows: Section 2 presents the material and methods defining the various modules designed for the health monitoring framework. Section 3 presents the results and discussion of the analysis done in this study, followed by the article's concluding remarks in Section 4.

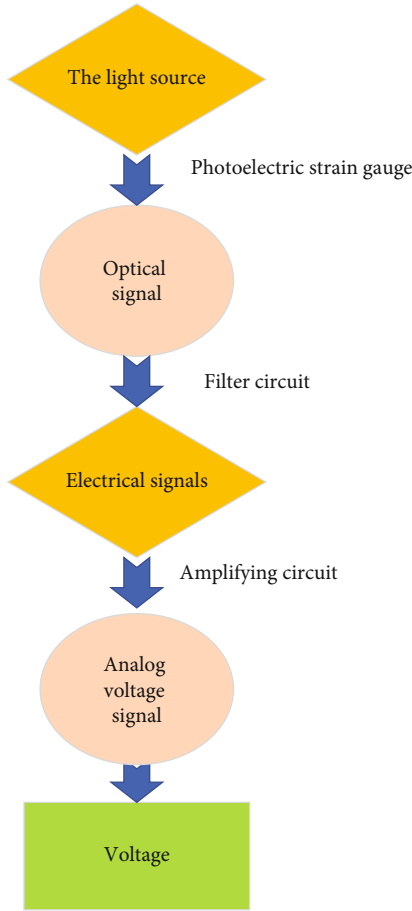


FIGURE 6: The diagram of the heart rate acquisition module.

## 2. Materials and Methods

The health monitoring system using IoT consists of various modules like pulse acquisition module, body temperature acquisition module, heart rate acquisition module, and blood pressure acquisition module. All these frameworks are elaborated in this section.

**2.1. The Framework of the Health Monitoring System Based on the Internet of Things.** The health monitoring and medical information system based on the Internet of Things integrate technologies such as wireless networks and mobile computing, aiming to provide patients with remotely receivable sensing, sound, image, and video multimedia information, enhancing medical diagnosis accuracy the quality of clinical services. The patient's blood pressure, heart rate, body temperature, pulse, and other information can be collected accurately by wearing related equipment. Information is transmitted using sensor network technologies such as Zigbee, Wi-Fi, Bluetooth, ultrawideband, and short-range wireless transmission, as shown in Figure 2.

**2.2. The Framework of Health Monitoring Terminal System Based on Internet of Things Human.** In the human health monitoring system based on the Internet of Things, the terminal system is mainly responsible for collecting and moni-

toring normal human health data. When abnormal data occurs, the terminal's alarm system will raise the alarm. At this time, it is necessary to conduct research and analysis on abnormal data and perform timely data processing. For example, the monitor's specific situation is confirmed first, and then, emergency rescue measures are carried out. Therefore, monitoring various indexes of the subjects is highly critical. To sum up, based on the existing research state quo and results and the market demand, the terminal system's hardware framework is designed for human health monitoring based on the Internet of Things. The terminal is mainly divided into a health monitoring project module, a data acquisition module, a data receiving module, a data transmission module, a data processing module, and a display and alarm module, as shown in Figure 3.

**2.3. Pulse Acquisition Module.** Generally speaking, the photoelectric pulse sensor is divided into two types: transmitted wave monitoring and reflected wave monitoring according to how to detect light [42]. Their key components are the same (i.e., stable light source and light-receiving sensor). The impulse data sensor of Rohm Semiconductor Group is selected in the study, as shown in Figure 4.

**2.4. Body Temperature Acquisition Module.** In this study, the voltage output integrated temperature sensor is selected for the health monitoring system terminal, and the hardware circuit is designed. The digital conversion of the output analog signal is realized through the displayer, as shown in Figure 5.

The temperature sensor converts the temperature signal into a voltage output, performs low-pass filtering on the output signal to remove noise, and then amplifies the temperature sensor output voltage to a voltage level by the amplifier circuit [43].

**2.5. Heart Rate Acquisition Module.** The light volume method's principle is to measure the heart rate using the difference in the blood vessel's light transmittance caused by the pulse's beating [44]. The light source is converted into an optical signal using a photoelectric sensor, and the optical signal is then converted into an electrical signal by a filter circuit. The selected wavelength is 650 nm-750 nm. The signal flow of the heart rate sensor is shown in Figure 6.

When the light passes through human peripheral blood vessels, the volume change caused by pulse congestion affects the light source's light transmittance. The light signal reflected by the photoelectric converter through the human body's peripheral blood vessels is converted and output by the amplifier circuit. The heart rate is output in analog voltage. This value is acquired using the heart rate acquisition module.

**2.6. Blood Pressure Acquisition Module.** Blood pressure monitoring methods can be divided into the direct method and indirect method (Oscillometric method). The indirect method avoids the direct method's shortcomings, such as being complicated and traumatic [45]. It monitors the pressure value on the body surface using the relationship between the vessel's pressure and the FM flow change. It is easy to operate, hygienic and concise without particularly severe

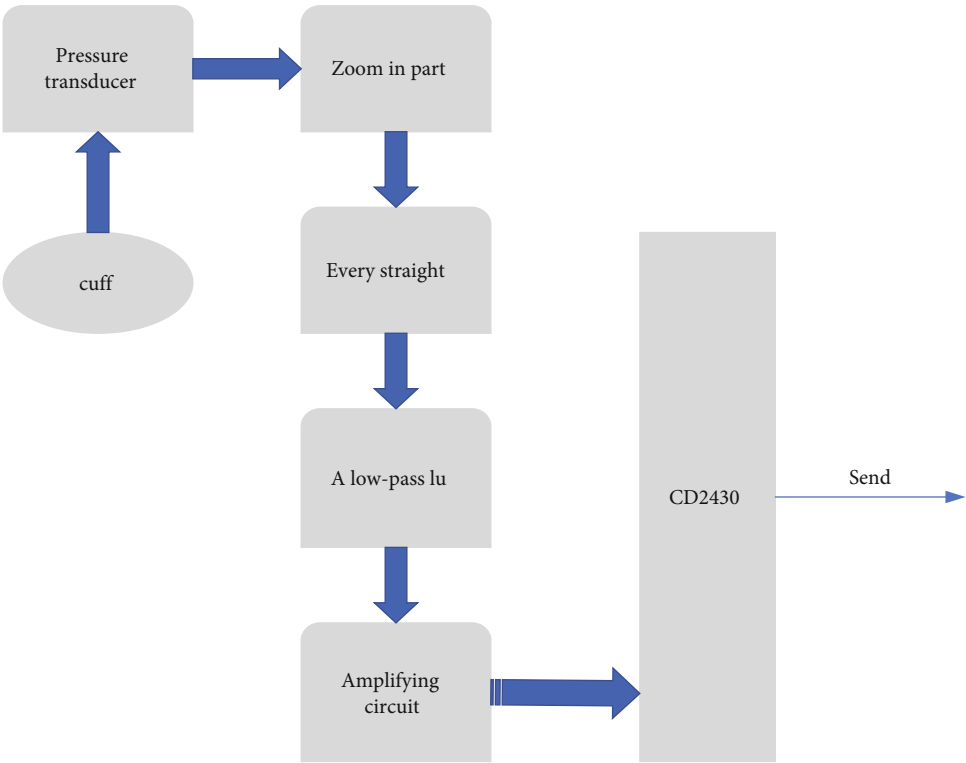


FIGURE 7: The diagram of the blood pressure acquisition module.

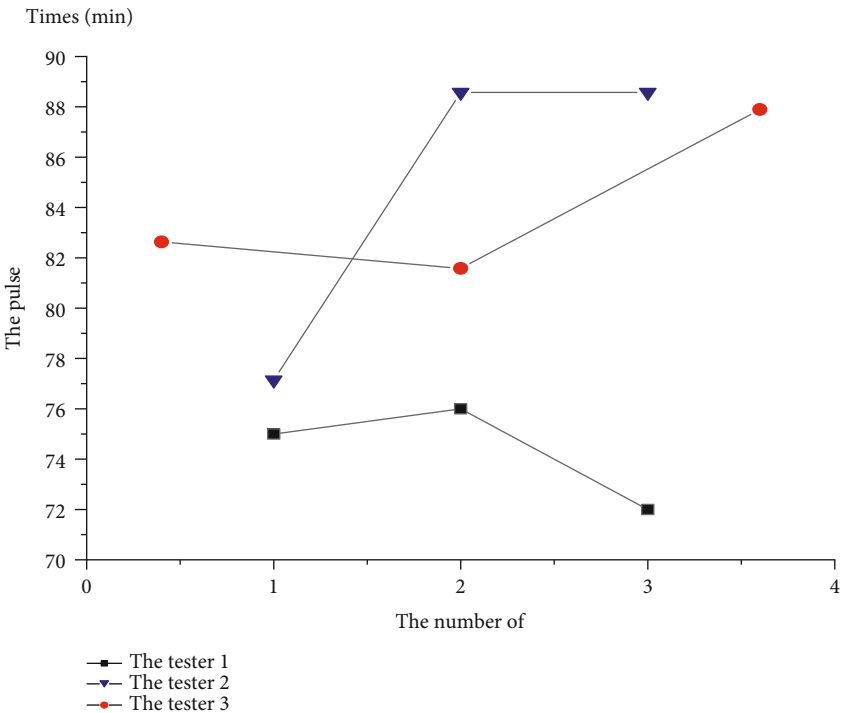


FIGURE 8: The pulse test results.

medical restrictions, and does not harm health. As a result, the indirect method is more commonly used. Not only is the blood pressure monitored without any trauma to the human body but the monitored values are also more accurate [6–15]. The system diagram is shown in Figure 7.

The signal acquisition and processing are dependent on the op-amp LM324. The sensor is a BP300 sensor, which is sensitive, accurate, and precise. Besides, air pumps, resistors, and capacitors are also necessary components. The pressure sensor converts the pressure signal by converting the blood

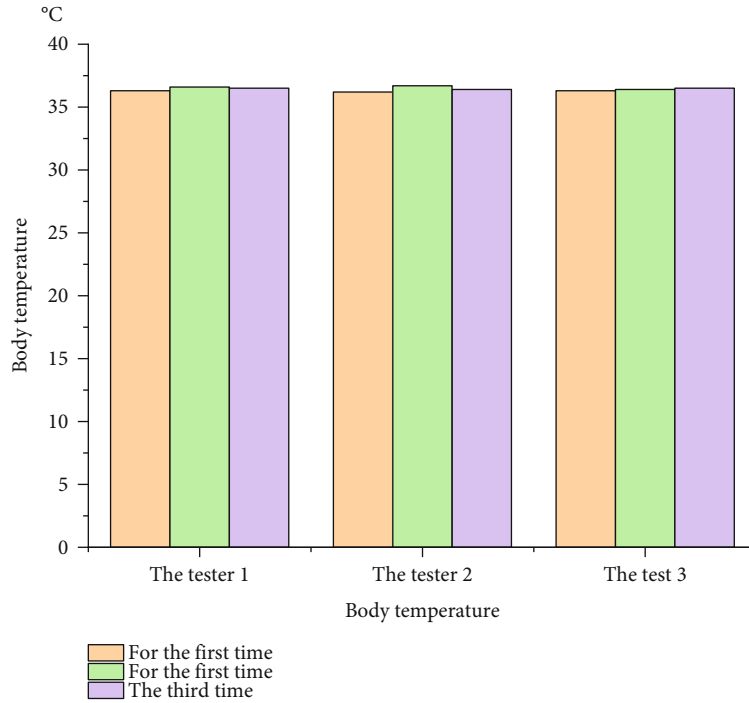


FIGURE 9: The temperature test results.

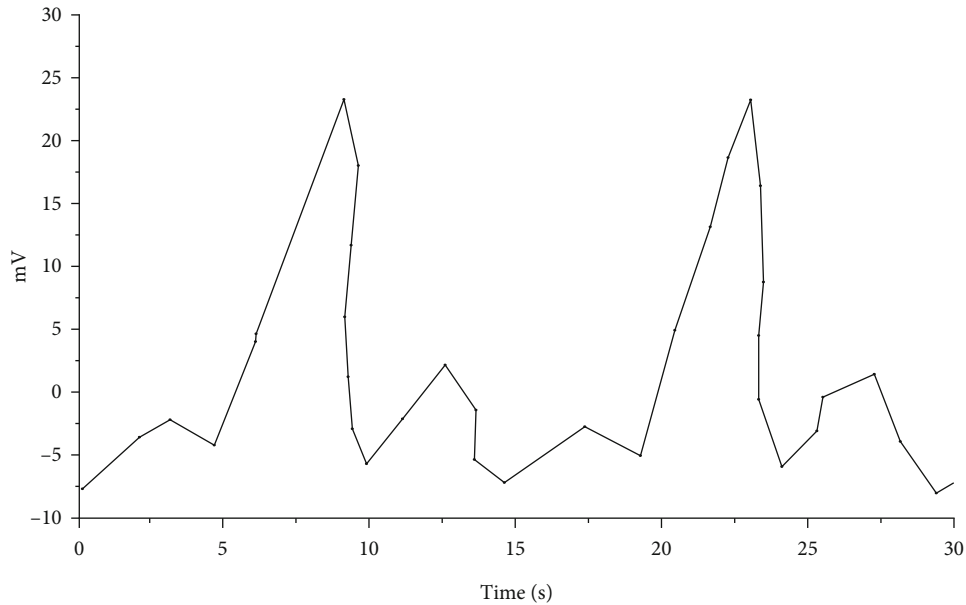


FIGURE 10: The 30-second ECG.

flow pressure signal in the inflatable bandage into a voltage signal close to the microcontroller's voltage amplitude. The one-chip computer collects and processes the signal and is responsible for the control of the entire circuit.

### 3. Results and Discussion

The experimentation outcomes are analyzed in this section discussing various compliances and assessing outcomes obtained from their implementation. Various modules like

pulse acquisition, body temperature monitoring, ECG, and physiological information acquisition are observed in the upcoming subsections.

**3.1. Compliance Test of the Pulse Acquisition Module.** It is evident from the pulse test results that the three subjects' pulse values are all within the normal range (the pulse rate of an average adult is 70~90 beats/min). The pulse signal acquisition test is performed three times for each person, and the average pulse value acquired is 78, 78, and 79 (beats/min),

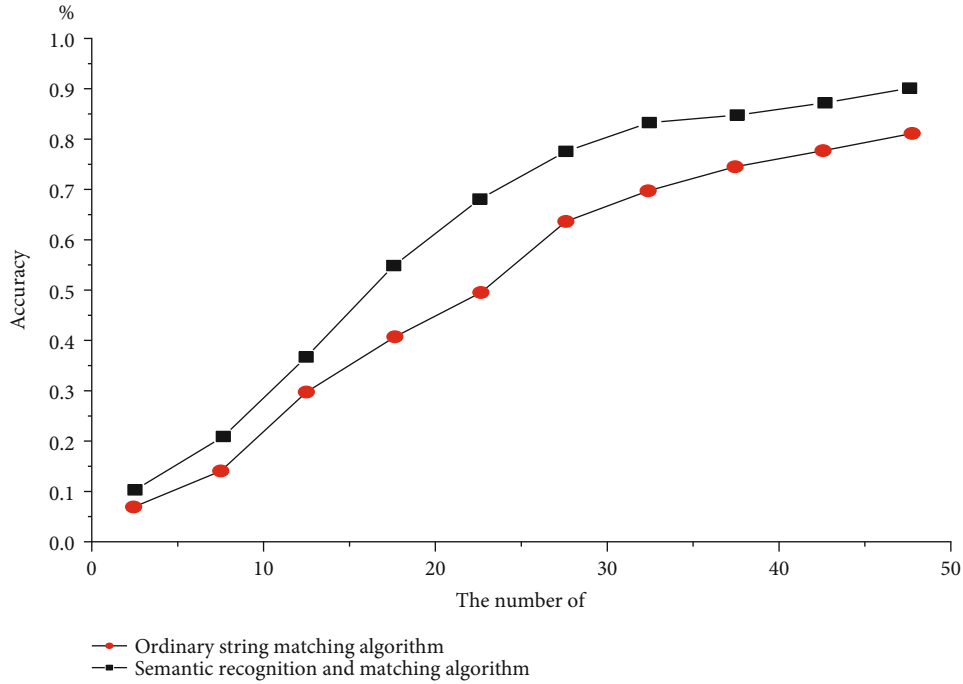


FIGURE 11: The comparison of keyword matching.

respectively. The thermometer's corresponding values are 77, 79, and 78, indicating that the system's test results are relatively accurate, as shown in Figure 8.

Although there is deviation sometimes, it is within the acceptable range. This is because the sensor of the pulse acquisition module is associated with the circuit design. It can be further improved in the future to acquire more accurate results.

**3.2. Compliance Test of Body Temperature Acquisition Module.** Three people were selected as test subjects to conduct temperature measurements to make reasonable judgments on the temperature monitoring module's performance to evaluate the system's accuracy more rigorously.

As shown in Figure 9, three persons' temperature using a thermometer is 36.4°C, 36.7°C, and 36.5°C, respectively. The temperature test was carried out three times for each person, and the average of each person acquired by the system is 36.5°C, 36.4°C, and 36.5°C, respectively. It is evident that this system's measurements are very close to those of a thermometer and can monitor body temperature. It also indicates that the temperature test of this system is relatively stable.

**3.3. Compliance Test of ECG Information Acquisition Module.** In monitoring the ECG information collection module, the first step is to update or load the user's latest ECG measurement record information. Simultaneously, the corresponding detailed operation page will be displayed so that the real-time ECG image is acquired. Considering that the ECG data points are complicated, slight adjustments can be performed in the image's functional area to achieve the best

results to view a particular segment's image curve. The ECG operation interface is shown in Figure 10.

**3.4. The Compliance Test of the Physiological Information Acquisition Module.** It is found that as the number of keywords input by users increases, whether it is a traditional character matching system or not, the accuracy to obtain information is further raised, as shown in Figure 11, to verify the rationality of the semantic recognition and matching system and improve the traditional character matching system, through simulation experiments.

Therefore, in addition to measuring pulse and temperature, users should also be provided with more physiological-related information to understand their physical condition better.

## 4. Conclusion

In the study, the wireless sensor technology is combined with the human health monitoring terminal based on the Internet of Things to test the health-related indexes. The test results are analyzed. It is observed that the human health monitoring system of the Internet of Things is relatively stable and has functions such as an accurate collection of human health data, real-time monitoring and alarming, and evaluation of subjects. The subjects were assessed for temperature using the thermometer, which provides the temperature values of 36.4, 36.7, and 36.5 (°C), respectively, demonstrating relatively accurate and stable testability. Similarly, the pulse rate monitoring module employing the ECG observes the test outcomes of 78, 78, and 79 (times/min), respectively, similar to the medical pulse meter results.



The human health monitoring system based on the Internet of Things designed in this study has completed collecting the user's blood pressure, pulse, body temperature, heart rate, physiological information, and other vital sign data, which is suggested in practice. After long-term data collection, factors related to a potential risk prediction should be further explored in the future to expand the application of human health monitoring systems based on the Internet of Things. This will provide a scientific and effective basis for preventing and controlling chronic high-risk diseases in the near future.

## Data Availability

All data is shared in the manuscript.

## Conflicts of Interest

The authors declare that they have no conflicts of interest.

## Acknowledgments

The authors would like to thank for the support of the Taif University Researchers Supporting Project (No. TURSP-2020/10), Taif University, Taif, Saudi Arabia.

## References

- [1] C. O'Brien and C. Heneghan, "A comparison of algorithms for estimation of a respiratory signal from the surface electrocardiogram," *Computers in Biology and Medicine*, vol. 37, no. 3, pp. 305–314, 2007.
- [2] R. E. Nappi, E. Martini, L. Cucinella et al., "Addressing vulvovaginal atrophy (VVA)/genitourinary syndrome of menopause (GSM) for healthy aging in women," *Frontiers in Endocrinology*, vol. 10, p. 561, 2019.
- [3] A. Bansal, S. Kumar, A. Bajpai et al., "Remote health monitoring system for detecting cardiac disorders," *IET Systems Biology*, vol. 9, no. 6, pp. 309–314, 2015.
- [4] G. Dhiman, D. Oliva, A. Kaur et al., "BEPO: a novel binary emperor penguin optimizer for automatic feature selection," *Knowledge-Based Systems*, vol. 211, p. 106560, 2021.
- [5] K. Gatsis and G. J. Pappas, "Wireless control for the IoT," in *Proceedings of the Second International Conference on Internet-of-Things Design and Implementation*, pp. 341–342, 2017 Apr 18.
- [6] S. Kaur, L. K. Awasthi, A. L. Sangal, and G. Dhiman, "Tunicate swarm algorithm: a new bio-inspired based metaheuristic paradigm for global optimization," *Engineering Applications of Artificial Intelligence*, vol. 90, p. 103541, 2020.
- [7] G. Dhiman and A. Kaur, "Spotted hyena optimizer for solving engineering design problems," in *2017 International Conference on Machine Learning and Data Science (MLDS)*, pp. 114–119, Noida, India, 2017.
- [8] G. Dhiman and A. Kaur, "STOA: a bio-inspired based optimization algorithm for industrial engineering problems," *Engineering Applications of Artificial Intelligence*, vol. 82, pp. 148–174, 2019.
- [9] G. Dhiman and A. Kaur, "A hybrid algorithm based on particle swarm and spotted hyena optimizer for global optimization," in *In Soft computing for problem solving*, pp. 599–615, Springer, Singapore, 2019.
- [10] A. Kaur and G. Dhiman, "A review on search-based tools and techniques to identify bad code smells in object-oriented systems," in *In Harmony search and nature inspired optimization algorithms*, pp. 909–921, Springer, Singapore, 2019.
- [11] G. Dhiman and A. Kaur, "Optimizing the design of airfoil and optical buffer problems using spotted hyena optimizer," *Designs*, vol. 2, no. 3, p. 28, 2018.
- [12] A. Kaur, S. Kaur, and G. Dhiman, "A quantum method for dynamic nonlinear programming technique using Schrödinger equation and Monte Carlo approach," *Modern Physics Letters B*, vol. 32, no. 30, p. 1850374, 2018.
- [13] P. Singh, G. Dhiman, and A. Kaur, "A quantum approach for time series data based on graph and Schrödinger equations methods," *Modern Physics Letters A*, vol. 33, no. 35, p. 1850208, 2018.
- [14] G. Dhiman and A. Kaur, "HKn-RVEA: a novel many-objective evolutionary algorithm for car side impact bar crashworthiness problem," *International Journal of Vehicle Design*, vol. 80, no. 2/3/4, p. 257, 2019.
- [15] A. Kaur, S. Jain, S. Goel, and G. Dhiman, "A review on machine-learning based code smell detection techniques in object-oriented software system(s)," *Recent Advances in Electrical & Electronic Engineering (Formerly Recent Patents on Electrical & Electronic Engineering)*, vol. 14, no. 3, pp. 290–303, 2021.
- [16] M. Poongodi, M. Hamdi, A. Sharma, M. Ma, and P. K. Singh, "DDoS detection mechanism using trust-based evaluation system in VANET," *IEEE Access*, vol. 7, pp. 183532–183544, 2019.
- [17] J. Dogra, S. Jain, A. Sharma, R. Kumar, and M. Sood, "Brain tumor detection from MR images employing fuzzy graph cut technique," *Recent Advances in Computer Science and Communications*, vol. 13, no. 3, pp. 362–369, 2020.
- [18] G. Rathee, A. Sharma, R. Kumar, F. Ahmad, and R. Iqbal, "A trust management scheme to secure mobile information centric networks," *Computer Communications*, vol. 151, pp. 66–75, 2020.
- [19] H. B. Hassen, N. Ayari, and B. Hamdi, "A home hospitalization system based on the Internet of things, Fog computing and cloud computing," *Informatics in Medicine Unlocked*, vol. 20, p. 100368, 2020.
- [20] M. M. Islam, A. Rahaman, and M. R. Islam, "Development of smart healthcare monitoring system in IoT environment," *SN Computer Science*, vol. 1, no. 3, 2020.
- [21] F. Rezaeibagha and Y. Mu, "Practical and secure telemedicine systems for user mobility," *Journal of Biomedical Informatics*, vol. 78, pp. 24–32, 2018.
- [22] S. O. Agnisarman, K. Chalil Madathil, K. Smith, A. Ashok, B. Welch, and J. T. McElligott, "Lessons learned from the usability assessment of home-based telemedicine systems," *Applied Ergonomics*, vol. 58, pp. 424–434, 2017.
- [23] F. Mugica, À. Nebot, S. Bagherpour, L. Baladón, and A. Serrano-Blanco, "A model for continuous monitoring of patients with major depression in short and long term periods," *Technology and Health Care*, vol. 25, no. 3, pp. 487–511, 2017.
- [24] V. Tamilselvi, S. Sribalaji, P. Vigneshwaran, P. Vinu, and J. GeethaRamani, "IoT based health monitoring system," in *2020 6th International Conference on Advanced Computing and Communication Systems (ICACCS)*, pp. 386–389, Coimbatore, India, 2020.



- [25] A. D. Acharya and S. N. Patil, "IoT based health care monitoring kit," in *2020 Fourth International Conference on Computing Methodologies and Communication (ICCMC)*, pp. 363–368, Erode, India, 2020.
- [26] S. Banerjee and S. Roy, "Design of pulse rate and body temperature monitoring system with Arduino via wifi and android-based gadget," *International Journal of Technology and Engineering Studies*, vol. 2, no. 5, pp. 302–306, 2016.
- [27] M. J. Gregoski, M. Mueller, A. Vertegel et al., "Development and validation of a smartphone heart rate acquisition application for health promotion and wellness telehealth applications," *International Journal of Telemedicine and Applications*, vol. 2012, Article ID 696324, 2012.
- [28] J. J. Oresko, Z. Jin, J. Cheng et al., "A wearable smartphone-based platform for real-time cardiovascular disease detection via electrocardiogram processing," *IEEE Transactions on Information Technology in Biomedicine*, vol. 14, no. 3, pp. 734–740, 2010.
- [29] S. Trivedi and A. N. Cheeran, "Android based health parameter monitoring," in *2017 International Conference on Intelligent Computing and Control Systems (ICICCS)*, pp. 1145–1149, Madurai, India, 2017.
- [30] S. P. Kumar, V. R. Samson, U. B. Sai, P. M. Rao, and K. K. Eswar, "Smart health monitoring system of patient through IoT," in *2017 International Conference on I-SMAC (IoT in Social, Mobile, Analytics and Cloud) (I-SMAC)*, pp. 551–556, Palladam, India, 2017.
- [31] M. R. Desai and S. Toravi, "A smart sensor interface for smart homes and heart beat monitoring using WSN in IoT environment," in *2017 International Conference on Current Trends in Computer, Electrical, Electronics and Communication (CTCEEC)*, pp. 74–77, Mysore, India, 2017.
- [32] S. Kumar and Z. Raza, "Internet of Things: possibilities and challenges," in *Fog Computing: Breakthroughs in Research and Practice*, pp. 1–24, IGI Global, 2018.
- [33] A. M. Koya and P. P. Deepthi, "Plug and play self-configurable IoT gateway node for telemonitoring of ECG," *Computers in biology and medicine*, vol. 112, p. 103359, 2019.
- [34] M. Masud, G. S. Gaba, S. Alqahtani et al., "A lightweight and robust secure key establishment protocol for Internet of Medical Things in COVID-19 patients care," *IEEE Internet of Things Journal*, pp. 1–1, 2020.
- [35] J. Lin, J. Y. Pai, and C. C. Chen, "Applied patent RFID systems for building reacting HEPA air ventilation system in hospital operation rooms," *Journal of medical systems*, vol. 36, no. 6, pp. 3399–3405, 2012.
- [36] J. J. Rodrigues, D. B. Segundo, H. A. Junqueira et al., "Enabling technologies for the Internet of Health Things," *IEEE Access*, vol. 6, pp. 13129–13141, 2018.
- [37] C. Stergiou, K. E. Psannis, B. G. Kim, and B. Gupta, "Secure integration of IoT and cloud computing," *Future Generation Computer Systems*, vol. 78, pp. 964–975, 2018.
- [38] P. M. Kumar, S. Lokesh, R. Varatharajan, G. C. Babu, and P. Parthasarathy, "Cloud and IoT based disease prediction and diagnosis system for healthcare using Fuzzy neural classifier," *Cloud and IoT based disease prediction and diagnosis system for healthcare using Fuzzy neural classifier*, vol. 86, pp. 527–534, 2018.
- [39] N. J. Vickers, "Animal communication: when I'm calling you, will you answer too?," *Current Biology*, vol. 27, no. 14, pp. R713–R715, 2017.
- [40] M. Al Yami and D. Schaefer, "Fog computing as a complementary approach to cloud computing," in *2019 International Conference on Computer and Information Sciences (ICCIS)*, pp. 1–5, Sakaka, Saudi Arabia, 2019.
- [41] N. V. Panicker and A. S. Kumar, "Tablet PC enabled body sensor system for rural telehealth applications," *International Journal of Telemedicine and Applications*, vol. 2016, Article ID 5747961, 9 pages, 2016.
- [42] R. Miramontes, R. Aquino, A. Flores et al., "PlalMoS: a remote mobile healthcare platform to monitor cardiovascular and respiratory variables," *Sensors (Basel)*, vol. 17, no. 12, p. 176, 2017.
- [43] P. Bellavista, J. Berrocal, A. Corradi, S. K. Das, L. Foschini, and A. Zanni, "A survey on fog computing for the Internet of Things," *Pervasive and mobile computing*, vol. 52, pp. 71–99, 2019.
- [44] H. Sun, H. Yu, G. Fan, and L. Chen, "Energy and time efficient task offloading and resource allocation on the generic IoT-fog-cloud architecture," *Peer-to-Peer Networking and Applications*, vol. 13, no. 2, pp. 548–563, 2020.
- [45] H. Kaur and S. K. Sood, "Energy-efficient IoT-fog-cloud architectural paradigm for real-time wildfire prediction and forecasting," *IEEE Systems Journal*, vol. 14, no. 2, pp. 2003–2011, 2019.