

Research Summary: SKIIN Switzerland Website Copy (v7)

1. User Goals and Deliverable Requirements

The user has asked for a **complete overhaul** of the SKIIN Switzerland website copy guide based on multiple iterations (pre-CEO v4, v5, v6, v6.1 and the upcoming v7). Key requirements include:

- **Respect the prescribed site architecture.** The site must include Home, Solutions, Partners (with subsections for GPs, cardiologists, telemedicine providers and corporate employers/insurers), How It Works (Process, Reimbursement, Technology, Clinical Evidence), About Us (Company & Mission, Our Team & Medical Advisors, Testimonials, Compliance & Legal, Contact) and Support. **There is no patient page**; patient-facing content belongs on the main Home page.
- **Maintain defined CTAs.** Three patient CTAs—“**Start Your Free Assessment**,” “**Check Insurance Coverage**” and “**Questions? Read our FAQ →**”—must appear across the site. Professional CTAs (e.g., “Book a Demo,” “Join Our GP Network,” “Integrate SKIIN,” “Get a Corporate Quote”) are reserved for partner pages. The user notes that the CTAs were mishandled in v6.0; this must be corrected.
- **Integrate the Silent Triad.** The product now offers **10-day ECG monitoring**, **ambulatory blood pressure monitoring (ABPM)** and **sleep analysis**. Each modality should be explained clearly. ABPM must be acknowledged as the gold standard for diagnosing hypertension: measurements occur every 15–30 min during the day and 30–60 min at night pmc.ncbi.nlm.nih.gov, and ABPM detects masked or nocturnal hypertension pmc.ncbi.nlm.nih.gov. Sleep analysis should note that nocturnal arrhythmia prevalence jumps from 53 % in people without sleep-breathing disorders to 92 % in those with severe obstructive sleep apnoea pmc.ncbi.nlm.nih.gov.
- **Move MVCP to the General Practitioner page.** In the pre-CEO version, a dedicated MVCP page existed. The CEO now wants the **Myant Virtual Clinic Portal (MVCP)** content merged into the general practitioner subpage in Partners and removed from standalone pages.
- **Eliminate the patient partner subsection.** Partner pages target only healthcare professionals (GPs, cardiologists, telemedicine providers and corporate/insurers).

Patient-facing content should not appear here.

- **Use evidence-based messaging.** Claims must be supported by credible sources: 66 % vs 9 % detection when extending monitoring beyond 24 hours [pmc.ncbi.nlm.nih.gov](https://pubmed.ncbi.nlm.nih.gov/), 93.7 % comfort preference for patch monitors [pmc.ncbi.nlm.nih.gov](https://pubmed.ncbi.nlm.nih.gov/), 70 % of AF episodes being asymptomatic [pmc.ncbi.nlm.nih.gov](https://pubmed.ncbi.nlm.nih.gov/) and AF causing approximately 20–30 % of ischaemic strokes heartandstroke.ca. ABPM's status as the reference standard for hypertension diagnosis is supported by the HOPE Asia guidelines [pmc.ncbi.nlm.nih.gov](https://pubmed.ncbi.nlm.nih.gov/).
- **Update mission & heritage narrative.** The product is developed by **Myant** in Canada and enhanced by the acquisition of **Nanoleq**, an ETH Zurich spin-off. Avoid misrepresenting the technology as ETH-developed; emphasise the acquisition in 2024 and the establishment of Myant Europe.
- **Adjust voice & tone.** Avoid shallow words like “revolution” or “transformation,” use urgent yet empathetic phrasing and highlight longevity and quality-of-life benefits. Messaging must be **patient-centric**, emphasising comfort, preventive urgency and family impact.
- **Provide a detailed change log** documenting what changed between versions (v4 → v5 → v6 → v6.1 → v7) and highlighting deviations from the CEO's requirements.

Deliverables include:

1. **Research summary (this document)** summarising context, attachments and external evidence.
2. **Tree-of-thought (TOT.md):** a structured map of entities (pages, sections, CTAs, features, audiences) and their relationships.
3. **Brainstorming & evaluation (BRAINSTORM.md):** candidate features/components scored for inclusion.
4. **Planning document (planning.md)** and **task list (todo.md)** with expert feedback and completion tracking.
5. **Detailed change log (change_log.md)** summarising how copy evolved from v4 to v7 and identifying misalignments.
6. **Final production-ready copy specification (Version 7.0)** that integrates the CEO comments, follows the site architecture and includes all necessary pages and sections.

2. Primary Sources Reviewed

2.1 Pre-CEO Copy Specification (Version 4.0 – July 23, 2025)

The pre-CEO spec establishes the site structure and messaging themes for SKIIN Switzerland. Key points include:

- **Website architecture:** Home, Solutions (14-day Holter, Tritest/3X Screening), Partners (GPs, cardiologists, telemedicine providers, corporate), How It Works (Process, Reimbursement, Technology, Clinical Evidence), About Us (Company & Mission, Our Team & Advisors, Blog & Resources, Testimonials, Compliance & Legal, Contact) and Support. The CEO emphasised that **no patient page** should exist under Partners.
- **Hero CTAs:** Each hero variant features the same CTAs (“Start Your Free Assessment,” “Check Insurance Coverage,” “Questions? Read our FAQ →”), which direct to an eligibility/coverage form.
- **Problem/solution narrative:** Up to 70 % of arrhythmias are silent [pmc.ncbi.nlm.nih.gov](https://pubmed.ncbi.nlm.nih.gov/); extended monitoring (beyond 24 hours) detects significantly more arrhythmias [pmc.ncbi.nlm.nih.gov](https://pubmed.ncbi.nlm.nih.gov/); atrial fibrillation contributes to 20–30 % of strokes heartandstroke.ca. The spec emphasises the comfort revolution (wire-free, soft, washable garment), longevity, emotional storytelling and Swiss medical excellence.
- **Partners and MVCP:** The v4 spec included a combined physicians page with targeted subsections for GPs, cardiologists and telemedicine providers. It also featured a standalone **Myant Virtual Clinic Portal (MVCP)** page describing real-time ECG monitoring, comprehensive analysis tools, patient management dashboards, integrated reporting and security & compliance features. This page included CTAs (“Request Portal Access,” “Schedule a Demo,” “View Portal Guide”) and emphasised Swiss data residency and ISO 27001 compliance. The CEO later requested that MVCP content be incorporated into the GP page and that the separate MVCP page be removed.
- **Additional sections:** The pre-CEO spec contained a **Blog** page and a **Heart-Age Tool** (not included in the v6 spec) and offered more detailed pricing options (3-day, 5-day, 10-day self-pay packages) with cost breakdowns. It emphasised insurance reimbursement pathways and a blog for thought leadership.

2.2 Version 6.0 Copy Guide

Version 6.0 updates the pre-CEO spec in response to the CEO’s comments and marketing

objectives. Highlights include:

- **Messaging refresh:** Hero headlines emphasise preventive urgency and longevity (“Screen early. Live longer.”), remove hyperbolic terms like “revolution,” and integrate the **Silent Triad** narrative (arrhythmia, hypertension, sleep apnoea). The version clarifies that the garment is water-resistant, washable and removable.
- **Expanded technology narrative:** ABPM and sleep analysis are introduced alongside ECG monitoring under the slogan “**One System. Three Vital Signs.**” The AI analysis pipeline is explained: data flow from the textile band to the smartphone app, encrypted cloud, AI analysis via the DeepRhythm Platform and cardiologist review. Certifications (MDR Class IIa, Swissmedic, ISO 13485, ISO/IEC 27001) are prominent.
- **Mission & heritage:** The About section clarifies that Myant developed the technology in Canada and acquired Nanoleq (an ETH Zurich spin-off) for Swiss R&D. The section emphasises Swiss precision, data protection and the goal of enabling people to live younger, longer.
- **Unified partners page:** The physicians page is merged into the Partners page with subsections for patients, GPs, cardiologists, telemedicine providers and corporate wellness. Each subsection features tailored value propositions and CTAs (“Join Our GP Network,” “Book a Demo,” “Integrate SKIIN,” “Get a Corporate Quote”). **However, this inclusion of a “For Patients” subsection contradicts the CEO’s directive to avoid a patient page in the partner section.**
- **Clinical evidence & screening guidance:** Statistical claims are backed by peer-reviewed studies: 66 % vs 9 % detection rates with extended monitoring [pmc.ncbi.nlm.nih.gov](https://pubmed.ncbi.nlm.nih.gov/), patient comfort with patch monitors [pmc.ncbi.nlm.nih.gov](https://pubmed.ncbi.nlm.nih.gov/), 70 % silent AF episodes [pmc.ncbi.nlm.nih.gov](https://pubmed.ncbi.nlm.nih.gov/), 20–30 % stroke linkage heartandstroke.ca and ABPM as the gold standard [pmc.ncbi.nlm.nih.gov](https://pubmed.ncbi.nlm.nih.gov/). Sleep apnoea’s impact on arrhythmia prevalence is also noted [pmc.ncbi.nlm.nih.gov](https://pubmed.ncbi.nlm.nih.gov/).
- **Reduced distractions:** The v6.0 spec removes the blog, heart-age tool and micro-conversion elements, focusing conversions on the eligibility form and professional demo sign-ups.
- **Remaining issues:** CTAs appear inconsistent across sections; the MVCP content is still referenced separately rather than being fully integrated into the GP page; the patient subsection under Partners remains; and some original copy has been replaced by placeholders or pseudo-instructions, missing polished final text.

3. Key External Evidence

- **Silent AF and stroke risk:** Up to **70 %** of atrial fibrillation episodes are asymptomatic[pmc.ncbi.nlm.nih.gov](https://pubmed.ncbi.nlm.nih.gov/). AF contributes to about **20–30 %** of ischaemic strokesheartandstroke.ca. Early detection via continuous monitoring helps prevent strokes and guides timely treatment.
- **Extended monitoring superiority:** A 14-day patch monitor detected arrhythmias in **66 %** of patients compared with **9 %** using a 24-hour Holter monitor[pmc.ncbi.nlm.nih.gov](https://pubmed.ncbi.nlm.nih.gov/). Longer monitoring windows capture intermittent arrhythmias that would otherwise be missed.
- **Patient comfort:** Studies show that patch monitors are preferred by **93.7 %** of patients over traditional Holter devices[pmc.ncbi.nlm.nih.gov](https://pubmed.ncbi.nlm.nih.gov/), emphasising the comfort revolution.
- **Carbon-fibre electrodes durability:** Textile electrodes maintain functionality after at least **50 wash cycles**[pmc.ncbi.nlm.nih.gov](https://pubmed.ncbi.nlm.nih.gov/), ensuring long-term usability.
- **ABPM as gold standard:** Ambulatory blood pressure monitoring measures BP every **15–30 min** during the day and **30–60 min** at night and is regarded as the **reference standard** for diagnosing hypertension[pmc.ncbi.nlm.nih.gov](https://pubmed.ncbi.nlm.nih.gov/). ABPM can detect masked hypertension and nocturnal dipping[pmc.ncbi.nlm.nih.gov](https://pubmed.ncbi.nlm.nih.gov/).
- **Sleep analysis & arrhythmia:** Nocturnal arrhythmia prevalence increases dramatically in individuals with severe obstructive sleep apnoea—from **53 %** to **92 %**[pmc.ncbi.nlm.nih.gov](https://pubmed.ncbi.nlm.nih.gov/)—highlighting the need for combined sleep and ECG monitoring.

4. High-Level Observations

- **Multiple version iterations** have introduced complexity and misalignment. Some original copy has been replaced with placeholders (e.g., the MVCP section), and some CTAs have been omitted or modified incorrectly. A careful audit is needed to restore clarity and completeness.
- **The final v7 copy specification** must abide by the CEO's instructions, emphasising preventive urgency, longevity and comfort; integrating ABPM and sleep analysis; eliminating the patient partner page; relocating MVCP to the GP page; and ensuring CTAs are consistent across the site.

- **A comprehensive change log** is required to document the evolution from v4 to v7, highlighting which changes were intentional, which deviated from requirements and how v7 resolves outstanding issues.


5. Additional Context from the Existing Website

During a review of the current implementation at **smartholter.netlify.app** (a staging version of the SKIIN Switzerland site), several differences emerged between the website's structure and the Version 7 copy specification. Understanding these differences is critical for adapting the final copy to the real UI without reinventing the design.

5.1 Home Page Layout


The home page is dominated by a **split-hero** design. On the left, a headline ("Clinical Precision Healthcare") and subheadline emphasise clinical accuracy and trust, with CTAs labelled "**Start Clinical Assessment**" and "**Book Assessment.**" A badge ("Certified by the Federal Office of Public Health (BAG)") appears above the headline. The right side contains an image of a smiling woman using her phone. Beneath the hero, the site presents several sections:

1. **Statistics Cards:** Three visual cards convey statistics: 70 % of arrhythmias remain unnoticed, 30 % of people with arrhythmias have strokes, and 50 % more arrhythmias are detected with 14-day monitoring

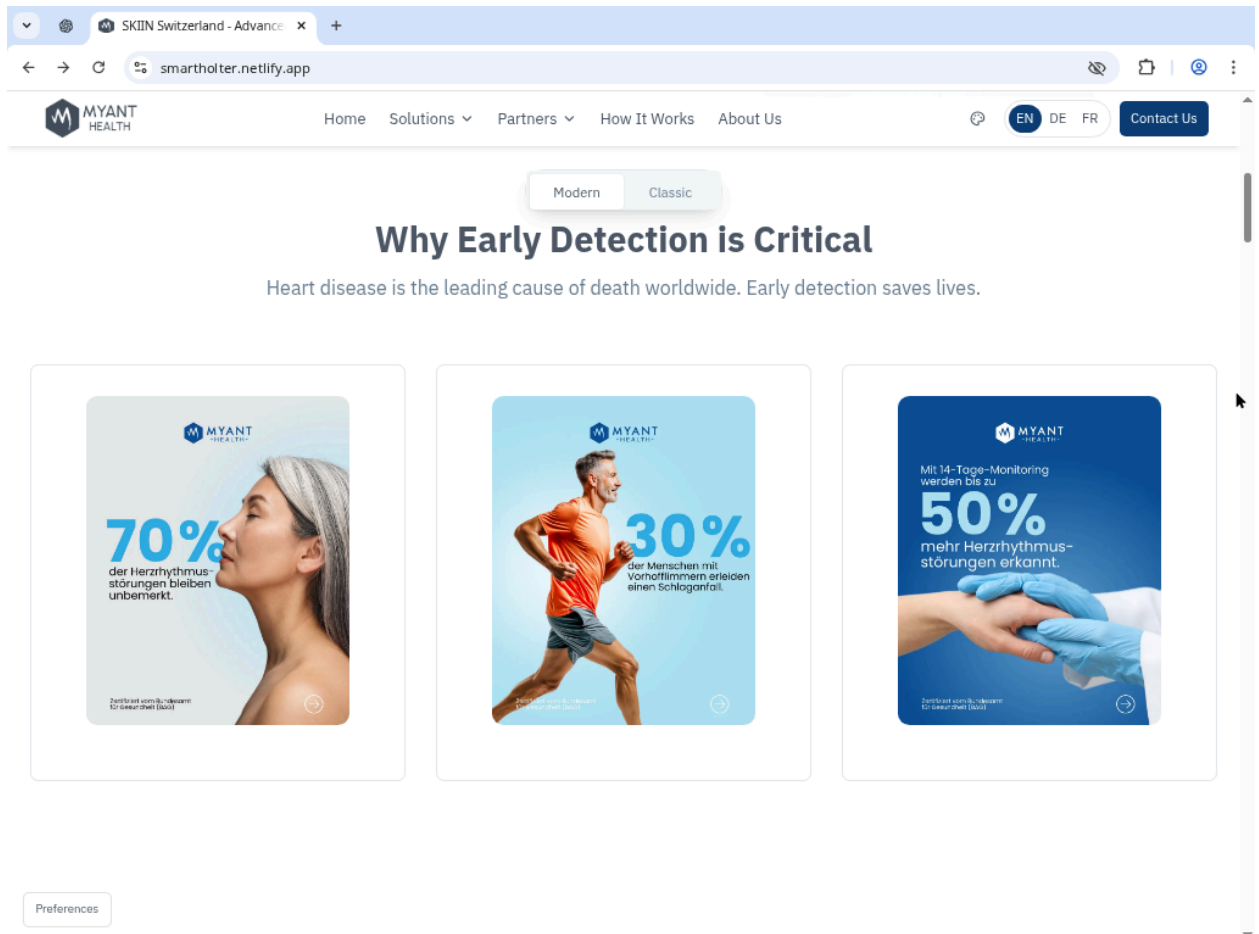


smartholter.netlify.app. These cards are visually prominent and accompanied by concise captions.

2. **Educational Videos:** A section titled “Understanding Heart Health Monitoring” includes two video thumbnails that explain cardiac assessments at home and why continuous monitoring matters

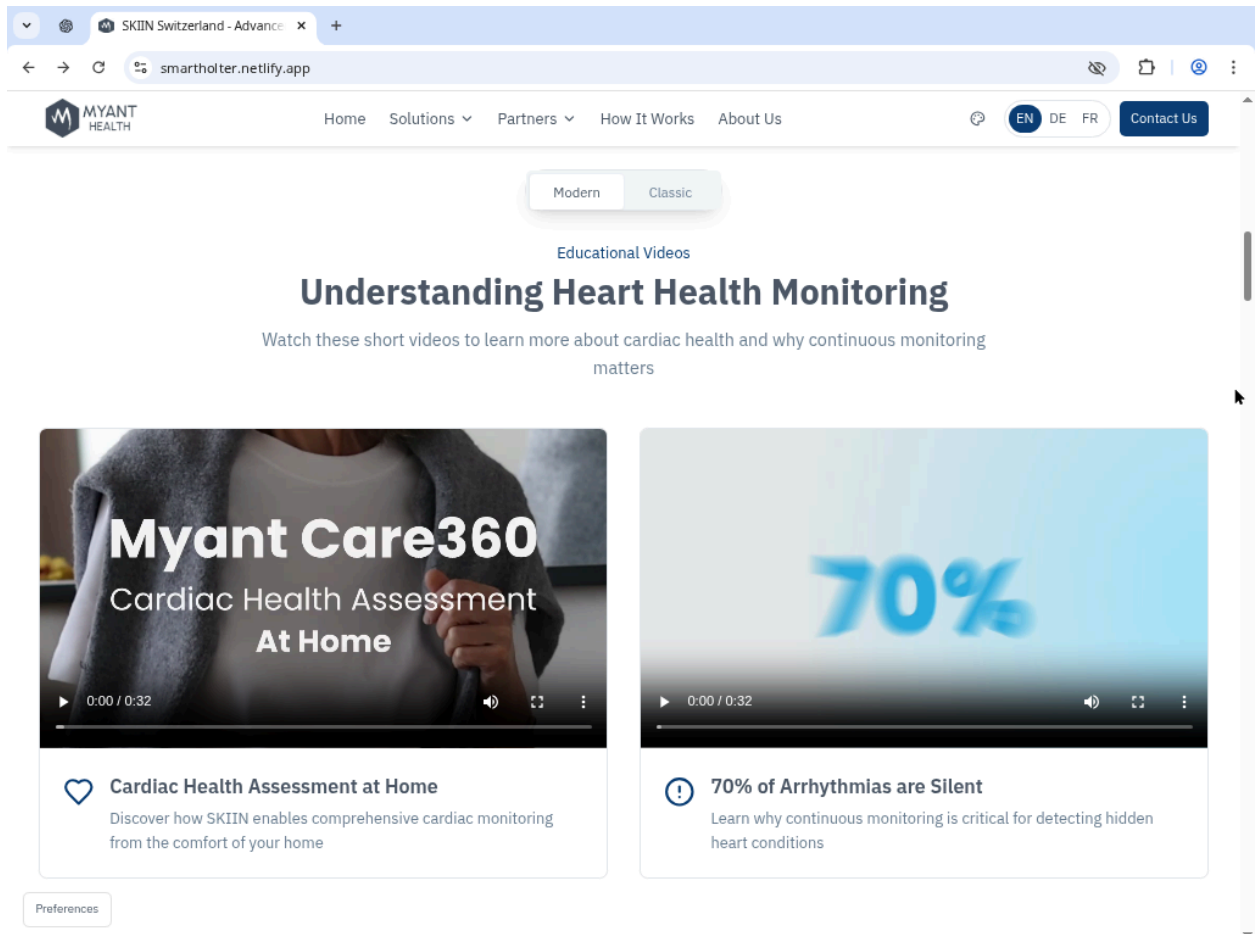


smartholter.netlify.app.

3. **SKIIN by the Numbers:** Four large numbers (95 % detection accuracy, 14 days continuous monitoring, 100 % insurance coverage, 24/7 real-time analysis) summarise key benefits

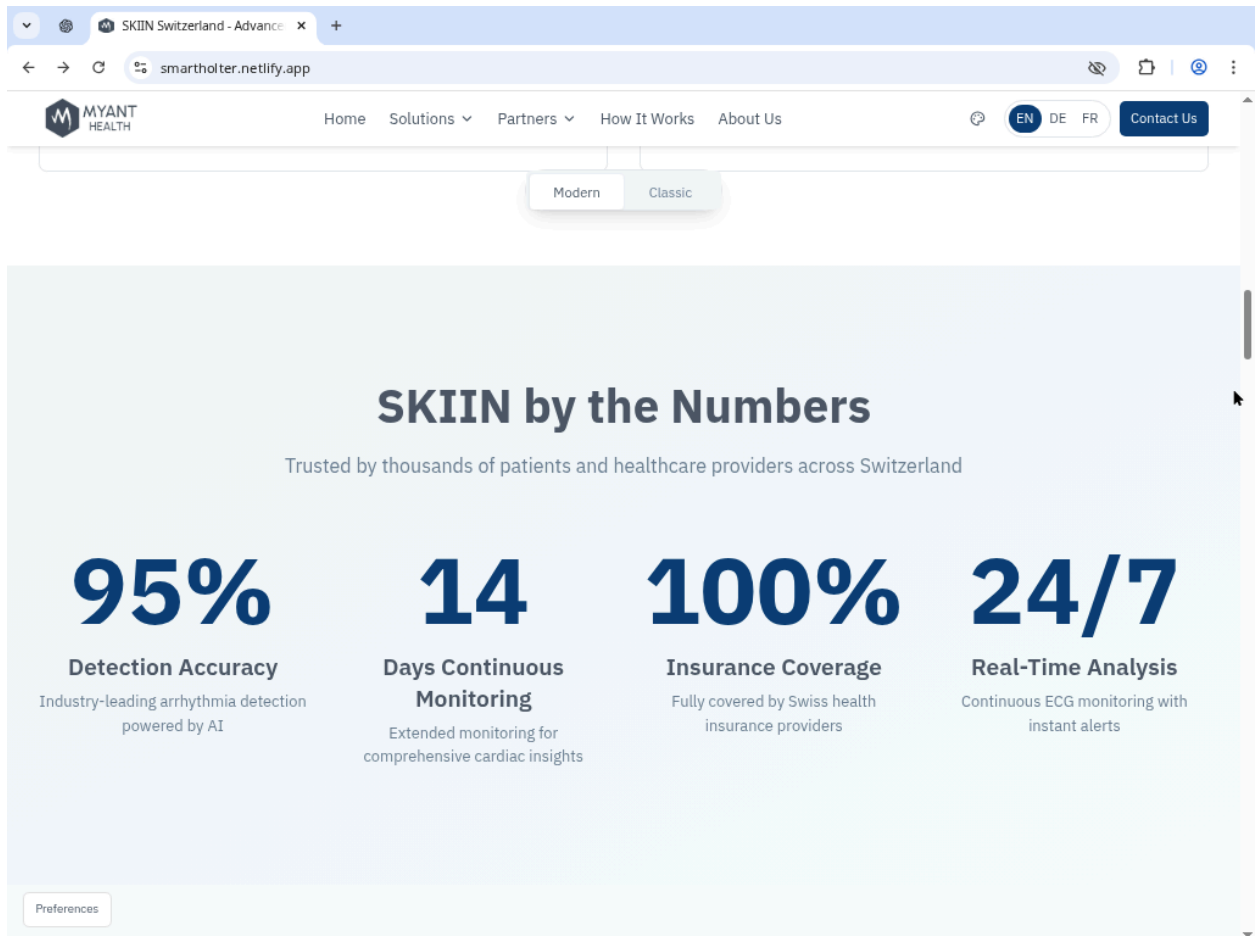


smartholter.netlify.app.

4. **Clinically Proven Technology:** This section lists four trust markers (98.6 % accuracy rate, published research, FDA & CE certified, cardiologist endorsed)

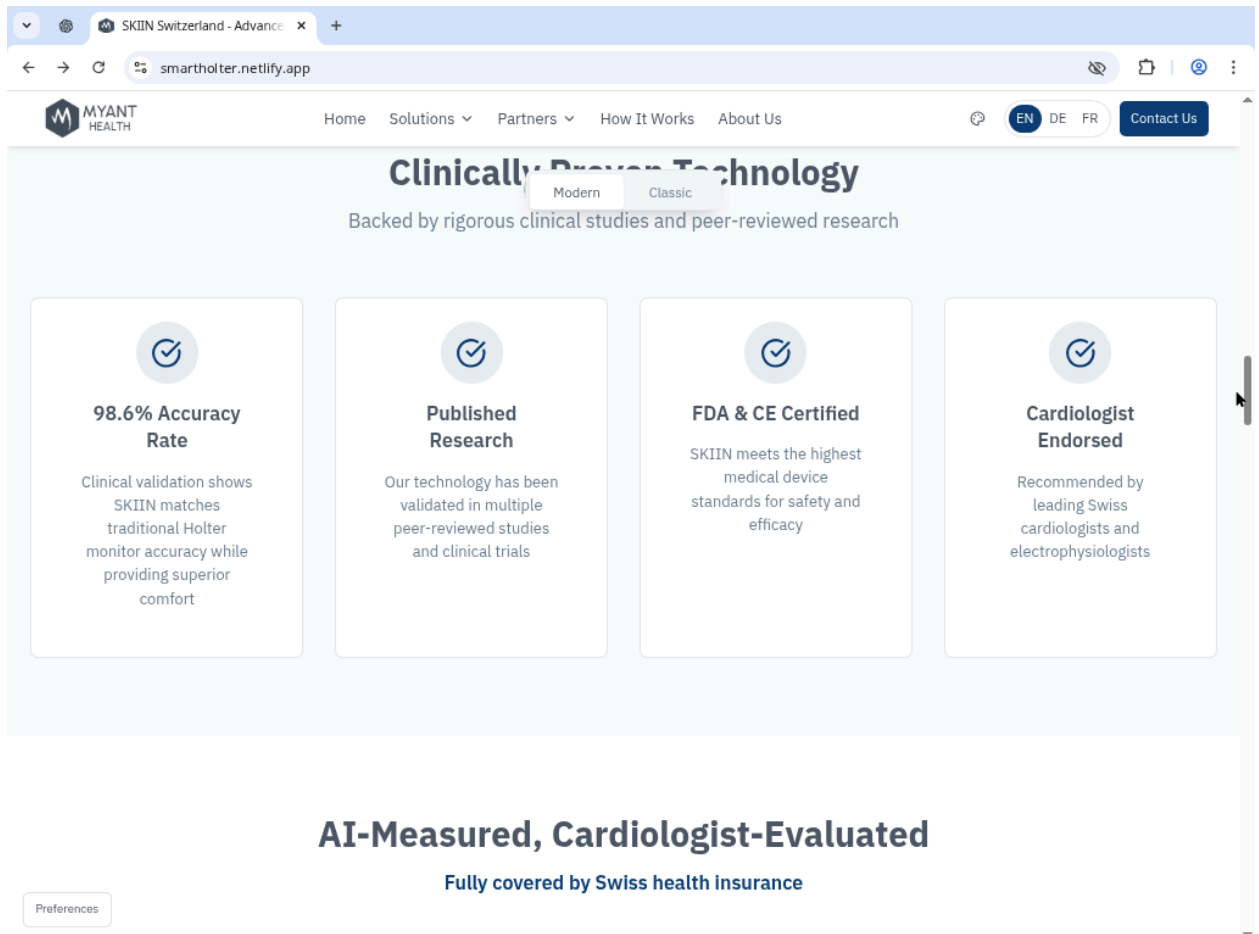


smartholter.netlify.app.

5. **AI-Measured, Cardiologist-Evaluated:** Four icons summarise comfortable monitoring, AI analysis, cardiology expertise and insurance coverage

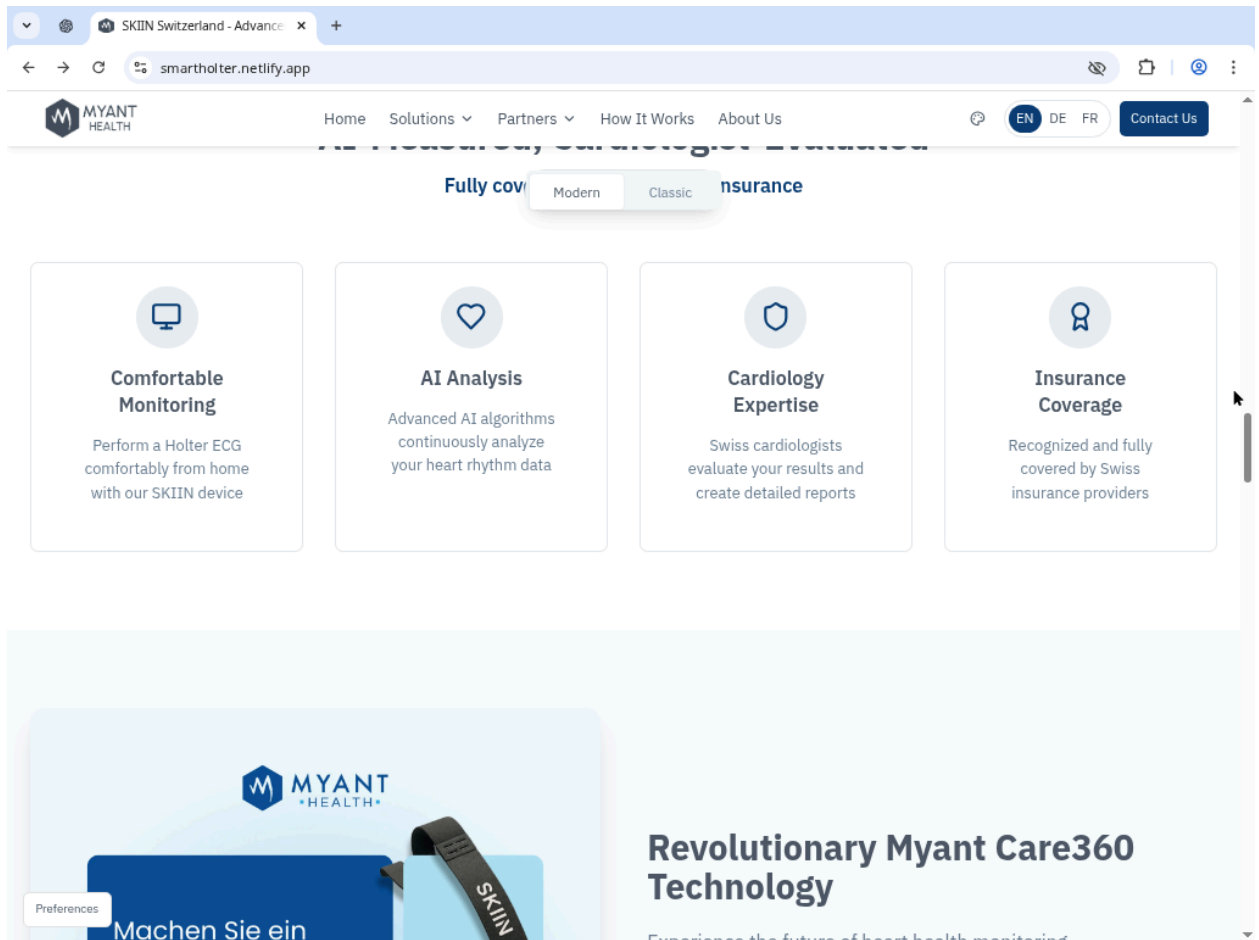


smartholter.netlify.app.

6. **Revolutionary Myant Care360 Technology:** A two-column layout pairs a graphic with a list of features such as 14-day continuous monitoring, real-time AI analysis, Swiss cardiologist validation and seamless data transmission

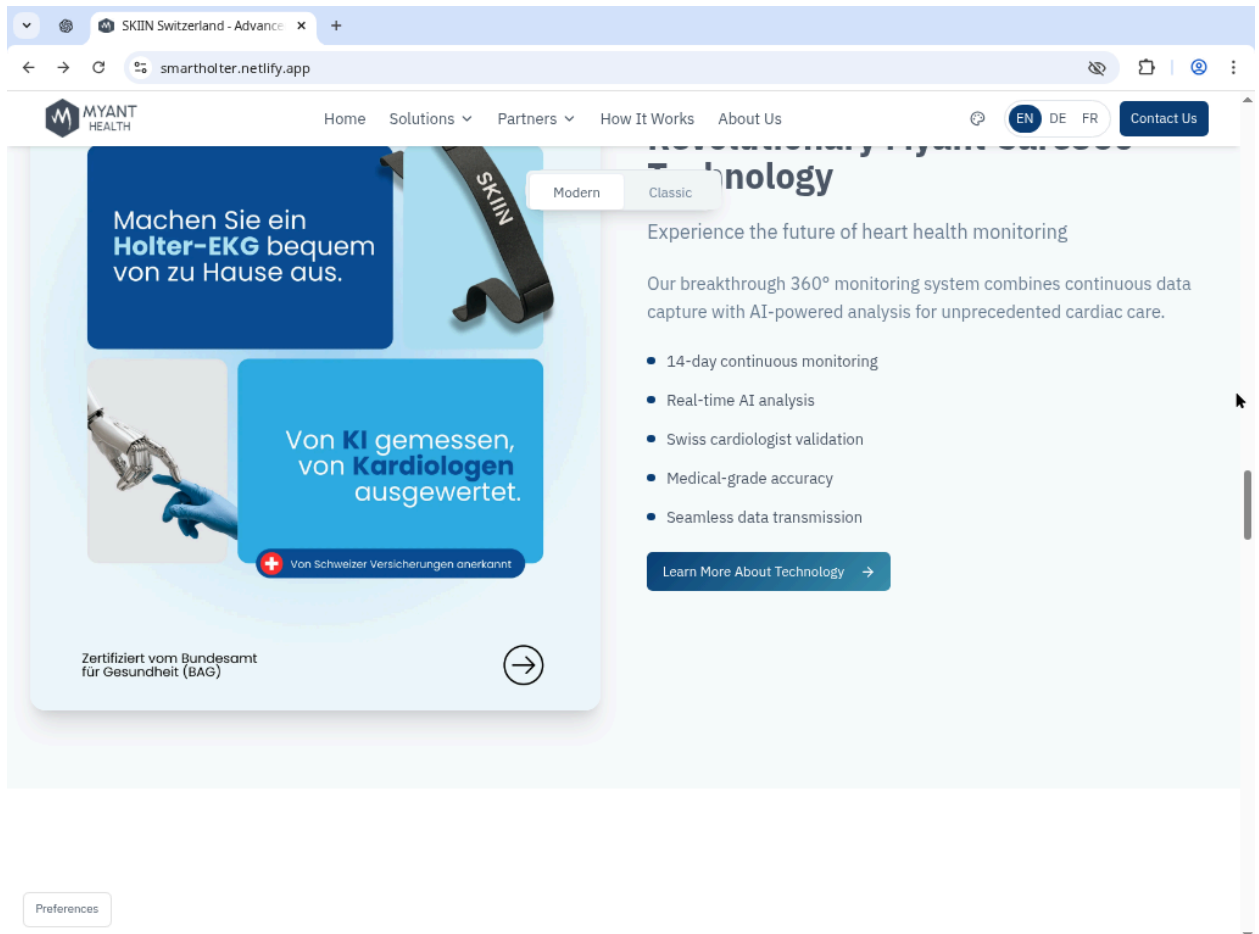


smartholter.netlify.app.

7. **Process Section:** A five-step journey explains referral, delivery, wearing the device, monitoring and receiving results

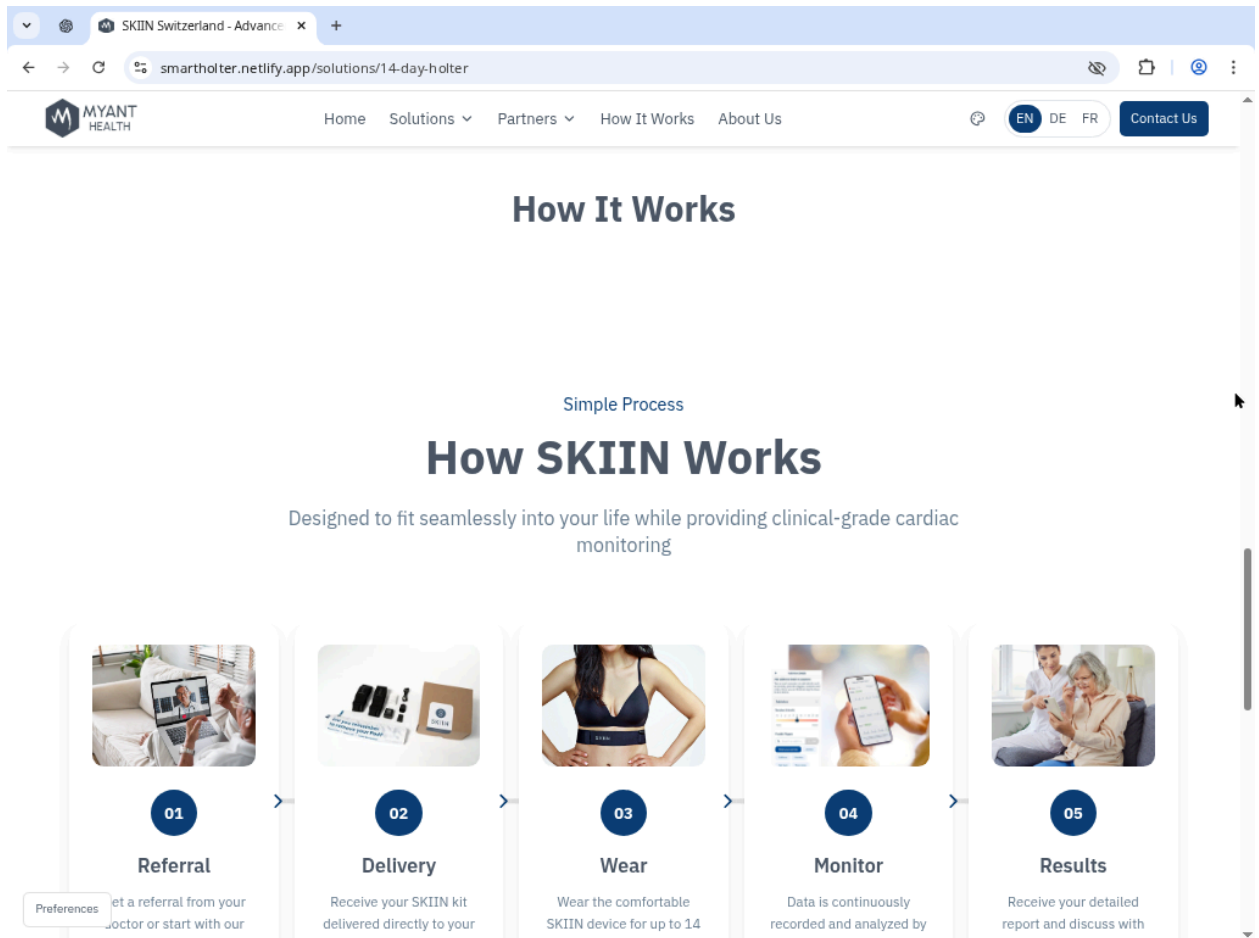

smartholter.netlify.app.

8. **Myant Virtual Clinic Portal (MVCP):** A dedicated section on the home page introduces the MVCP dashboard and its capabilities, including real-time ECG review, patient data management, collaborative care and AI-powered analysis

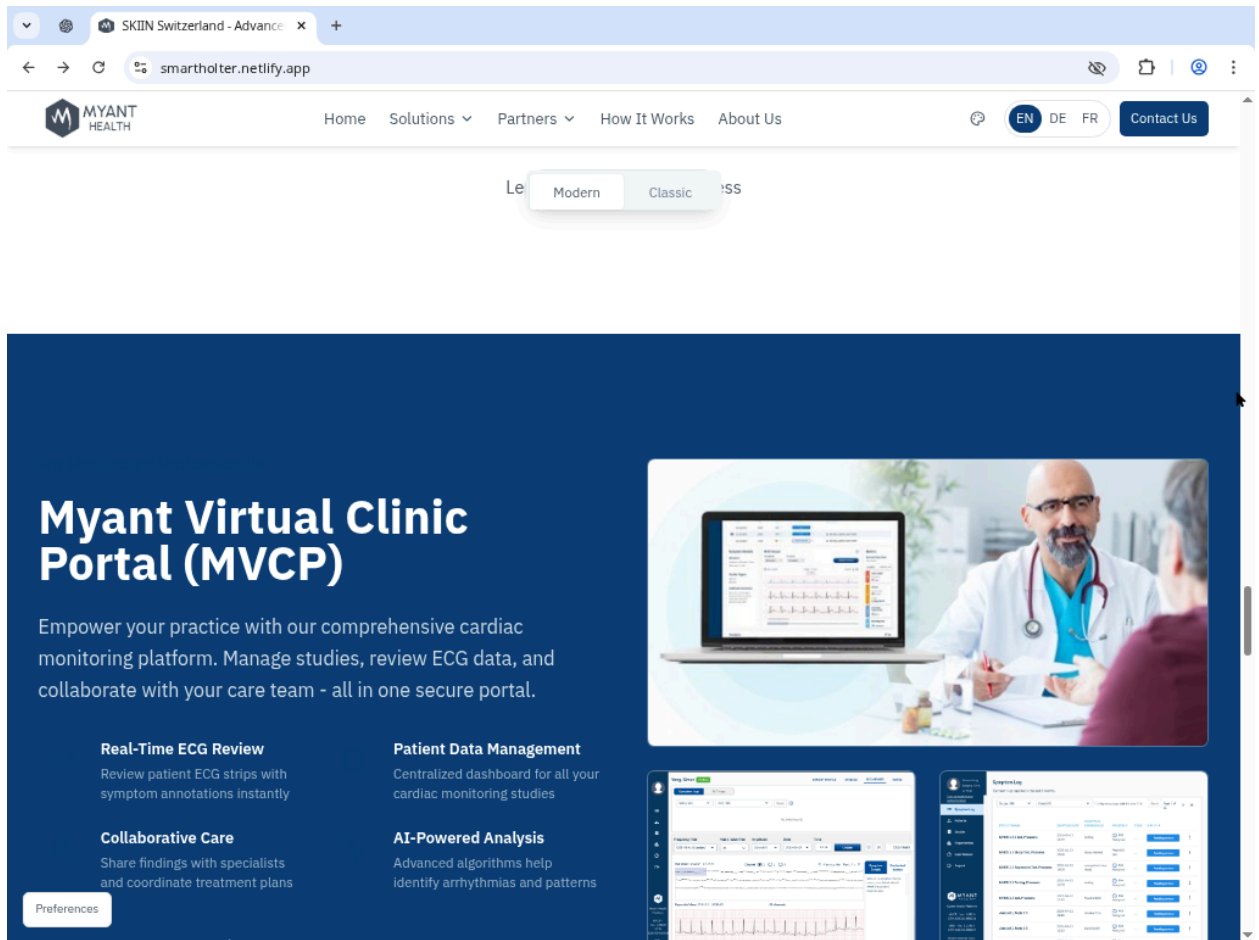

smartholter.netlify.app.

9. **Insurance Coverage:** A section emphasises that SKIIN is recognised and covered by Swiss basic insurance, with bullet points listing coverage details and reimbursement support

SKIIN Switzerland - Advance x +

← → ↻ smartholter.netlify.app

MYANT HEALTH Home Solutions Partners How It Works About Us EN DE FR Contact Us

SKIIN is recognized and covered by Swiss health insurance when medically prescribed

Navigate the Swiss healthcare system with confidence. Our team helps ensure proper coverage for your cardiac monitoring needs.

- ✓ Covered by basic insurance when prescribed
- ✓ No out-of-pocket costs for qualifying patients
- ✓ Reimbursement support included
- ✓ Direct billing available

Krankenversicherung.

Zertifiziert vom Bundesamt für Gesundheit (BAG)

Know Your Heart Risk

Understanding your cardiovascular risk can save your life


Preferences **Silent Atrial Fibrillation**
Often asymptomatic but increases

Cardiac Arrhythmias
Irregular heartbeats that can be life-

Heart Disease Prevention
Early detection enables prevention


smartholter.netlify.app.

10. **Know Your Heart Risk:** Three cards highlight silent atrial fibrillation, cardiac arrhythmias and heart disease prevention

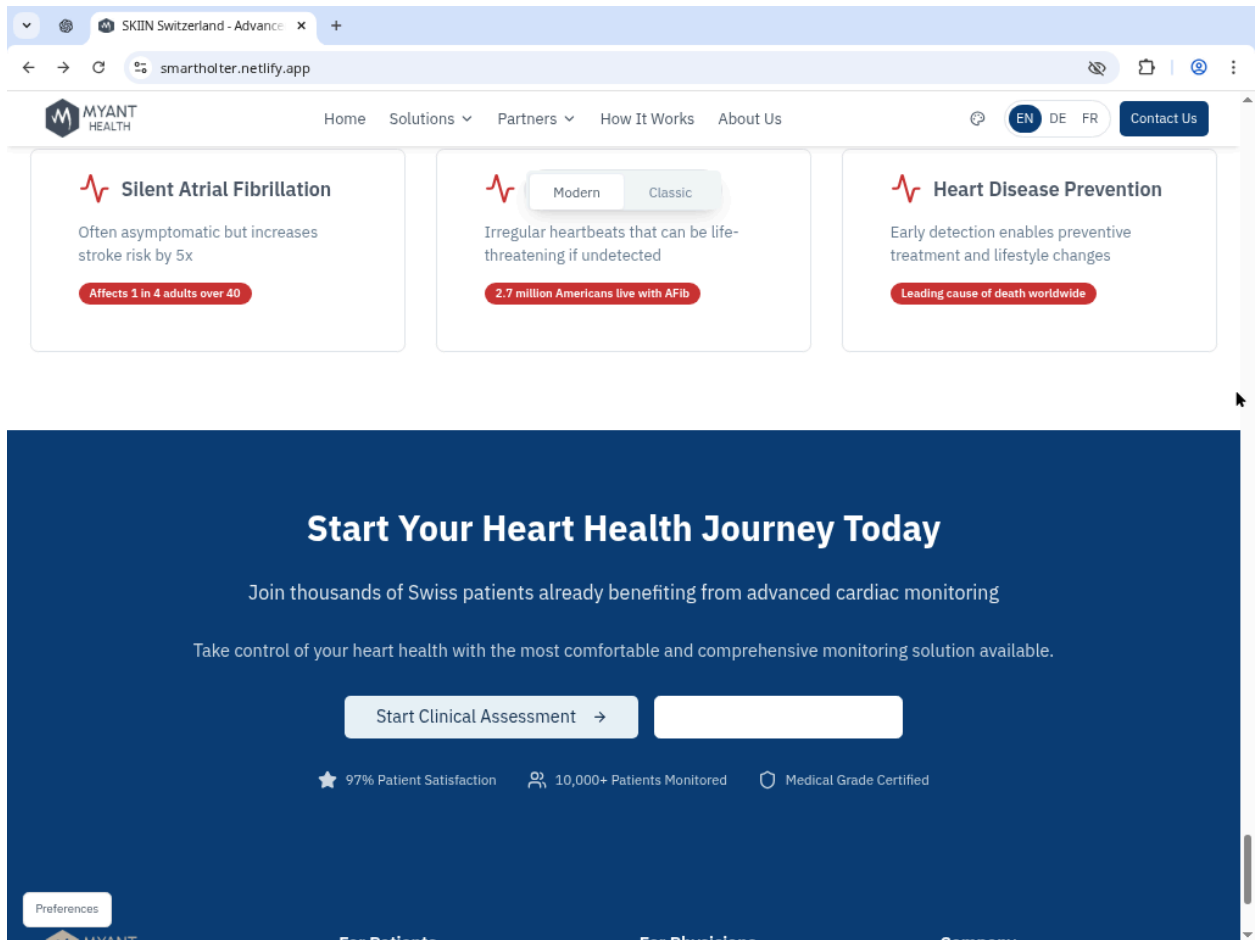

smartholter.netlify.app.


11. **Final CTA:** A blue banner invites visitors to “Start Your Heart Health Journey Today” and features a single CTA (“Start Clinical Assessment”) with supporting statistics (patient satisfaction, patients monitored)

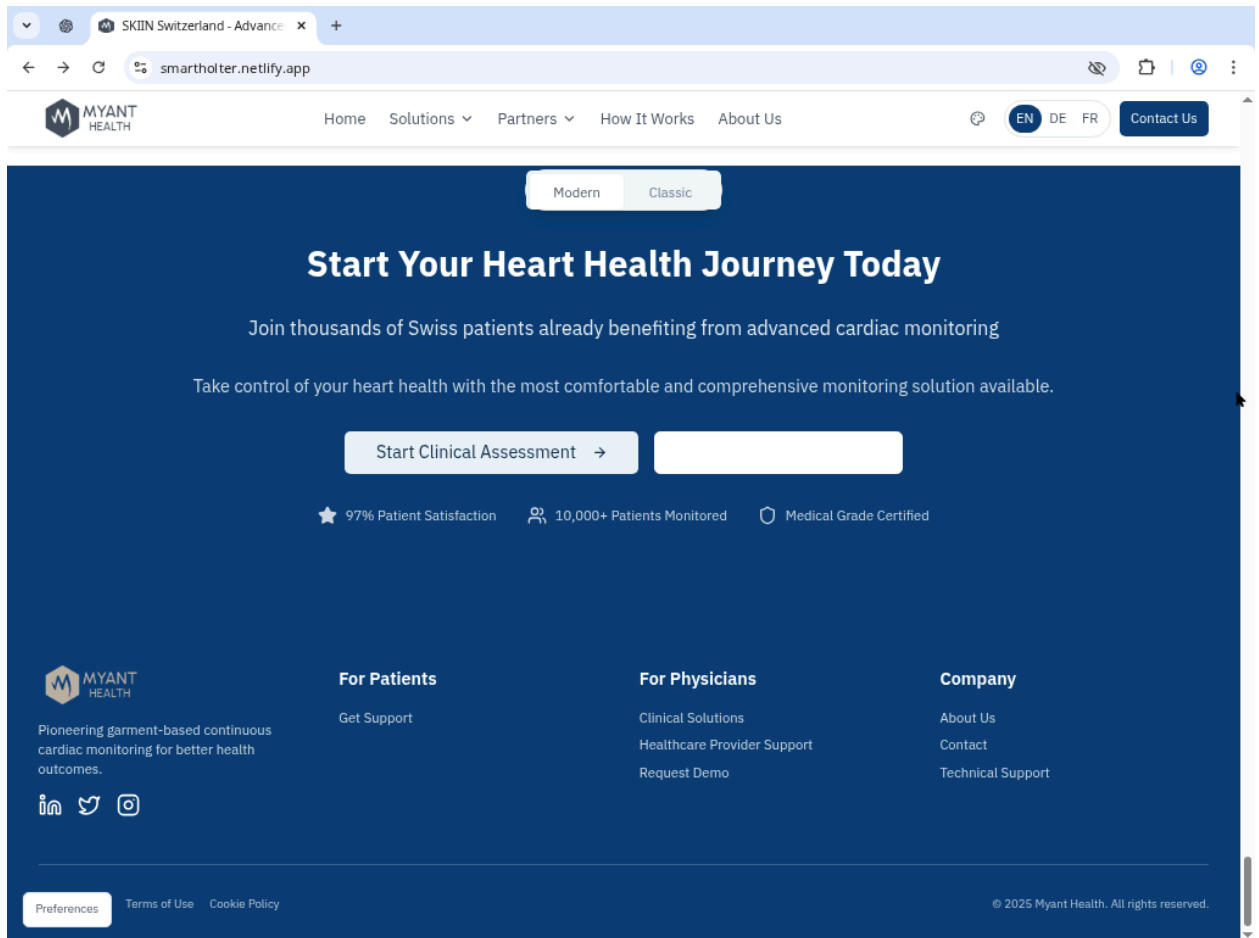

smartholter.netlify.app.

5.2 Solutions Page (14-Day Holter ECG)

The solutions page for the 14-Day Holter ECG retains a similar layout to the home page. The hero features an image of a woman wearing the SKIIN band, a badge (“CE Certified Medical Device”), the headline “14-Day Holter ECG,” a subheadline emphasising comfort and clinical expertise, and a single CTA (“Check Eligibility”)

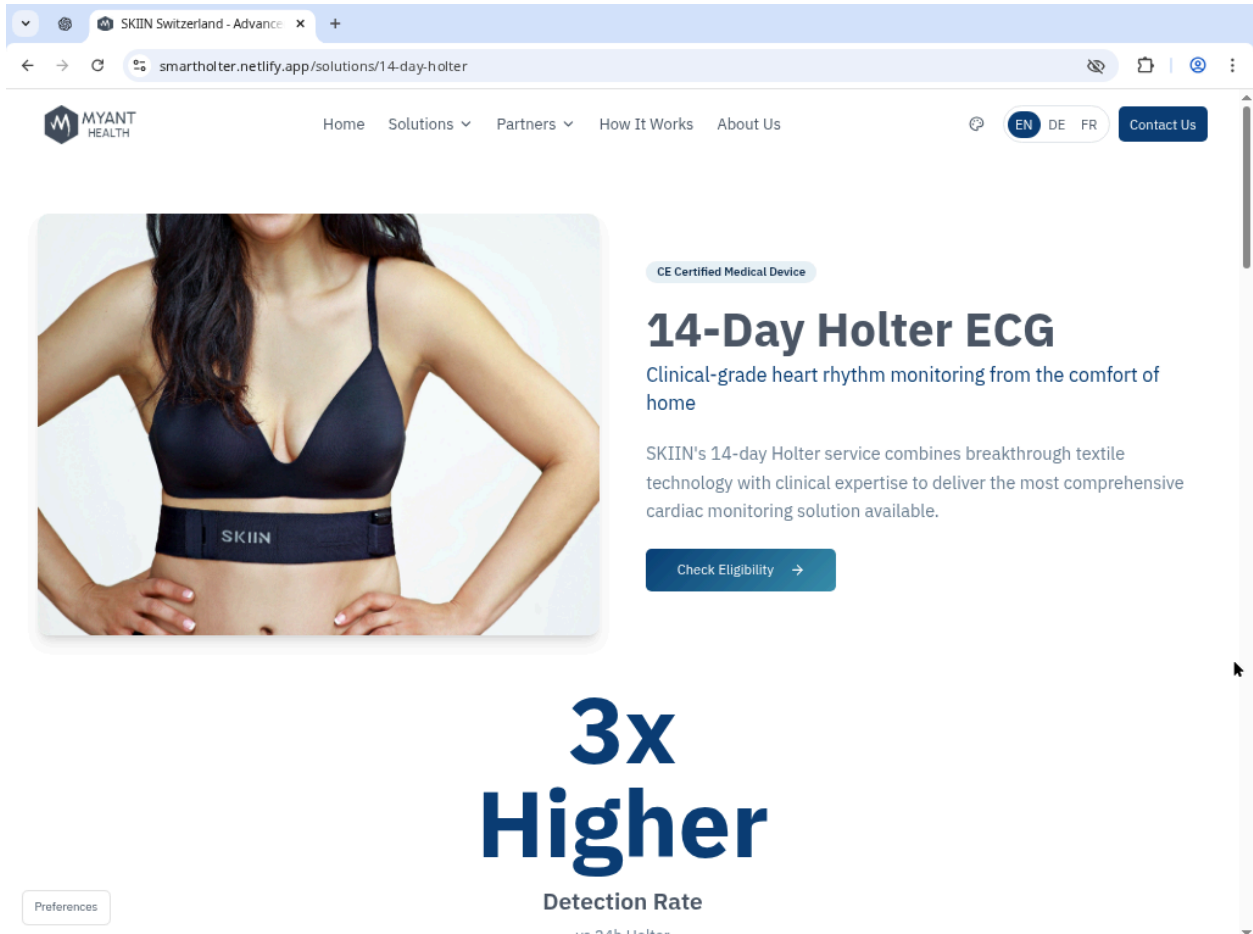

smartholter.netlify.app. Subsequent sections include the “3× Higher Detection Rate” call-out, a feature comparison table (“SKIIN vs Traditional Holter”), the five-step process diagram and another final CTA. The overall tone is clinical and emphasises extended monitoring and detection efficacy.

5.3 Key Gaps between the Copy Specification and the Current Website

1. **Hero messaging and CTAs:** The website’s hero emphasises “Clinical Precision Healthcare” and uses CTAs like “Start Clinical Assessment” and “Book Assessment,” whereas the v7 spec proposes preventive and patient-friendly headlines with CTAs “Start Your Free Assessment,” “Check Insurance Coverage” and a FAQ link. Aligning the spec with the UI may require harmonising language and ensuring CTAs correspond to a single eligibility form.
2. **14-Day vs 10-Day Monitoring:** The live site references a 14-day Holter service and claims a three-fold improvement in detection rate, whereas the v7 spec emphasises a 10-day screening. Deciding whether to adopt a 10-day or 14-day duration (or offering

both) is a critical alignment decision.

3. **MVCP Placement:** The home page contains a prominent MVCP section, but the CEO has instructed that MVCP content should appear only on the General Practitioner page. The copy spec must reconcile this discrepancy by either removing MVCP from the home page or ensuring that the GP page captures all MVCP details.
4. **Additional Sections:** The website features segments not present in the v7 spec, such as “Educational Videos,” “SKIIN by the Numbers,” “Clinically Proven Technology,” “AI-Measured, Cardiologist-Evaluated,” “Revolutionary Myant Care360 Technology,” “Know Your Heart Risk” and a comparative features checklist. Integrating or adapting these sections can make the copy spec more consistent with the UI.
5. **Insurance Coverage Section:** The site devotes a section to explaining that SKIIN is covered by Swiss health insurance, whereas the v7 spec combines insurance information within pricing. Separating insurance coverage from pricing could better match the UI.
6. **Partner Pages and Professional CTAs:** The home page includes professional CTAs (e.g., “Request Demo” in the MVCP section) that may confuse patients. The spec should ensure that professional CTAs appear only on partner pages or be clearly demarcated.

By documenting these gaps, we can plan modifications that adapt the v7 copy to the current website’s structure while preserving the CEO’s requirements and marketing objectives.

5.4 New Guidance from CEO Comments (July 24 2025)

After submitting Version 7.1, the CEO provided additional feedback. Key directives include:

- **Rename the Features Section to Product Section:** The CEO wants to emphasise product benefits rather than generic “features.” The Product section should follow the bullet list shown in the provided screenshot (extended monitoring, shortened wait times, seamless referrals, comfortable band, AI precision, fast turnaround, proven technology, Health Canada licensed). This ensures that value propositions are clear and aligns with the current UI.
- **Insert the phrase “If you have no symptoms but still want to be checked”** in the pricing note. This language reassures asymptomatic visitors that self-pay screening is a valid option and encourages preventive action.
- **Expand the Technology page into narrative paragraphs.** The outline previously used on the Technology page must be replaced with full copy that explains carbon-electrode

technology, ambulatory BP cuff, sleep analysis, the sensor→app→cloud→AI→cardiologist pipeline and security/compliance. The narrative should also highlight that SKIIN is the first piece of textile designed to diagnose the heart and include a carousel visual describing the data flow.

- **Emphasise the Silent Triad, chronic conditions and longevity.** The copy should describe how arrhythmia, hypertension and sleep apnoea interact, why chronic conditions require regular screening and how the upcoming SKIIN 3X Screening™ will monitor all three modalities. This reinforces the company's vision of preventive health and longevity.
- **Clarify GP billing rules.** General practitioners can only bill for consultation and patient onboarding; interpretation is the cardiologist's responsibility. This must be reflected on the Partners page and in the TOT.

These new directives will be incorporated into Version 7.2 and reflected in the updated planning, brainstorming and change log documents.

2. Additional Context for UI Iteration (24 July 2025)

After delivering Versions 7.2 and 7.1, the user requested a deeper review of the **live website UI** (<https://smartholter.netlify.app/>) and the copy specifications to ensure alignment and iterate on existing components. The goal is to map the complete copy from **v7.1** (the CEO-aligned version) to the current UI components, identify gaps and propose new or modified components for a future update. Key observations include:

- **Hero Section:** The current home page hero (under the “Modern” theme) features the headline “**Clinical Precision Healthcare**” and CTAs “**Start Clinical Assessment**” and “**Book Assessment.**” This contrasts with the Version 7 hero copy, which emphasises preventive health urgency, comfort and family control. The new hero should adopt the **Vincent’s variant** (Headline: “*Heart Disease Is the #1 Killer — When Was Your Last Heart Check?*”) and the standard CTAs. The hero design includes a split layout with text on the left and an image on the right[121463520507852†screenshot].
- **Statistics Section:** Immediately below the hero is a **Why Early Detection Is Critical** section with three cards showing 70 %, 30 % and 50 % statistics[235987424365000†screenshot]. This design aligns with the **Statistics Section** in our copy spec, but the copy must be updated to reflect accurate statistics (70 % silent arrhythmias, 20–30 % stroke link, 66 % vs 9 % detection) and include footnotes.

- **Educational Videos:** The live site includes an **Educational Videos** section featuring two short videos on cardiac health and silent arrhythmias[667505432939530†screenshot]. This component is not described in v7.1 or v7.2; we need to decide whether to keep these videos (and update their descriptions) or replace them with other educational content.
- **SKIIN by the Numbers & Clinically Proven Technology:** A combined **numbers** and **technology** section shows four metrics (detection accuracy, days of continuous monitoring, insurance coverage, real-time analysis) followed by four trust cards (accuracy rate, published research, FDA & CE certified, cardiologist endorsed)[553560217291829†screenshot]. Our v7.1 spec includes similar sections (**SKIIN by the Numbers** and **Clinically Proven Technology**), but the numbers must be updated (e.g., 95 % detection accuracy, 10 days continuous monitoring). We should adapt the design to accommodate our updated metrics and textual copy.
- **AI-Measured, Cardiologist-Evaluated:** The site uses a four-card section labelled “**AI-Measured, Cardiologist-Evaluated**” with cards for comfortable monitoring, AI analysis, cardiology expertise and insurance coverage[979310607466692†screenshot]. Our v7.1 copy spec replaces the **Features Section** with a **Product Section** containing eight bullet points. We need to reconcile this by either condensing our eight benefits into four categories or expanding the UI to accommodate all eight items.
- **Myant Care360 Technology:** The current site includes a “**Revolutionary Myant Care360 Technology**” section with an image of the SKIIN band and a five-item bullet list: 14-day continuous monitoring, real-time AI analysis, Swiss cardiologist validation, medical-grade accuracy, seamless data transmission[631927473953222†screenshot]. Our v7.1 copy emphasises that “revolution” is inappropriate; instead, the section should be titled “**Myant Care360 Technology**” and follow the eight-point bullet list from the Product section. We should also update the monitoring duration (10 days) and remove hyperbolic language.
- **Process Section:** The **How SKIIN Works** section depicts a 5-step journey (Referral, Delivery, Wear, Monitor, Results) using cards with icons[294393807844794†screenshot]. Our v7.1 process narrative matches this structure but updates descriptions (e.g., emphasising self-assessment, 10-day monitoring and AI analysis). The UI design is compatible; we just need to update the copy and ensure translation.
- **Myant Virtual Clinic Portal (MVCP):** The home page includes a large blue section promoting the MVCP with features such as real-time ECG review, patient data management, collaborative care and AI-powered analysis[782037975639679†screenshot]. In v7.1, the MVCP content is moved to the **General Practitioner** page and summarised briefly in the cardiologist section. We must decide whether to remove this section from the home page or convert it into a smaller call-out

linking to the partner pages.

- **Comparison Table:** The site presents a **How SKIIN Compares** table contrasting SKIIN with traditional monitors across factors like monitoring duration, data transmission and patient comfort[810302637999466†screenshot]. Our v7.1 spec does not explicitly include a comparison table, but the concept supports the Product section's value propositions. We should determine whether to keep, update or replace this table.
- **Insurance Coverage & Pricing:** A section titled "**Comprehensive Insurance Coverage**" outlines that SKIIN is covered by Swiss health insurance when prescribed and lists benefits (no out-of-pocket costs, reimbursement support, direct billing)[379169971394415†screenshot]. Below this, a "**Know Your Heart Risk**" section features cards about silent AF, cardiac arrhythmias and heart disease prevention[799235110776073†screenshot]. Our v7.1 copy splits insurance and pricing into separate sections and includes a self-pay table with a note for asymptomatic users. We need to propose how to display pricing and risk information within the existing design.
- **Final CTA:** The page ends with a dark blue "**Start Your Heart Health Journey Today**" section encouraging visitors to start the clinical assessment[799235110776073†screenshot]. The copy emphasises patient benefits and includes icons for patient satisfaction and patients monitored. Our v7.1 spec's final CTA has similar intentions but slightly different wording ("Take control of your heart health today").

In addition to reviewing the live site, we examined the repository's **component inventory** and **visual architecture** documents. The repository uses **shadcn/ui** components and React with TypeScript. Key components include **HeroSection**, **StatisticsSection**, **ProblemSolutionSection**, **FeaturesSection**, **ProcessSection**, **MvcpSection**, **ComparisonSection**, **InsuranceSection**, **RiskSection**, **CTASection** and various partner-specific components. Our mapping file (**component_mapping_gap_analysis.md**) already aligns these components with the v7.2 copy. We will extend this mapping to v7.1, noting that the product section now has eight benefits and the technology narrative is expanded.

The next steps involve constructing a detailed tree-of-thought mapping, brainstorming how to adapt the v7.1 copy to existing UI components, performing a gap analysis to identify new component requirements, planning tasks and creating an updated copy specification with UI component assignments. We will document these in **TOT.md**, **BRAINSTORM.md**, **planning.md** and **todo.md**, using the above observations and citations as evidence.

This research summary serves as a foundation for constructing the tree-of-thought, brainstorming potential improvements, planning the work and drafting the final copy specification.

Extended Tree-of-Thought Diagram:

Tree-of-Thought Diagram: SKIIN Switzerland Website Architecture & Entities

This diagram breaks down the entities (pages, sections, modalities, audiences) and their relationships for the SKIIN Switzerland website (Version 7.0). Entities are defined as relevant, specific (≤ 5 words), novel, faithful to source content and found anywhere in the content.

1. Website Architecture (Top-Level Pages)

- **Home** – Patient-focused landing page.
 - **Hero Section** – Multiple A/B testing variants share a common structure: badge, headline, subheadline, emotional subheadline and CTAs. **Variant A (default)** follows Vincent’s “Urgency & Longevity” theme and is prioritised per the CEO’s directive. It uses the headline “Heart Disease Is the #1 Killer — When Was Your Last Heart Check?”, a subheadline noting that **70 %** of arrhythmias show no symptoms and can cause strokes if undetected and an emotional subheadline emphasising longevity (“Longevity means more birthdays — for you, and for those who love you most”). CTAs remain consistent across variants: **Start Your Free Assessment** (primary), **Check Insurance Coverage** (secondary) and **Questions? Read our FAQ** → (text link).
 - **Statistics Section** – Three call-outs (70 % silent AF; 20–30 % AF-related strokes; 66 % vs 9 % detection; ABPM gold standard may appear as a fourth card).
 - **Problem/Solution Framework** – Narrative: silent danger, waiting and wondering, brief snapshot vs long view. Introduce comfort revolution, longevity and quality of life.
 - **Product Section** – Present a benefits-driven overview of the tri-modal system. Key points include: extended monitoring for deeper insight (e.g., 10-day screening catches intermittent arrhythmias); shortened wait times and earlier detection; swift, seamless referrals via MVCP; comfortable textile-based band that is water-resistant and removable; AI-powered precision using CNN/Transformer models; fast turnaround (results within 24–48 hours); proven

technology trusted by clinics and cardiologists; and licensing by Health Canada in addition to MDR Class IIa and Swissmedic.

- **Process Section** – 5-step journey for patients: eligibility assessment, kit delivery, monitoring, report generation, next steps with physician; note MVCP involvement for clinicians.
- **SKIIN by the Numbers** – Four metrics summarising detection accuracy, monitoring duration, insurance coverage and real-time analysis.
- **Clinically Proven Technology** – Trust markers highlighting accuracy, published research, MDR & CE certification and cardiologist endorsement.
- **AI-Measured, Cardiologist-Evaluated** – Four pillars: comfortable monitoring, AI analysis, cardiology expertise and insurance coverage.
- **Myant Care360 Technology** – Overview of continuous monitoring, real-time AI, Swiss cardiologist validation, medical-grade accuracy and seamless data transmission.
- **Know Your Heart Risk** – Three call-outs about silent AF, arrhythmias and heart disease prevention.
- **Insurance Coverage & Pricing** – Separate sections: coverage explanation (no out-of-pocket costs, reimbursement support) and transparent self-pay options (3/5/10 days).
- **Testimonials** – Patient stories and quotes from medical advisors; emphasise comfort, peace of mind and family impact.
- **CEO's Message** – A brief quote from Tony Chahine, founder and CEO of Myant, is integrated near the final CTA on the home page. It underscores the mission to normalise cardiac screening, make it as routine as dental check-ups and empower people to take control of their heart health.