


Separating chemical and temporal station calibration

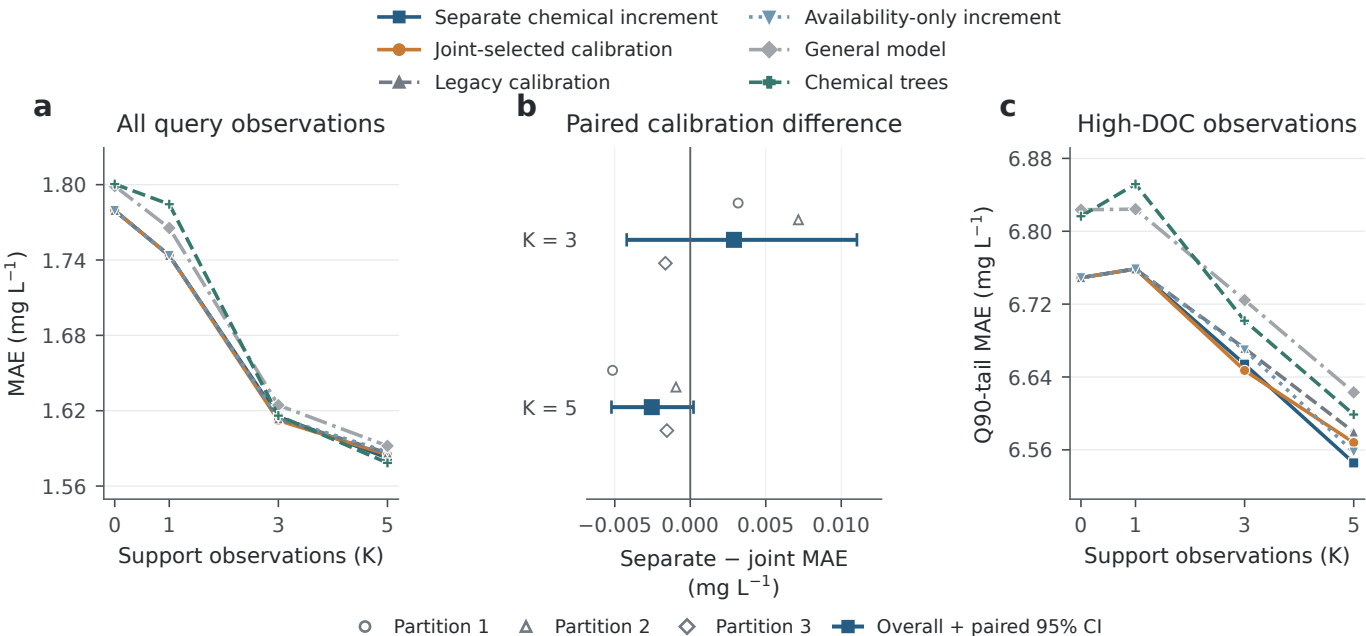

Negative paired differences favor the separate chemical increment.

Equal partition means · 5,000 joint station-bootstrap draws · Dots are partition means