


Current-source DOC reconstruction in an external basin

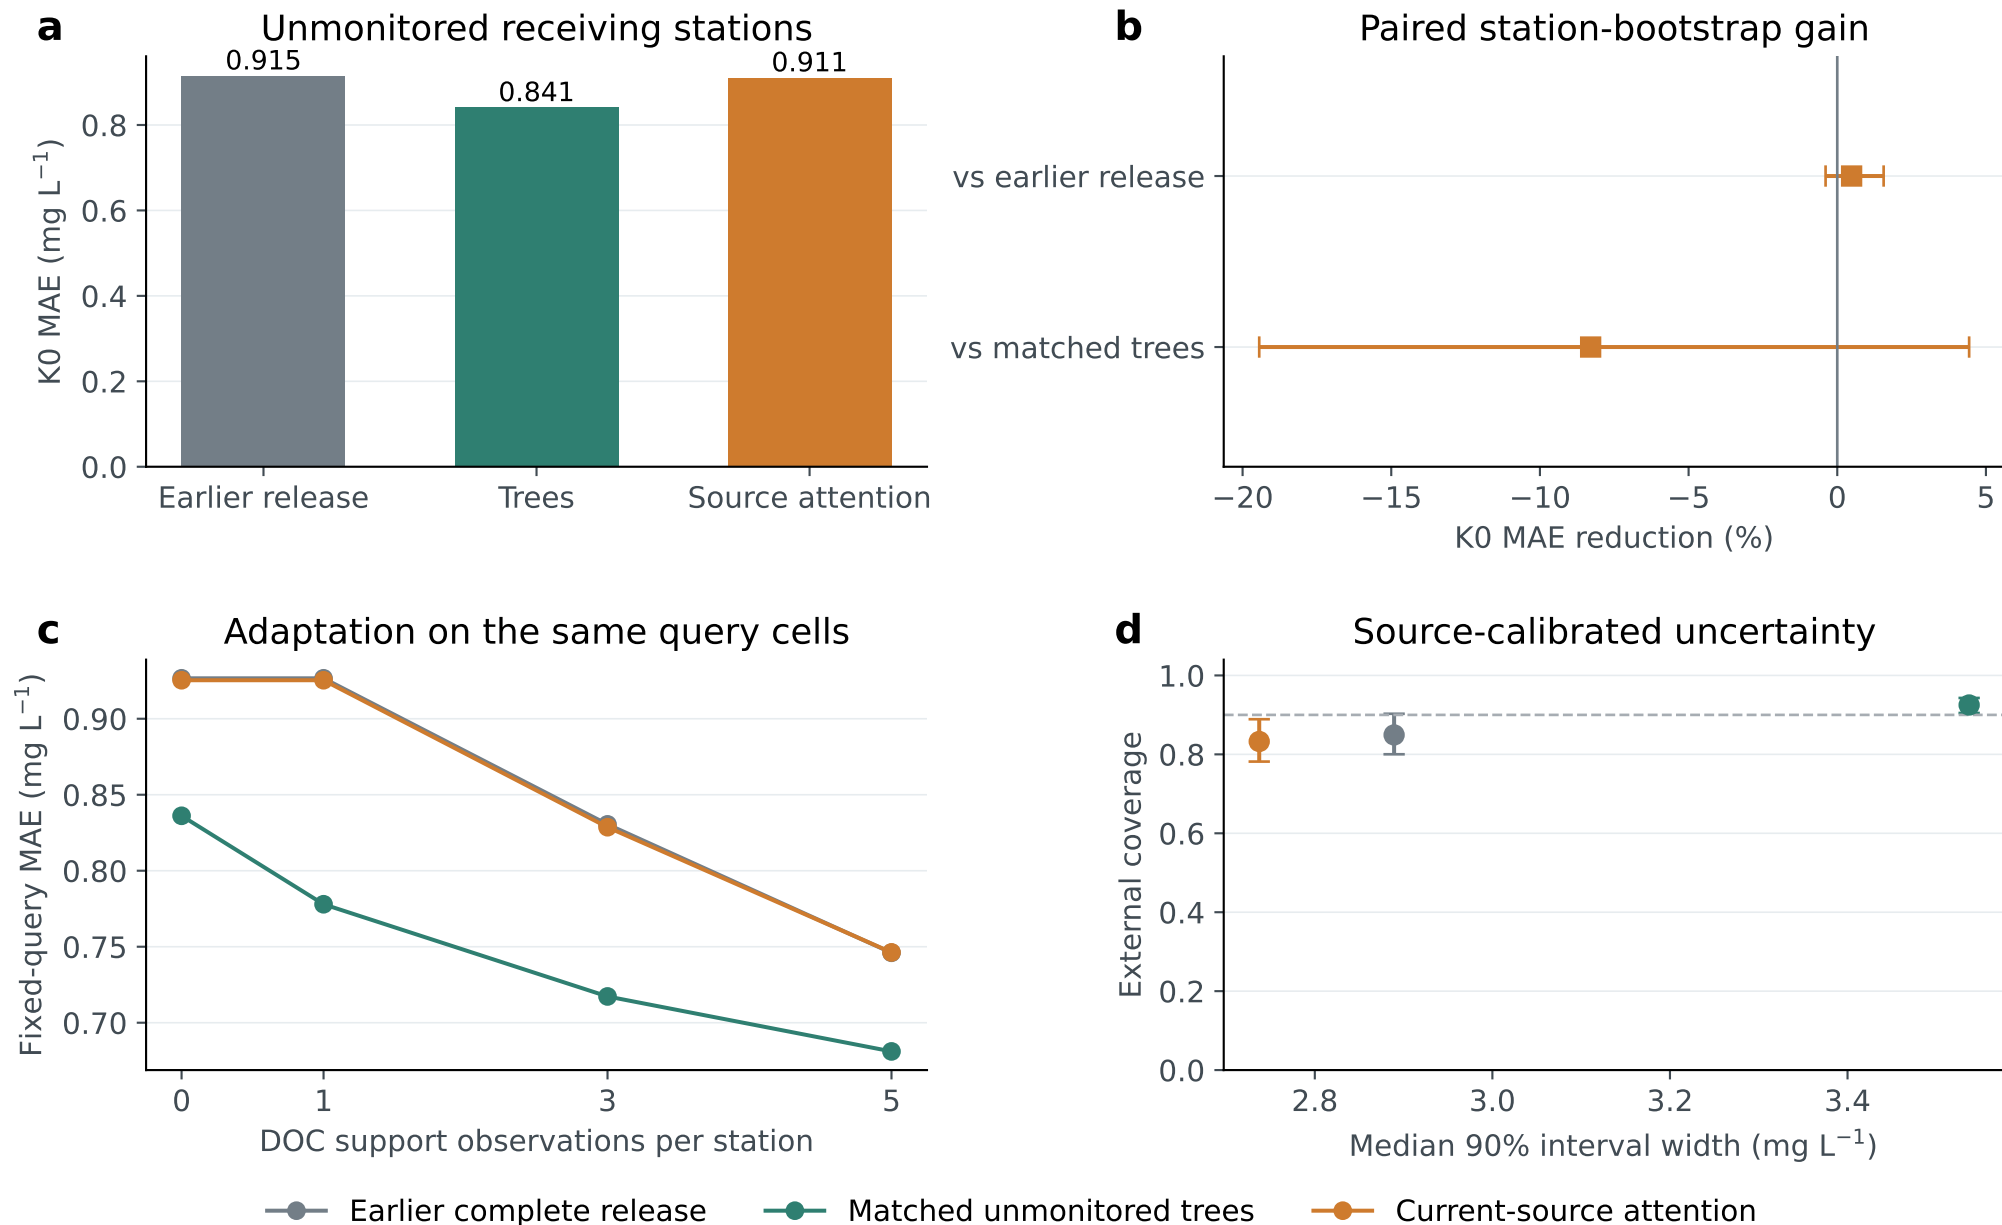

HUC02040104 · 130 stations · five-seed ensemble · previously inspected external case

K0: no external DOC calibration. K curves: designated support only. Intervals: source validation only.