

Reading the onset at 50 % instead of 10 % of the peak: error N1 0.98 → 0.64 ms, N2 5.2 → 3.9 ms (51 patients)

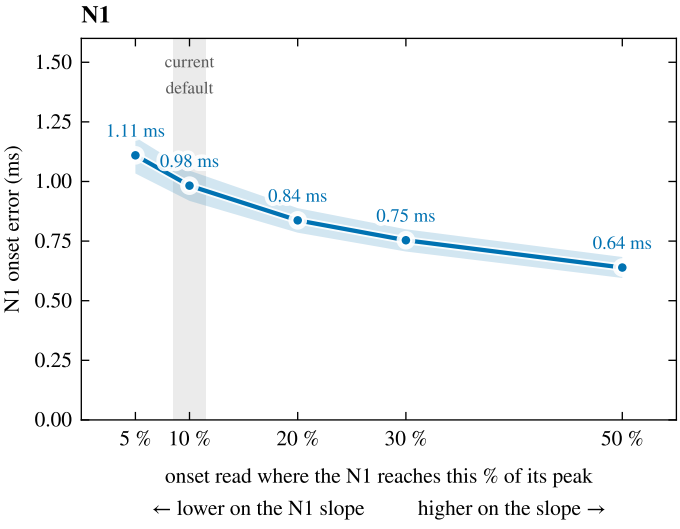

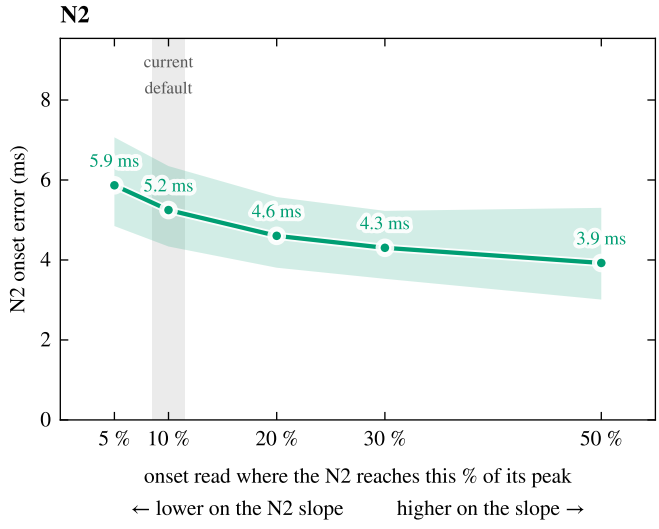

Onset: first time the fitted N1 or N2 reaches the given % of its peak. Error: |fitted onset - true onset| in ms, both read at the same %.

Truth: known N1 and N2 added to real recorded noise. Per patient: median over contacts. Line: mean of 51 patients. Band: 95 % confidence interval over patients.