Copyright© 2021-2026 NEWPONG Co.,Ltd. All rights reserved.

LSSA

LSSA User Manual

NPUM-200(US) Rev.12 2026.03.03

Eng.ver

Copyright© 2021-2026 NEWPONG Co.,Ltd. All rights reserved.

Reference before use

This user manual contains all the information to help users understand how to control and operate the product. If you have any question or problem regarding handling the product, do not hesitate to contact us. Manufacturer and official agency shall not be responsible for any problem occurring from misuse or violation of descriptions in the user manual or any problem occurring from unqualified operator.

The product and company means each LSSA and NEWPONG in this user guide.
Please use the product in a right and safe manner after reading marked danger, warning, caution, and notice in this manual in detail.

Copyright© 2021-2026 NEWPONG Co.,Ltd. All rights reserved.

1. WARNINGS AND PRECAUTIONS 4

2. GENERAL 15

3. INSTALLATION AND CONNECTION 21

4. INSTRUCTION FOR USE 24

5. CLEANING AND MAINTENANCE 29

6. TROUBLE SHOOTING 32

7. PRODUCT SPECIFICATION 34

8. PRODUCT WARRANTY 36

Copyright© 2021-2026 NEWPONG Co.,Ltd. All rights reserved.

1. WARNINGS AND PRECAUTIONS

Failure to comply with the following safety information may result in serious injury or device damage.

1.1. General Caution

1) Please check the product and accessories before use.
   - Always check the condition of accessories before use.
   - Be sure to check the connection status of accessories and equipment before use.
   - Do not place surgical equipment or other electrical appliances close to each other.
   - Be sure to fully read and familiarize yourself with the user manual before use.
   - All accessories must be sterilized by steam prior to use.
2) Avoid operating the product which has visible damage. It may harm to patients.
3) Please understand this user guide before use. Otherwise, it may harm to people or damage the product.
4) Misuse of the product can harm to patients. The people who are well trained and properly understood dangerousness and benefit of the product have to use.
5) Safety and effectiveness of the product and components have been confirmed. Accordingly, safety and efficiency coincides with function requirement.
6) Please use only compatible accessories supplied, as the safety and effectiveness of the products and parts have been confirmed.
7) This equipment is an ultrasonic surgical device and should be operated by qualified medical professionals trained in the safe performance of surgical procedures in accordance with the safety guidelines described in this manual to ensure safe use of ultrasonic energy and medical devices.
8) Before using the machine, beware of following precautions.
   - Check the connection status of the power cord and accessories, and that the equipment is working properly.
   - Check the grounding and make sure that grounding is secure. And do not touch the power plug with wet hands.
   - Do not modify the equipment.
   - When using the equipment with other devices, use it after thorough inspection that there is no impact on the equipment.
9) When installing the device, note the following:
   - Install in a place where water is not nearby.
   - Install in a place where it will not adversely affect air pressure, temperature, humidity, wind, sunlight, salinity, air containing ionic components.
   - Pay attention to safety conditions such as vibration and shock (including transportation and movement).
   - Install in a location that can accurately supply power, voltage, frequency and power consumption.
10) When using the device, note the following:
   - Equipment and patients should be monitored carefully for abnormalities during use.
   - If an abnormality is found in the device or patient, immediately put the patient in a safe state, stop the operation of the device and take appropriate action.

Copyright© 2021-2026 NEWPONG Co.,Ltd. All rights reserved.

- Avoid patient being contacted by the equipment.

11) After using the device, note the following:
   - Return the operation switch to the pre-use state according to its order and disconnect the power supply.
   - Do not pull the cable or apply excessive force when removing the cord.
12) When storing, note the following:
   - Store in a place where air pressure, temperature, humidity, wind, sunlight, salinity, ions, etc. will not adversely affect.
   - Beware of safety conditions such as vibration and physical impact (including transportation and movement).
   - Do not store in chemical storage or gas generating area.
   - Do not store near water.
   - Clean up accessories (cords, etc.) and put them together.
13) Changes in the configuration of equipment and accessories or the use of accessories with unintended specifications may require reevaluation of additional requirements according to IEC60601-1.
14) All components connected to this equipment use the components provided by NEWPONG Co., Ltd. If components not provided by the company are used, there is a possibility that the inspection and operation status of the equipment may not be confirmed, and the equipment may not work.
15) All serious accidents related to equipment should be reported to the competent authorities of the Member State where the manufacturer, user and patient are located.

Division	Timescale	Example for accident
Serious public health threat	Immediately (without any delay that could not be justified) but not later than 2 calendar days after awareness by the manufacturer of this threat.	· Possibility of multiple deaths occurring at short intervals.
Death or inanticipated serious deterioration in state of health	Immediately (without any delay that could not be justified) after the manufacturer established a link between the device and the event but not later than 10 elapsed calendar days following the date of awareness of the event.	· Death · Serious burns injuries · Electric shock
Others	Immediately (without any delay that could not be justified) after the manufacturer established a link between the device and the event but not later than 15 elapsed calendar days following the date of awareness of the event.	· In the case of Serious / Major, Minor, Negligible in the 2.5.1.

Copyright© 2021-2026 NEWPONG Co.,Ltd. All rights reserved.

1.2. General Warning

1) Use of accessories, transducers and cables other than those specified or provided by the manufacturer of this equipment could result in increased electromagnetic emissions or decreased electromagnetic immunity of this equipment and result in improper operation.
2) Electric devices have potential electric shocks. Please establish education policy and procedure for risk factors related to electric devices. Only qualified person, who has proper service documents for the electricity shock, can repair this device.
3) To avoid risk of electric shock, keep this equipment dry. Do not expose this equipment to high humidity, moisture or liquids.
4) If the user uses accessories other than those specified, the safety and performance of the device may be impaired. Use only the specified accessories.
5) Do not move the equipment and its components during use of equipment.
6) To prevent the risk of electric shock, this equipment must be connected to a power supply (hospital grade AC outlet) with a protective earth.
7) Unintended operation may occur due to equipment failure.
8) Do not leave the patient with probe inserted.
9) If operator uses another accessory besides listing of this device or unapproved accessory for substitution of its original accessory, electromagnetic compatibility(EMC) would be emitted or its resistance for EMC would be decreased.
10) If accessory, which is not compatible equivalently with safety requirements, is used, it may downgrade the safety level. Please review if accessories around patient and its safety certificates are compatible with [IEC 60601-1] or [IEC 60601-1-2]. It may harm to people or damage the product.
11) If operator uses other accessories beside designated accessories, it may downgrade the device's safety and performance. Please use only designated accessories.
12) Do not press the Foot Switch with excessive force.
13) The foot switch should be placed on a flat surface and kept from tipping over during use.
14) Do not step on the foot switch when it is upside down.
15) Press only one foot switch button at a time. Do not press multiple buttons simultaneously.
16) Use the foot switch in a location where it is protected from water as much as possible.

1.3. Operating Environment & Electrical Safety Guidelines

1) NP-200 is classified as Class 1 and Type BF for electric shock.
2) Do not operate NP-200 near flammable anesthetics and solvents.
3) Use of this equipment adjacent to or stacked with other equipment should be avoided because it could result in improper operation. If such use is necessary, this equipment and the other equipment should be observed to verify that they are operating normally.
4) Failure to use this equipment in the specified type of shielded location could result in degradation of the performance of this equipment, interference with other equipment or interference with radio services.

Copyright© 2021-2026 NEWPONG Co.,Ltd. All rights reserved.

5) This equipment has been tested for radiated RF immunity only at selected frequencies, and use nearby of emitters at other frequencies could result in improper operation.
6) Please check whether electric specification of building is compatible with electric specification of device. Power of every device which is connected to outlet of stand has to accord with electrical requirements written in the back side of stand. Otherwise, it may cause damage to patients and product.
7) To Avoid the Risk Of Electric Shock, This Equipment Must Only Be Connected To A Supply Mains With Protective Earth
8) Do not use this unit for multiple socket-outlets. Using multiple socket-outlets or extending the power cord may cause damage to the equipment.
9) Equipotential stud should be connected to the protective earthing conductor in hospital by a proper connecting device. If the connection to the earth is not completely established, there is a potential risk that the patient or the operator could be injured by electric shock.
10) Portable RF communications equipment (including peripherals such as antenna cables and external antennas) should be used no closer than 30 cm (12 inches) to any part of "NP-200", Including cables specified by the manufacturer. Otherwise, degradation of the performance of this equipment could result.
11) Use of this equipment adjacent to or stacked with other equipment should be avoided because it could result in improper operation. If such use is necessary, this equipment and the other equipment should be observed to verify that they are operating normally.
12) Failure to use this equipment in the specified type of shielded location could result in degradation of the performance of this equipment, interference with other equipment or interference with radio services.
13) This equipment has been tested for radiated RF immunity only at selected frequencies, and use nearby of emitters at other frequencies could result in improper operation.
14) If the equipment overheats, stop using it immediately and turn off the power.
15) If operator feels that the handpiece is discomfortable to grab due to hitting, please either add more anesthetic solution or stop using the handpiece.
16) Use the probe in a way that prevents it from bending as much as possible.
17) Do not touch the connector contacts with bare hands or metallic objects. This may result in electric shock or device malfunction.
18) Always ensure that the connector is securely and properly connected before attaching it to the patient.
19) When the connector is detached, take care to prevent the exposed area from coming into contact with the patient’s skin or body.
20) Do not modify, disassemble, or tamper with the device’s connectors or terminals.
21) Use only patient cables and connectors specified by the manufacturer. The use of incompatible accessories may compromise patient safety.
22) All exposed metal parts of the device are designed with protective grounding. Do not alter or bypass this safety feature under any circumstances.

Copyright© 2021-2026 NEWPONG Co.,Ltd. All rights reserved.

1.4. IEC Electrical Safety & EMC Specifications

Table 1-1 IEC Electrical Safety Specifications

Device Description	
Class Ⅰ, Type BF Equipment, IPX0, not AP/APG	
Mode of Operation: Non-continuous	
Electrical Isolation	· Leakage current conforms to IEC 60601-1 · Dielectric withstanding voltage conforms to IEC 60601-1
EMC Emissions and Susceptibility: NP-200 Ultrasonic Surgical Unit has been tested and found to comply with the limits for medical devices to the IEC 60601-1-2:2014. These limits are designed to provide reasonable protection against harmful interference in a typical medical installation. This Equipment uses, and can radiate RF energy and, if not installed and used in accordance with the instruction given below, may cause harmful interference to other devices in the vicinity. However, there is no guarantee that interference will not occur in a particular installation.	

1.5. Electromagnetic Field Information according to IEC 60601-1-2

Table 1-2 IEC EMC Specifications (Emissions)

Guidance and manufacturer's declaration – electromagnetic emissions		
The LSSA is intended for use in the electromagnetic environment specified below. The customer or the user of the LSSA should assure that it is used in such an environment.		
Emission test	Compliance	Electromagnetic environment - guidance
RF emissions CISPR 11	Group 1	The LSSA uses RF energy only for its internal function. Therefore, its RF emissions are very low and are not likely to cause any interference in nearby electronic equipment.
RF emissions CISPR 11	Class A	The EMISSIONS characteristics of this equipment make it suitable or use in industrial areas and hospitals (CISPR 11 class A). If it is used in a residential environment (for which CISPR 11 class B is normally required) this equipment might not offer adequate protection to radio-frequency communication services. The user might need to take mitigation measures, such as relocating or re-orienting the equipment.
Harmonic emissions IEC 61000-3-2	Class A	
Voltage fluctuations / flicker emissions IEC 61000-3-3	Complies	

Table 1-3 IEC EMC Specifications (Immunity)

Guidance and manufacturer's declaration – electromagnetic Immunity			
The LSSA is intended for use in the electromagnetic environment specified below. The customer or the user of the LSSA should assure that it is used in such an environment			
Immunity	IEC 60601 Test level	Compliance level	Electromagnetic environment - guidance

Copyright© 2021-2026 NEWPONG Co.,Ltd. All rights reserved.

Electrostatic Discharge (ESD) IEC 61000-4-2	± 2,4,6,8 kV Contact	± 2,4,6,8 kV Contact	Floor should be wood. Concrete or ceramic tile. If floors are covered with synthetic material. The relative humidity should be at least 30%.
	± 2,4,8,15 kV air	± 2,4,8,15 kV air	
Electrical fast Transient/burst IEC 61000-4-4	± 2 kV for power Supply lines	± 2 kV for power Supply lines	Main power quality should be that of a typical commercial or hospital environment.
	± 1 kV for input/output lines	± 1 kV for input/output lines	
Surge IEC61000-4-5	± 0.5, 1 kV line(s) to line(s)	± 1 kV line(s) to line(s)	Main power quality should be that of a typical commercial or hospital environment.
	± 0.5,1,2 kV line(s) to ground	± 2 kV line(s) to ground	
Voltage dips, short interruptions and voltage Variations on power supply input lines IEC 61000-4-11	< 0% UT (>100% dip in Ut) for 0.5cycle	< 0% UT (>100% dip in Ut) for 0.5cycle	Main power quality should be that of a typical commercial or hospital environment. If the user of the NP-200 requires continued operation during power main interruptions, it is recommended that the NP-200 ne powered from an uninterruptible power supply.
	0% UT (100% dip in UT) for 1cycle	0% UT (100% dip in UT) for 1cycle	
	70% UT (30% dip in UT) for 25cycle	70% UT (30% dip in UT) for 25cycle	
	< 0% UT (>100% dip in UT) for 250cycle	< 0% UT (>100% dip in UT) for 250cycle	
Power frequency (50,60Hz) Magnetic field IEC 61000-4-8	30 A/m	30 A/m	Power frequency magnetic fields should be at levels characteristic of a typical location in a typical commercial or hospital environment.
NOTE U^T is the a.c. main voltage prior to application of the test level.			

Guidance and manufacturer's declaration – electromagnetic Immunity			
The LSSA is intended for use in the electromagnetic environment specified below. The customer or the user of the LSSA should assure that it is used in such an environment			
Immunity	IEC 60601 Test level	Compliance level	Electromagnetic environment - guidance

Copyright© 2021-2026 NEWPONG Co.,Ltd. All rights reserved.

Conducted RF IEC 61000-4-6	3 Vrms 150kHz to 80MHz 6 Vrms ISM bands @ 150 kHz to 80 MHz	3 Vrms 6 Vrms	Potable mobile RF communications equipment should be used no closer any part of the NP-200, including cables, than the recommended separation distance calculated from the equation applicable to the frequency of the transmitter. Recommended separation distance $d = 1{,}2\sqrt{P}$ $d = 1{,}2\sqrt{P}$ 80MHz to 800 MHz $d = 2{,}3\sqrt{P}$ 800MHz to 2.5 GHz where P is the maximum output power rating of the transmitter in watts (W) according to the transmitter manufacturer and d id the recommended separation distance in meters(m).
Radiated RF IEC 61000-4-3	3V/m 80MHz to 2.7 GHz	3 V/m	Field strengths from fixed RF transmitters, as deter-mined by an electromagnetic site survey, a should be less than the compliance level in each frequency range. interference may occur in the vicinity of equipment marked with the following symbol :
NOTE 1) at 80 MHz and 800 MHz, the higher frequency range applies. NOTE 2) These guidelines may not apply in all situations. Electromagnetic propagation is affected by absorption and reflection from structures, objects and people.			
[a] Field strengths from fixed transmitters, such as base stations for radio (cellular/cordless) telephones and land mobile radios, amateur radio, AM and FM radio broadcast and TV broadcast cannot be predicted theoretically with accuracy. To access the electromagnetic environment due to fixed RF transmitters, an electromagnetic site survey should be considered. If the measured filed strength in the location in which the EUT is used exceeds the applicable RF compliance level above, the EUT should be observed to verify normal operation. If abnormal performance is observed, additional measures may be necessary, such as reorienting or relocating LSSA. [b] Over frequency range 150 kHz to 80 MHz, filed strengths should be less than 3 v/m.			

1) Precautions regarding sources of EM energy that:
   - emit levels of EM energy that exceed the immunity test levels of the referenced EMC standards used, or EMI Tesitng has verified the release of the product.
   - have other emission characteristics to which the medical device has not been tested for immunity: N/A
2) Specifications of the wireless communication for medical devices with RF wireless functions: N/A
3) Any maintenance instructions needed to ensure that the medical device remains safe and performs as intended with regard to EM disturbances throughout the expected service life.
4) Stop using the device if it operates erratically or if the display malfunctions due to the EM disturbances.

Copyright© 2021-2026 NEWPONG Co.,Ltd. All rights reserved.

5) Markings affixed to the medical device and warnings for certain types of known EM environments, such as in or near an MRI scanner. Medical devices intended for use in the MR environment that have not been shown to be MR Safe or MR Conditional should be marked with the ASTM F2503 symbol for MR Unsafe. (See ASTM F2503-13 Standard Practice for Marking Medical Devices and Other Items for Safety in the Magnetic Resonance Environment.)

1.6. Precaution During Ultrasonic Procedure

1.6.1 Cautions for Patient

1) To use this equipment, you should use the dedicated accessory supplied by NEWPONG Co., Ltd. according to the user's manual to prevent potential danger.
2) To stop the ultrasonic output, you can release the right button on the foot switch to stop
3) Press the left footswitch button to select modes. Mode changes are disabled during output.
4) Any physical deformation inside or outside the device is prohibited.
5) Failure of the equipment could result in an unintended increase of output power.
6) To avoid the risk of electric shock, this equipment must be connected to the supply mains with protective earth.
7) After checking the patient status and considering the clinical treatment guide line, set up the proper parameter.
8) Use the machine with prescription and instruction of medical specialist.
9) Avoid the treatment to the pregnancy and children.
10) Avoid the treatment to patient who has progressive dermatitis or treat after consultation with medical specialist.
11) Prohibit the treatment to the acute disease patient who has over 38°C body temperature with bloody condition
12) Prohibit the treatment to abnormal blood pressure, infectious and tubercular patients.
13) Prohibit the treatment to malignant tumor and heart disease patients.
14) Prohibit the treatment to patients who can have the hemotelangiosis from the liver function disturbance and from the long use of steroid hormone.
15) Prohibit the treatment the patients who has legal communicable disease.
16) Use of this device is limited to those physicians who, by means of residency training or sanctioned continuing medical education, have demonstrated proficiency in suction lipoplasty.
17) This device should be used with extreme caution in patients with chronic medical conditions such as diabetes, heart or lung disease, circulatory diseases.
18) Loss of blood and fluid is predictable based on suction volume. Capability of providing adequate, timely replacement of these components is essential for patient safety.
19) Probe, handpiece, and wrench must be sterilized prior to use.
20) The outcome of the procedure may vary depending on the age of the patient, the site of the operation, and the surgeon's experience.

Copyright© 2021-2026 NEWPONG Co.,Ltd. All rights reserved.

21) Due to ultrasonic energy, the temperature of the handpiece area rises, and there is a possibility of inadvertent use. In the case of the continuous mode, 10 minutes rest when using for 3 minutes, and in the case of the pulse mode, 10 minutes rest when using for 7 minutes.
22) This equipment is designed safely through General requirements for basic safety and essential performance (IEC60601-1) and risk management process to minimize the possibility of risk. However, user and patient may still be exposed to residual risks such as:
    - Endangerment of patient or user's life (ex. Death, Electric shock)
    - Serious burns injuries
    - Minor burn injuries
    - Tissue damage
    - Delay of surgery
    - Occur problem in product (ex. Trouble in product, fire in product)
    - Inconvenient
23) Caution: Federal law (USA) restricts these devices to sale by or on the order of a physician

1.6.2 Precautions for maintenance

1) Remove the foot switch from the device and store.
2) Avoid bending the cable connector between the main body and the handpiece or foot switch.
3) Regular inspection of products and components is recommended.
4) Ensure that the Main Body does not come into contact with water.
5) When reusing products that have not been used for a long time, check for safe operation before use.
6) You should avoid environments that can be heated by direct sunlight
7) Care must be taken not to damage the handpiece by falling on the floor. Care must be taken as it may cause defects.
8) Keep the power cable disconnected from the outlet during non-use.
9) Store carefully against incline, vibration, impact, etc.
10) Avoid storing chemicals in places where gas is generated.
11) It should be stored in consideration of hygiene, and it is recommended to disinfect the skin contact area especially when reusing it.
12) When cleaning the surface of the product, it is recommended to wipe it with a soft tissue or gauze.

1.7. Side Effect

When using an ultrasound surgical device, the following side effects may occur depending on the indications.

1) Bleeding
2) Hematoma
3) Hypoalbuminemia
4) Anemia
5) Inflammation and infection at the surgical site
6) Seroma

Copyright© 2021-2026 NEWPONG Co.,Ltd. All rights reserved.

7) Bruising and Swelling
8) Hypoesthesia
9) Residual Lumps and Irregularities
10) Localized Fibrosis

1.8. Indication/Contraindication

1) Indication
   - Plastic and Recinstruction Surgery
   - Orthopedic Surgery
2) Contraindication

Do not treat the patients who fall on each of the following subparagraphs

- Pregnant women
- Patients with cardiac pacemakers or defibrillator
- Patients with open wound on the area of treatment
- Patients with chronic conditions such as diabetes, blood clotting disorders, heart, lung or circulatory diseases, or have vascular problems including general circulation problems and coagulation problems associated with certain medications
- Collagen, the presence of scarring or connective tissue disorders, lupus erythema, endocrine disorders, pregnancy or pregnancy, or other active diseases that may affect or increase the risk of the procedure

1.9. Symbol Definition

	Equipotentiality		Separate collection for WEEE
	Refer to instruction manual/booklet		Type BF Applied part
SN	Serial Number	90% 10%	Humidity Limitation
60°C 0°C	Temperature Limit	106kPa 80kPa	Atmospheric pressure limitation
	Date of Manufacture		Manufacturer
	General warning sign		Caution

Copyright© 2021-2026 NEWPONG Co.,Ltd. All rights reserved.

	Warning, electricity	NON STERILE	Non-sterile
	Stand-by		“OFF”
	“ON”		

Copyright© 2021-2026 NEWPONG Co.,Ltd. All rights reserved.

2. General

2.1. Introduction

NP-200 of Newpong Co., Ltd. is an ultrasonic surgical unit designed to fragment and emulsify subcutaneous fatty tissues using ultrasound frequency vibrations. The NP-200 generates ultrasonic vibrations through the piezoelectric effect of PZT ceramic crystals embedded in the NP-200 handpieces. When electrical energy is supplied from the main control unit, these PZT crystals rapidly expand and contract, converting electrical signals into mechanical ultrasonic vibrations. These vibrations are transmitted to the attached probe, which delivers the mechanical action required for tissue fragmentation and emulsification.

The NP-200 is equipped with an electronic control system that allows the operator to adjust the vibration amplitude and frequency. It offers two operating modes, Continuous Mode and Pulse Mode.

2.2. Intended Use

LSSA is intended for the fragmentation and emulsification of subcutaneous fatty tissues for aesthetic body contouring. LSSA is indicated for use in the following surgical specialists when the fragmentation and aspiration of adipose tissue is desired:

- Plastic and Reconstruction Surgery
- Orthopedic Surgery

2.3. Composition

NP-200 is consisted of below parts.

Please check whether the below parts are included in the package or there any damages of main body or accessories. Applied part to patient is only “PROBEs”.

Table 2-1. Basic Composition

No.	Shape	Name	Description	Remark
1		NP-200 Main body	LED indicator for User Interface Jog wheel for Adjusting Ultrasonic power	1EA
2		B HANDPIECE	Convert electric power to ultrasonic power (IPX7) With BL, BM, BS PROBE	1EA
3		F Handpiece	Convert electric power to ultrasonic power (IPX7) With FM, FS PROBE	1EA

Copyright© 2021-2026 NEWPONG Co.,Ltd. All rights reserved.

4		Foot Switch	On and Off output of the ultrasonic power (IPX6)	2EA
5		PROBE	Convert the ultrasonic power to mechanical vibration energy BL PROBE (Ø3.7mm), BM PROBE (Ø2.9mm), BS PROBE (Ø1.8mm), FM PROBE (Ø1.2mm), FS PROBE (Ø0.9mm)	Optional
6	 (For FM, FS) (For BL, BM, BS)	SPANNER (WRENCH)	Connect or disconnect the PROBE with the handpiece For BL, BM, BS, FM, FS PROBE	1EA
7		Power Cord	AC Power Connection	1EA
8		Operator Manual	Operating Instruction for use	1EA

Copyright© 2021-2026 NEWPONG Co.,Ltd. All rights reserved.

2.4. Descriptions

2.4.1. Main Body

1) Front View of the Main Body

Figure 2-1. NP-200 Front View

No.	Item name	Description
1	Lapsed Time	Display Ultrasonic Output Lapsed Time.
2	Output Power Level	Output Power Level (1~5 Level)
3	Continuous Mode	Continuous Mode Indicator White : B Handpiece, Blue : F Handpiece
4	Pulsed Mode	Pulsed Mode indicator White : B Handpiece, Blue : F Handpiece
5	Handpiece Connector	Handpiece Connector
6	Jog wheel	Controller to adjust output power(Turn counterclockwise to reduce by one level, turn clockwise to increase by one level)
7	Output Indicator	Indicates that ultrasonic output is in progress

2) Rear view of the Main body

Figure 2-2. NP-200 Rear View

No.	Function	Description
1	Time Check button	Blinks the current time on Timer
2	Time Reset button	Reset the timer.
3	Protective Earth Terminal	Terminal for connecting Protective Ground Cable

Copyright© 2021-2026 NEWPONG Co.,Ltd. All rights reserved.

4	Foot Switch Connector	The connector for Foot Switch.
5	Foot Switch Connector	The connector for Foot Switch. *Foot switches do not work at the same time. it works individually.
6	Main power switch	Input: (100-240) V~ On and Off Main Power I: AC On, O: AC off
7	Power cable socket	Connect power cable

2.4.2. Accessories

1) Handpiece

The handpiece (including the cable) does not have any intended contact with the patient during medical procedures.

① B Handpiece

It is used in connection with BL, BM, and BS Probe and converts electrical signals into ultrasonic waves.

No.	Name	Description
1	The Front End	Connections to BL, BM, and BS Probe
2	Cable	Silicon Cable
3	Connector	Connect to the Main Body's Handpiece Connector
4	Cap	Cap
5	Handpiece Cap	Handpiece cap

Copyright© 2021-2026 NEWPONG Co.,Ltd. All rights reserved.

② F Handpiece

It is used in connection with FM and FS Probe and converts electrical signals into ultrasonic waves.

No.	Name	Description
1	The Front End	Connections to FM and FS Probe
2	Cable	Silicon Cable
3	Connector	Connect to the Main Body's Handpiece Connector
4	Cap	Cap
5	Handpiece Cap	Handpiece cap

2) Foot Switch

It is an accessory that controls the on/off of the Ultrasonic wave output, which can be changed to C mode and P mode when the left mode switch is operated, and the output is transmitted when the start switch is operated.

No.	Name	Description
1	Mode Switch	Used when changing to Continuous mode and Pulse mode
2	Start(On/Off) Switch	Use to turn the output on
3	Cable	Cable
4	Connector	Connect to the Main Body's Foot Switch Connector

Copyright© 2021-2026 NEWPONG Co.,Ltd. All rights reserved.

3) Probe

The probe transmits ultrasonic vibration.

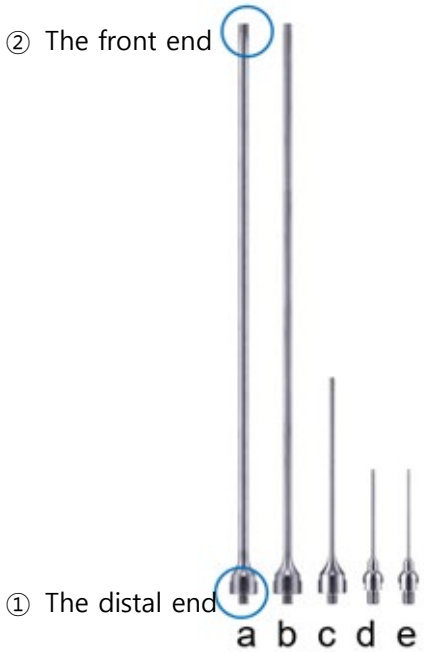

No.	Name	Description
a	BL Probe	Using with B Handpiece
b	BM Probe	
c	BS Probe	
d	FM Probe	Using with F Handpiece
e	FS Probe	
No.	Name	Description
1	The distal end	The part that engages with the handpiece.
2	The front end	The part where ultrasonic energy is transmitted.

Copyright© 2021-2026 NEWPONG Co.,Ltd. All rights reserved.

3. Installation and Connection

Please note following articles when “NP-200” is installed

1) It is recommended that this device is installed at an airy or ventilated space because it has slight heat during operating.
2) Be sure to use linear or grounded power supply to prevent against malfunctions by electrical effects.
3) Do not try to get the power cord wet.
4) Do not connect the power cord to main body if it is damaged.
5) Do not share an outlet with other devices. There is potential for the fire by abnormal generated heat if several devices share an outlet.
6) If possible, please avoid direct sunlight.
7) Be careful not to damage by shock.
8) Install the device at the flat location.
9) Install the device away from dust or inflammables.
10) To facilitate disconnection of the power supply in an emergency, install the equipment with a minimum distance of 15 cm between the rear of the equipment and the wall, and install it in a location where access to the equipment is not obstructed by obstacles or walls.
11) Be careful not to block the exhaust vent as heat accumulates on the top and back of the equipment when the equipment is used continuously.

3.1. Transport and Fix

Please follow the below process when “NP-200” is moving to another place.

1) Before moving the device, turn off the device first. And remove the power cable.
2) Be careful for probe and handpiece drop.
3) After moving to another place, connect the power cable.
4) During the output of "NP-200”, moving of mainbody or removing of accessories is prohibited.
5) If device should be moved by elevator or through slope, please use the packing box.
6) Do not push PROBE socket with heavy material from the top. It may cause the damage of PROBE socket.

3.2. Power and cable connection

1) Connect the power cord to power supply and "NP-200"'s power cord socket which is located at the left of back side.
2) Activate the device Switching "Main Power Switch” which is located above the power cord socket.

⚠ Warning	Check the fixed condition of power cord when the power cord is connected to the power cord socket. Check the connection of power cord and be careful not to loosen. Any problem or damages on the device can be caused by disconnection of power during operation.

Copyright© 2021-2026 NEWPONG Co.,Ltd. All rights reserved.

3.3. Foot switch connection

1) Connect the Foot switch cord to “Foot switch connector” located at the right of back side.
2) Align the protrusion of the socket with the slit of the connector before connecting them.
3) The footswitch can be used alternately by connecting both. When one switch operates, the other foot switch does not work.

Figure 3-1. NP-200 Footswitch connection

3.4. Handpiece connection

1) Connect the Handpiece to "Handpiece connector” located at the left of front side.
2) Align the engravings on the socket and connector before connecting them.
3) Check whether the cord is connected firmly.

Figure 3-2. NP-200 Handpiece connection

⚠ Warning	If there are foreign substances (such as body fluids or tissues) inside the Handpiece Connector terminal, using it as is may cause a fire or malfunction.

3.5. Handpiece and PROBEs connection

Follow the instruction for fixing the PROBE into handpiece;

(1) Remove the cap of the handpiece by turning it around to expose horn.
(2) Put the PROBE in to the horn and turning it clockwise to connect with handpiece.
(3) For fixing the PROBE firmly using wrench and re-cap the cap of handpiece.
(4) It is recommended that operator turns on the power after installing handpiece.
(5) Check if the power cord is connected properly. And do not touch the device with wet hand to avoid the electric shock.

Copyright© 2021-2026 NEWPONG Co.,Ltd. All rights reserved.

Figure 3-3 Fixing the PROBE wrench

PROBE, wrench, and handpiece are parts that require sterilization before use. Also the user is required to wear a sterilized clothes and gloves.

⚠ Warning	Manufacturer do not has acceptance and no responsibility for the any trouble or damages caused by consumable items beside original connector or cable which was supplied by manufacturer.

Check the followings after turning on the power of "NP-200".

- Press the ON/OFF button and check whether the power is supplied and device is operated.
- Check if the all images are displayed on the screen.
- Pour sterilized saline into a bowl, immerse the tip of the probe, and press the foot switch for 2-3 seconds to check if the output is functioning properly.

Copyright© 2021-2026 NEWPONG Co.,Ltd. All rights reserved.

4. Instruction for Use

4.1. Sterilization

4.1.1. Sterilization option

The Ultrasonic handpiece and instruments may be combined or separated for sterilization according to your facility's capabilities and the sterilization methods descried below.

All components(Handpiece, Probe, Wrench) must be disassembled and sterilized separately.

Note. Use only FDA-cleared sterilization wraps, pouches, or other appropriate sterile barrier systems validated for the intended sterilization cycle to maintain device sterility.

4.1.2. Instruments

Applicable instruments: B HANDPIECE, F HANDPIECE, PROBEs(BL, BM, BS, FM and FS), WRENCH.

Follow your institution's guidelines for the following types of sterilization. Autoclave cycles longer than those shown in the Table 4-1. will slowly degrade the performance and useful life of the handpiece.

⚠ Caution	DO NOT unscrew hex-shaped cable connection on the back of the Handpiece.
⚠ Caution	DO NOT use chlorinated cleaning agents (bleach) on the Handpiece.
⚠ Caution	DO NOT use abrasive cleaning agents on the Handpiece.

4.1.3. Sterilization Methods for Instruments

Sterilization Method	Recommended Parameters	
Cycle Times for Gravity-Displacement Steam Sterilization Cycles	Temperature	132 °C
	Sterilization Time	15 minutes
	Drying Time	30 minutes
Cycle Times for Dynamic-Air-Removal Steam Sterilization Cycles	Temperature	132 °C
	Sterilization Time	4 minutes
	Drying Time	30 minutes

Table 4-1. Sterilization Methods for Instruments

If using an autoclave to sterilize the handpiece, remove the handpiece as soon as possible when the autoclave dry cycle is completed. Do not let the handpiece sit in a hot autoclave beyond the recommended drying period. Let the Handpiece cool at least 30 minutes before use, 2 hours is preferable. The handpiece may be rinsed in sterilized water or sterilized saline for more rapid cooling.

Copyright© 2021-2026 NEWPONG Co.,Ltd. All rights reserved.

4.2. Starting the system

4.2.1. Power On

Check the connection of power cable at the bottom behind of the product, then push the power button(Figure 4-1) for the ON status in the side of product. After connecting the handpiece and footswitch to the main body, turn on the power and the LED will be displayed as shown in Figure 4-2.

Figure 4-1. ON/OFF

Figure 4-2. Initial UI state

4.2.2. Check handpiece and footswitch connection

If the handpiece is not connected to the main body, Er 21 (Figure 4-3.) is displayed and if the footswitch is not connected to the main body, Er 23 is displayed. (Figure 4-4.)

Figure 4-3. Handpiece Disconnected

Figure 4-4. Foot Switch Disconnected

When the B HANDPIECE is connected to the main body, the LED displayed in continuous mode is white(Figure 4-5), and when the F HANDPIECE is connected to the main body, the LED displayed in continuous mode is displayed in blue(Figure 4-6).

Figure 4-5. B HANDPIECE Connected

Figure 4-6. F HANDPIECE Connected

4.2.3. Select Output Level

The ultrasonic output level can be set from level 1 to 5. It can be adjusted using the jog wheel on the front of the product, with clockwise rotation increasing the level and counterclockwise rotation decreasing the level. Each level is numbered from 1 to 5. The number of LEDs and the digits indicate each level. While the ultrasound is being output, the output level does not change even if the jog wheel is turned.

Copyright© 2021-2026 NEWPONG Co.,Ltd. All rights reserved.

Figure 4-7. Indication of output level

4.2.4. Select Output Mode

It can be selected by changing the continuous mode and pulse mode by pressing the mode switch(Foot Switch) of the foot switch. LED is indicated when continuous mode selected, LED is indicated when pulse mode selected.

Figure 4-8. Continuous Mode

Figure 4-9. Pulse Mode

⚠ Caution	Operation Time and Thermal Safety To prevent handpiece overheating and ensure patient safety, please strictly observe the operation and rest times according to the selected output mode: ► **Continuous Mode:** Max. 3 minutes of use followed by a 10-minute rest period. ► **Pulsed Mode:** Max. 7 minutes of use followed by a 10-minute rest period.

4.2.5. Ultrasonic wave output

Press the start switch of the foot switch (Figure 4-10. Foot Switch) to output ultrasonic. When ultrasonic are output, the ultrasonic output indicator lights up and the timer starts (Figure 4-11). The buzzer indicating ultrasonic output sounds once every 2 seconds. When you release the switch, the output stops, and simultaneously, the timer stops, allowing you to check the equipment usage time. The ultrasonic output indicator turns off and the buzzer stops sounding

Figure 4-10. Foot Switch

Figure 4-11. Output Indicator

Copyright© 2021-2026 NEWPONG Co.,Ltd. All rights reserved.

4.2.6. Timer Reset

The timer operates while the ultrasonic wave is output to display the usage time. Pressing the reset button (Figure 4-12) on the rear of the Main Body will reset the usage time back to 00:00.

Figure 4-12. Indication of timer

4.3. Operation

1) The patient's choice and surgical area are determined through consultation with the patient and medical judgment of the doctor.
2) Before using this device, the amount and method of injection of the anesthetic solution shall be determined by the doctor.
3) Use of this device in surgery
   ① In order to insert the probe of this device into the body, a 3-5 mm skin is incised.
   ② Connect the probe of this equipment to the handpiece and Position the front end of the probe at the incised skin.
   ③ With the probe entering the target area, press the foot switch to generate an output. Do not step on the footswitch before inserting the probe.
   ④ The user does not stop the stroke of the probe while the ultrasonic output goes out by stepping on the footswitch.
   ⑤ To change the direction of the probe, take back the probe front end to the entry point and then change the direction.
   ⑥ In order to maintain ultrasoinc wave output, bending of the probe is prevented as much as possible. The hand holding the handle need to move as straight as possible, and check the probe end with the hand not holding the handpiece.
   ⑦ Be careful not to touch the skin with the probe front end inside the body.
   ⑧ Operator can place wet gauze on the skin to prevent frictional thermal damage by between cannula or probe in the area where the skin contacts the probe.
   ⑨ The end point of device use is until there is a loss of resistance in the probe movement.

⚠ Caution	DO NOT lay the LSSA Handpiece on the patient when not in use.

4) After using the device, the soft tissue remaining in the body is evacuated using a suction device or manual syringe approved in the country, which is referred to the literature below.

Reference :

(1) Rod J. Rohich, Samel J. Beran, Jeffrey M. Kenkel. *ULTRASOUND-ASSISTED LIPOSUCTION.* St. Louis, Quality Medical

Copyright© 2021-2026 NEWPONG Co.,Ltd. All rights reserved.

Publishing, Inc., 1998, pp.382-383.

(2) Shridharani SM, Broyles JM, Matarasso A. *Liposuction devices: technology update.* Med Devices (Auckl). 2014 Jul 21;7:241-51. doi: 10.2147/MDER.S47322. PMID: 25093000; PMCID: PMC4114741.

5) Operation Environment

① Temperature: +10°C to +30°C

② Relative Humidity: 30 to 75%(non-condensing)

③ Atmospheric pressure: 800 to 1060hPa

4.4. System Off

Please follow instruction below to off the system safely.

- Turn off the "NP-200" by Push the Power button
- Turn off the Main Power switch by switching from I to O
- Disconnect the handpiece cable, footswitch cable and power cord.

Copyright© 2021-2026 NEWPONG Co.,Ltd. All rights reserved.

5. Cleaning and Maintenance

5.1. Maintenance and storage

5.1.1. Maintenance

1) Always unplug the AC power cord and cables before cleaning the Main Body and handpiece.
2) This Main Body, handpiece, probe and wrench must be kept clean and hygienic with proper care.
3) Do not submerge the socket at the end of the handpiece in water.
4) During cleaning, make sure to completely remove any moisture from the socket at the tip of the handpiece. Failure to do so may result in an electrical short.
5) Immediately remove all impurities of outside the device and accessories after treatment.
6) Do not break the handpiece cable.
7) If the device has not been used for a long time, check firstly whether the device is working in safety.
8) Avoid the environment that temperature can be increased by direct sunlight.
9) Regular inspection for device and accessories is recommended.
10) After clean the device, check the main body and accessories seriously. If the device is old or damaged, do not use the device.
11) Remove the power of device before cleaning and maintenance. Otherwise, it may harm to people or damage the product.
12) Some chemical cleaning products may have conductivity and make some scraps. The products remain with conductivity dusts or scraps. Do not use the products for electrical part and do not use spray cleaning products for any surfaces.

5.1.2. Storage

1) Separate a power cord from the outlet.
2) Store the device avoiding a wet place.
3) Be careful with the bad influence like air containing atmospheric pressure, temperature, humidity, ventilation, dust and salty.
4) Be careful with incline, vibration and shock.
5) Do not store the device in storage place for chemicals and place where generates gas.
6) Store the device without power cord by using cover as like vinyl when the device is stored in a long time
7) If the device has not been used over a month, check whether the device works in safety.
8) Store with consideration of sanitation, sterilization before reuse of contact point with skin is recommended.
9) Store this NP-200 in a clean, dry and non-corrosive atmosphere under the conditions below.
   - Temperature: 0 °C to + 60 °C
   - Relative Humidity: 10 to 90 % (non-considering)
   - Atmospheric pressure: 800 to 1 060 hPa

Copyright© 2021-2026 NEWPONG Co.,Ltd. All rights reserved.

5.2. Equipment Cleaning

5.2.1. Method of Equipment Cleaning

1) Use a soft cotton to clean the Main body.
2) Use a soft cotton, which has a suitable moisture without greasy, to clean product surface.
3) Turn off "NP-200"s power and separate the power cord before cleaning. Also all accessories are separated. Do not soak the device in water and do not trickle any liquid down to the case.
4) Do not use alcohol to clean the front side of device. Alcohol may cause a scratch or damage of acrylic.

5.2.2. Method of Accessories Cleaning

1) Wash the product with room temperature water for 30 seconds.
2) Dilute Endozime AW in a 1:250 ratio in 20°C to 30°C constant water. (4ml/1L constant water)
3) Soak the product for at least 2 minutes.
4) Remove any contaminants with a soft brush.
5) Rinse the Endozime AW product 2-3 times with room temperature water.
6) Dry at a dryer temperature of 110°C for 40 minutes. (After removing the sample, wipe it with sterile gauze and dry it in a clean tray for 1 hour.)

⚠ Warning	- Prevent cleaning solution to contact with eyes, skin, or clothing. - Avoid generating and breathing mists of cleaning solution. - Wash thoroughly with soap and water after handling the cleaning solution and before eating, drinking, chewing gum, using tobacco or using the toilet. - Remove and wash for cleaning solution contaminated clothing before reuse. - Seal the cleaning solutions and store. - Avoid spilling liquids into the Main Body during cleaning. - Avoid getting cleaning materials inside the Foot switch Port and the AC Power inlet. - ※ Do not immerse the socket at the tip of the handpiece in water during cleaning.

5.3. Regular inspection

1) It is recommended that "NP-200" is inspected regularly once a year like as other medical devices.
2) For a symptom of corrosion or damage, check regularly. Otherwise, it may harm to people or damage the product.
3) Only qualified service person or trained person trained/authorized by manufacturer can repair the device due to its electrical shock.

5.3.1. Instruction of Inspection

Inspection Order	Description
1. Power supply	1) Connect only the main body to the power supply to turn on the device. 2) Check if the "Er 23" code appears on the UI screen
2. Footswitch recognition	1) Properly attach the footswitch to the main body. 2) Verify that the "Er23" code converted to "Er 21" code

Copyright© 2021-2026 NEWPONG Co.,Ltd. All rights reserved.

3. Handpiece recognition	1) Properly attach the Handpiece to the main body. 2) Verify that all error messages are disappeared and correct indicators are light up according to the handpiece type 3) Connect a different type of handpiece to make sure the correct indicator lights up(Optional)
4. Footswitch Operation	1) Press the footswitch mode button and check if the mode indicator changes.
5. Ultrasonic Output	1) Connect the probe to the handpiece and submerge 50–75% of the probe in distilled water. 2) Press the output button on the footswitch to emit ultrasonic for approximately 5 seconds. 3) Turn the jog wheel to check if the output level adjusts properly. 4) Check whether the UI indicators for ultrasonic emission are functioning properly.

1) After inspection, wipe the probe clean with a dry cloth to ensure no residue remains. Before use, be sure to follow the sterilization process recommended by the manufacturer.
2) Never emit ultrasound while the probe is exposed to air. This may cause damage to the handpiece and probe.

5.4. Product Lifetime and Probe Change Guidance

Lifetime of the NP-200 is determined by SMPS electrolytic condenser. SMPS electrolytic condenser lifetime is 5,000 hours and expectation used time is 3 hours/day. So, lifetime of our product is 5 years.

		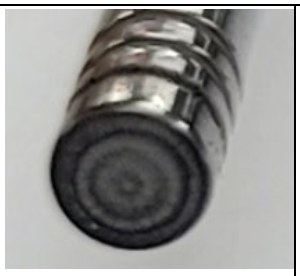	
unused	usable	Replacement recommended	Must be replaced
		Possibility of abnormal output	abnormal output

5.5. Disposal of Equipment

When disposing of the product, it must be separated and recycled. For disposal of waste residue, please contact the manufacturer, NEWPONG Co., Ltd., or the place where you purchased the product.

Copyright© 2021-2026 NEWPONG Co.,Ltd. All rights reserved.

6. Trouble shooting

6.1. Corrective action for emergency

⚠ Warning	Nobody beside authorized person can disassemble the device. Manufacturer has no responsibility for the broken device or damaged person if the device is disassembled discretionally.
⚠ Warning	In case of unintended malfunction or showing a sign, immediately stop operating and follow to trouble shooting procedures below.

If following troubles happen, please check the trouble shooting below before contact to manufacturer.

Situation and indications	Checklist	Solution
Smell of burning or sound of explosion in product		Separate power cord from outlet.
		Immediately call manufacturer.
When connection of Handpiece is not recognized.	It happens when the Handpiece is not connected well.	Restart the device after substitute the Handpiece.
		If it doesn't work with substituted Handpiece, contact us immediately.
Burn damage on the skin		Immediately have a cooling massage on the treated area. Prescribe steroid and spread an Ointment for burns depending on the situation.
When the LED indicator light is damaged		Discontinue use and treatment of the product immediately.
		Turn the power OFF and unplug the power cable from the outlet.
		Contact the manufacturer immediately.
Power supply is not working	Check whether the outlet or socket of wall is working and check whether the plug is inserted properly.	Check whether the power cord is connected well into main body.
		If the device is still not working though check all lists above, please call manufacturer.
The device does not turn off	Check the power cord and reset the working of ON/OFF button.	It the situation is repeated though check the working of ON/OFF button two to three times, please call manufacturer.

Copyright© 2021-2026 NEWPONG Co.,Ltd. All rights reserved.

6.2. Error Message

When error occurs, an error message is displayed with the alarm sound.

Display	Error Type	Error detail	Trouble shooting
Er10	1 Initial Fail	Hardware Error	1. Reboot the device 2. Contact to manufacturer or supplier
Er21	2 External Connection Status	HP Not Connected	1. Check handpiece connection 2. Re-connect handpiece cable 3. Test with other handpiece 4. Contact to manufacturer or supplier
Er23		Foot Switch Not Connected	** One Foot switch connected ** 1. Check Foot switch connection 2. Re-connect Foot switch cable ** Two Foot switch connected ** 1. IF one of them is working, there is no error message. Test with other foot switch and figure out whether it is foot switch problem or port problem. 2. If error message pop-up, test with other foot switch. 3. Contact to manufacturer or supplier

Copyright© 2021-2026 NEWPONG Co.,Ltd. All rights reserved.

7. Product specification

7.1. Mechanical Specification

<table>
<tr><th colspan="2">Item</th><th>Description</th></tr>
<tr><td colspan="2">Model Name</td><td>NP-200</td></tr>
<tr><td colspan="2">Classification and type for electrical shock</td><td>Class I, Type BF</td></tr>
<tr><td colspan="2">Input Power</td><td>(100 – 240) V~, (50/60) Hz</td></tr>
<tr><td colspan="2">Maximum Power Dissipation</td><td>200VA</td></tr>
<tr><td colspan="2">PROBE Tuning Frequency Range</td><td>37.5 kHz ± 2%, 31 kHz ± 2%</td></tr>
<tr><td colspan="2">Output Acoustic power</td><td>
<table>
<tr><th>Mode</th><th>BL</th><th>BM</th><th>BS</th><th>FM</th><th>FS</th></tr>
<tr><td>Continuous</td><td>17W~40W±10%</td><td>15W~37W±10%</td><td>14W~36W±10%</td><td>8W~22W ±10%</td><td>8W~20W ±10%</td></tr>
<tr><td>Pulse</td><td>12W~30W±10%</td><td>11W~28W±10%</td><td>11W~27W±10%</td><td>7W~19W ±10%</td><td>6W~18W ±10%</td></tr>
</table>
</td></tr>
<tr><td rowspan="2">Operation Mode</td><td>Continuous</td><td>Continuous Output</td></tr>
<tr><td>Pulse</td><td>Pulsed Output (Duty Cycle : 50%)</td></tr>
<tr><td colspan="2">Main Body</td><td>D 396mm x W 397mm x H 128mm</td></tr>
<tr><td colspan="2">B HANDPIECE</td><td>264mm(without cable), 32Φ, IPX7</td></tr>
<tr><td colspan="2">F HANDPIECE</td><td>205mm(without cable), 28Φ, IPX7</td></tr>
<tr><td colspan="2">Foot Switch</td><td>IPX6</td></tr>
<tr><td colspan="2">Mobility</td><td>Portable ME equipment</td></tr>
<tr><td colspan="2">Language</td><td>English</td></tr>
<tr><td colspan="2">S/W Version</td><td>NP200_MAIN_APP_2.00.00</td></tr>
</table>

7.2. Intended conditions of use

Considerations	Condition
Frequency of use	Depend on the operators and patients.
Location	In hospital environment
Mobility	Portable ME equipment

Copyright© 2021-2026 NEWPONG Co.,Ltd. All rights reserved.

7.3. Intended user profile (Operator Profile)

Considerations	Requirement description
Education	Physicians who, by means of formal professional training or sanctioned continuing medical education (including supervised operative experience).
Knowledge	- At least graduate from a surgical college. - International language(English), Local Language. - Arabic numerals and international units.
Language understanding	- Local language
Experience	- surgical or dermatologist
Permissible impairments	- Mild reading vision impairment or vision corrected to log MAR 0.2 - Average degree of aging-related short term memory impairment - Impaired by 40 % resulting in 60 % of normal hearing at 500 Hz to 2 kHz

Copyright© 2021-2026 NEWPONG Co.,Ltd. All rights reserved.

8. Product Warranty

Product name		LSSA
Model name		NP-200
Product license number [1)]		
Serial number		
Warranty (from the date of installation)		Main body : 24 months (except accessories) Handpiece & Footswitch : 6 months
Purchase date		
Client	Hospital : Address : Name : Tel :	
Seller		
Manufacturer		NEWPONG Co., Ltd

※ Thank you for your purchasing of NEWPONG's product.

※ This device is passed the restrict quality control and inspection process.

※ Standard compensation for repair, exchange and refund is compliant with [Consumer Injury and Compensation rule] of Ministry of Strategy and Finance.

※ Service center will repair in free of charge during warranty period if the device has a trouble under normal conditions during warranty period.

※ Please inform manufacturer or seller the model name, serial number, purchasing date and trouble matter if the device has a trouble under normal conditions during warranty period

※ Any unauthorized modification on this device are prohibited.

※ Main Body and accessories disposal should be done complying with disposed according to the hospital management regulations or WEEE policies.

Copyright© 2021-2026 NEWPONG Co.,Ltd. All rights reserved.

NEWPONG Co., Ltd
#1216 SJ Technoville, 278, Beotkkot-ro, Geumcheon-gu, Seoul, Korea
Tel. +82-2-541-0145
FAX. +82-2-541-0147
E-mail: info@newpong.com