


CIFAR-100, M4: Final-20 validation accuracy standard deviation

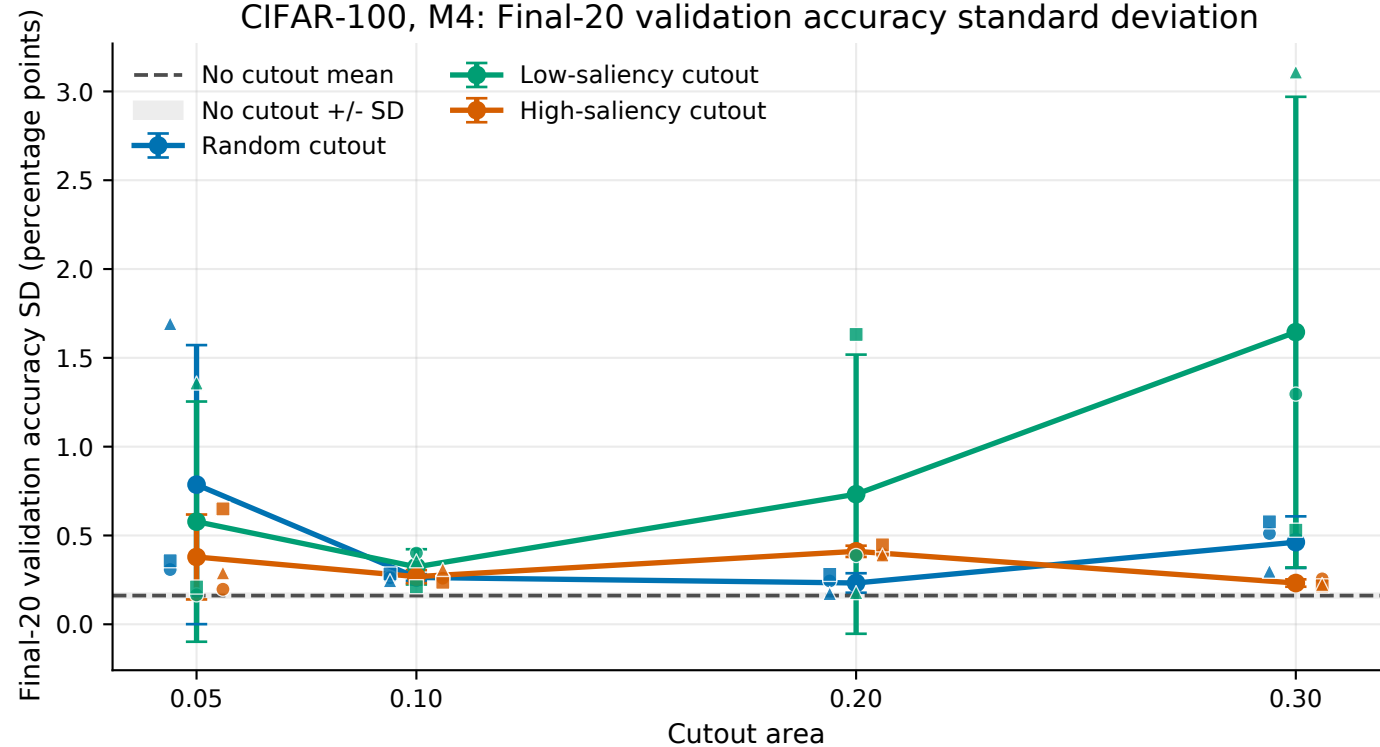

Mean across seeds; error bars and the baseline band show +/-1 sample SD across seeds.