

Detection of Arrhythmia Using Weightage-based Supervised Learning System for COVID-19.

Yashodhan Ketkar^a, Sushopti Gawade^b

^aDepartment of Information Technology Engineering, Pillai College of Engineering, Panvel, 410206, Maharashtra, India

^bDepartment of Computer Engineering, Pillai College of Engineering, Panvel, 410206, Maharashtra, India

ARTICLE INFO

Keywords:

Arrhythmia Detection
Automated Model Generation
Automated Model Training
Machine Learning In Healthcare
Supervised Learning Algorithm
Weightage based Model Selection

ABSTRACT

COVID-19 disease became a global pandemic in the last few years. This disease was highly contagious, and it quickly spread throughout several countries. Its infection can lead to severe implications in its victims, including cardiovascular issues. This complication develops in some people with a history of cardiovascular illness, whereas it emerges in others after COVID-19 infection. Cardiovascular problems are the primary cause of mortality in COVID-19 patients and are used to predict disease prognosis. Identifying arrhythmia from abnormalities in patient ECG signals is one approach to the detection of cardiovascular disorders. This is a laborious and time-consuming procedure that can be automated. The proposed method selects the most suitable model for this task. The selection is done through the weightage generated from the user's requirements. The proposed method uses supervised learning to identify abnormalities in ECG waves. The models provided by the selection system during tests were able to meet user requirements. The models achieved up to 97% accuracy and 97% precision in predictive tasks.

1. Introduction

COVID-19 has been widespread in recent years. It targets the human respiratory system, causing severe respiratory issues. Depending on a person's condition and the prevalence of comorbidities, this disease can be fatal. Cardiovascular comorbidities are frequent in COVID-19 disease. Cardiovascular comorbidities are also problematic to diagnose in the absence of suitable equipment. Checking for arrhythmia in patients is one approach to detection. Arrhythmia is the irregular beating of the heart. Arrhythmia is detected by examining ECG signals. Because COVID-19 has put a strain on the medical personnel, detection takes longer than usual. Increased Internet connectivity has led to the use of machine learning and artificial intelligence (AI) for service in a variety of sectors. This increases research in the field of machine learning and has an impact on machine learning in a variety of domains. One of them is the medical and healthcare businesses. Machine learning is used to detect and categorize viruses and other microorganisms in patients. In medical applications, machine learning algorithms have already been shown to be quite useful.

The machine learning system may be used to scan these ECG signals and detect them. These signs may be detected considerably faster and more efficiently using supervised learning techniques. In such exact classification problems, supervised algorithms have previously been demonstrated to be quicker than unsupervised techniques. Once taught, this algorithm may also be utilized to make future predictions.


There are several supervised algorithms accessible, allowing us to select the best method for our purposes. This phase can be automated in the case of the general population. A few methods may be pre-programmed into the system, and

the computer can then train and pick the best model for the supplied dataset. This will free up medical personnel to focus on patient care and problem-solving.

2. Literature Review

Babapoor-Farrokhran, Rasekhi, Gill, Babapoor and Amanullah (2020) suggests that arrhythmia is one of the most common symptoms in patients with COVID19. Arrhythmia was found in 7% of all 19 Wuhan COVID cases and 14.8% of patients with poor outcomes. Mulia, Maghfirah, Rachmi and Julario (2021) states that 17% of patients hospitalized in China were diagnosed with arrhythmia. Mulia et al. conducted a review of 10 eligible studies (5,193 patients) for analysis and found that atrial arrhythmia was present in 9.2% of cases. A review by Liu, Chen and Zeng (2020a) of 17 studies with (5,815 patients) showed that arrhythmia was detected in 9.3% of COVID-19 cases. Yarmohammadi, Morrow, Dizon, Biviano, Ehlert, Saluja, Waase, Elias, Poterucha, Berman et al. (2021) suggest that only 8% of patients with arrhythmia had prior cardiovascular conditions. also mentioned that 56% of patients showed symptoms after the COVID-19 infection.

Sun, Wang, Zhao and Yan (2020) used an ensemble classifier to detect the anomalies in the ECG signal. This approach, which combines multiple classifiers for prediction, has proven effective because the accuracy of the ensemble classifier is significantly higher than that of a single classifier. Few authors used this approach to improve the prediction accuracy of supervised learning models. Huang, Chen, Zeng, Cao and Li (2020) used the maximal overlap wavelet packet transform ensemble with a neural network and achieved satisfactory results. Rajak, Shrivastava and Vidushi (2020) used the ensemble approach to predict the results of the students. Rajak et al. states the model was

 ketkaryapr19me@student.mes.ac.in (Y. Ketkar); sgawade@mes.ac.in (S. Gawade)

able to predict the correct results even with a small amount of training data. Liu, Lou and Huang (2020b) compared the FLINK-based iForest ensembled algorithms against the sklearn-iForset and other algorithms. Liu et al. concluded that the Flink-iForest algorithm showed better performance than off-shelf algorithms. Imbrea (2021) used the AutoML algorithm and tools on data streams. Imbrea concluded that the default classifiers can be used with AutoML tools for accurate prediction. With AutoML tools, prediction systems can be automated.

Chopade, Chopade and Gawade (2022) used machine learning for the prediction of end-of-semester results. Chopade, Chopade and Gawade (2022) used SVM, KNN, and DT models. Chopade, Chopade and Gawade (2022) concluded that the machine learning system performed satisfactorily, with SVM achieving up to 78% accuracy.

Siddiqui, Morales-Menendez, Huang and Hussain (2020) extracted appropriate features for the detection of epileptic seizures. Siddiqui et al. preprocessed data and used ML algorithms on the data. Siddiqui et al. concluded that the supervised learning models showed more effectiveness than the unsupervised learning models. Jha and Kolekar (2020) used a commercial classifier for the detection of arrhythmia. Jha and Kolekar used ECG signals from patients and applied a custom SVM classifier. Jha and Kolekar concluded that the algorithm was a successful and efficient detection of arrhythmia.

Marathe, Gawade and Kanekar (2021) used supervised learning algorithms for the early detection of heart disease and diabetes disease. Marathe, Gawade and Kanekar (2021) concluded that the model performed satisfactorily.

Hannun, Rajpurkar, Haghpanahi, Tison, Bourn, Turakhia and Ng (2019) used neural networks to process raw ECG signals and make predictions. While Sannino and De Pietro (2018) used small neural networks for efficient recognition processes. Both studies concluded that artificial neural networks are extremely efficient and accurate in the prediction of anomalies.

Chen, Mazomenos, Maharatna, Dasmahapatra and Niranjan (2013) showed that the LDA classifier can outperform the SVM classifier in low-performance environments and lightweight systems. The self-learning algorithm makes the system more dynamic and adaptable to incoming signals. Lei, Li, Dong and Vai (2007) used adaptive fuzzy algorithms to classify ECG signals. Lei et al. stated that the algorithm showed satisfactory results, but it requires former classification patterns results. The RPA system can be used in these systems for easier integration of machine learning with dynamic data Ketkar and Gawade (2021). Rehmat, Hassan, Khalid and Dilawar (2022) used ECG signals of COVID-19 patients for patient monitoring. Rehmat et al. used LSTM, SVM, and MLP algorithms to monitor data. Rehmat et al. suggest that machine learning with robotics can provide better results.

Dev, Wang, Nwosu, Jain, Veeravalli and John (2022) used a multi perceptron neural network for stroke predictions. The neural network showed high accuracy. Dev et al.

were able to achieve up to 78% accuracy. Dev et al. suggested that the model can produce better results with a larger training dataset. Chang, Bhavani, Xu and Hossain (2022) used artificial intelligence to detect heart disease. Chang et al. concluded that the algorithms achieved up to 83% accuracy. Chang et al. also concluded that the system was able to comply with the HIPAA regulations.

Verma and Gawade (2021) used machine learning algorithms to predict crop growth rates. Verma and Gawade were able to get good insights into the field with the help of machine learning. Verma and Gawade concluded that the use of machine learning will result in minimizing the complexity and increasing yield in farming.

Atanasova, Todorovski, Džeroski and Kompare (2008) used a two-year dataset collected by Glumo Lake and used their expertise to train and select models. A mixed approach of data-driven and knowledge-driven modeling is used for the success of the application. Lee and Lin (2000) used loo rate and stop criteria for model selection. Lee and Lin investigated eight different issues and found that a larger loo rate was more desirable. Lee and Lin also suggested that modeling difficulties can only be found by careful numerical calculations.

Malkomes, Schaff and Garnett (2016) used a novel kernel to get the dataset description. Malkomes et al. concluded that this approach led to the discovery of invisible models. Malkomes et al. also state that this approach reduces the amount of human interaction. Calcagno and de Mazancourt (2010) created a new model using the glmulti package. These models are unique and flexible. The model is automatically optimized to provide a multi-model interface. This approach allows you to quickly explore a large set of models for selection purposes. Garcia and Lõndero (2021) optimized parameters with a genetic algorithm. Garcia and Lõndero successfully used a genetic algorithm to reduce uncertainty from the prediction results. These methods can be used for the automated model selection system.

3. Dataset and Method

3.1. Mathematical Model

Figure 1 shows the approach toward the selection of a suitable model. With this system, we can handle up to N models. Equation (1) shows the mathematical formula used to calculate the V scores of the models. These V scores will allow the system to select the appropriate model.

$$V_{score} = \left(\sum_{x=1}^5 w_x P_x \right) - w_6^2 P_6 \quad (1)$$

3.2. Method

The Figure 2, shows the basic architecture of the automated model training and selection system. The data is collected from the user and processed by the application. This data is stored as training and testing datasets.

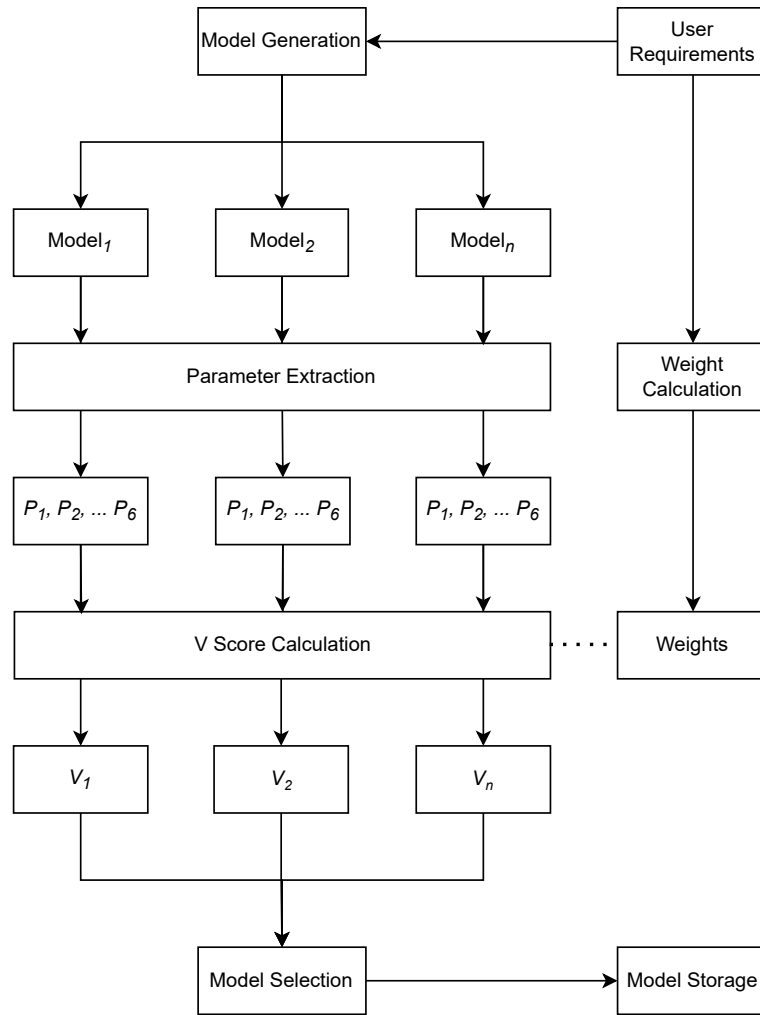


Figure 1: Model Selection Approach

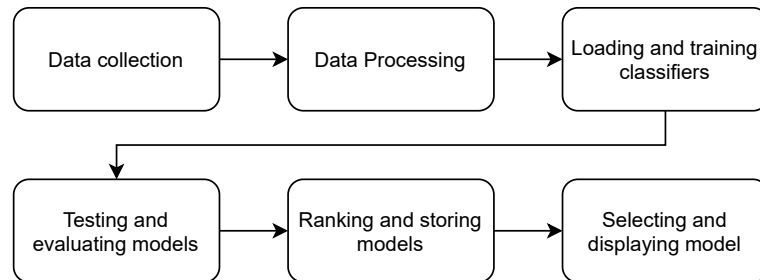


Figure 2: Training and Selection Process

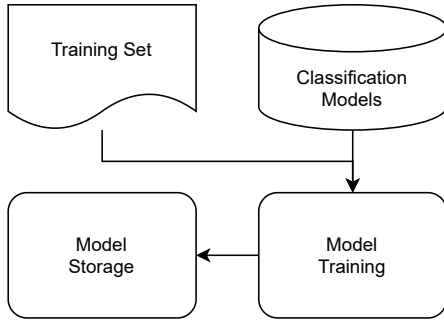


Figure 3: Training Process

Figure 3, shows the training process. In this process, the training dataset is loaded into the system. Premade classification model templates are accessed by the system and trained with provided data. These trained models are stored by the system for the next step.

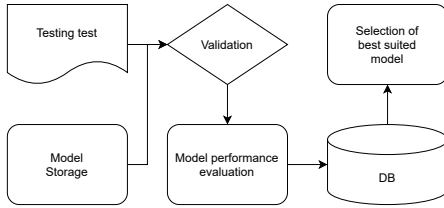


Figure 4: Selection Process

The Figure 4, shows the selection process. In this process, the testing dataset is used for the evaluation of the trained models. The trained models are ranked with respect to the performance evaluation. These ranks are used with the help of the tuning parameters to select the best-suited model. This model is stored as the best model for future classification.

3.3. Dataset

The ECG readings in this paper are obtained from the MIT-BIH arrhythmia database [8]. This database is used for automated training and evaluation. This dataset was published in 1999 by MIT-BIH as an open-source database; it consists of training and testing datasets. This database is further divided into four equal parts for analysis. Each training set contains 21888 signals, and the testing set contains 5473 signals.

4. Results And Testing

During the automated training and selection process, the SVM classifier is selected as the best-suited model for dataset 1, dataset 2, and dataset 4. Whereas RF classifier is selected as the best-suited model for dataset 3.

Performance metrics used for evaluation were Accuracy, F1, Precision, Recall, Area under ROC Curve, and Total prediction time. The weightage assigned to these metrics for ranking was 1.0, 0.8, 0.4, 0.4, 0.4, 0.25 respectively. Where higher value means higher priority.

4.1. Performance Evaluation

The models are tested with a testing dataset obtained from the MIT-BIH database. The testing dataset consists of 5473 signals. Figures 5 to 8 shows that model trained with automated system produced satisfactory results. Few models like KNN, RF, and SVM performed better than other models (DT) at the cost of higher prediction time. Whereas MLP models produced good overall results with lower prediction time. Tables 1 to 4 show the performance of the models on their respective datasets in detail.

4.2. Performance Error Calculation

For error calculation, best models are tested against training datasets of other models. Figures 9 to 13 shows the average error introduced when models are tested against training datasets of other models. This chart shows that KNN, MLP, and SVM models introduced minimum errors, whereas DT and RF models introduced large amounts of error. Figure 13 also shows that SVM model produced similar error across all datasets. This smaller difference in error suggests that the SVM classifier can be used for classification tasks of similar nature. Tables 5 to 24 show the performance of the models when tested on other datasets in detail.

5. Conclusion and Future work

In this paper, we present a novel system. The system provides the end user ability to train the best-suited model for the problem. With the current COVID-19 pandemic, this system can be employed by healthcare professionals for the detection of anomalies such as arrhythmia in patients. The system is tested with the ECG MIT-BIH arrhythmia database. The models trained and selected by the system showed good classification performance, these models also performed satisfactorily against training datasets of other models suggesting good general classification performance.

Future work will involve the use of other freely available datasets to test the general classification performance of the system as well as testing the current system in a real-time environment. Also modifying the system to work with non-labeled databases by employing unsupervised learning methods.

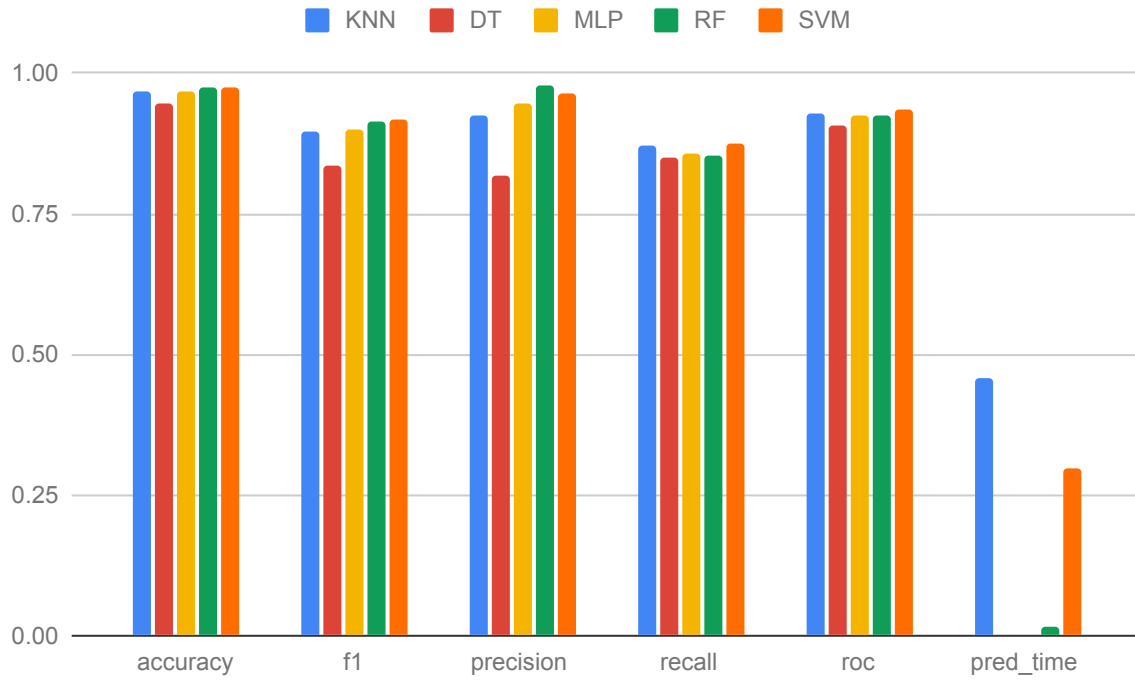


Figure 5: Performance Results Dataset 1

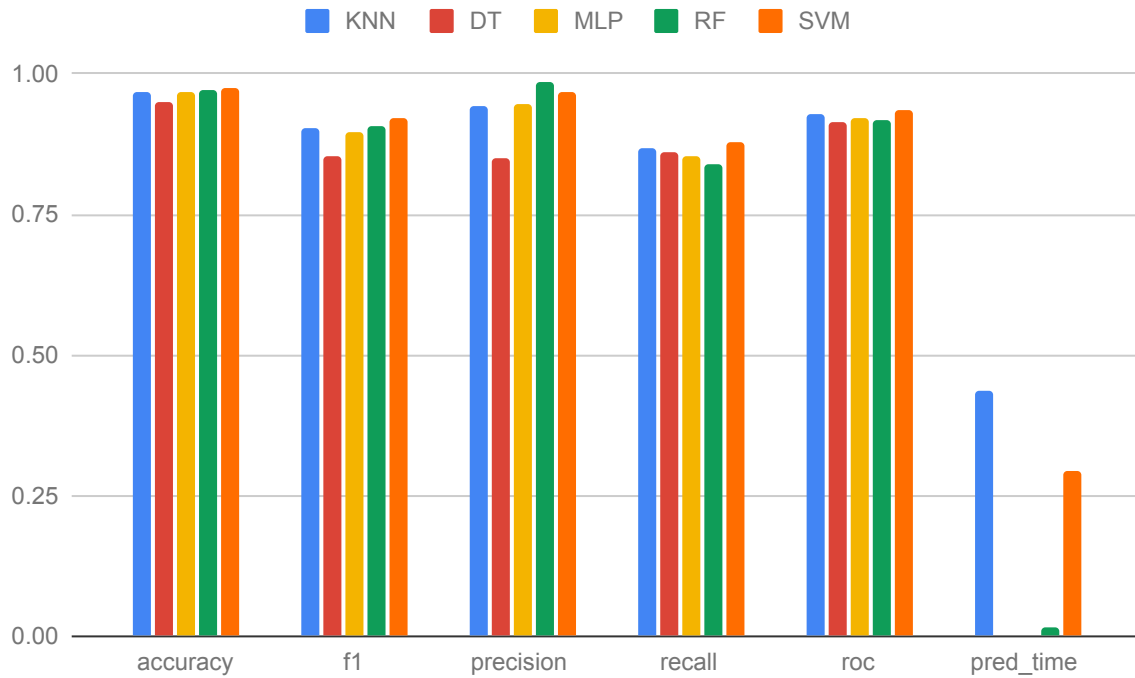


Figure 6: Performance Results Dataset 2

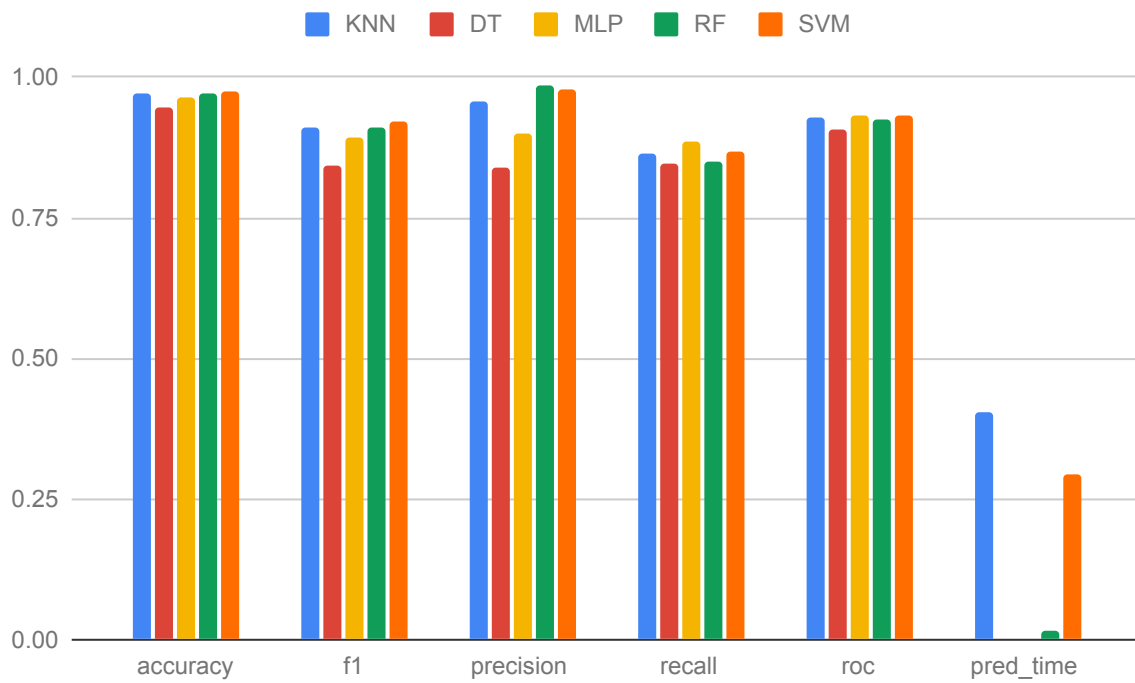


Figure 7: Performance Results Dataset 3

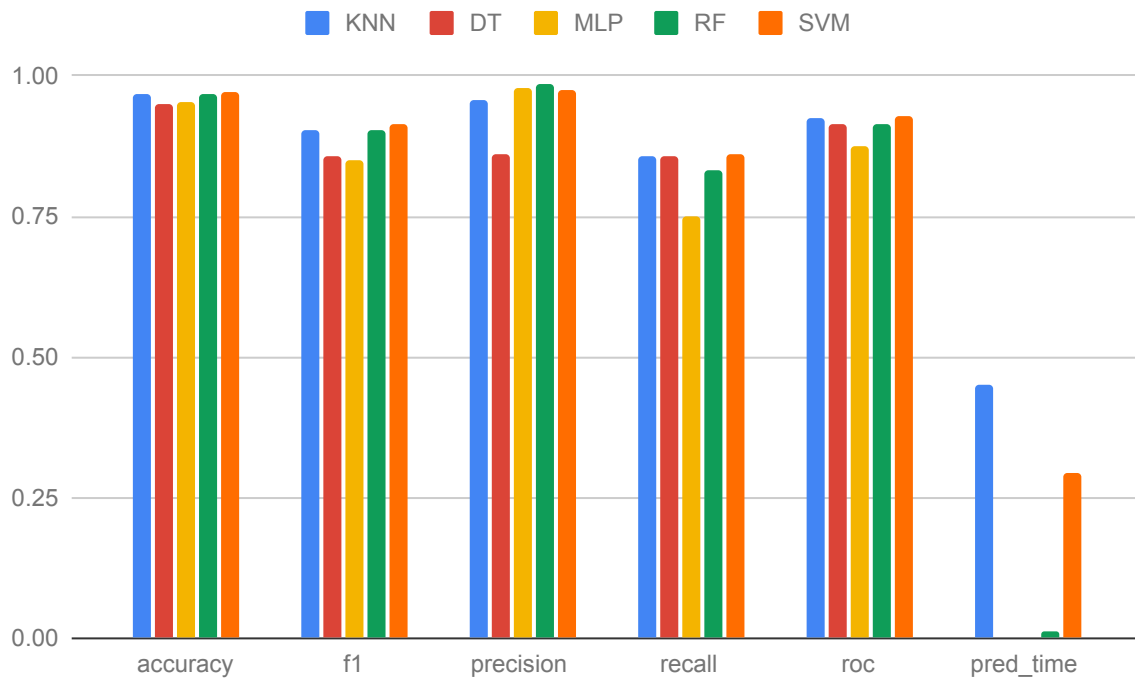


Figure 8: Performance Results Dataset 4

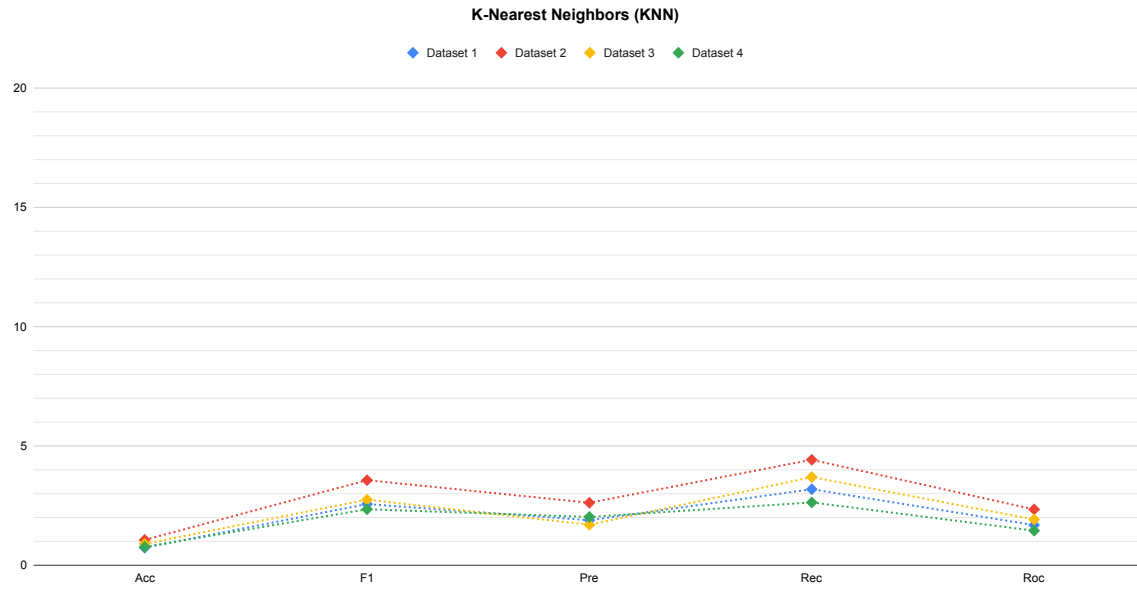


Figure 9: Average Error for K-Nearest Neighbors (KNN) model

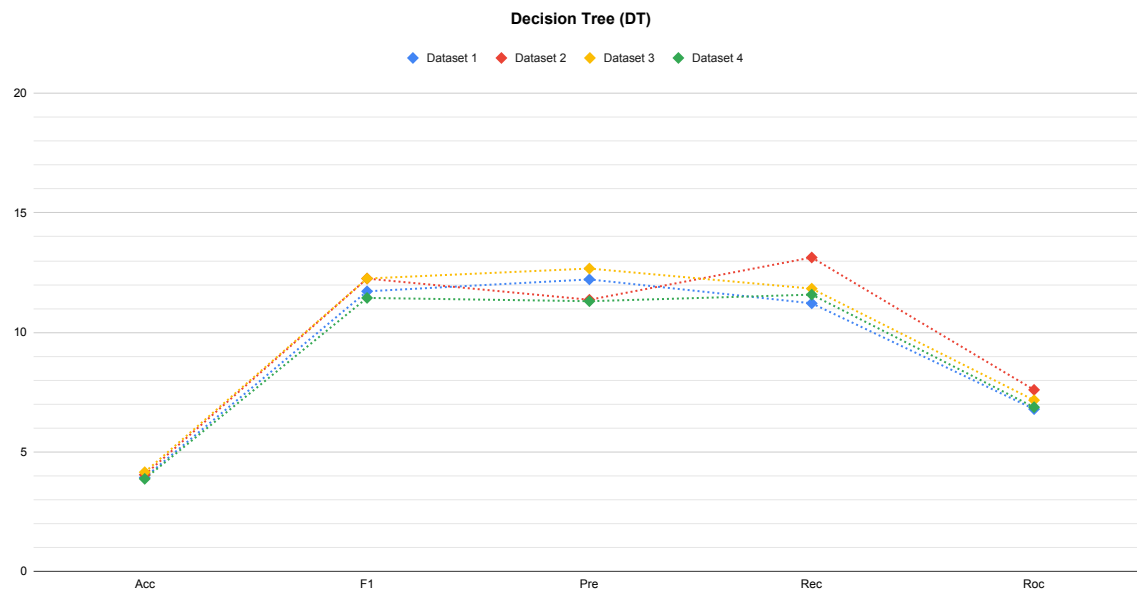


Figure 10: Average Error for Decision Tree (DT) model

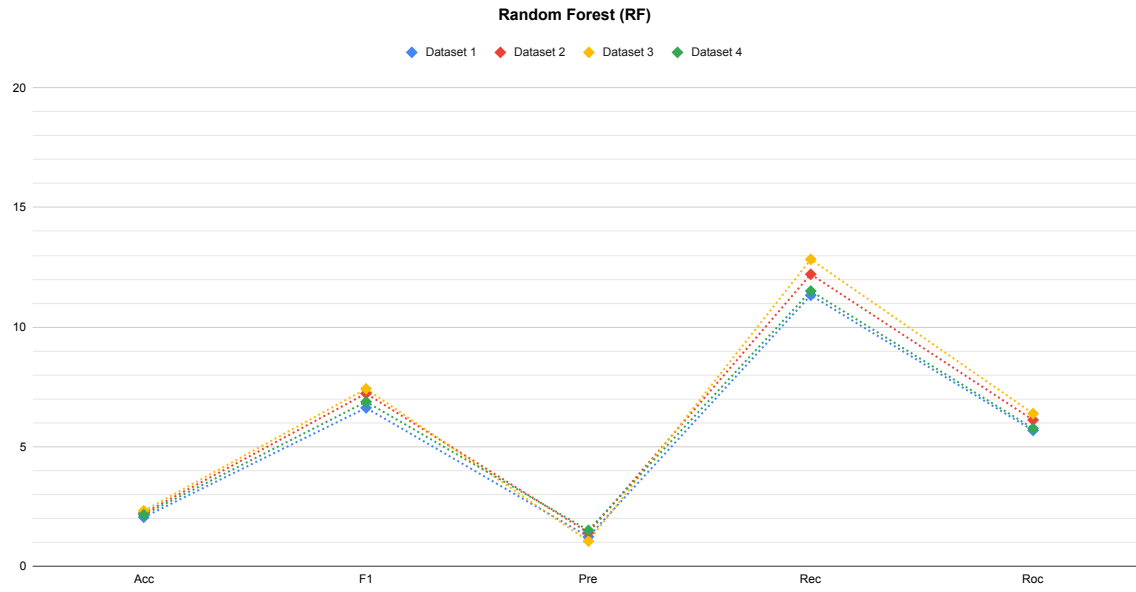


Figure 11: Average Error for Random Forest (RF) model

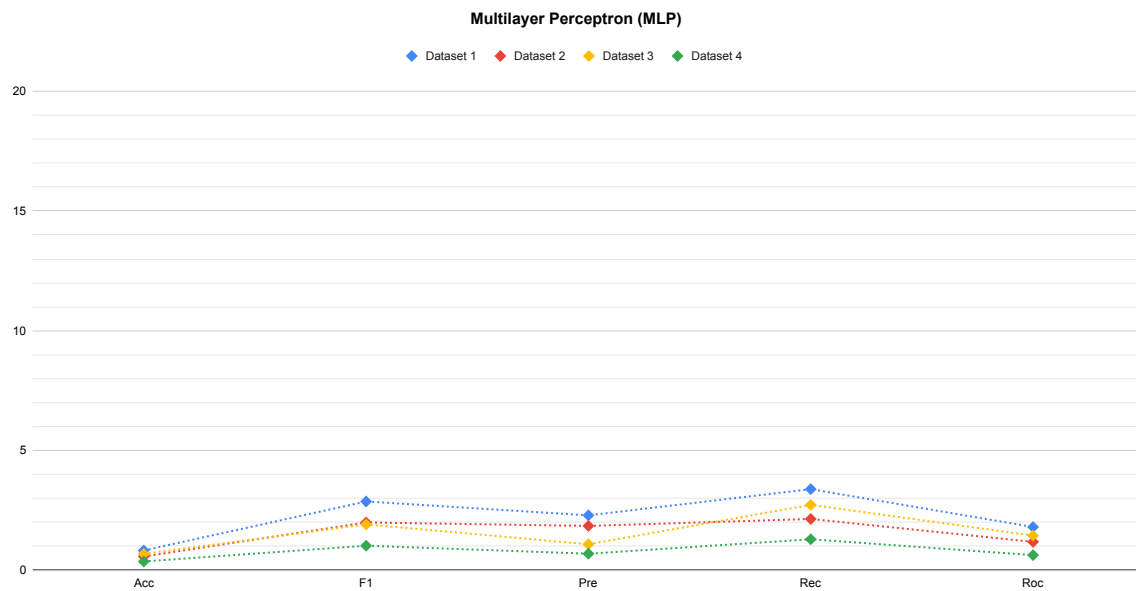


Figure 12: Average Error for Multilayer Perceptron (MLP) model

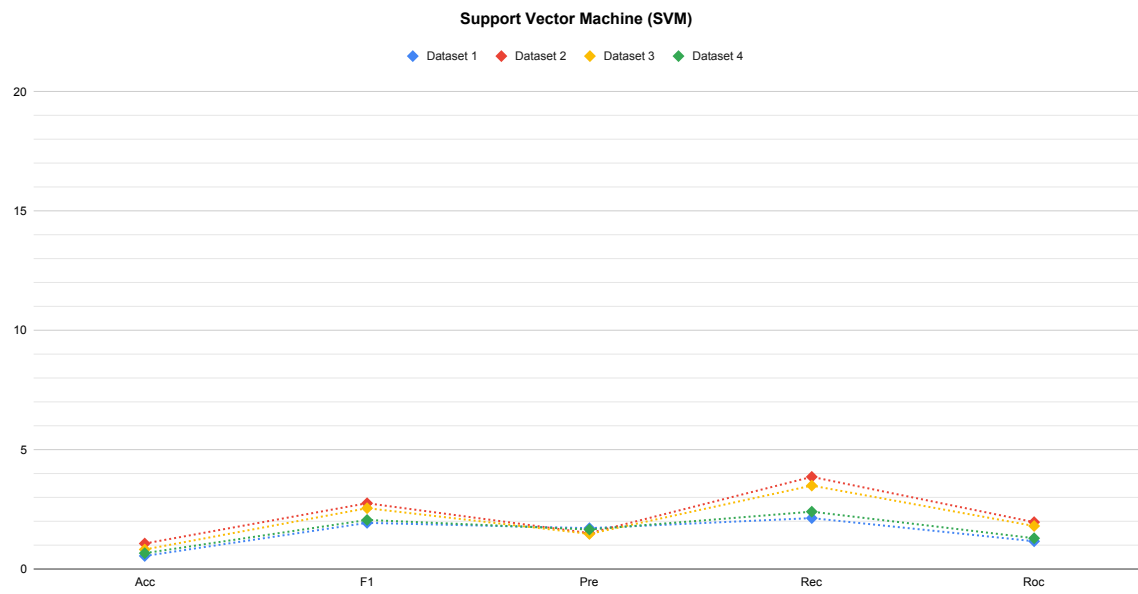


Figure 13: Average Error for Support Vector Machine (SVM) model

Table 1

Performance of models trained on dataset 1

Metric	KNN	DT	MLP	RF	SVM
Accuracy	96.72	94.46	96.89	97.33	97.40
F1	89.71	83.43	90.05	91.30	91.69
Precision	92.53	81.86	94.71	97.95	96.43
Recall	87.06	85.06	85.84	85.50	87.40
ROC	92.84	90.68	92.45	92.57	93.38
Time(s)	0.457	0.001	0.002	0.015	0.297

Table 2

Performance of models trained on dataset 2

Metric	KNN	DT	MLP	RF	SVM
Accuracy	96.83	95.04	96.69	97.09	97.46
F1	90.28	85.50	89.73	90.75	92.15
Precision	94.25	84.90	94.73	98.60	96.79
Recall	86.63	86.09	85.23	84.05	87.93
ROC	92.77	91.48	92.13	91.90	93.66
Time(s)	0.435	0.001	0.003	0.014	0.295

Table 3

Performance of models trained on dataset 3

Metric	KNN	DT	MLP	RF	SVM
Accuracy	97.07	94.64	96.41	97.22	97.44
F1	90.93	84.30	89.34	91.21	92.00
Precision	95.82	83.81	90.13	98.37	97.81
Recall	86.53	84.80	88.57	85.02	86.85
ROC	92.87	90.73	93.29	92.36	93.22
Time(s)	0.404	0.001	0.002	0.017	0.293

Table 4

Performance of models trained on dataset 4

Metric	KNN	DT	MLP	RF	SVM
Accuracy	96.84	94.99	95.34	96.88	97.15
F1	90.52	85.73	85.01	90.37	91.39
Precision	95.71	85.91	97.83	98.65	97.41
Recall	85.86	85.55	75.15	83.37	86.07
ROC	92.52	91.28	87.40	91.56	92.79
Time(s)	0.452	0.001	0.002	0.014	0.294

Table 5

Performance of Decision Tree model trained on dataset 1

Metric	Dataset 1	Dataset 2	Dataset 3	Dataset 4
Accuracy	0.98	0.94	0.94	0.94
F1	0.96	0.85	0.85	0.84
Precision	0.95	0.83	0.84	0.83
Recall	0.96	0.86	0.85	0.85
ROC	0.97	0.91	0.91	0.90

Table 6

Performance of Decision Tree model trained on dataset 2

Metric	Dataset 1	Dataset 2	Dataset 3	Dataset 4
Accuracy	0.94	0.98	0.94	0.94
F1	0.84	0.96	0.84	0.85
Precision	0.85	0.96	0.85	0.85
Recall	0.82	0.96	0.84	0.84
ROC	0.89	0.97	0.90	0.90

Table 7

Performance of Decision Tree model trained on dataset 3

Metric	Dataset 1	Dataset 2	Dataset 3	Dataset 4
Accuracy	0.94	0.94	0.98	0.94
F1	0.84	0.84	0.96	0.83
Precision	0.84	0.83	0.95	0.83
Recall	0.84	0.85	0.96	0.84
ROC	0.90	0.90	0.97	0.90

Table 8

Performance of Decision Tree model trained on dataset 4

Metric	Dataset 1	Dataset 2	Dataset 3	Dataset 4
Accuracy	0.94	0.94	0.95	0.98
F1	0.85	0.85	0.85	0.96
Precision	0.85	0.85	0.85	0.96
Recall	0.85	0.84	0.85	0.96
ROC	0.91	0.90	0.91	0.97

Table 9

Performance of K-Nearest Neighbors model trained on dataset 1

Metric	Dataset 1	Dataset 2	Dataset 3	Dataset 4
Accuracy	0.97	0.97	0.97	0.96
F1	0.93	0.91	0.90	0.90
Precision	0.96	0.95	0.94	0.94
Recall	0.90	0.87	0.87	0.87
ROC	0.94	0.93	0.93	0.93

Table 10

Performance of K-Nearest Neighbors model trained on dataset 2

Metric	Dataset 1	Dataset 2	Dataset 3	Dataset 4
Accuracy	0.96	0.97	0.96	0.96
F1	0.90	0.93	0.90	0.89
Precision	0.94	0.96	0.94	0.94
Recall	0.86	0.90	0.86	0.85
ROC	0.92	0.94	0.92	0.92

Table 11

Performance of K-Nearest Neighbors model trained on dataset 3

Metric	Dataset 1	Dataset 2	Dataset 3	Dataset 4
Accuracy	0.96	0.96	0.97	0.96
F1	0.90	0.90	0.93	0.90
Precision	0.95	0.95	0.96	0.94
Recall	0.86	0.86	0.89	0.86
ROC	0.92	0.92	0.94	0.92

Table 12

Performance of K-Nearest Neighbors model trained on dataset 4

Metric	Dataset 1	Dataset 2	Dataset 3	Dataset 4
Accuracy	0.96	0.96	0.96	0.97
F1	0.90	0.90	0.90	0.92
Precision	0.94	0.95	0.94	0.96
Recall	0.86	0.86	0.87	0.89
ROC	0.92	0.92	0.93	0.94

Table 13

Performance of Multilayer Perceptron model trained on dataset 1

Metric	Dataset 1	Dataset 2	Dataset 3	Dataset 4
Accuracy	0.97	0.96	0.96	0.96
F1	0.92	0.89	0.89	0.89
Precision	0.97	0.95	0.94	0.95
Recall	0.88	0.85	0.85	0.85
ROC	0.93	0.92	0.92	0.92

Table 14

Performance of Multilayer Perceptron model trained on dataset 2

Metric	Dataset 1	Dataset 2	Dataset 3	Dataset 4
Accuracy	0.96	0.97	0.96	0.96
F1	0.90	0.91	0.90	0.90
Precision	0.95	0.97	0.94	0.95
Recall	0.85	0.87	0.85	0.85
ROC	0.92	0.93	0.92	0.92

Table 15

Performance of Multilayer Perceptron model trained on dataset 3

Metric	Dataset 1	Dataset 2	Dataset 3	Dataset 4
Accuracy	0.96	0.96	0.96	0.96
F1	0.89	0.89	0.90	0.88
Precision	0.89	0.89	0.90	0.89
Recall	0.88	0.88	0.91	0.88
ROC	0.93	0.93	0.94	0.93

Table 16

Performance of Multilayer Perceptron model trained on dataset 4

Metric	Dataset 1	Dataset 2	Dataset 3	Dataset 4
Accuracy	0.95	0.95	0.95	0.95
F1	0.85	0.85	0.85	0.86
Precision	0.97	0.97	0.97	0.98
Recall	0.75	0.75	0.75	0.76
ROC	0.87	0.87	0.87	0.88

Table 17

Performance of Random Forest model trained on dataset 1

Metric	Dataset 1	Dataset 2	Dataset 3	Dataset 4
Accuracy	0.99	0.97	0.97	0.97
F1	0.98	0.91	0.91	0.91
Precision	0.99	0.98	0.97	0.98
Recall	0.96	0.85	0.85	0.85
ROC	0.98	0.92	0.92	0.92

Table 18

Performance of Random Forest model trained on dataset 2

Metric	Dataset 1	Dataset 2	Dataset 3	Dataset 4
Accuracy	0.96	0.99	0.97	0.97
F1	0.90	0.97	0.91	0.90
Precision	0.98	0.99	0.97	0.98
Recall	0.83	0.96	0.85	0.84
ROC	0.91	0.98	0.92	0.91

Table 19

Performance of Random Forest model trained on dataset 3

Metric	Dataset 1	Dataset 2	Dataset 3	Dataset 4
Accuracy	0.96	0.97	0.99	0.97
F1	0.90	0.90	0.97	0.90
Precision	0.98	0.98	0.99	0.98
Recall	0.83	0.84	0.96	0.83
ROC	0.91	0.91	0.98	0.91

Table 20

Performance of Random Forest model trained on dataset 4

Metric	Dataset 1	Dataset 2	Dataset 3	Dataset 4
Accuracy	0.96	0.97	0.97	0.99
F1	0.90	0.91	0.90	0.97
Precision	0.98	0.98	0.97	0.99
Recall	0.84	0.84	0.85	0.95
ROC	0.91	0.92	0.92	0.97

Table 21

Performance of Support Vector Machine model trained on dataset 1

Metric	Dataset 1	Dataset 2	Dataset 3	Dataset 4
Accuracy	0.97	0.97	0.97	0.97
F1	0.93	0.92	0.91	0.91
Precision	0.98	0.97	0.96	0.96
Recall	0.89	0.87	0.87	0.87
ROC	0.94	0.93	0.93	0.93

Table 22

Performance of Support Vector Machine model trained on dataset 2

Metric	Dataset 1	Dataset 2	Dataset 3	Dataset 4
Accuracy	0.97	0.98	0.97	0.97
F1	0.91	0.94	0.91	0.91
Precision	0.97	0.98	0.96	0.96
Recall	0.86	0.89	0.86	0.86
ROC	0.92	0.94	0.93	0.92

Table 23

Performance of Support Vector Machine model trained on dataset 3

Metric	Dataset 1	Dataset 2	Dataset 3	Dataset 4
Accuracy	0.97	0.97	0.98	0.97
F1	0.91	0.92	0.94	0.91
Precision	0.97	0.97	0.98	0.97
Recall	0.85	0.87	0.89	0.87
ROC	0.92	0.93	0.94	0.93

Table 24

Performance of Support Vector Machine model trained on dataset 4

Metric	Dataset 1	Dataset 2	Dataset 3	Dataset 4
Accuracy	0.97	0.97	0.97	0.97
F1	0.91	0.91	0.91	0.93
Precision	0.97	0.96	0.96	0.98
Recall	0.85	0.86	0.86	0.88
ROC	0.92	0.93	0.93	0.94

References

- Atanasova, N., Todorovski, L., Džeroski, S., Kompare, B., 2008. Application of automated model discovery from data and expert knowledge to a real-world domain: Lake glumšø. *ecological modelling* 212, 92–98.
- Babapoor-Farrokhran, S., Rasekhi, R.T., Gill, D., Babapoor, S., Amanullah, A., 2020. Arrhythmia in covid-19. *SN Comprehensive Clinical Medicine* 2, 1430–1435.
- Calcagno, V., de Mazancourt, C., 2010. glmulti: an r package for easy automated model selection with (generalized) linear models. *Journal of statistical software* 34, 1–29.
- Chang, V., Bhavani, V.R., Xu, A.Q., Hossain, M., 2022. An artificial intelligence model for heart disease detection using machine learning algorithms. *Healthcare Analytics* 2, 100016.
- Chen, T., Mazomenos, E.B., Maharatna, K., Dasmahapatra, S., Niranjana, M., 2013. Design of a low-power on-body ecg classifier for remote cardiovascular monitoring systems. *IEEE Journal on Emerging and Selected Topics in Circuits and Systems* 3, 75–85.
- Chopade, S., Chopade, S., Gawade, S., 2022. Multimedia teaching learning methodology and result prediction system using machine learning. *Journal of Engineering Education Transformations* 35.
- Dev, S., Wang, H., Nwosu, C.S., Jain, N., Veeravalli, B., John, D., 2022. A predictive analytics approach for stroke prediction using machine learning and neural networks. *Healthcare Analytics* 2, 100032.
- Fazeli, S., 2018. ECG heartbeat categorization dataset. URL: <https://www.kaggle.com/shayanfazeli/heartbeat>, accessed on 15 April 2022.
- Garcia, L.G., Lôndero, V., 2021. A parameter optimizer based on genetic algorithm for the simulation of carbonate facies. *Intelligent Systems with Applications* 12, 200057.
- Hannun, A.Y., Rajpurkar, P., Haghpanahi, M., Tison, G.H., Bourn, C., Turakhia, M.P., Ng, A.Y., 2019. Cardiologist-level arrhythmia detection and classification in ambulatory electrocardiograms using a deep neural network. *Nature medicine* 25, 65–69.
- Huang, J.S., Chen, B.Q., Zeng, N.Y., Cao, X.C., Li, Y., 2020. Accurate classification of ecg arrhythmia using mowpt enhanced fast compression deep learning networks. *Journal of Ambient Intelligence and Humanized Computing* , 1–18.
- Imbrea, A.I., 2021. Automated machine learning techniques for data streams. *arXiv preprint arXiv:2106.07317* .
- Jha, C.K., Kolekar, M.H., 2020. Cardiac arrhythmia classification using tunable q-wavelet transform based features and support vector machine classifier. *Biomedical Signal Processing and Control* 59, 101875.
- Ketkar, Y., Gawade, S., 2021. Effectiveness of robotic process automation for data mining using uipath, in: 2021 International Conference on Artificial Intelligence and Smart Systems (ICAIS), pp. 864–867. doi:10.1109/ICAIS50930.2021.9396024.
- Lee, J.H., Lin, C.J., 2000. Automatic Model Selection for Support Vector Machines. Technical Report. Information Engineering Graduate Institute of Taiwan University.
- Lei, W.K., Li, B.N., Dong, M.C., Vai, M.I., 2007. Afc-ecg: An adaptive fuzzy ecg classifier, in: *Soft computing in industrial applications*. Springer, pp. 189–199.
- Liu, Q., Chen, H., Zeng, Q., 2020a. Clinical characteristics of covid-19 patients with complication of cardiac arrhythmia. *Journal of Infection* 81, e6–e8.
- Liu, Y., Lou, Y., Huang, S., 2020b. Parallel algorithm of flow data anomaly detection based on isolated forest, in: 2020 International Conference on Artificial Intelligence and Electromechanical Automation (AIEA), IEEE. pp. 132–135.
- Malkomes, G., Schaff, C., Garnett, R., 2016. Bayesian optimization for automated model selection. *Advances in Neural Information Processing Systems* 29.
- Marathe, N., Gawade, S., Kanekar, A., 2021. Prediction of heart disease and diabetes using naive bayes algorithm. *International Journal of Scientific Research in Computer Science, Engineering and Information Technology* , 447–453.
- Mulia, E.P.B., Maghfirah, I., Rachmi, D.A., Julario, R., 2021. Atrial arrhythmia and its association with covid-19 outcome: a pooled analysis. *Diagnosis* 8, 532–535.
- Rajak, A., Shrivastava, A.K., Vidushi, 2020. Applying and comparing machine learning classification algorithms for predicting the results of students. *Journal of Discrete Mathematical Sciences and Cryptography* 23, 419–427.
- Rehmat, M.A., Hassan, M.A., Khalid, M.H., Dilawar, M., 2022. Next level of hospitalisation through smart icu. *Intelligent Systems with Applications* 14, 200080.
- Sannino, G., De Pietro, G., 2018. A deep learning approach for ecg-based heartbeat classification for arrhythmia detection. *Future Generation Computer Systems* 86, 446–455.
- Siddiqui, M.K., Morales-Menendez, R., Huang, X., Hussain, N., 2020. A review of epileptic seizure detection using machine learning classifiers. *Brain informatics* 7, 1–18.
- Sun, Z., Wang, C., Zhao, Y., Yan, C., 2020. Multi-label ecg signal classification based on ensemble classifier. *IEEE Access* 8, 117986–117996.
- Verma, M.S., Gawade, S.D., 2021. A machine learning approach for prediction system and analysis of nutrients uptake for better crop growth in the hydroponics system, in: 2021 International Conference on Artificial Intelligence and Smart Systems (ICAIS), IEEE. pp. 150–156.
- Yarmohammadi, H., Morrow, J.P., Dizon, J., Biviano, A., Ehlert, F., Saluja, D., Waase, M., Elias, P., Poterucha, T.J., Berman, J., et al., 2021. Frequency of atrial arrhythmia in hospitalized patients with covid-19. *The American Journal of Cardiology* 147, 52–57.