


Q-KNEE QUANTUM-ASSISTED MRI ANALYSIS REPORT

Research prototype — quantum-assisted ACL / meniscal tear-risk triage. Not a certified medical device.


Patient & Study Information

Patient ID	DEMO-001	Scan Date	2026-08-30
Patient Name	Test Patient	Modality	MRI Knee
Date of Birth	1990-01-01	Referring Physician	Dr. A. Example
Clinical Indication	Chronic knee pain, rule out ACL/meniscal tear		

Imaging — MRI Slice & Risk-Targeted Grad-CAM Overlay

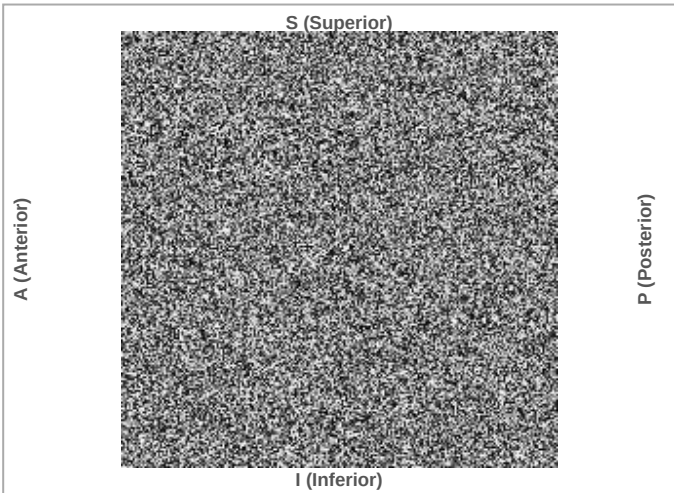

Original MRI Slice

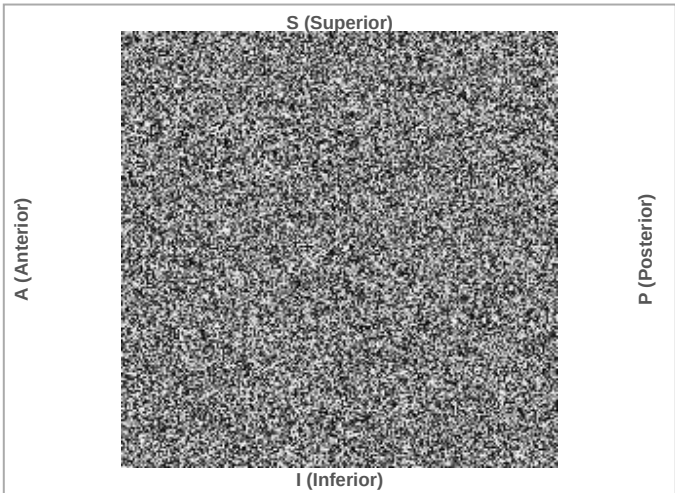

Grad-CAM Risk-Region Overlay

Diagnostic Breakdown

Region	Tear Risk	Risk Tier	Classification
ACL	72.0%	HIGH	TEAR LIKELY
Meniscus	31.0%	LOW	NO TEAR INDICATED

Quantum Circuit Inference Latency

Feature Extraction	Dim. Reduction	Quantum Circuit Inference	Total (End-to-End)
18.40 ms	1.20 ms	42.70 ms	62.30 ms

Inference backend: live

CLINICAL DISCLAIMER: This report is generated by Q-Knee, a research-prototype quantum-assisted decision-support tool. It is NOT a validated diagnostic device and has NOT been reviewed or cleared by any regulatory authority. Findings are probabilistic risk estimates only and must not be used, in isolation or otherwise, as the basis for diagnosis or treatment. All results require independent interpretation and confirmation by a qualified, licensed radiologist or orthopedic clinician.

Digitally signed (placeholder, non-cryptographic) by Q-Knee Automated Analysis System — generated 2026-08-30 11:03:04 — signature ref: FF14F62DAA6EA139