HERMON LABORATORIES

CALIBRATION
839.03

CERTIFICATE

CALIBRATION CERTIFICATE № *181541-1*

Calibrated Item:	Professional High Frequency and RF Meter, 10 MHz to 8 GHz, 20 V/m
Manufacturer:	LATNEX
Type (Model):	HF-B8G
Serial number:	230500026
HL number:	None
Customer:	Galit, Raanana, Israel
Received status:	Poor isotropy
Returned status:	Calibrated. Poor isotropy. Tamper-resistance seal is not required
Calibration interval agreed with customer:	24 months

Date of calibration:	30-Aug-2026
Calibration location:	Hermon Laboratories, Binyamina, Israel
Calibration environment:	24°C; 34% RH; 1005 hPa
Calibration procedure reference:	Prb_RF-E_CP-8
Calibration remarks:	PH alignment (probe shaft is positioned perpendicular to the applied E-field vector and perpendicular to the propagation direction), See Annex 1.
Measurement uncertainty reference:	Prb_RF-E_CP-8

Calibrated by A. Beliavskii, Test Engineer **Approved by** G. Shleimovich, Quality manager

The measurement uncertainty was derived from ISO “Guide to the expression of uncertainty of measurement” with a coverage factor k = 1.96 which yields probability of 95 %.

All measurement instrumentation is traceable to the National and International Standards. Supporting documentation relative to traceability is on the laboratory file and is available for examination upon request.

The standards and instruments used in the calibration system conform to the present requirement of ISO/ IEC 17025-2017 and ANSI/NCSL Z540-1-1994.

Hermon Laboratories Ltd.
Hatachana St., POB 23, Binyamina 30500 Israel
Phone: +972 4 628 8001, **Fax:** +972 4 628 8277
Email: mail@hermonlabs.com, www.hermonlabs.com

This certificate shall not be reproduced except in full, without written approval of Hermon Laboratories

CALIBRATION DATA

Frequency response and linearity

Frequency, MHz	Applied field, V/m	Measured field, V/m	Deviation, dB	Correction factor [1)]	Measurement uncertainty, dB
1800	6.01	7.27	1.66	0.83	±1.4
1800	3.00	2.44	-1.80	1.23	±1.4
1800	15.02	14.91	-0.06	1.01	±1.4
2800	6.00	14.66	7.75	0.41	±1.4

[1)] Multiply the monitor reading by correction factor.


This certificate shall not be reproduced except in full, without written approval of Hermon Laboratories

Isotropy check

Frequency, MHz	Applied field, V/m	Measured correction factor	Measured anisotropy, dB [1)]	Measurement uncertainty, dB
1800	6.01	0.914 (max) / 0.454 (min)	3.04	±1.40

[1)] Calculated as:
$20\times\mathrm{Log}_{10}(CF_{max}/(CF_{min}\times CF_{max})^{0.5})$ for linear units (V/m, A/m);
$10\times\mathrm{Log}_{10}(CF_{max}/(CF_{min}\times CF_{max})^{0.5})$ for power units (mW/cm², W/m²);
where CF_{max} and CF_{min} are maximum and minimum measured correction factor.

Isotropy pattern (measured field deviation, dB)

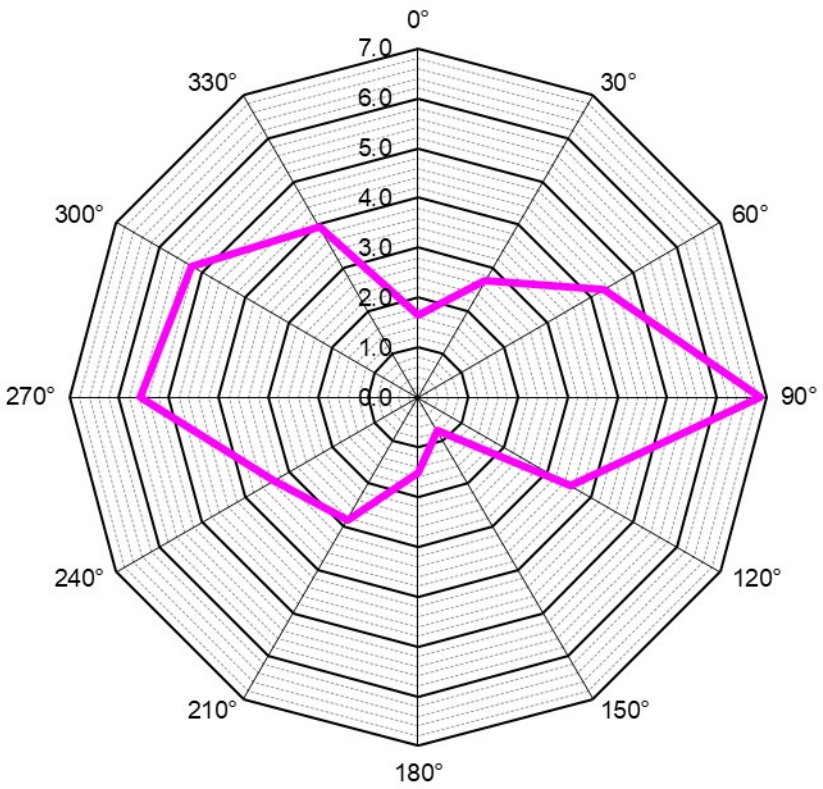


LIST OF EQUIPMENT USED IN CALIBRATION

HL No	Description	Manufacturer	Model	Ser. No	Due cal
2667	Signal generator, 9 kHz - 3.3 GHz	Rohde & Schwarz	SML03	101909	17-Nov-26
4874	Generator SGMA RF Source, 1.0 MHz up to 12.75 GHz	Rohde & Schwarz	SGS-100A	101377	12-Sep-26
4343	Signal Generator, 100 kHz to 40 GHz	Rohde & Schwarz	SMB 100A	175291	01-Jun-28
4884	Average Power Sensor, 9 kHz - 6 GHz, -67 to 23 dBm	Rohde & Schwarz	NRP-Z91	100005	17-Jun-27
3619	Laser distance meter	Leica	DISTO D3	180752021	06-Mar-27
5566	Universal Power Sensor, 10 MHz - 18 GHz, -67 to 23 dBm	Rohde & Schwarz	NRP-Z21	104400	01-Dec-27
4095	BI-Directional Coaxial Coupler, 50 - 1000 MHz, 500W	Narda	3020A	43286	05-Aug-28
5997	Coupler coaxial bi-directional 1 - 4 GHz, 20 dB	Narda	3022	60129	09-Sep-26
4021	Power Amplifier 1 to 2.5 GHz, 25 W and 1.8 to 4 GHz, 10 W	Hermon Laboratories	A 0.7-4	0001	04-Jun-27
659	Amplifier 1 to 4 GHz, 55 W	Milmega	AS0104-55/55B	971386	04-Dec-26
7821	Single-band Power Amplifier, 380 MHz to 6 GHz, 180W	Rohde & Schwarz	BBA300-CDE180	101338	14-Jan-27
4220	Standard gain horn antenna, 1.7 to 2.6 GHz	A-INFOMW	JXTXLB-430-10	J20211010 22008	20-Nov-26
5713	Standard Gain Horn Antenna 2.6-3.95 GHz ,WR 284, 10 dB	A-INFO(HK) Limited	LB-284-10-C-NF	J20206686 6	17-Nov-26
5033	Anechoic chamber, 6.5×3.5×3m	RDT Equipment & Systems	SM101	NA	04-Mar-28
2212	Tape-measure, 10 m / 33 in	The Stanley works Israel Ltd	33-443	2212	01-Jul-28

ANNEX 1

Probe alignment at calibration
(PH alignment according to IEEE Std 1309)

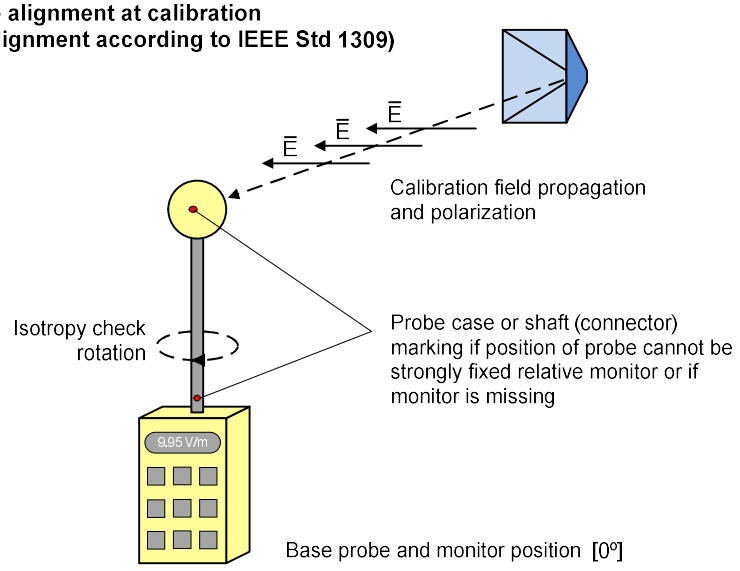

END OF DOCUMENT

This certificate shall not be reproduced except in full, without written approval of Hermon Laboratories