



(a) five arms: only the split position and the decoder width change

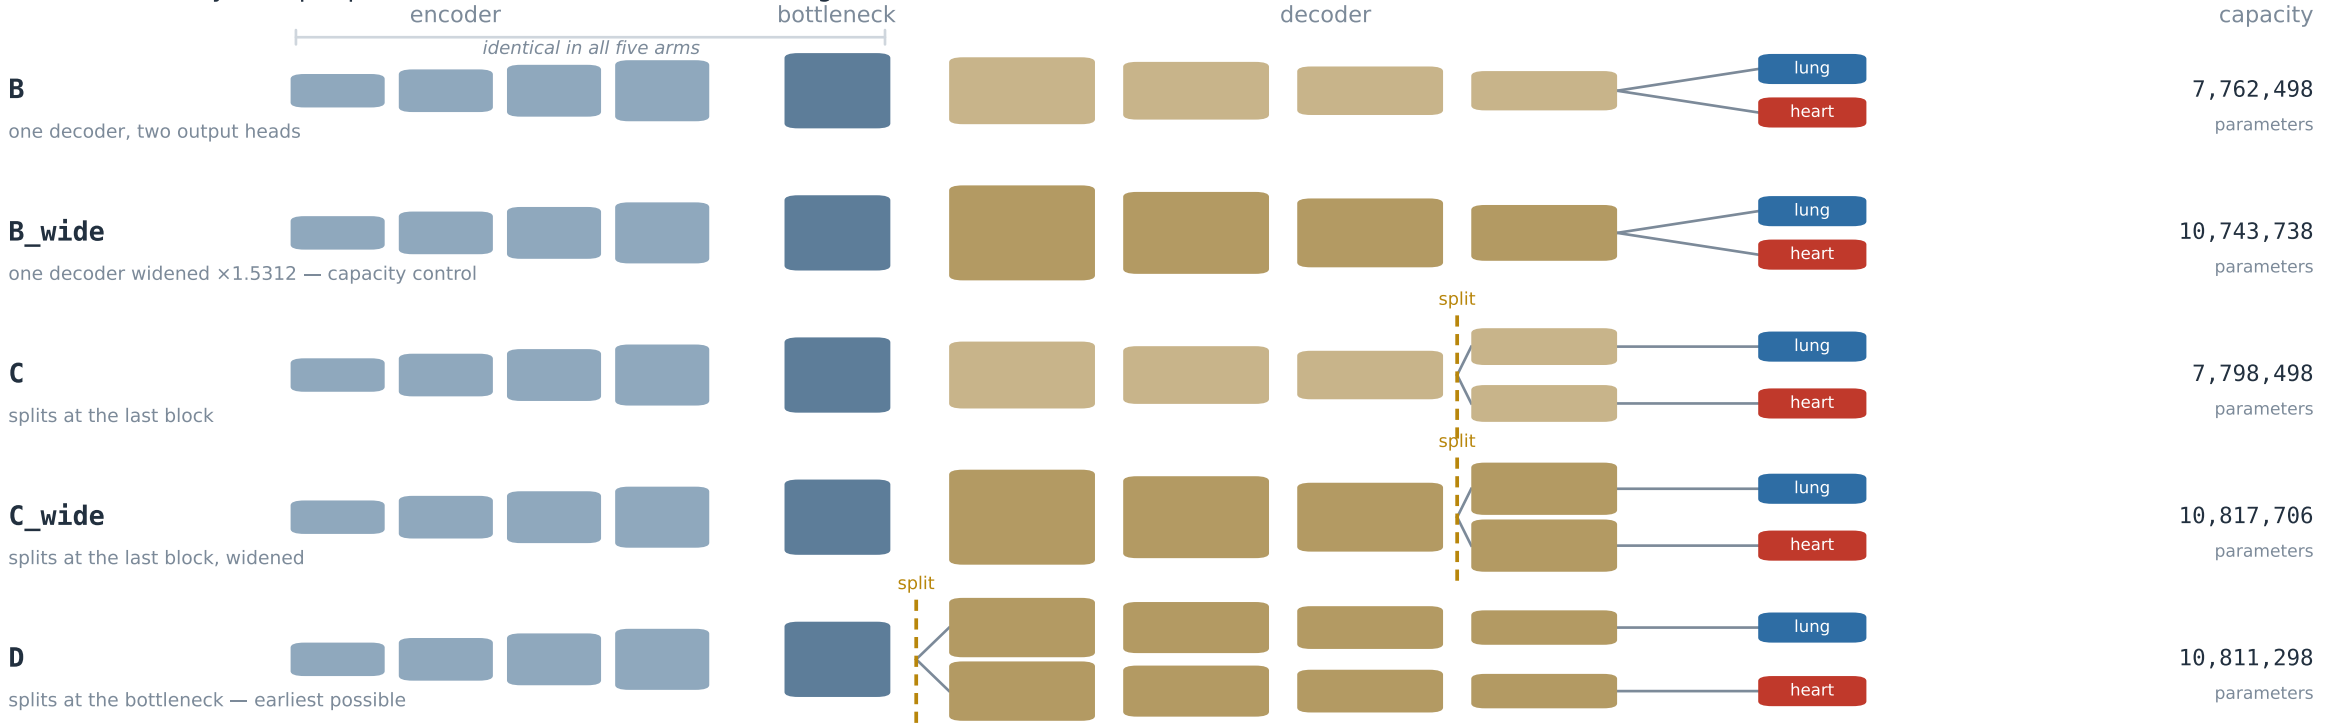

Held constant: encoder, block structure, L1 loss with 1.0/1.0 weights, Adam 1e-3 cosine to 1e-5, batch 16, ≤ 200 epochs with early stopping, no augmentation, one dataset-wide normalisation, the same 58 seeds on the same data. Primary contrast D - B_{wide}: +0.63% parameters, identical supervision.

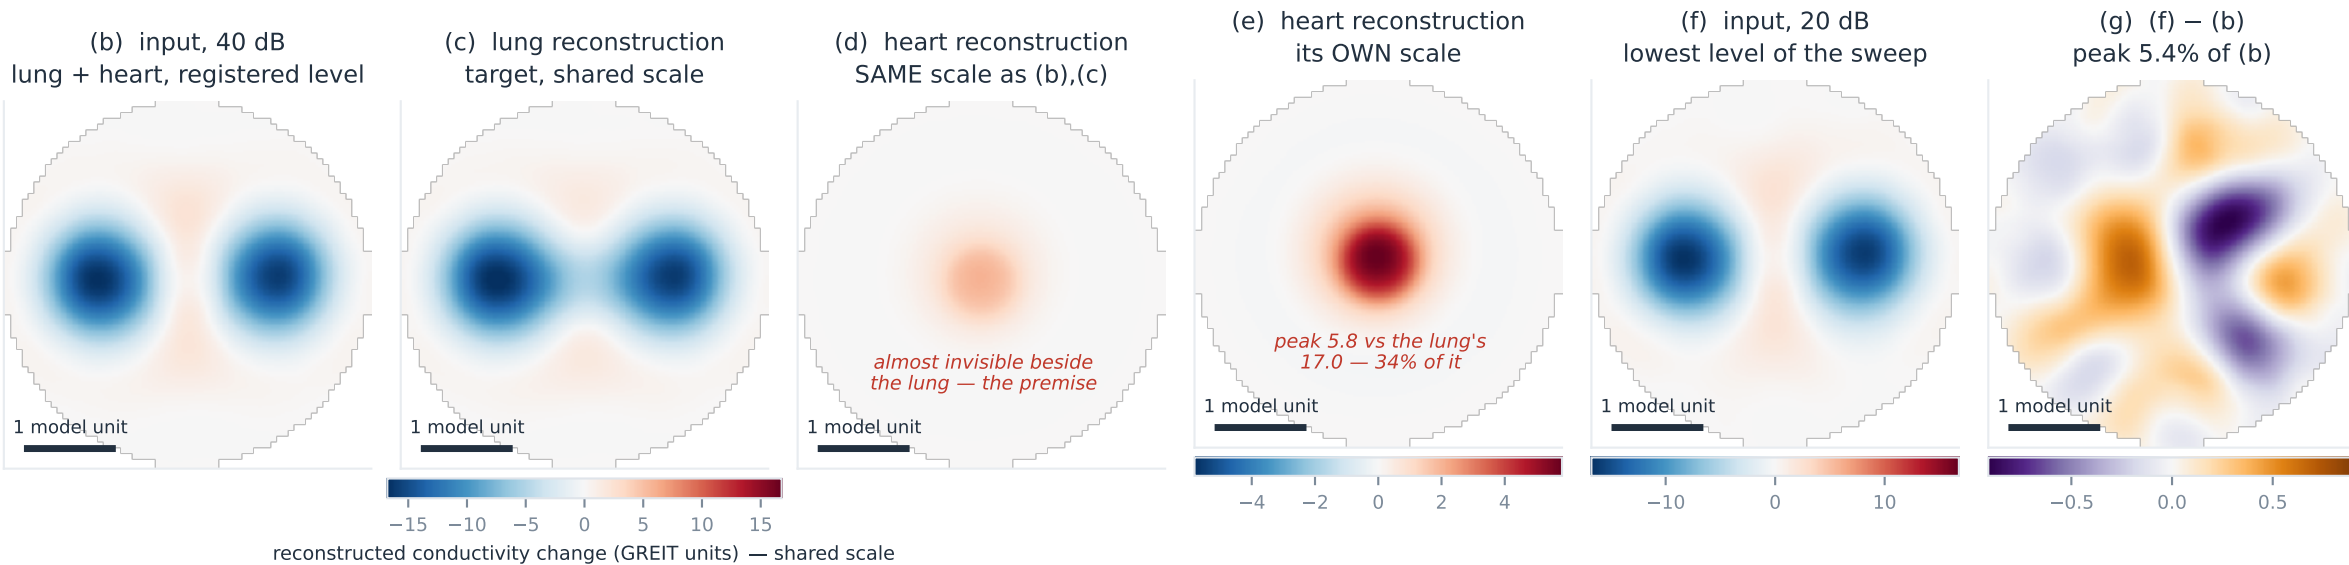

(b)–(g): one test-split geometry (index 1945), the median heart radius of the test split; every panel is an EIDORS GREIT reconstruction (three forward and three inverse solves per sample: mixed, lung only, heart only).

(d) and (e) are the SAME reconstruction on two scales; that gap is what the decoder branch is meant to address, and heart DSC is the registered primary endpoint

(g) GREIT is a regularised inverse and suppresses measurement noise before image space: 40→20 dB changes this input by 5.4% of peak yet costs 8.8 heart-DSC points (arm B wide, 58 seeds). Scale bars are model units; 64 px = 4 units.