FOR MATERNITY ONLY




STORAGE *- PCA pumps are located in recovery (EXT 841831)*

SWITCHING ON *– Open the latch using the PCA key – (found on CD Keys). Press the ON button*

LOADING THE SYRINGE

- *Open pump door by gently depressing latch. Door opens towards you*
- *Gently open syringe clamp. Drive head automatically retracts.*
- *Place (primed) syringe vertically within body of pump, wings inserted into slot (ensure patient disconnected or line clamped)*
- *Close syringe clamp, securing syringe (also reads syringe diameter/volume)*
- *Close pump door. Press and hold **I** or touchscreen (engage drive head)*
- *Confirm correct syringe using **II** on the touch screen*

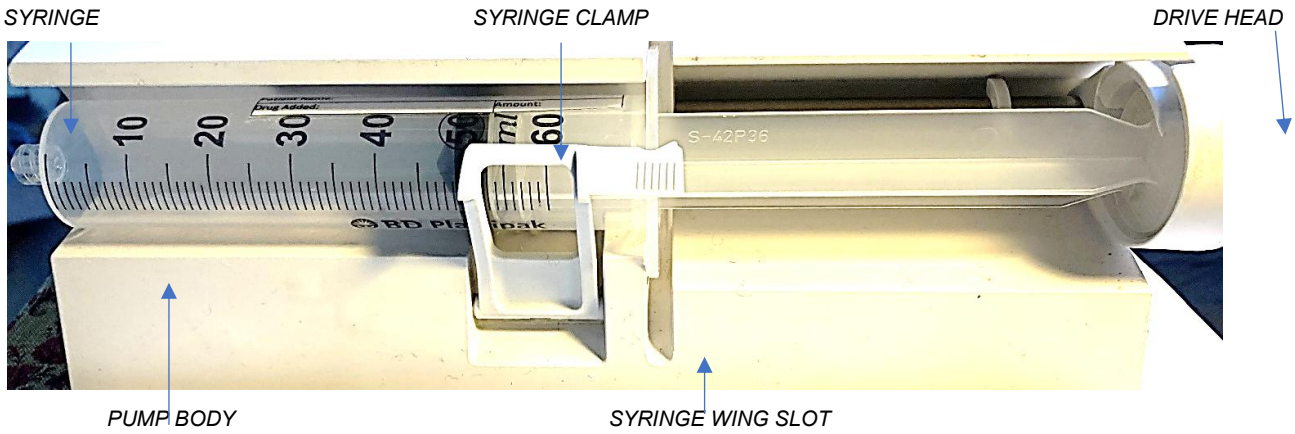

HARD KEYS

- ***RATE*** *window will only ever show ml/hr*
- ***DATA*** *window for entering passwords, variable rates, information requested on touchscreen*
- ***DATA*** *window will display cumulative dose (mls) administered when pump is running*

PATIENT HANDSET

- *Handset light is configured to flash during lockout period and continuous light when patient bolus is available*
- *The handset can be pressed upside down on a hard surface e.g., table-top*

PROGRAMMING

- *Password for Maternity folder* ***5511***
- *On the homepage, select appropriate Drug folder (press drug folder on touchscreen)*
- *Choose drug e.g., Morphine, Fentanyl or Remifentanil*
- *Remifentanil PCA are set up by Anaesthetists only*
- *Enter Drug Password* ***1115*** *when prompted into* ***DATA*** *window and confirm.*

REMIFENTANIL ONLY – Changing the patient weight



- *Enter the patient weight using the up/down keys in the DATA window*

MORPHINE, FENTANYL & REMIFENTANiL

- *Confirm bolus dose using* ***II*** *or the touch screen*
- *Confirm lockout time using* ***II*** *or the touch screen*

- *Press **START** to commence infusion*
- *PCA is infusing when the green syringe illuminated in small LED screen, red dots running across RATE and DATA windows and Green Syringe on touchscreen*
- *If **RATE NOT SET** page is displayed during programming, press **Menu** and press **PCA** mode to return to Homepage (this occurs if time limit is breached during programming, or programming is interrupted)*

***CLINICIAN BOLUS**: Only available with Morphine and Fentanyl PCAs*

- *The **Bolus** option is displayed on the shortcut menu when drug is infusing*
- *Press **Bolus***
- *Enter **Pain Team (5363)** Password in **DATA** Window and confirm*
- *Confirm default bolus or amend bolus dose in **DATA** Window*
- *Press **II** (hard key) pump auto-delivers bolus*
- *Patient lockout period starts again*
- *If a patient or clinician bolus is interrupted (e.g., occlusion). when restarted, the screen will offer the option of completing the interrupted dose.*
- *IF COMPLETION IS SELECTED THE PUMP RECORDS THIS AS A CLINICIAN BOLUS AS PATIENT HAS NOT PRESSED THE BUTTON.*
- *Refer to cumulative totals for total amount received.*

BOLUS HISTORY

- *Press Green Syringe on the Touch screen*
- *1st page displays total boluses administered/refused since infusion commenced. Press **II** for 2nd page to display hourly breakdown of demands.*
- *Also access the INFO Screen **(status/help)** for the event log/history. Available in shortcut and menu. Records/retains previous 500 events.*
- *Displays remaining volume in syringe, duration of current protocol, lockout time remaining, battery life.*

***PCA MODE** – to alter programmed drug settings*

- *Press **STOP.** Press **MENU***
- *Press **PCA MODE***
- *Enter Drug Password **1115** in **DATA** window and confirm, follow instructions*

PRESSURE READING

- *Press **MENU***
- *Press **OCCLUSION LIMIT***
- *Line pressure: defaulted at 600mm/Hg maximum 1000mm/Hg*
- *Can be raised/lowered according to clinical need, will default back to 600mm/Hg when drug changed/pump turned off*

NEW THERAPY *- Enables change of drug without turning pump off/on*

- *Press **STOP***
- *Press **MENU***
- *Press **NEW THERAPY***
- *Enter Drug Password **1115** in **DATA** Window and confirm.*
- *Confirm New Therapy by pressing **II** (hard key only). Previous settings/history will be cleared*
- *Choose Folder, programme new infusion*

CHANGING BOLUS DOSE, LOCKOUT TIME OR BACKGROUND

- *Choose **PAIN TEAM ONLY** folder. Accessible to Anaesthetist and Acute Pain Team only*

ALERTS & ALARMS

- ***ALERT**: p  usually still infusing and is advisory e.g., Soft Limit reached*
- ***ALARM**: immediate attention is required, and the pump has stopped infusing (e.g., occlusion, door open, syringe empty)*
- *To silence auditory alarm press touchscreen or **II***
- ***CONSTANT ALARM**; may indicate internal fault: remove pump from power, press and hold ON/OFF button until silences, send to EBME for assessment.*

STANDBY MODE

- *To access **STANDBY** briefly press the **ON/OFF** key once*
- *Enter password **1115***
- *Standby will be displayed on touch screen*
- *The pump will not alarm*
- *The pump will retain the settings entered*
- *To cancel standby, press touchscreen*

TURNING PUMP OFF

- *Press **ON/OFF** button – enter **1115** password – hold **ON/OFF** button for 3 seconds, pump will power down, all history/programming will be cleared, pump is now zeroed and ready for next patient*

ALL PCA PATIENTS REQUIRE:

- *Oxygen via a nasal canula*
- *A continuous 5mls/hr infusion of 0.9% NaCl or Hartmann's solution*
- *A dedicated venflon*

DOCUMENTATION

- *Ensure the PCA, oxygen and fluids are prescribed via ePMA*
- *PCA observations should be documented on the relevant paperwork*