Ysbyty Gwynedd
Anaesthetics Department
Adran Anaestheteg

PAEDIATRICS

Ventilation of Children <20kg on Dewi Ward HDU: T1 Hamilton Set Up

Author(s): Dr Stephan Clements
Reviewer: Departmental Guideline Group

YG CG 807

FIRST APPROVED: DEC 2022 REVIEW BY: DEC 2025

Key Points

There are 2 set-ups for the Hamilton T1 ventilator. These are weight banded:

- Adult/Paed setup ≥20kgs = Coaxial breathing circuit
- Neo/Paed Setup <20kgs = Dual limb circuit

Each requires a slightly different arrangement for checking of the flow sensor & adaptor.

This guide provides information to set up the T1 with the Dual Limb circuit.

N.B. For <5kg patients, the Drager Atlan A350 flow sensor may not be sufficiently sensitive to deliver small tidal volumes, if the corrugated circuit is used, so cannot be relied upon.

Equipment

'Neonatal' circuit packs are located in the Hamilton Ventilator Bucket +/- bottom drawer of the Anaesthetic Machine.





Door Code: C12345

If they are missing, there are plenty in the main stores on Minfford ward (Door code C12345).

Connecting the Dual Limb Circuit Set





Inside the pack. Discard nCPAP



mini HME filters on each of the inspiratory & expiratory ports



Dual limb circuit attached (Blue sky above!)




Blue tube to Blue port
Clear tube to White



Flow sensor at patient

Keep the dumbbell shaped adaptor for the Preop flow sensor check (see below).

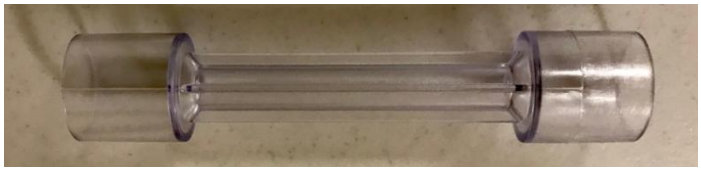

- For more info, here is a video:


https://www.youtube.com/watch?v=hVbD049umf8

PreOp Checks

Make sure the Neonatal patient group is selected at the top of the screen.


1. ***Tightness***: as per Adult set up.
2. ***Flow Sensor***:

Use the Dumbell shaped adaptor to perform this test:



3. ***O2 Sensor*** test: Only perform if not done within 1 month.

Trouble shooting if Preop Check Fails:

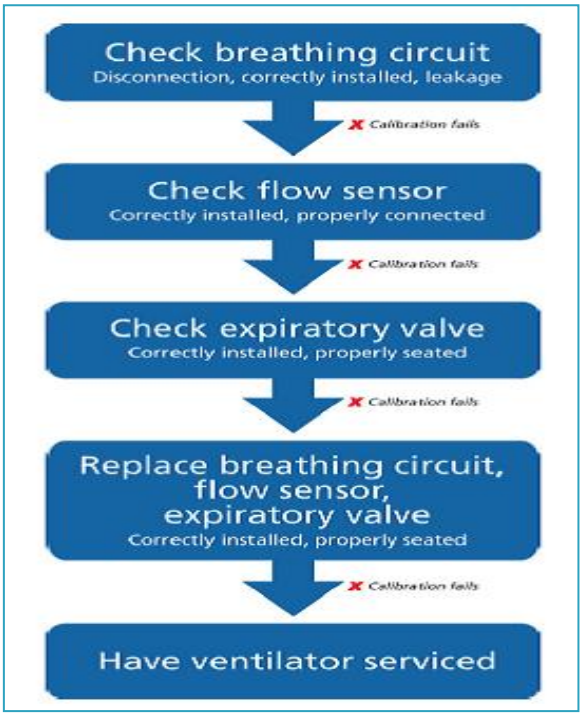

References

HAMILTON T1 QUICK MANUAL Pdf Download | ManualsLib