
BabyPAC 100 Ventilator
INSTRUCTIONS FOR USE

For neonates & infants up to 10kg in conjunction with end tidal capnography.

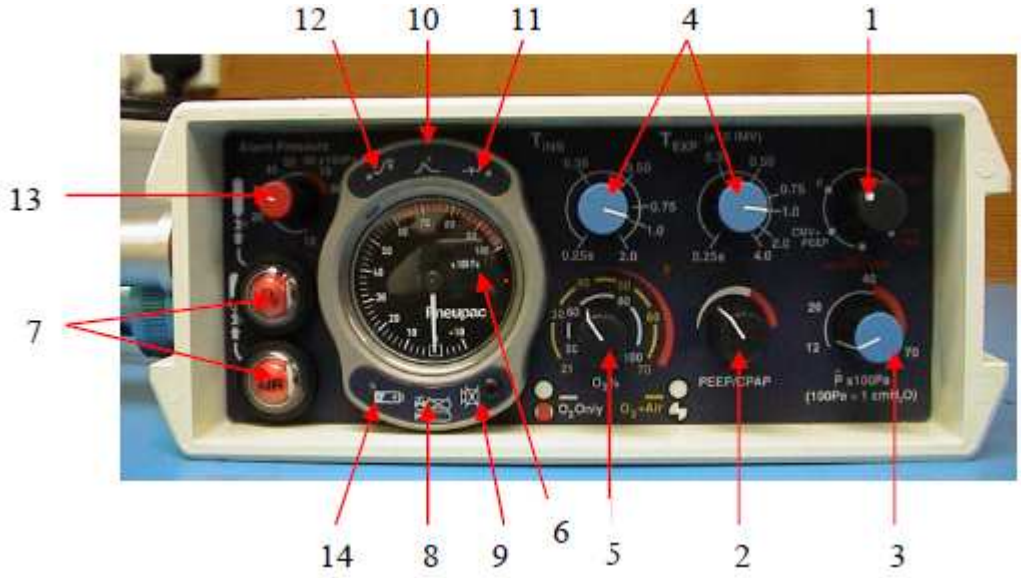

BEFORE ATTACHING TO PATIENT SET THE FOLLOWING:

- **Connect supply hose(s) to gas supply(ies)**
- **Check the visual alarms (7) have changed from red to white.**
- **Set the following:**

1. **Ventilator function (1):** Select CMV + Active PEEP
2. **PEEP/CPAP (2):** check it is at the low end of the scale. You will adjust this to the desired level once patient is attached using the pressure gauge (**6**).
3. **Inspiratory pressure (3):** check it is set to 12cm^{H2O} initially. You will adjust this to the desired level once patient is attached by looking at the chest expansion to estimate desired tidal volume.
4. **Respiratory Rate (4):** Adjust T_{INS} & T_{EXP} dials for the desired rate by referring to the printed table on the ventilator.
5. **Inspired Oxygen concentration (5):**
    - Oxygen only connected- Use the white markings (50-100%).
    - Oxygen & Air connected- Use the yellow markings (21-70%).
6. Ensure alarm pressure dial (**13**) is set to 30cm^{H2O}.

AFTER ATTACHING TO PATIENT:

- Adjust the inspiratory pressure (**3**) to the desired chest expansion (tidal volume).
- Adjust the PEEP to the desired level by observing the pressure dial (**6**).
- Check the green cycle indicator (**10**) flashes during each inflation.
- Temporarily disconnect the ventilator circuit at the connection closest to the patient to verify that the green cycle light (**10**) fails to illuminate during inspiration +/- disconnect alarm (**11**) sounds.

Additional functions:

8= single gas use indicator, **9**=alarm mute, **13**= Variable relief valve, **14**= Low battery alarm (The battery only powers the alarms)