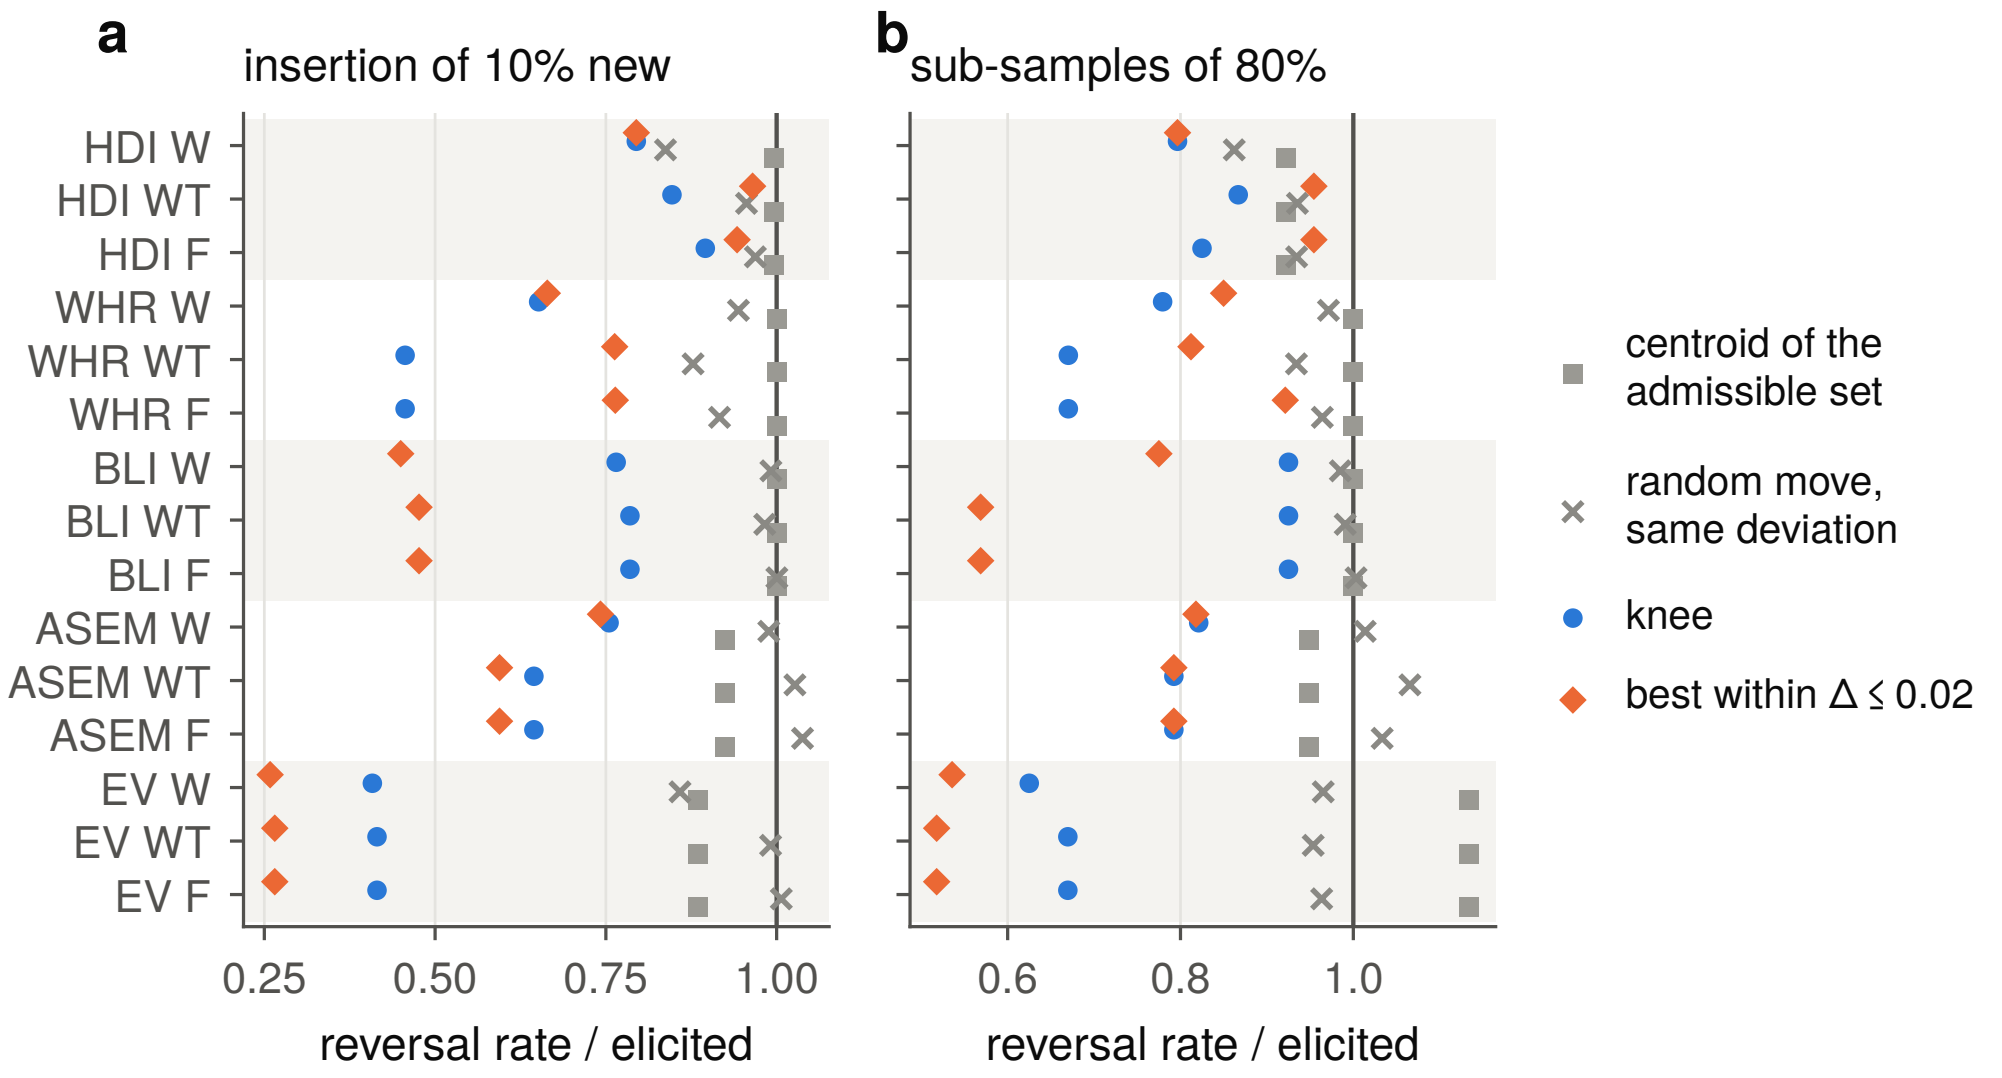
a
insertion of 10% new
b
sub-samples of 80%
HDI W
HDI WT
HDI F
WHR W
WHR WT
WHR F
BLI W
BLI WT
BLI F
ASEM W
ASEM WT
ASEM F
EV W
EV WT
EV F
0.25
0.50
0.75
1.00
0.6
0.8
1.0
reversal rate / elicited
reversal rate / elicited
centroid of the admissible set
random move, same deviation
knee
best within Δ ≤ 0.02