



I1 = -8.0000x10⁻¹
I2 = 1.1600x10⁰

FWHM
265ps

CH1
5x10²
COUNTS/DIV
V.EXPND
x 1
ACCUM NUM
x 1
SCAN
x 5000

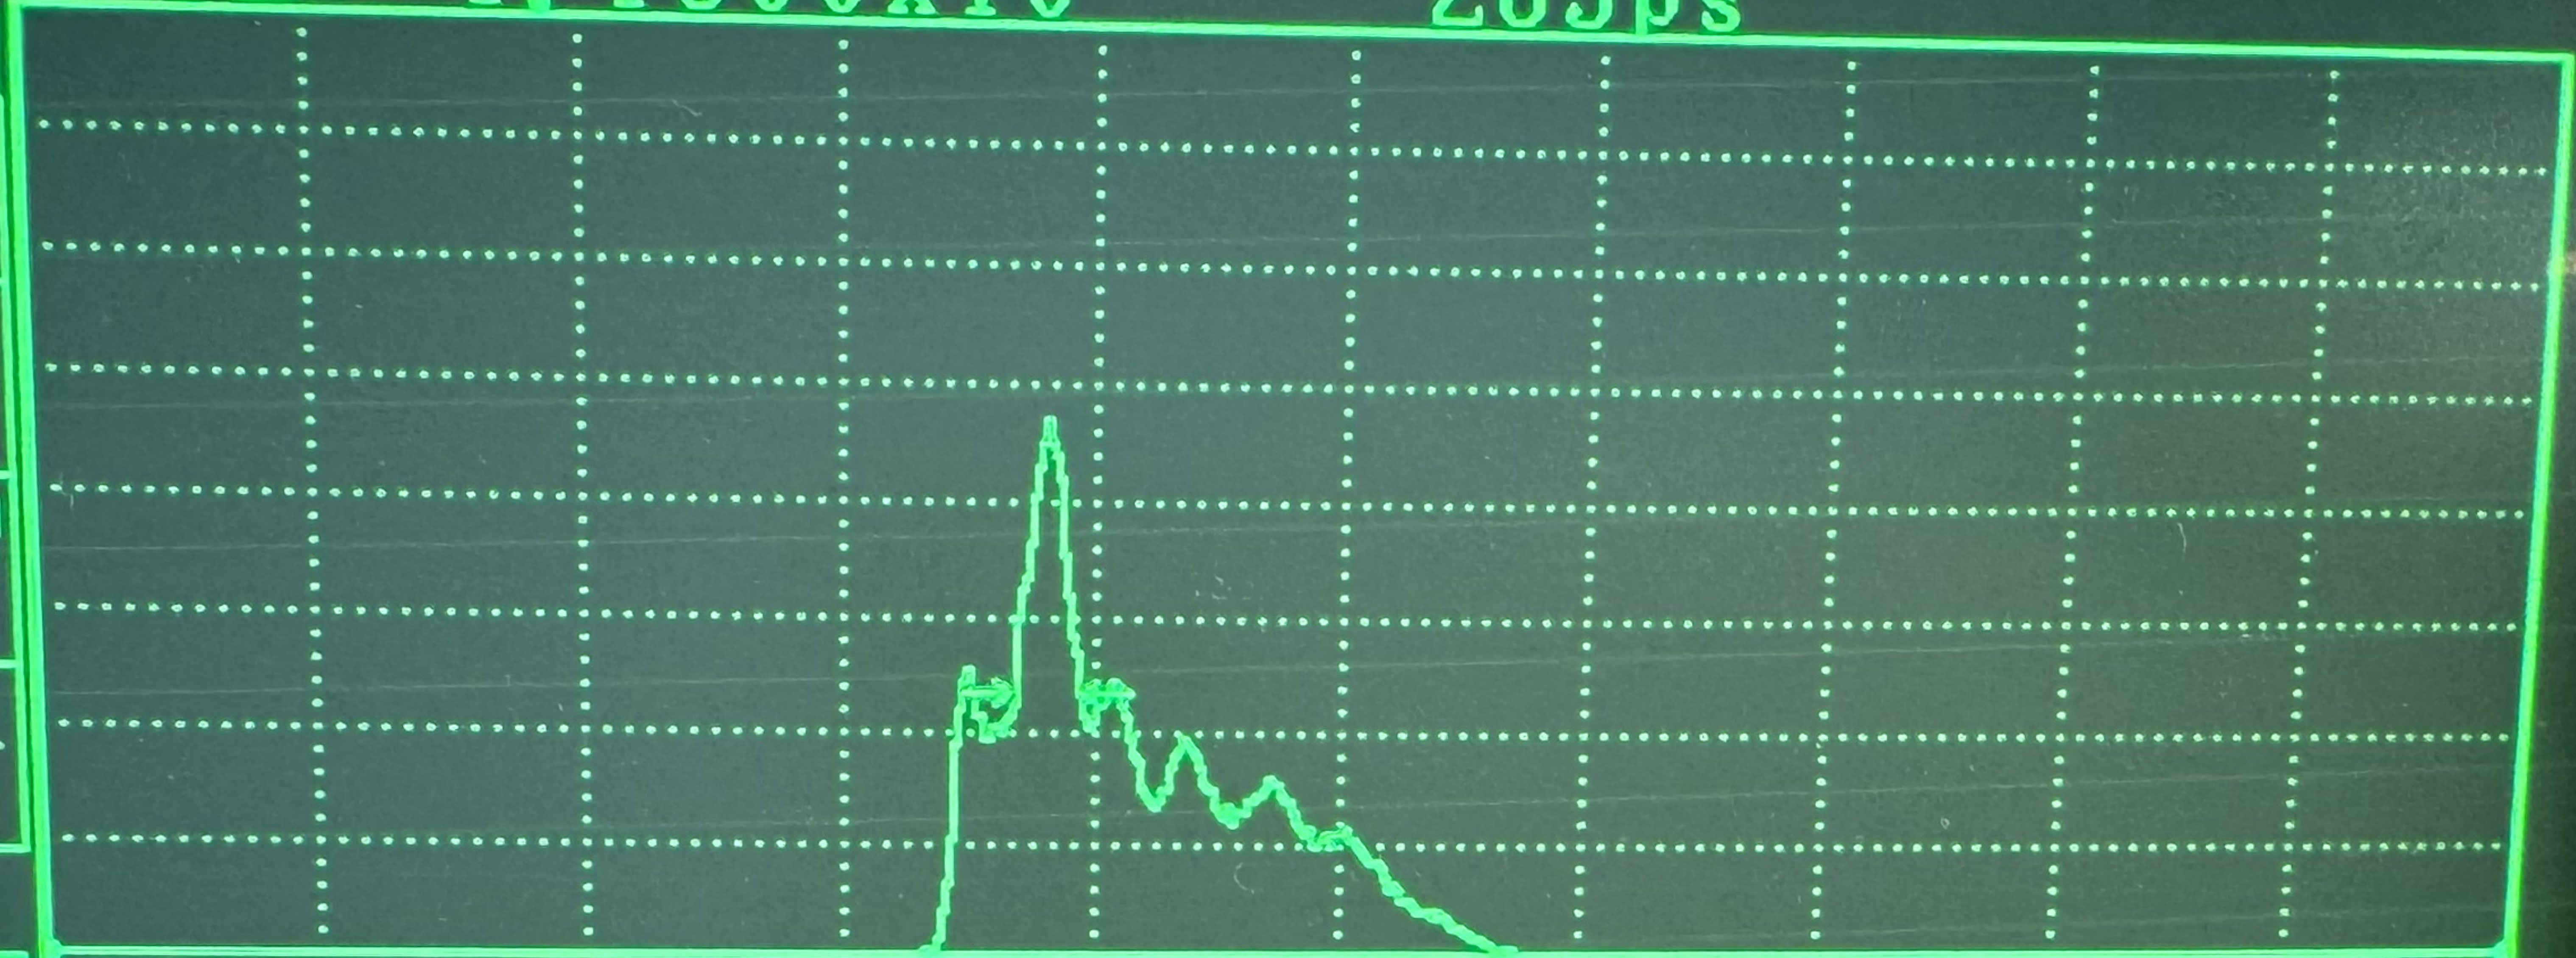

M4
2x10³
COUNTS/DIV
V.EXPND
x 1
ACCUM NUM
x 1
SCAN
x 5000

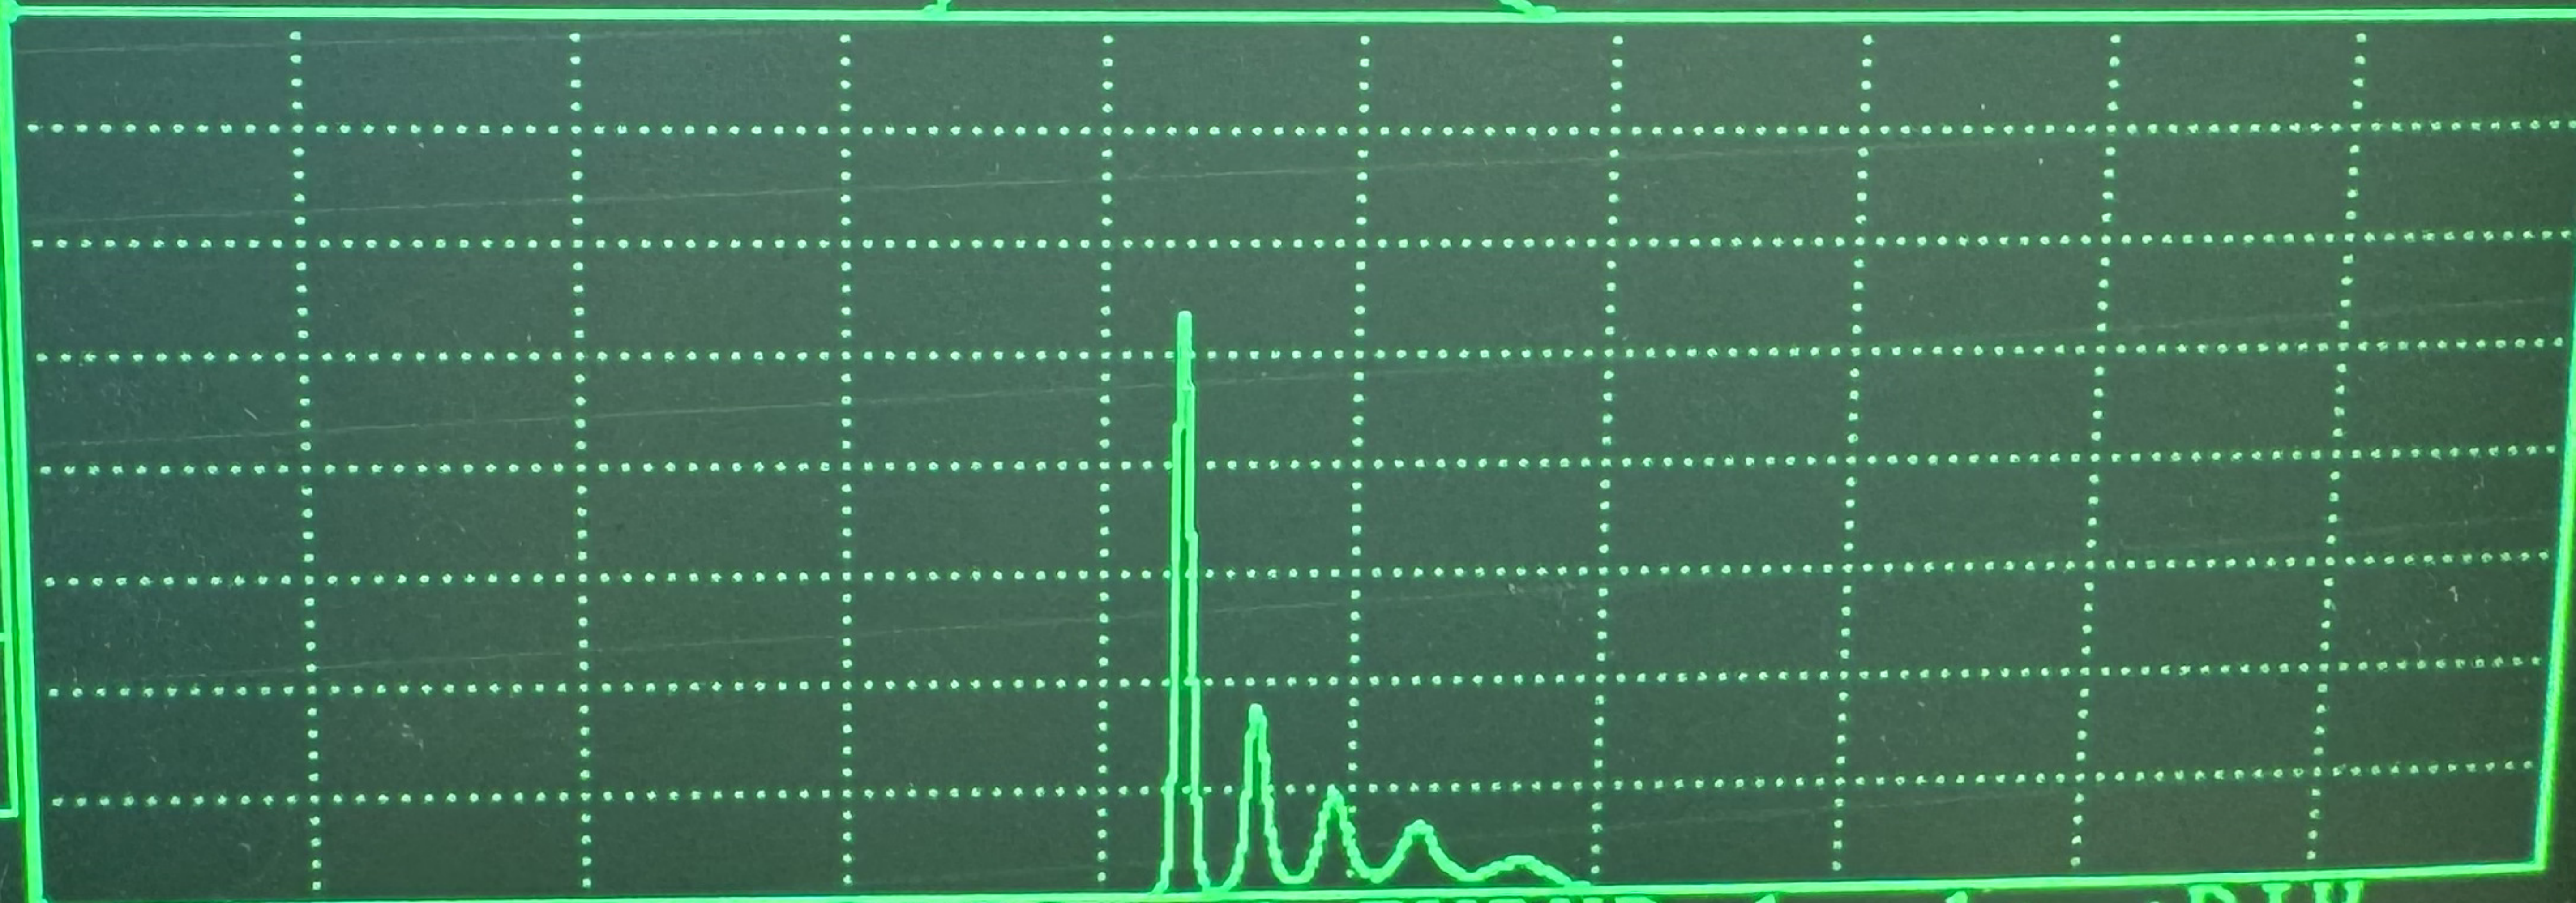

SAMPLE 4096 SCAN 5000 H. EXPND 1 1ns/DIV

DIRECTORY | SCALE : STORE : RECALL : FUNC