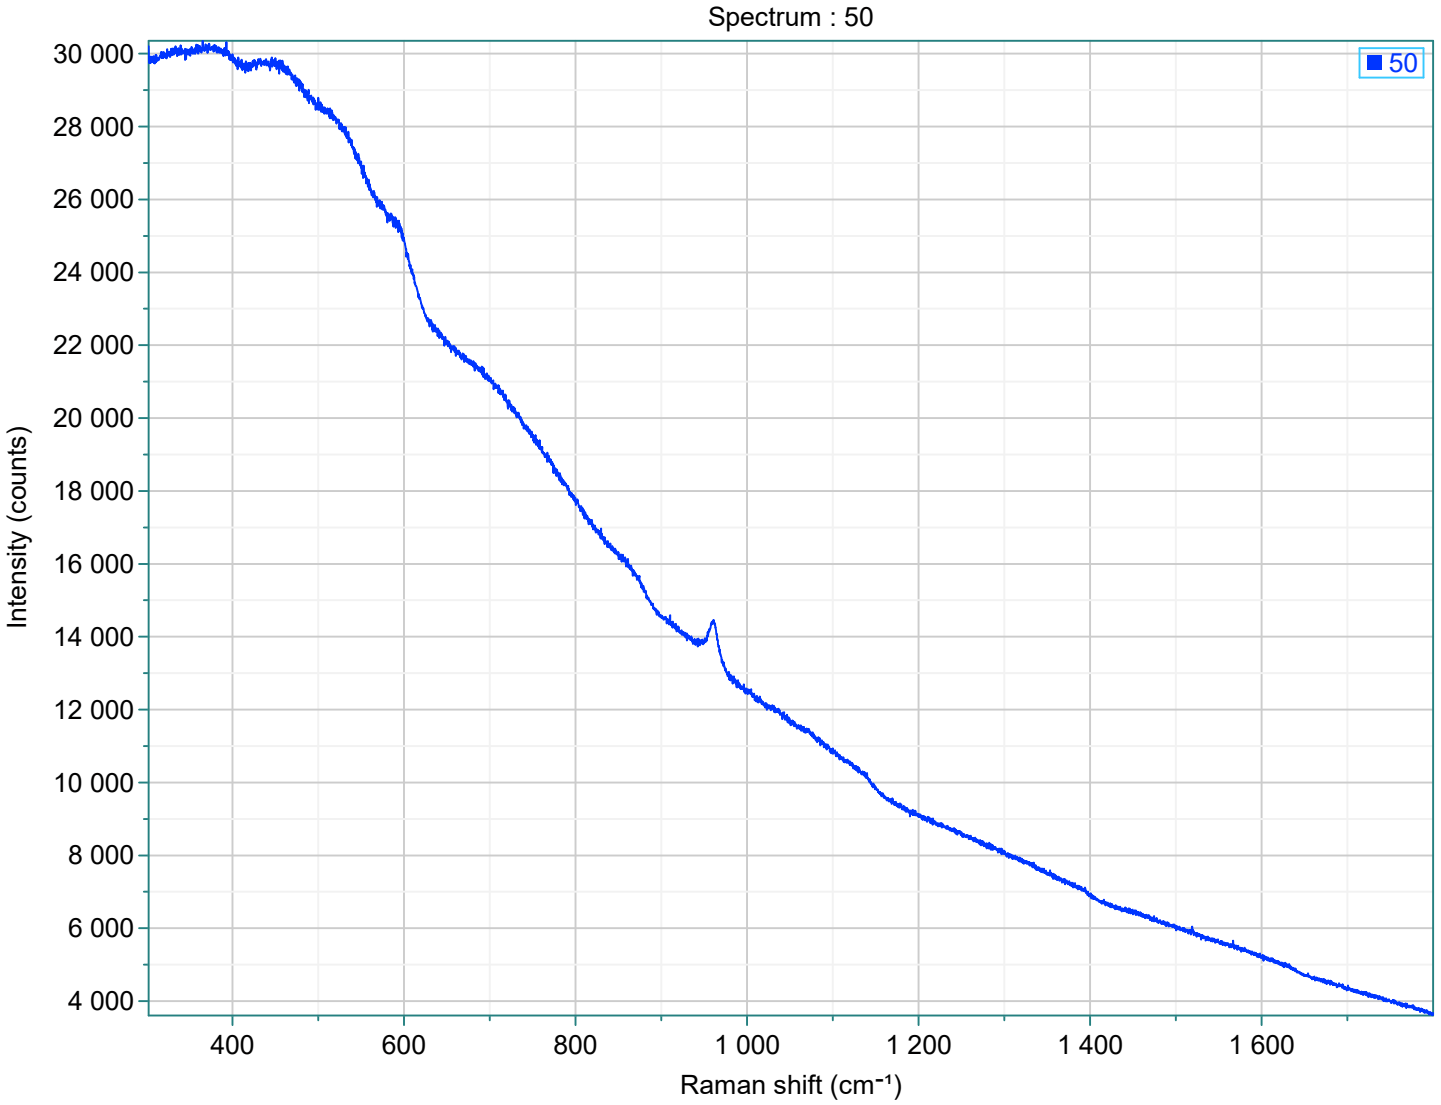


NOTES:

Date	11.04.2022 1...	Acq. time (s)	50	Accumulations	4	Laser	633nm_Edge
Spectro (nm)		Hole	150.001	Slit		Grating	1800 (450-85...
ND Filter	50%	Objective	x20_LWD	ICS correction	Off	Range (cm-¹)	

Powered by
LabSpec 6 from:

HORIBA Scientific