


Validation of Lidocaine HCL in Biovit Ampoule
Day 1
Standard A 01

Acquired by : mohdah
Sample Name : Standard A 01
Sample ID : Standard A 01
Tray# : 1
Vail# : 61
Injection Volume : 20 uL
Data Filename : Standard A 01.lcd
Method Filename : lidocaine assay in Biovit B12.lcm
Batch Filename : Repeatability.lcb
Report Filename : Default.lcr
Date Acquired : 2/26/2024 4:14:52 PM
Data Processed : 2/27/2024 9:10:14 AM

Chromatogram

Standard A 01 D:\...\HPLC 7\Data\Biovit amp\26-02-2024 Lidocaine\Standard A 01.lcd
mV

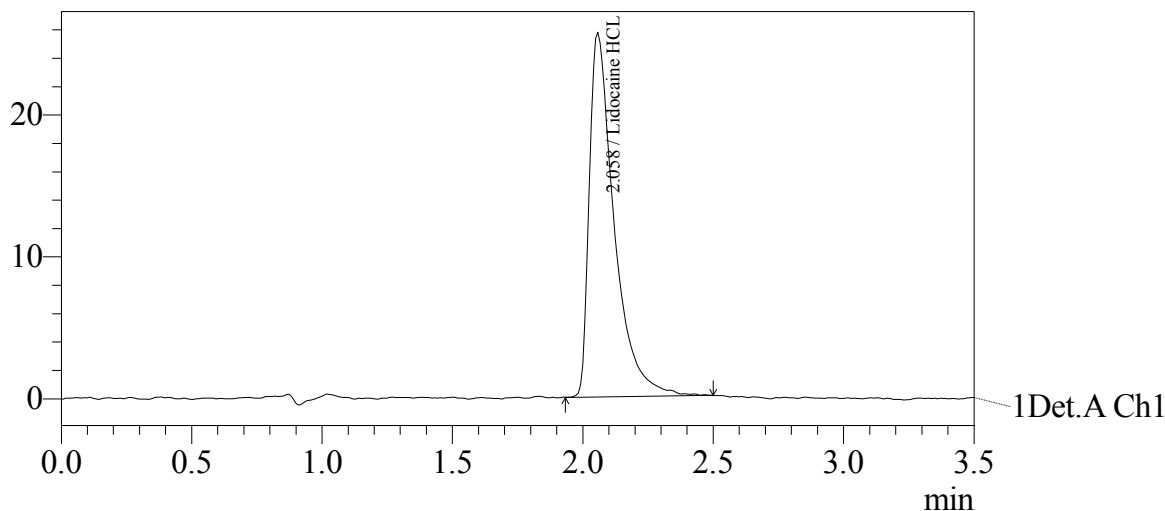

Quantitative Results D:\MS-Archive\HPLC 7\Data\Biovit amp\26-02-2024 Lidocaine\Standard A 01.lcd
Detector A

ID#	Name	Ret. Time	Area	Height	Conc.	Units
1	Lidocaine HCL	2.058	170515	24798	100.36	%