



Active Mesh Nebulizer

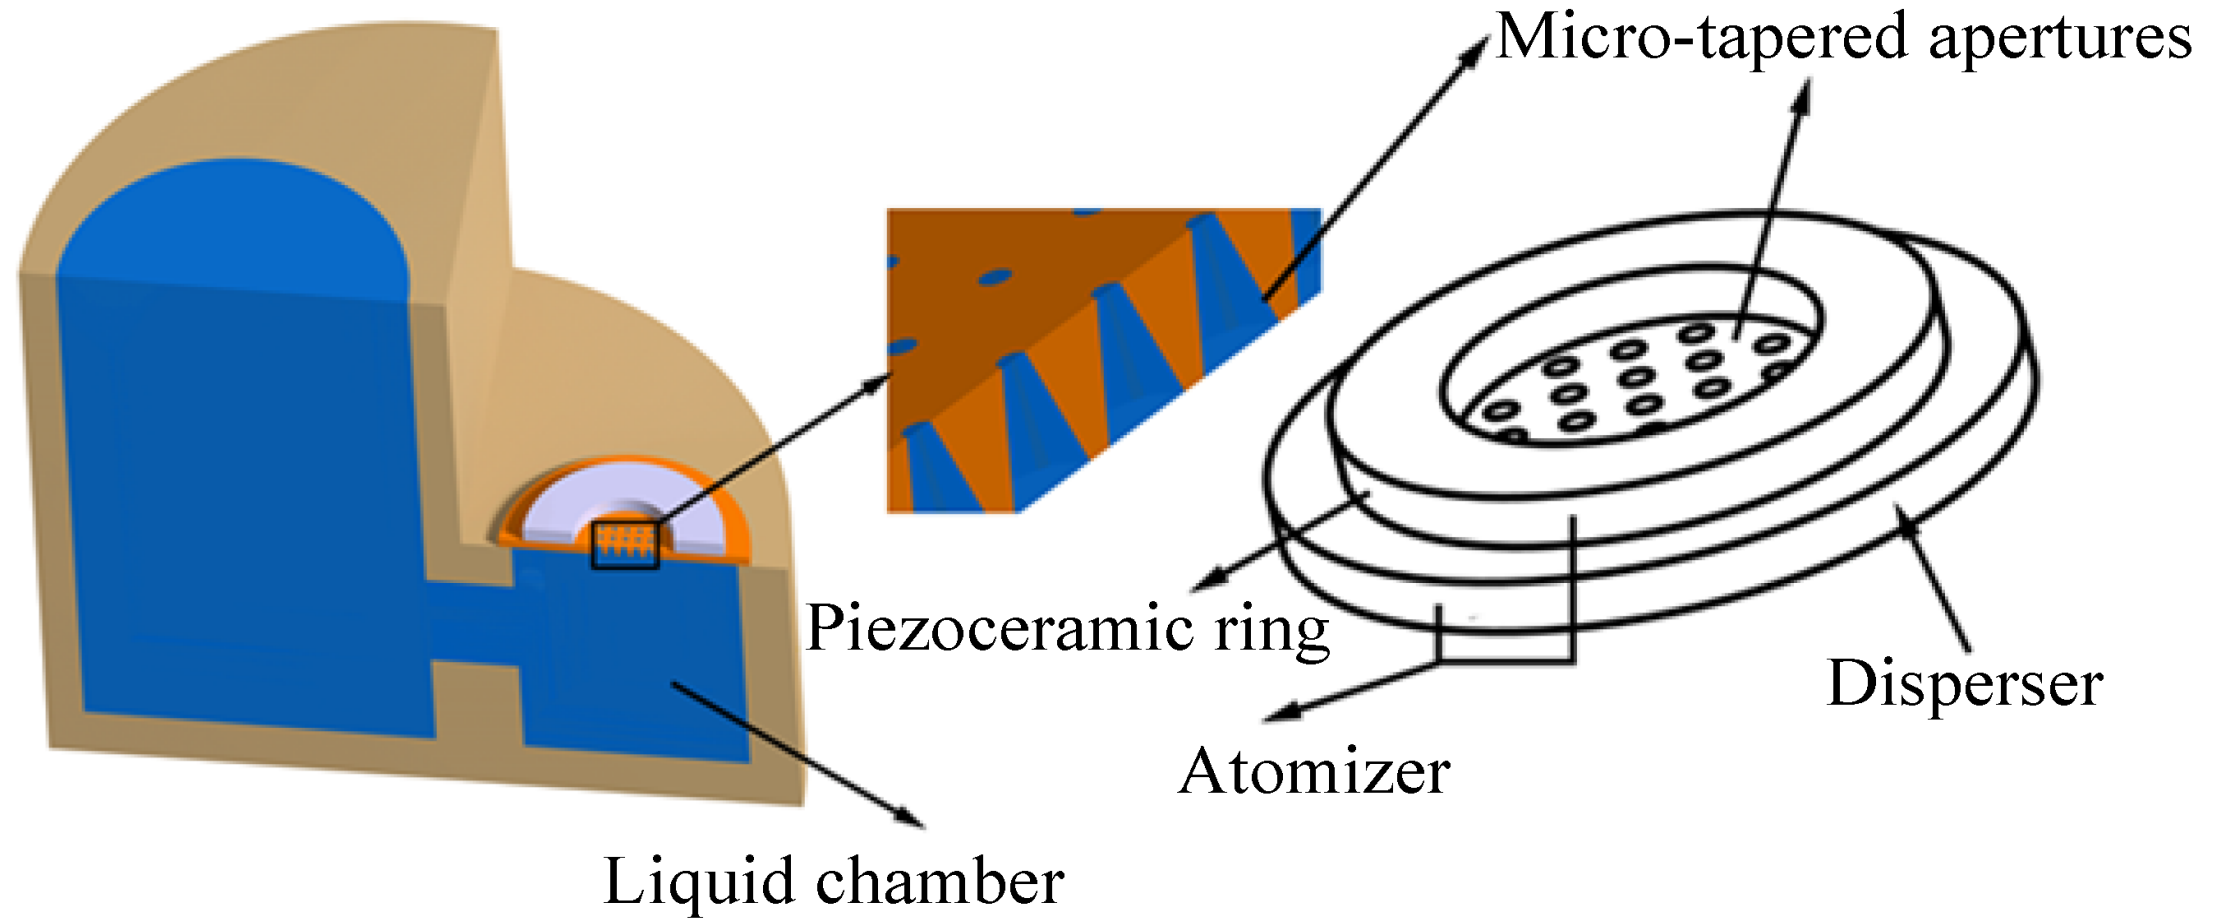

Driving Circuit

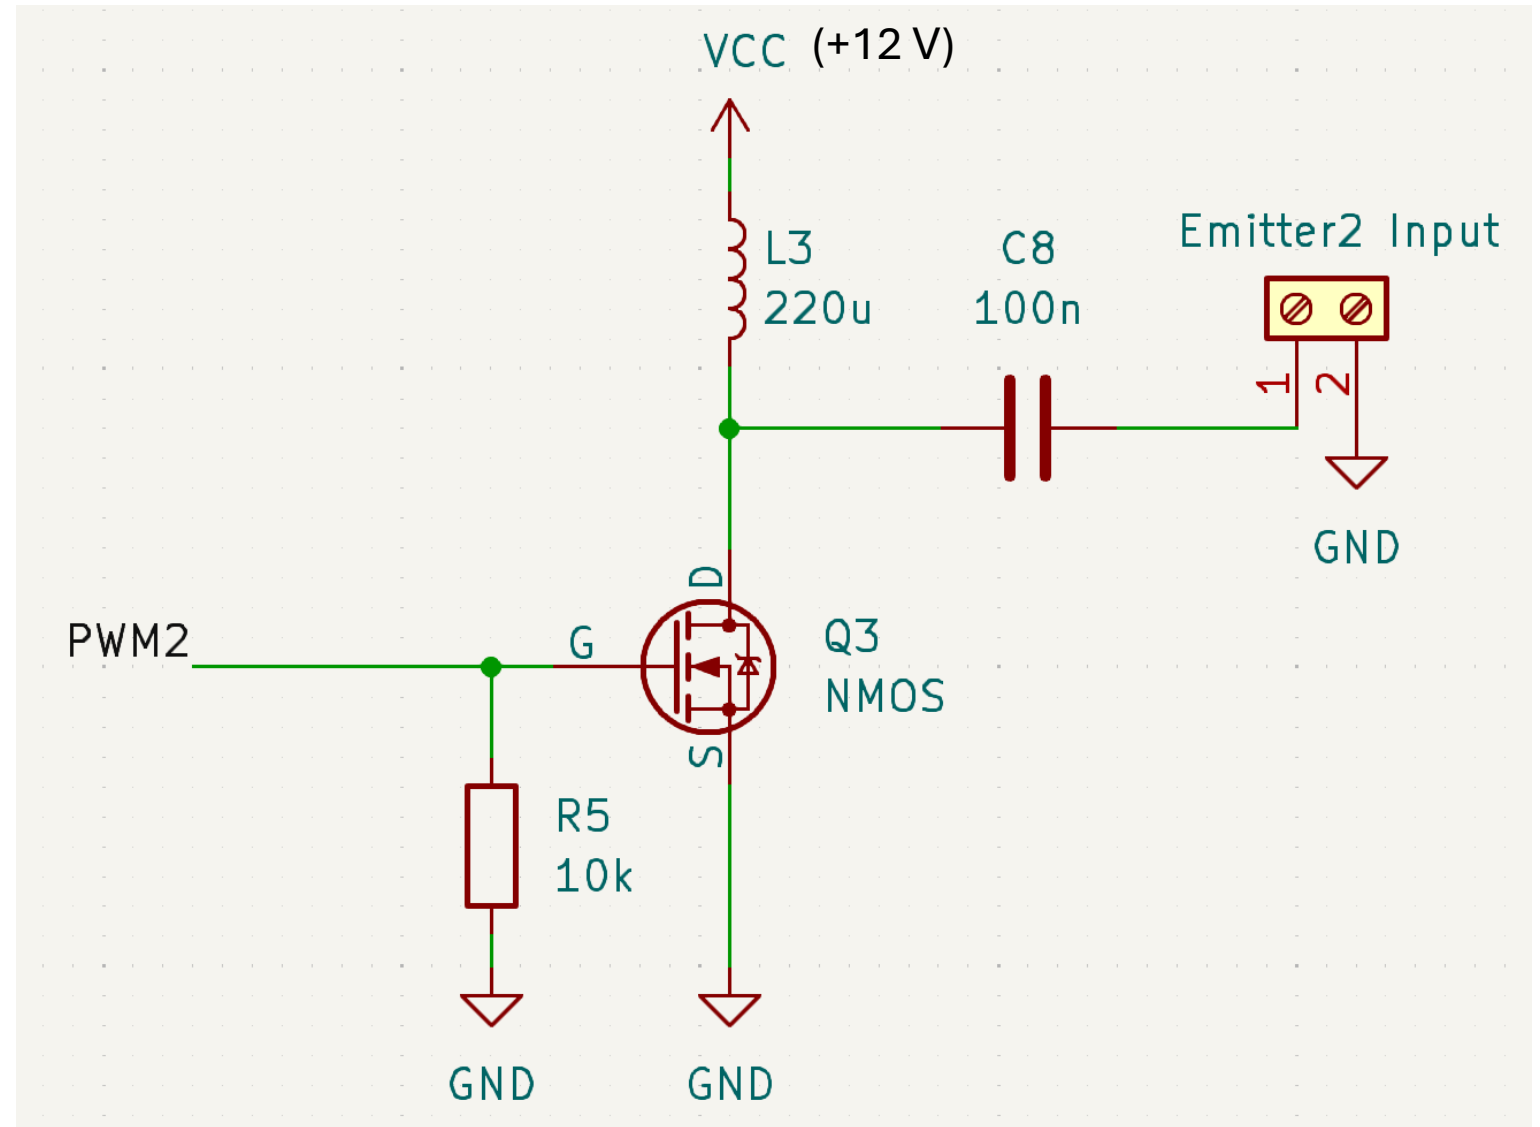

Things to Consider

- 1. Low rate of atomization (up to 0.025 ml/s or 25 μ l/s) for water.
- 2. Higher voltages may help achieve better atomization rates but risk damaging the transducer.
- 3. If the pressure of your liquid reservoir is too high, the liquid may leak through the mesh on its own.
- 4. Performance drops with more viscous liquids.
- 5. Liquids that crystalize on drying can clog the mesh. (e.g. tap water)