metamason™

The first and only 3D printed CPAP mask created to fit every individual uniquely and precisely.

811 W. 7th St. Suite 1146 Los Angeles, CA 90017
investor@metamason.com

Obstructive Sleep Apnea (OSA)

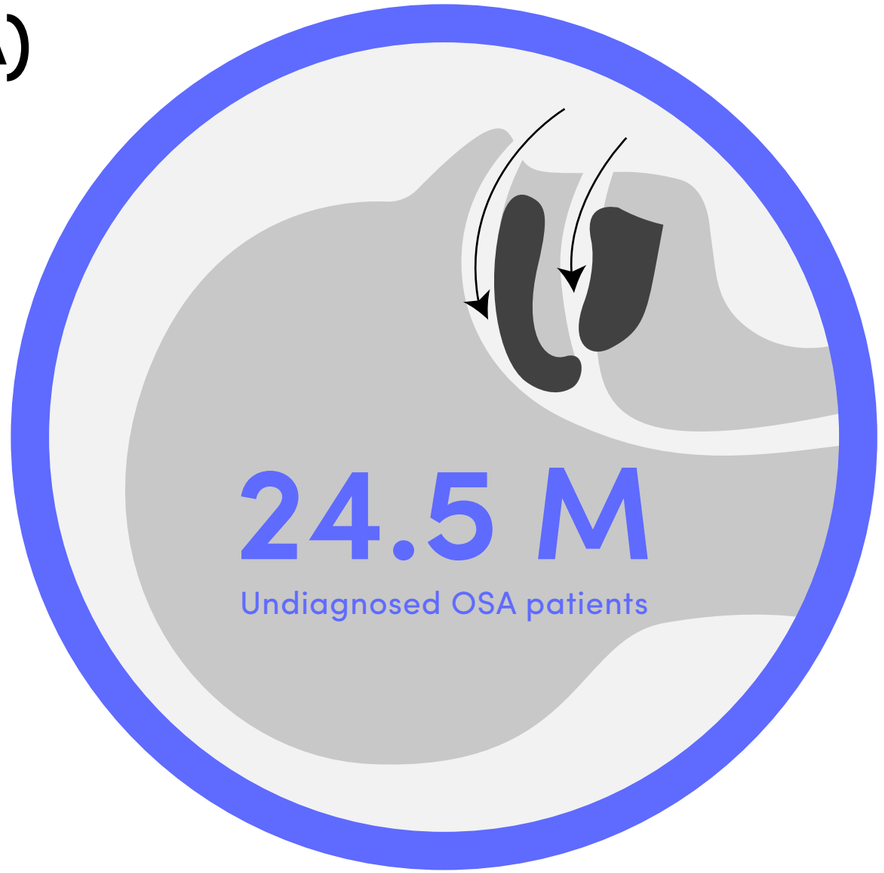

OSA is a disorder in which one's airway is obstructed during sleep, caused by the collapse of the airway walls and surrounding tissue.

12% of the U.S. adult population impacted by OSA

9% men

4% women

- In 2015, $12.4 billion was spent on the treatment of OSA
- Correlation to injuries, absenteeism, and lower productivity in the workplace
- OSA has the **same prevalence as each asthma and diabetes**

Prevalence of sleep apnea in other chronic illnesses:

Drug-Resistant Hypertension	83%
Obesity	77%
Congestive Heart Failure	76%
Diabetes	48%

80% remain undiagnosed

Source: Primary research with experts, U.S. Census (2014), Peppard "Increased Prevalence of Sleep-disordered Breathing in Adults." American Journal of Epidemiology (2013)

Continuous Positive Airway Pressure (CPAP)

CPAP is used to pump pressurized air through a tube and into a mask which then keeps a patient's airway open and unobstructed.

85%

of those diagnosed with OSA will be prescribed CPAP.

Although other therapies are available, CPAP remains the first line of treatment and is **100% effective when used.**

2017

$1.3 billion
Total US CPAP Market

$930 million
Total CPAP Mask Market

16.9 million
CPAP Masks Sold

-iData Positive Pressure Devices Market Report. Montserrat JM, Ferrer M, Hernadez L, Farre R, Vilagut G, Navajas S, Badia J, Carrasco E, DePablo J, Ballester E. A randomized placebo controlled study on the effectiveness of CPAP treatment. Am J Respir Crit Care Med 2001

A meta-analysis of 84 studies that evaluated sleeping characteristics and blood pressure identified "CPAP as the most efficacious treatment for OSA patients." Verifying the Relative Efficacy between CPAP Therapy and Its Alternatives for Obstructive Sleep Apnea: A Network Meta-analysis. Liu, Li, Zhou and Wang. Front Neurol. 2017 Jun 28;8:289. doi: 10.3389/fneur.2017.00289. eCollection 2017.

Poor Mask Fit Leads to Abandonment Of Treatment

All CPAP Masks on the market today are mass-produced in standard sizes (S, M, L, XL) with generic nasal plugs.

But no two faces or nostrils are the same.

- Patients try several masks before finding one that “almost fits”.
- Patients who switch their mask are at a 7x higher risk of abandoning therapy after switching than those who do not.
- Poor fit and comfort issues are the primary reason for high quit rate.

50%

of patients quit CPAP therapy within the first year!

Rates of initial acceptance of PAP masks and outcomes of mask switching
Adel Bachour & Pirjo Vitikainen & Paula Maasilta; Sleep Breath (2016) 20:733–738 DOI 10.1007/s11325-015-1292

The Metamason Solution

All Metamason CPAP masks are unique. They are custom-made for each patient and made possible through 3D scanning and printing.

African American Male

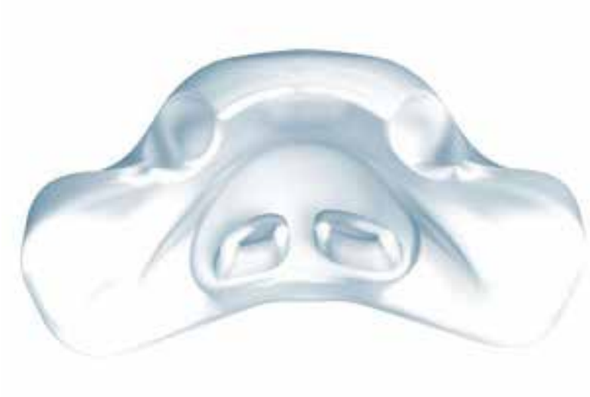

Asian Female

- Fits facial features instead of size range
- Patient specific nasal air seal
- Unique to each individual

Metamason Architechture

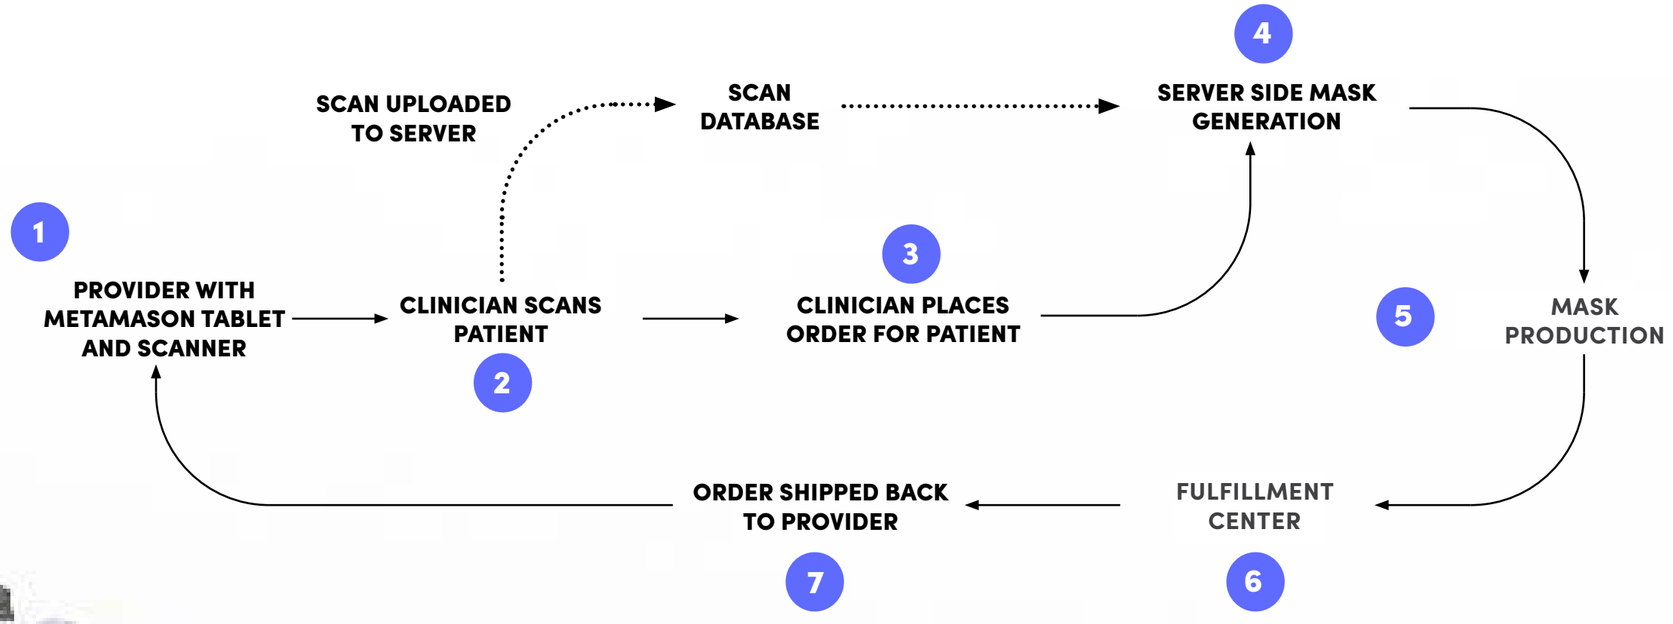

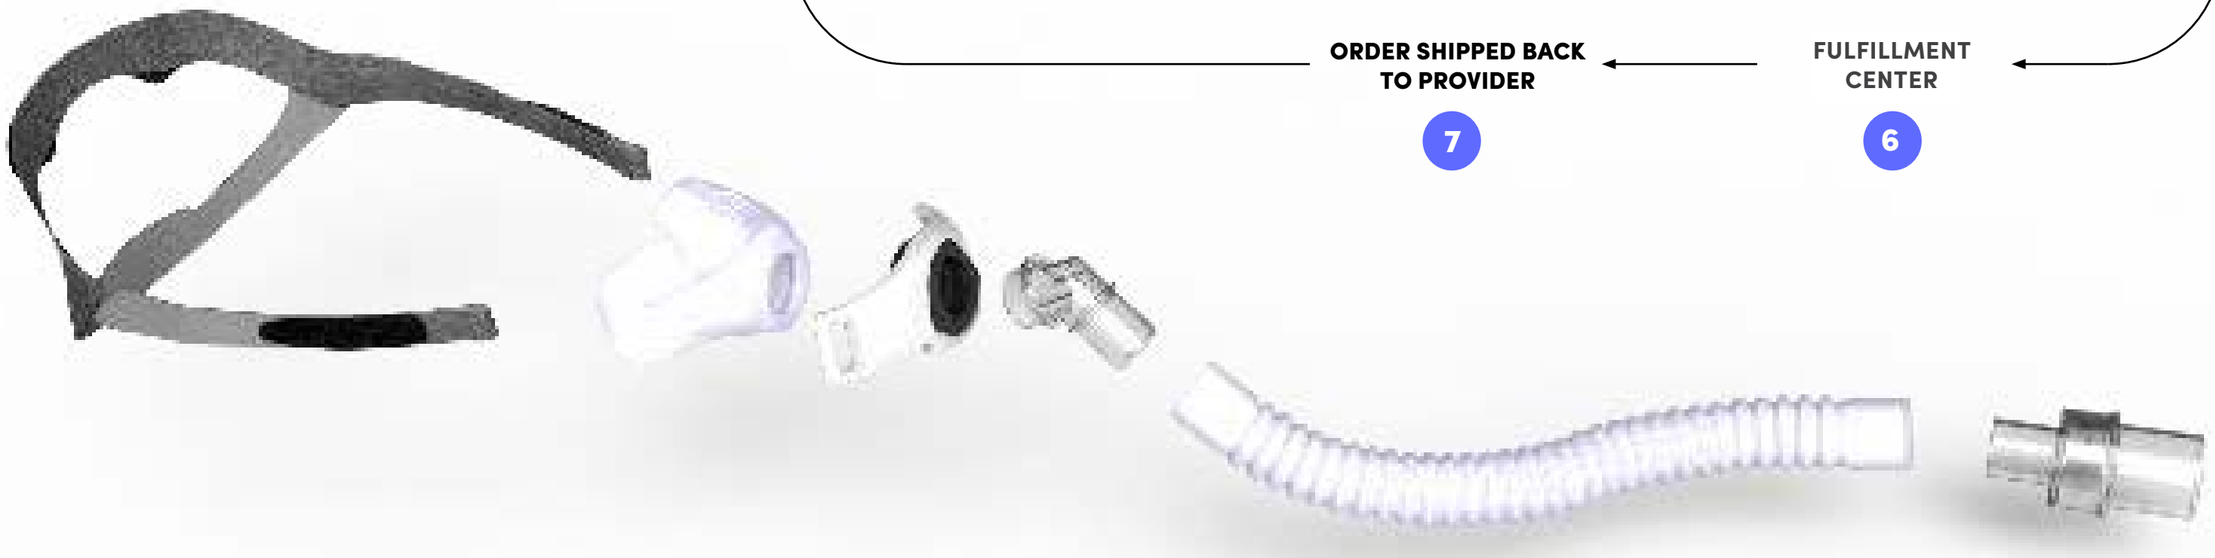

We took the traditional product development process and built it into an application. In a matter of minutes, a simple click of a button results in a CPAP mask unique tailored to the contours of each patient's face. We have created a platform that is both bespoke and scalable, capable of producing one mask or 10,000 with no direct input from a designer or engineer.

Design Algorithm

Over three years of software and product development went into the creation of our SCAN.FIT.PRINT pipeline. Our custom, cloud-based software is both scalable and completely automated. No matter the patients' face, our software always creates a mask design that performs to the highest standards.

SCAN GEOMETRY

SCAN LANDMARKS

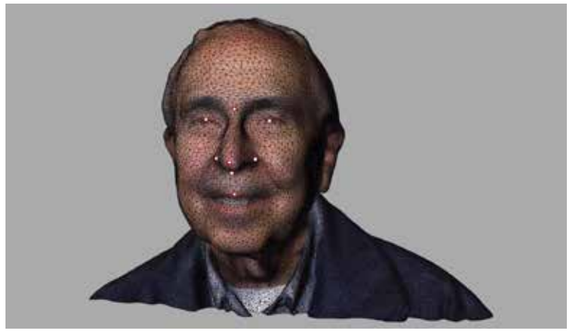

- Scans saved in HIPAA compliant database
- When an order is generated, our server-side mask software retrieves the scan and begins creating mask architecture
- Generates 68 unique landmarks used by the mask generation software to create patient-specific optimizations

METAMASON'S MASK SOFTWARE

- Custom cloud-based software
- After scanning, the mask design is generated in a matter of minutes
- Our proprietary software links design and manufacturing dynamically; if a design change is needed, production updates in seconds

3D MANUFACTURING FILE

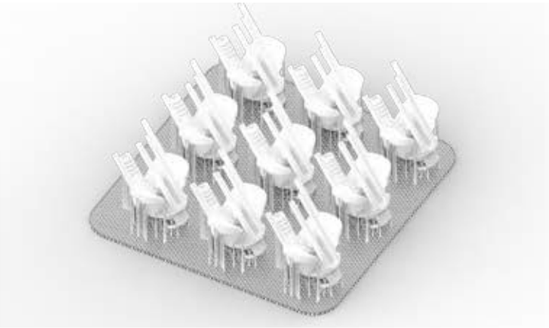

- Parts for immediate production
- Parts are properly orientated with built-in checks for failure reduction
- Electronically sent to 3D printer in minutes

MANUFACTURING

- Manufactured by our partner 3DSystems (NYSE: DDD)
- ISO-certified facility
- Leveraging state-of-the-art production machinery
- 2+ years of development to perfect our proprietary process

Intellectual Property

Our current portfolio captures the basics of our workflow to date. To support Metamason's wider strategy, current and future filings will focus on protecting four distinct areas of technology...

- Scan-to-Print pipeline
- Additive manufacturing processes
- New unique design features that our workflow allows
- Software platform

2 Patents Granted

Methods for additive manufacturing processes incorporating active deposition

8/11/2015, US9,102,099B1

US 14/321,046 (07/01/14)

Customized medical devices and apparel

11/22/2016, US9,498,593B2

US 14/102,370 (12/10/13), pct

3 Patents Pending

Customized CPAP Masks and Related Modeling Algorithms

US 62/373,866 (08/11/2017), pct

Systems and methods for additively manufacturing highly customized structures

US 14/615,389 (02/05/15), pct

Systems and methods for fabricating objects using investment molding techniques

US 14/173,549 (2/12/14), pct

Regulatory Progress

FDA 510(k)

CPAP Masks are Class II medical devices that require FDA Clearance.

A 510(k) is a premarket submission made to the FDA to demonstrate that a device to be marketed is at least as safe and effective (i.e. substantially equivalent) as a cleared device.

Paul Dryden
FDA Consultant
President, ProMedic Inc.

Paul has successfully taken over 600 respiratory devices through FDA clearance.

Biocompatibility Testing

Cytotoxicity	PASSED	12/3/2016
Intracutaneous Reactivity	PASSED	1/28/2017
Genotoxicity	PASSED	2/11/2017
Sensitization	PASSED	2/15/2017
Extractable & Leachable Spectrometry	PASSED	2/22/2017

Performance Testing

Resistance to Airflow	PASSED	1/2/2017
Exhaust Flow	PASSED	1/2/2017
Co2 Rebreathing	PASSED	1/2/2017
Dead-space Volume	PASSED	3/24/2017
Lifecycle Conditioning	PASSED	2/16/2017
Cleaning Conditioning	PASSED	3/16/2017
Manual Cleaning Validation	PASSED	3/16/2017

2016

- Q1 — Software Team on-boarding
- Q2 — Casting & Manufacturing Process R&D
- Q3
- Q4 — Start of 60 Day FDA Review
  Initiated Biocompatibility & Performance Testing

2017

- Q1 — Finalized Casting & Manufacturing Process
- Q2 — Completed FDA version of software
  Completed Performance Testing
- Q3 — 510(K) Application Official Submitted
- Q4 — Responses to FDA Questions
  FDA 30 Day Final Review

2018

- Q1 — **Anticipated 510(k) Clearance**

Clinical Success

Feasibility Study

Date Completed	**May 2017**
Subjects	**Compliant CPAP Users**
Subject Pool Size	**8**
Objectives	1. Assess Metamason's design & manufacturing process 2. Evaluate the functionality of Metamason's software 3. Evaluate sleep center's adaptation of novel work flow 4. Test patience acceptance of novel sleep technology
Location	**Tower Sleep Medicine** at Cedars-Sinai Medical Center

TOWER SLEEP
MEDICINE

Results

- Reduction in mask casting time from 8hrs to 1hr
- Reduction in scan to patient mask delivery time from 20 days to 10 days (industry standard is 30 days)
- Clinician acceptance of scanning process integrated into normal work flow
- Patient acceptance and high ratings for "ease of use"

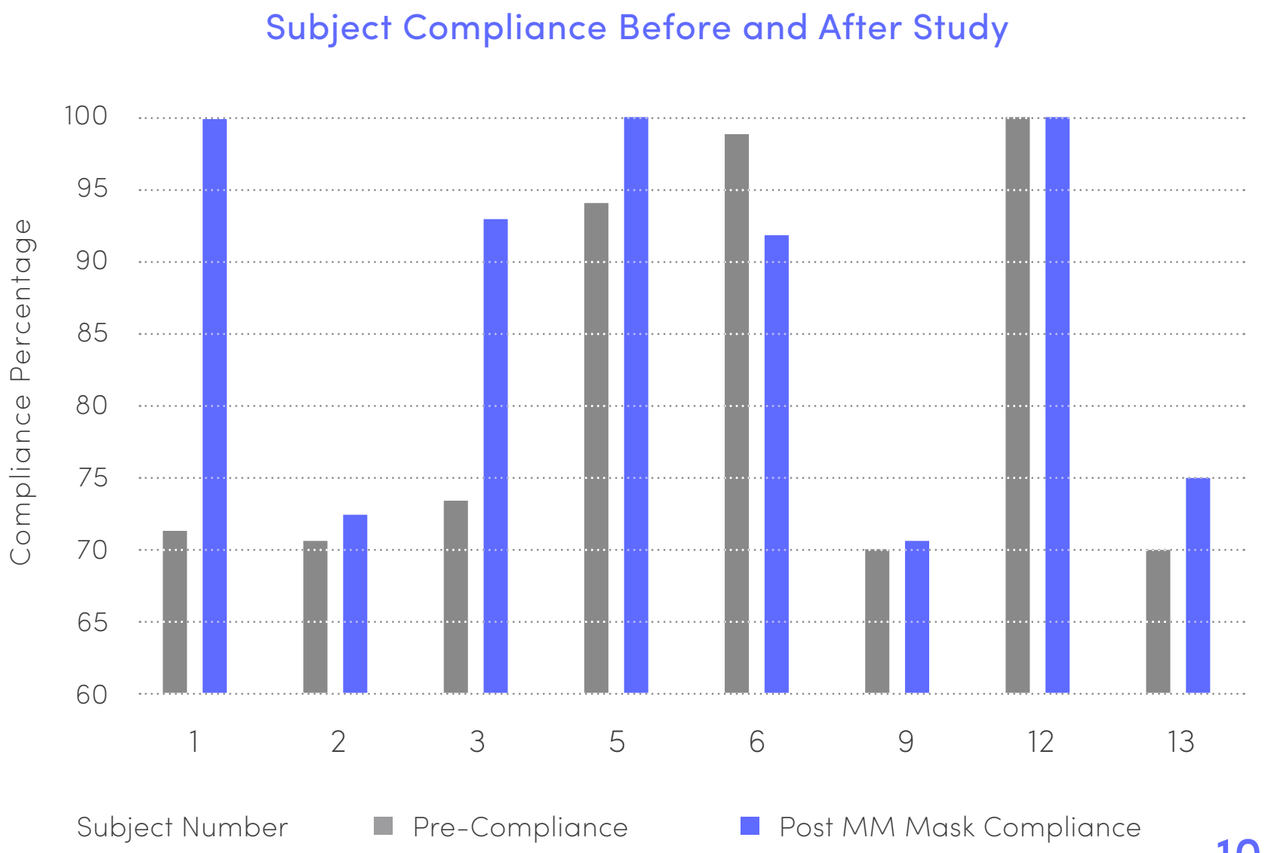

Addressable U.S. Market

YEAR	MASKS SOLD	MARKET VALUES
2013	8,231,767	$520.7M
2014	9,860,032	$620.1M
2015	11,986,360	$705.5M
2016	14,342,063	$815.8M
2017	**16,906,506**	**$930.6M**
2018	19,652,853	$1.05B
2019	22,549,596	$1.17B
2020	25,654,225	$1.28B
2021	28,654,896	$1.40B
2022	31,791,960	$1.52B
2023	34,939,277	$1.63B

US mask market annual growth forecast

8%

-iData Positive Pressure Devices Market Report

CPAP Machine & Mask Sales (U.S.)

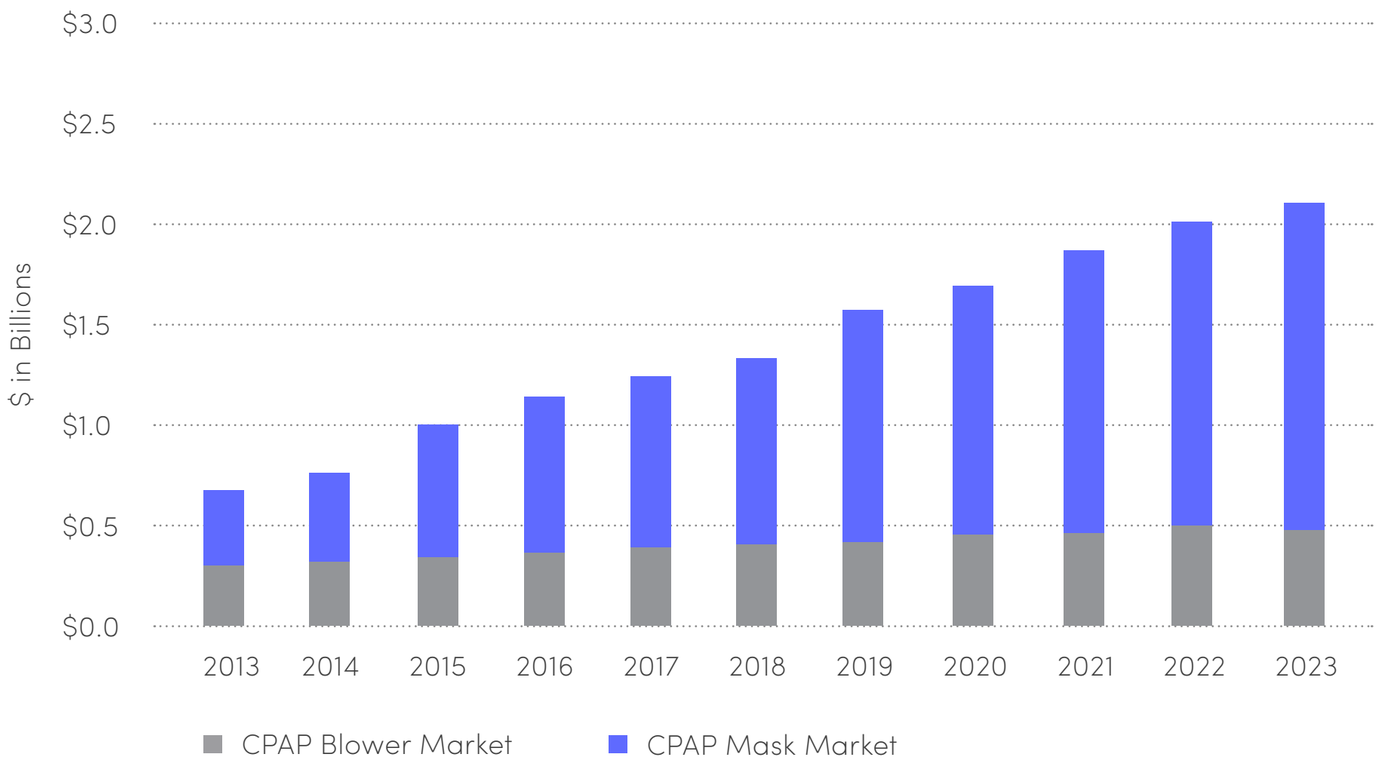

- Patients keep their CPAP blower machine, but replace their mask twice each year on average
- Increase in mask sales anticipated to be even greater with Metamason in the market since fewer patients will quit therapy.

-Citi Research, Deep Dive | Equities: 22 Nov 2016, Philips (PHG.AS)

Sales Channels

Durable Medical Equipment (DME) Providers

- 2,600 Unique DMEs (national & regional)
- National DMEs: 6000 locations, 40% market share
- Paid only on compliant patients
- Seeking market differentiation
- Seeking cash Sales

Value Proposition

Increased Compliance -> Resupply

Uninterrupted cash flow

Initially out-of-pocket

U.S. Department of Veterans Affairs

- $174M spend on CPAP in 2015
- 15% growth rate YOY
- Non-traditional purchaser
- Burdensome bureaucracy
- Less price sensitivity
- Requires FSS contract

Value Proposition

Reduced clinic wait time

Improved patient throughput

More effective, premium product

Sleep Physicians & Sleep Labs

- 7,000 board certified sleep physicians
- 3,000 accredited sleep Labs
- Biggest influencer (Rx)
- Focus on patient outcomes
- Patient satisfaction

Value Proposition

Improved health outcomes

Solution for pediatric patients

Provide potential new revenue path

Direct to Consumer (Online)

- Currently 5% of market and growing
- Promotes patient engagement
- Almost exclusively cash sales
- Patient convenience

Value Proposition

Expanded product offering

Higher margins

Increased consumer engagement

Our Team

Robin Randolph
Chief Marketing Officer

Prior:
Marketing Mgr, North America
Fisher & Paykel Healthcare
Director Market Initiatives, ResMed

Ryan Oenning
CPO Product Officer
Co-Founder

Prior:
Founder at Khora Design
MachineHistories

Lou Pizante
Chief Financial Officer/GC*

Prior:
CFO at GOOD
CEO of Mavent Inc.

Clifford Sarkin
Head Of Corp. Strategy & Dev.*
Co-Founder

Prior:
Director of Operations of
VideoSurf (acq. by MSFT 2011)
& Duda Mobile

Robyn Woidtke
VP Of Clinical*

Prior:
Founder at Sleep Apnea Risk
Associates

Charles Bohlen
VP Of Operations
Co-Founder

Prior:
Development at Mosaic Media
Group

* acting

Andrew Ferk
Lead Software Engineer

Charles Pyott
Senior Industrial Designer

Alexia Yang
Product Designer

Jake Dluhy
Front End Developer

Cory Pope
QA/Systems Analyst

Competitive Analysis

	Standard CPAP Masks	Truly Personalized CPAP Masks
Manufacturers	ResMed, PHILIPS RESPIRONICS, Fisher&Paykel	metamason™
Size Offerings	XS, S, M, L, XL	Infinite
Sizing Methodology	Sizing Guide (rudimentary ruler)	Optical Scan Accurate to 0.5mm
True Precision of Fit	Never	Always
Nair Openings	Symmetrical Only	Asymmetrical (i.e. exact match)
Bespoke Design Algorithm	None	Yes (cloud based)
Scanning Technology	No	Yes
Time to Market for New Versions	2-3 Years	Less Than 1 Year

Current & Future Financing

Series Seed 2

Intended Close	**Rolling Close**, Completed By **Oct. 31, 2017**
Intended Raise	**$1.5M**
Mechanism	**Convertible Note w/ Discount** on Series A
Major Milestones	1. FDA 510(k) Clearance - (Jan/Feb '18) 2. Completion of 20+ Subject Clinical Trial (April/May '18) 3. Controlled Market Release to select National DMEs 4. Notable First Adopter Agreements and LOIs 5. Initiate CEO Recruitment

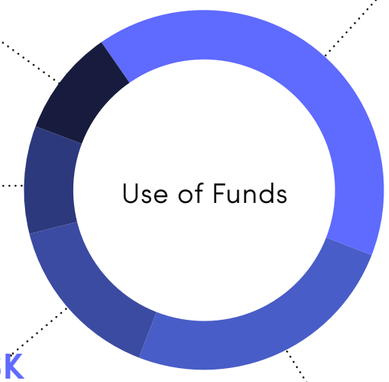

Clinical **$136K**
- Implementation of Market Validation Clinical Trial (20+ Subjects)

Regulatory **$135K**
- Completion of FDA Clearance Process

Sales & Marketing **$246K**
- Pre-Launch Marketing Activities
- Presence at 2 Industry Tradeshows
- Hiring Initial Sales Team (3 Regional Sales Managers)

Operations & Legal **$622K**
- Continued Operations
- IP Filings
- Chief Executive Officer

Product Development **$361K**
- Software Platform Development & Completion
- Hardware Accessory Prototyping & Development

Series A

Intended Close	May '18
Intended Raise	$8M - $10M
Anticipated Valuation	$35M - $40M (pre-money)

Objectives Full Product Launch

1. Federal Supply Schedule Contract and Rollout with VA
2. Expansion to National US and Canadian DMEs
3. Full US & Partial Canada D2C Launch
4. National Sales & Marketing Strategy Execution
5. Grow Sales & Customer Service Teams
6. Design, 510(k) Clearance, and Clinical Trials for Pediatric & Neonatal CPAP Mask Products
7. Pediatric & Neonatal CPAP Market Release

Notice

This Presentation is based on information supplied by Metamason Inc. It is furnished solely for use by prospective investors that are "accredited investors" to evaluate a potential investment.

This Presentation does not purport to be all inclusive or to contain all of the information that a prospective investor may require. Metamason Inc. does not make and expressly disclaims any specific representation or warranty as to the accuracy or comprehensiveness of any of the information contained herein and none may be implied.

This Presentation includes confidential and proprietary information and it is provided solely with the express understanding that such information will not be disclosed to any third party.

The sole purpose of this Presentation is to assist the recipient in deciding whether to proceed with investigation of the opportunity presented. It is not an offer to sell but only an announcement of an intention to seek inquiries. This Presentation shall not be construed to indicate that there has been no change in the potential investment since the date hereof.

THIS PRESENTATION IS AN EXPLORATION OF AN INVESTMENT INTO THE SECURITIES OF AN EARLY-STAGE COMPANY WITH A LIMITED OPERATING HISTORY. AN INVESTMENT IN SUCH SECURITIES IS SPECULATIVE AND INVOLVES A HIGH DEGREE OF RISK.

metamason™
The first and only 3D printed CPAP mask created to
fit every individual uniquely and precisely
811 W. 7th St. Suite 1146 Los Angeles, CA 90017
investor@metamason.com