

Filename: 2024-05-09 - 14.47.34.RNA




Default image (Contrast 100%)

Sample Info

Well	RINe	28S/18S (Area)	Conc. [ng/ul]	Sample Description	Alert	Observations
A1	-	-	89.7	Ladder		Caution! Expired ScreenTape device; Ladder
B1	-	-	2.13	LCM 3		Caution! Expired ScreenTape device; Sample concentration outside functional range for RINe and the assay
C1	-	-	2.31	LCM 10		Caution! Expired ScreenTape device; Sample concentration outside functional range for RINe and the assay

A1: Ladder

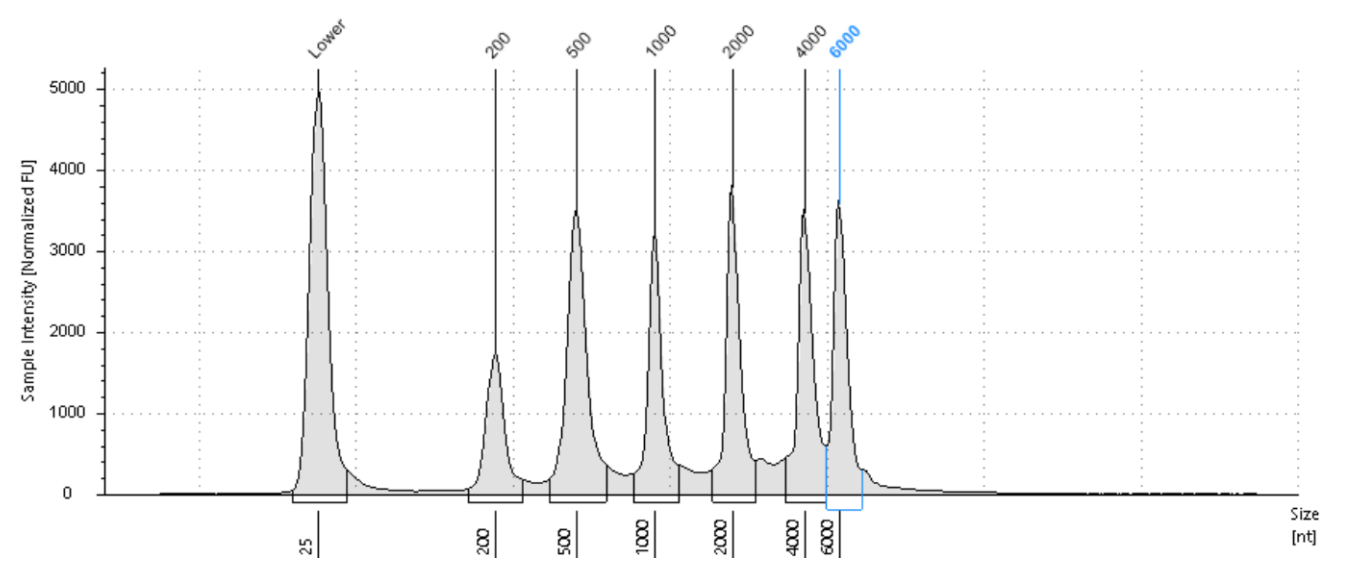


Sample Table

Well	RINe	28S/18S (Area)	Conc. [ng/μl]	Sample Description	Alert	Observations
A1	-	-	89.7	Ladder		Caution! Expired ScreenTape device; Ladder

Peak Table

Size [nt]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
25	40.0	40.0	4710	-		Lower Marker
200	8.23	-	121	10.50		
500	18.4	-	108	23.52		
1000	12.2	-	35.9	15.58		
2000	13.5	-	19.8	17.16		
4000	13.5	-	9.91	17.20		
6000	12.6	-	6.16	16.04		

B1: LCM 3

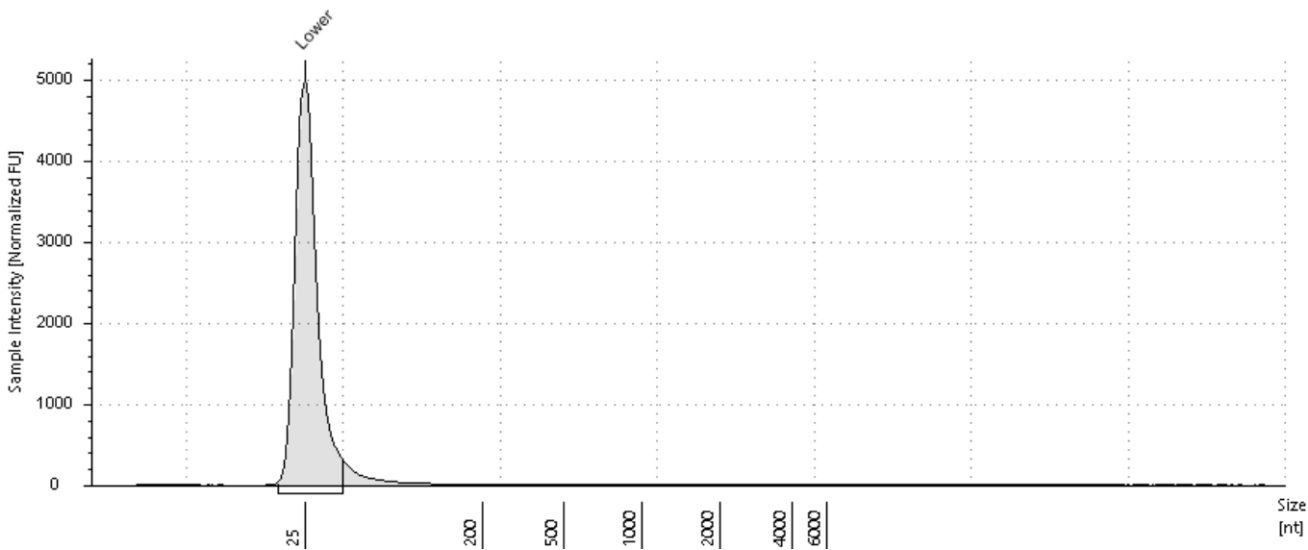


Sample Table

Well	RINe	28S/18S (Area)	Conc. [ng/µl]	Sample Description	Alert	Observations
B1	-	-	2.13	LCM 3		Caution! Expired ScreenTape device; Sample concentration outside functional range for RINe and the assay

Peak Table

Size [nt]	Calibrated Conc. [ng/µl]	Assigned Conc. [ng/µl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
25	40.0	40.0	4710	-		Lower Marker

C1: LCM 10

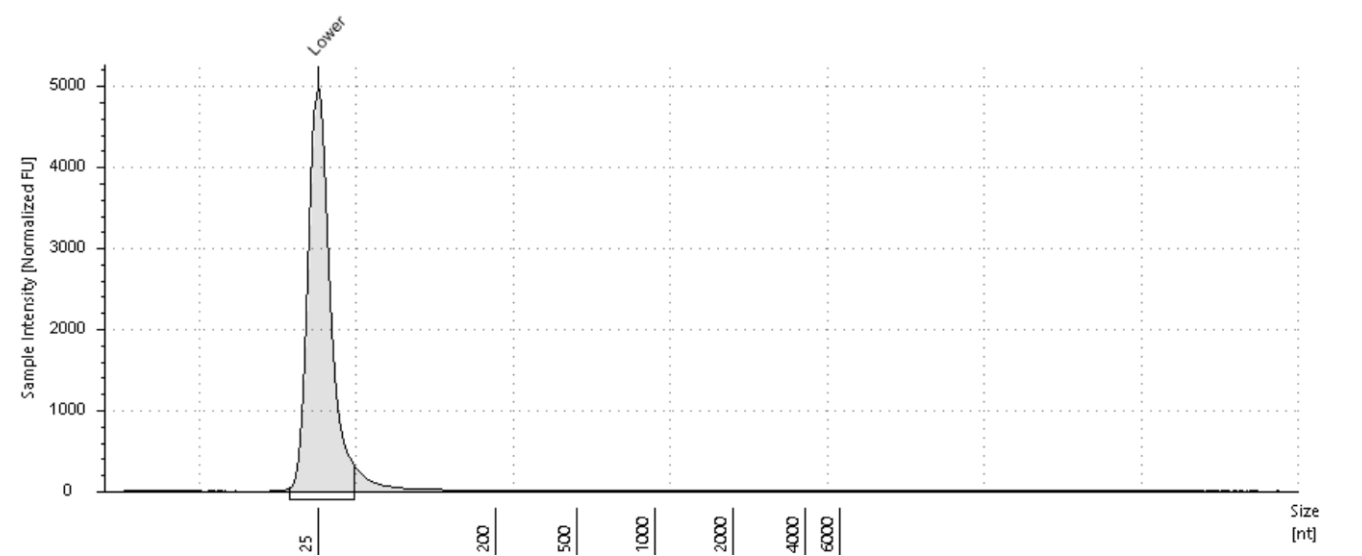

Sample Table

Well	RINe	28S/18S (Area)	Conc. [ng/µl]	Sample Description	Alert	Observations
C1	-	-	2.31	LCM 10	<div></div>	Caution! Expired ScreenTape device; Sample concentration outside functional range for RINe and the assay

Peak Table

Size [nt]	Calibrated Conc. [ng/µl]	Assigned Conc. [ng/µl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
25	40.0	40.0	4710	-		Lower Marker