



Filename: 2024-05-14 - 13.04.42.D5000

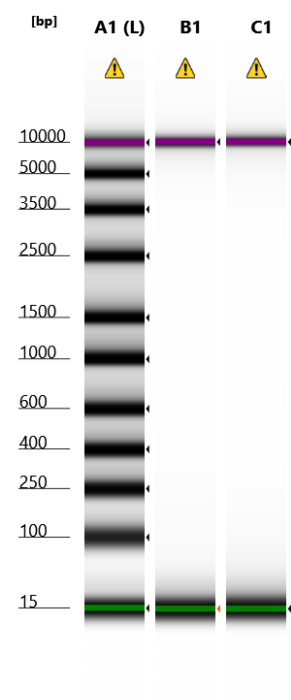

Sample Info

Well	Conc. [ng/μl]	Sample Description	Alert	Observations
A1	61.9	Ladder		Caution! Expired ScreenTape device; Ladder
B1		7		Caution! Expired ScreenTape device
C1		11		Caution! Expired ScreenTape device

A1: Ladder

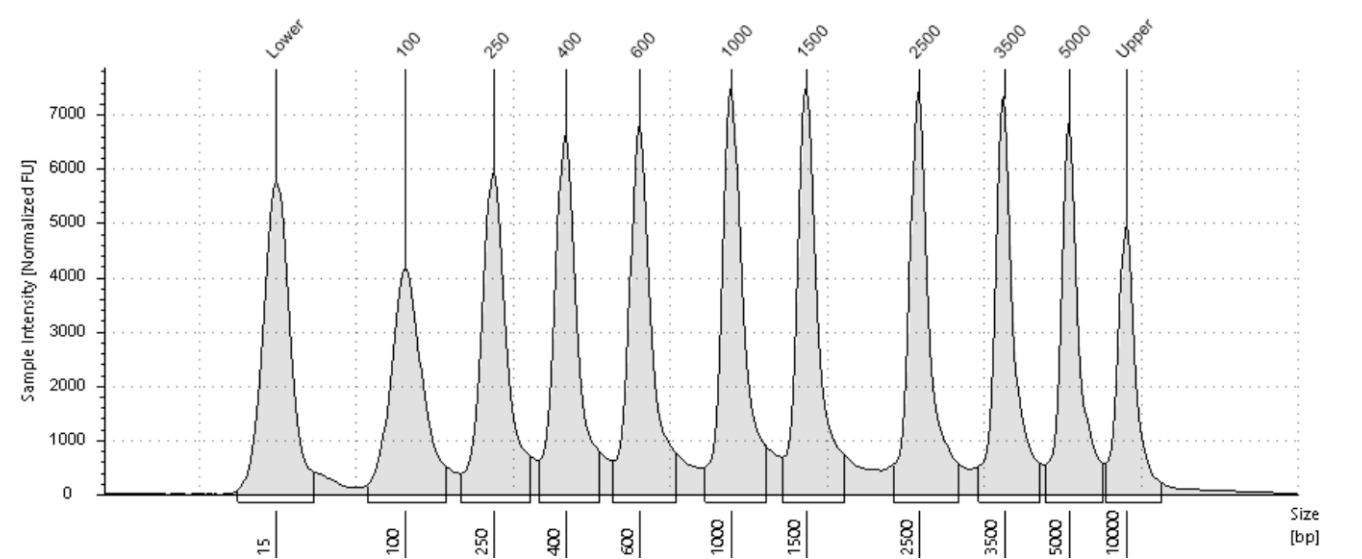


Sample Table

Well	Conc. [ng/μl]	Sample Description	Alert	Observations
A1	61.9	Ladder		Caution! Expired ScreenTape device; Ladder

Peak Table

Size [bp]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
15	6.51	-	668	-		Lower Marker
100	6.22	-	95.7	10.05		
250	6.97	-	42.9	11.27		
400	7.12	-	27.4	11.50		
600	7.18	-	18.4	11.61		
1000	7.54	-	11.6	12.20		
1500	7.26	-	7.45	11.74		
2500	7.04	-	4.33	11.38		
3500	6.56	-	2.88	10.60		
5000	5.97	-	1.84	9.65		
10000	3.25	3.25	0.500	-		Upper Marker

B1: 7

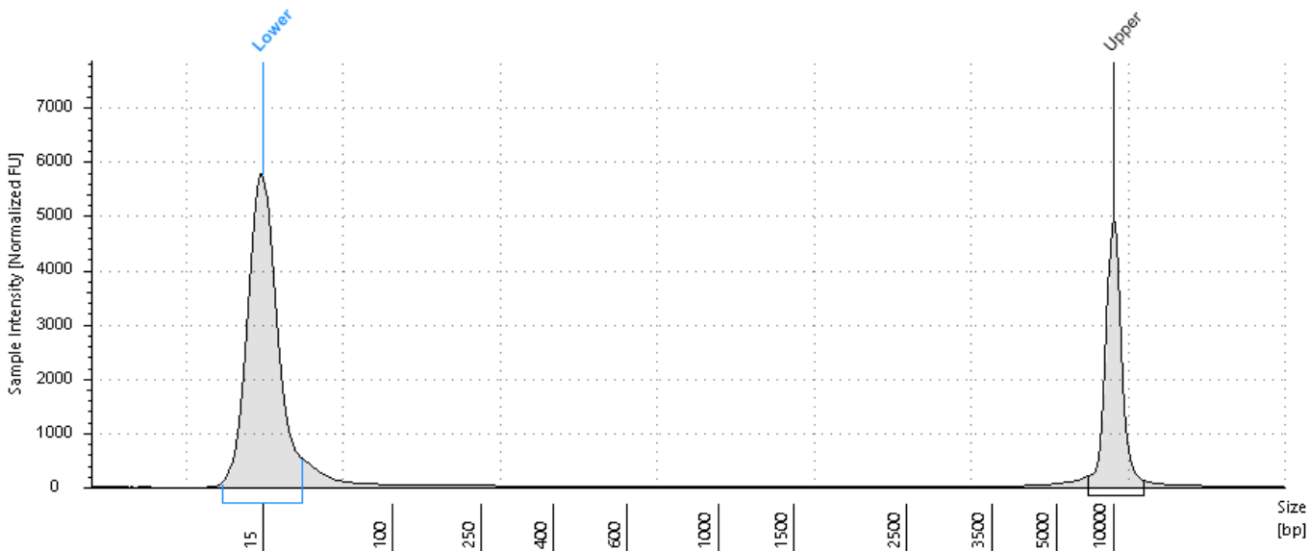


Sample Table

Well	Conc. [ng/μl]	Sample Description	Alert	Observations
B1		7		Caution! Expired ScreenTape device

Peak Table

Size [bp]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
15	7.02	-	720	-		Lower Marker
10000	3.25	3.25	0.500	-		Upper Marker

C1: 11

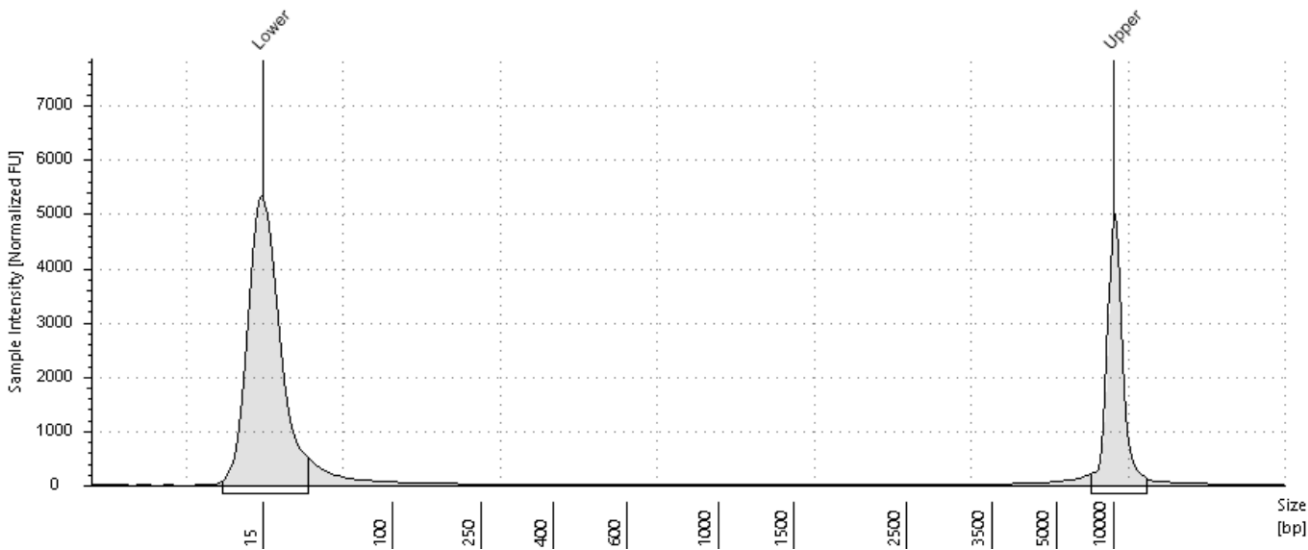

Sample Table

Well	Conc. [ng/μl]	Sample Description	Alert	Observations
C1		11		Caution! Expired ScreenTape device

Peak Table

Size [bp]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
15	7.14	-	732	-		Lower Marker
10000	3.25	3.25	0.500	-		Upper Marker