


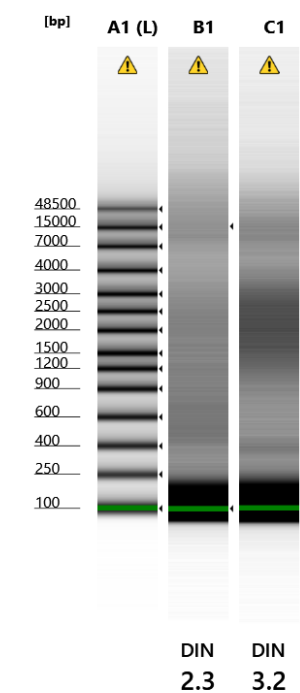


Filename: 2024-12-12 - 13.20.38.gDNA


Sample Info

Source	Well	DIN	Conc. [ng/ul]	Sample Description	Alert	Observations
	A1	-	88.7	Ladder		Caution! Expired ScreenTape device; Ladder
	B1	2.3	4.86	LCM_32		Caution! Expired ScreenTape device; Sample concentration outside functional range for DIN and the assay
	C1	3.2	4.56	LCM_33		Caution! Expired ScreenTape device; Sample concentration outside functional range for DIN and the assay



Default image (Contrast 76%), Image is Scaled to Sample

A1: Ladder

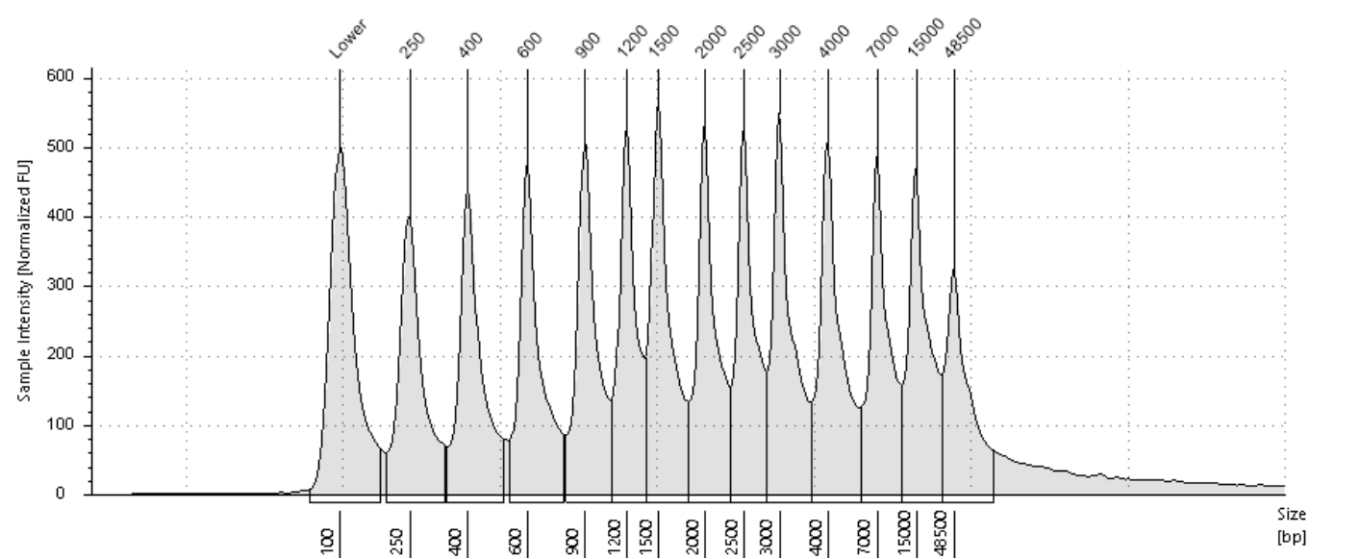


Sample Table

Source	Well	DIN	Conc. [ng/ul]	Sample Description	Alert	Observations
	A1	-	88.7	Ladder		Caution! Expired ScreenTape device; Ladder

Peak Table

Size [bp]	Calibrated Conc. [ng/ul]	Assigned Conc. [ng/ul]	% Integrated Area	From [bp]	To [bp]	Peak Molarity [nmol/l]	Peak Comment
100	8.50	8.50	-	67	171	131	
250	6.19	-	7.26	183	334	38.1	
400	6.44	-	7.55	337	510	24.8	
600	6.76	-	7.92	529	777	17.3	
900	6.66	-	7.80	784	1084	11.4	
1200	6.25	-	7.33	1084	1380	8.01	
1500	7.39	-	8.66	1380	1803	7.58	
2000	6.85	-	8.03	1803	2315	5.27	
2500	6.36	-	7.45	2315	2804	3.91	
3000	7.30	-	8.56	2804	3615	3.74	
4000	7.16	-	8.39	3615	5838	2.75	
7000	6.33	-	7.42	5838	11343	1.39	
15000	6.46	-	7.57	11343	24434	0.662	
48500	5.17	-	6.06	24434	84393	0.164	

B1: LCM\_32

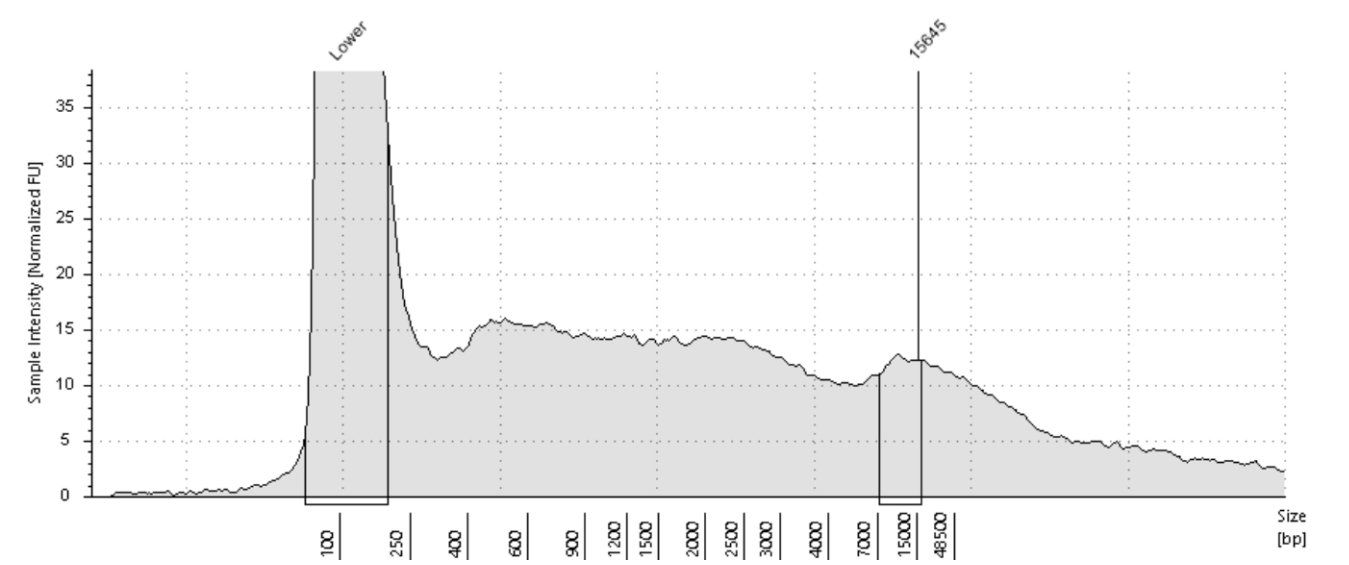


Sample Table

Source	Well	DIN	Conc. [ng/μl]	Sample Description	Alert	Observations
	B1	2.3	4.86	LCM_32		Caution! Expired ScreenTape device; Sample concentration outside functional range for DIN and the assay

Peak Table

Size [bp]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	% Integrated Area	From [bp]	To [bp]	Peak Molarity [nmol/l]	Peak Comment
100	8.50	8.50	-	63	188	131	
15645	0.269	-	100.00	7430	16469	0.0265	

C1: LCM\_33

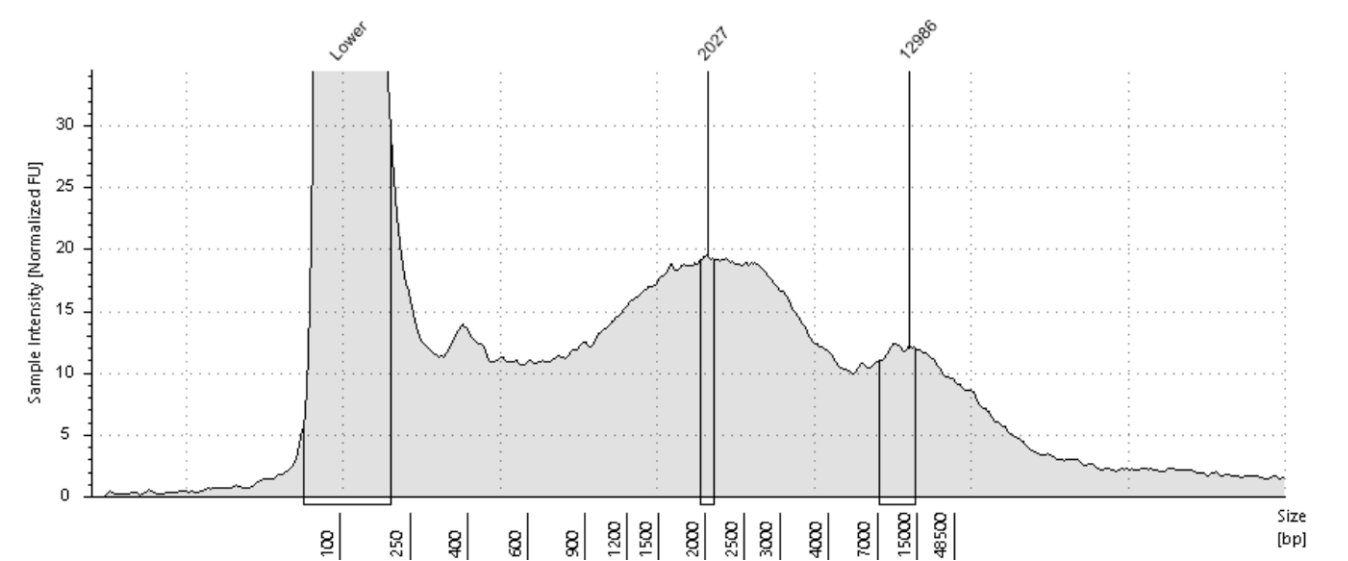

Sample Table

Source	Well	DIN	Conc. [ng/μl]	Sample Description	Alert	Observations
	C1	3.2	4.56	LCM_33		Caution! Expired ScreenTape device; Sample concentration outside functional range for DIN and the assay

Peak Table

Size [bp]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	% Integrated Area	From [bp]	To [bp]	Peak Molarity [nmol/l]	Peak Comment
100	8.50	8.50	-	62	195	131	
2027	0.149	-	39.70	1947	2108	0.113	
12986	0.226	-	60.30	7355	14778	0.0268	