


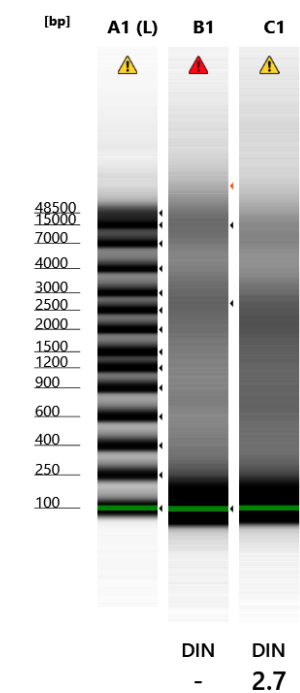



Filename: 2024-12-04 - 10.44.34.gDNA

Sample Info

Source	Well	DIN	Conc. [ng/ul]	Sample Description	Alert	Observations
	A1	-	79.4	Ladder		Caution! Expired ScreenTape device; Ladder; Sizing Changed
	B1	-	2.88	13		Caution! Expired ScreenTape device; Sample concentration outside functional range for DIN and the assay; DIN Edited (Ladder sizing changed)
	C1	2.7	3.23	14		Caution! Expired ScreenTape device; Sample concentration outside functional range for DIN and the assay; DIN Edited (Ladder sizing changed)



Default image (Contrast 100%), Image is Scaled to Sample

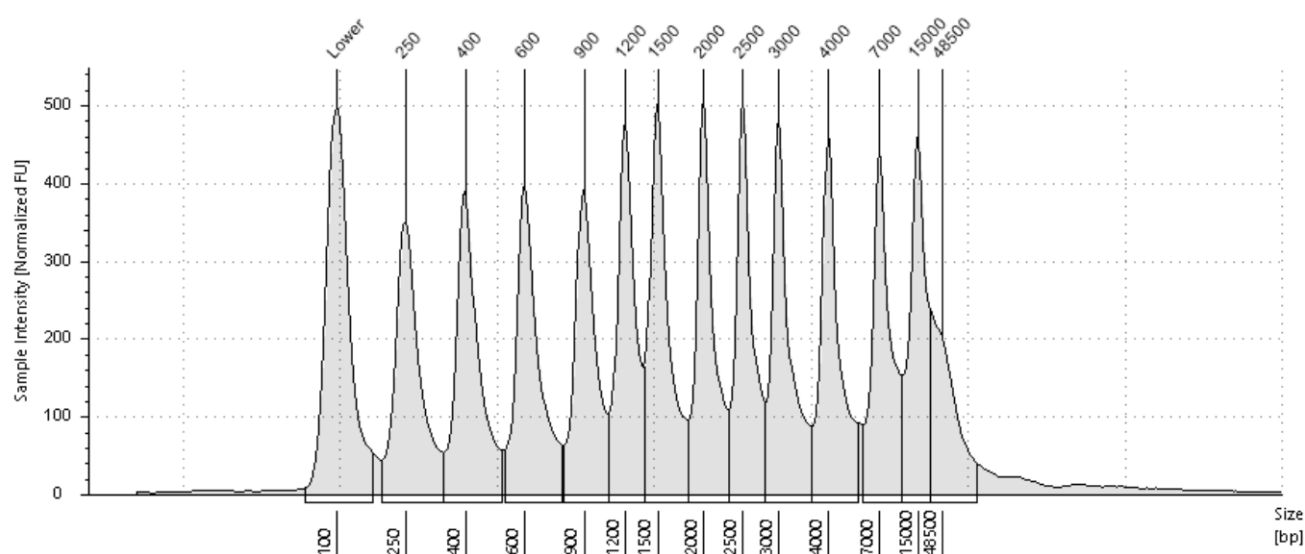
**A1: Ladder****Sample Table**

Source	Well	DIN	Conc. [ng/ul]	Sample Description	Alert	Observations
	A1	-	79.4	Ladder	⚠	Caution! Expired ScreenTape device; Ladder; Sizing Changed

**Peak Table**

Size [bp]	Calibrated Conc. [ng/ul]	Assigned Conc. [ng/ul]	% Integrated Area	From [bp]	To [bp]	Peak Molarity [nmol/l]	Peak Comment
100	8.50	8.50	-	66	161	131	
250	6.15	-	7.84	182	336	37.9	
400	6.41	-	8.16	336	515	24.6	
600	6.51	-	8.30	524	772	16.7	
900	5.92	-	7.54	779	1074	10.1	
1200	6.34	-	8.08	1074	1372	8.13	
1500	6.98	-	8.90	1372	1812	7.16	
2000	6.33	-	8.07	1812	2304	4.87	
2500	6.03	-	7.68	2304	2804	3.71	
3000	6.29	-	8.01	2804	3625	3.23	
4000	6.05	-	7.71	3625	5564	2.33	
7000	5.90	-	7.52	5809	10943	1.30	
15000	5.61	-	7.15	10943	19433	0.576	
48500	3.96	-	5.05	19433	95752	0.126	

B1: 13

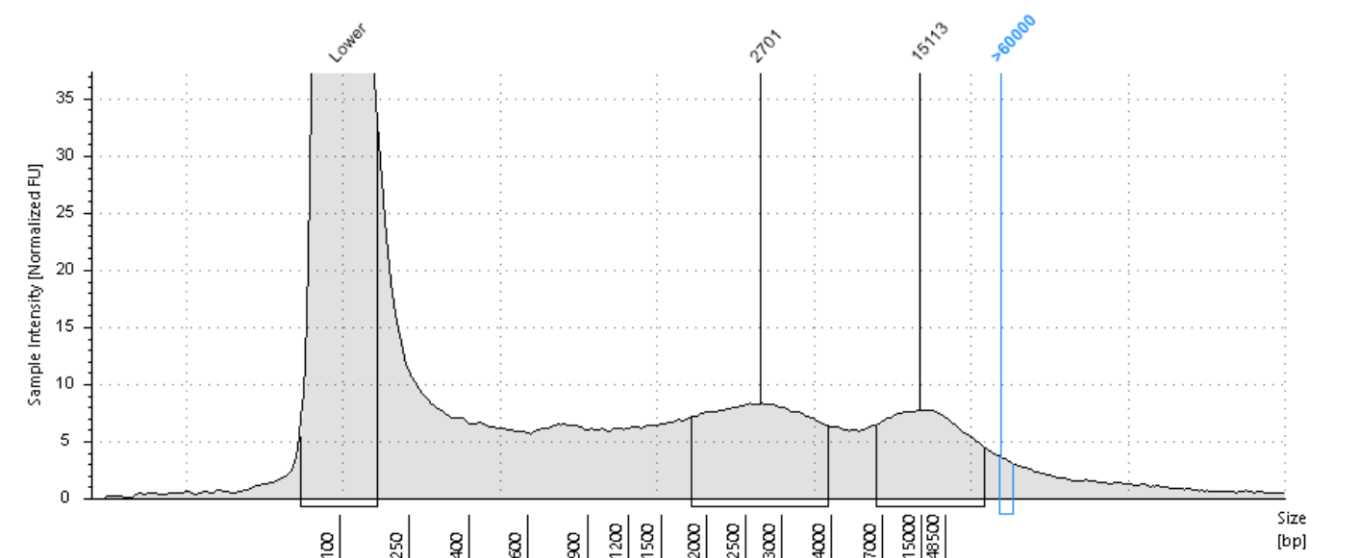


Sample Table

Source	Well	DIN	Conc. [ng/μl]	Sample Description	Alert	Observations
	B1	-	2.88	13		Caution! Expired ScreenTape device; Sample concentration outside functional range for DIN and the assay; DIN Edited (Ladder sizing changed)

Peak Table

Size [bp]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	% Integrated Area	From [bp]	To [bp]	Peak Molarity [nmol/l]	Peak Comment
100	8.50	8.50	-	59	166	131	
2701	0.609	-	57.60	1818	3946	0.347	
15113	0.421	-	39.83	6598	>60000	0.0429	
>60000	0.0272	-	2.57	>60000	>60000	-	

C1: 14

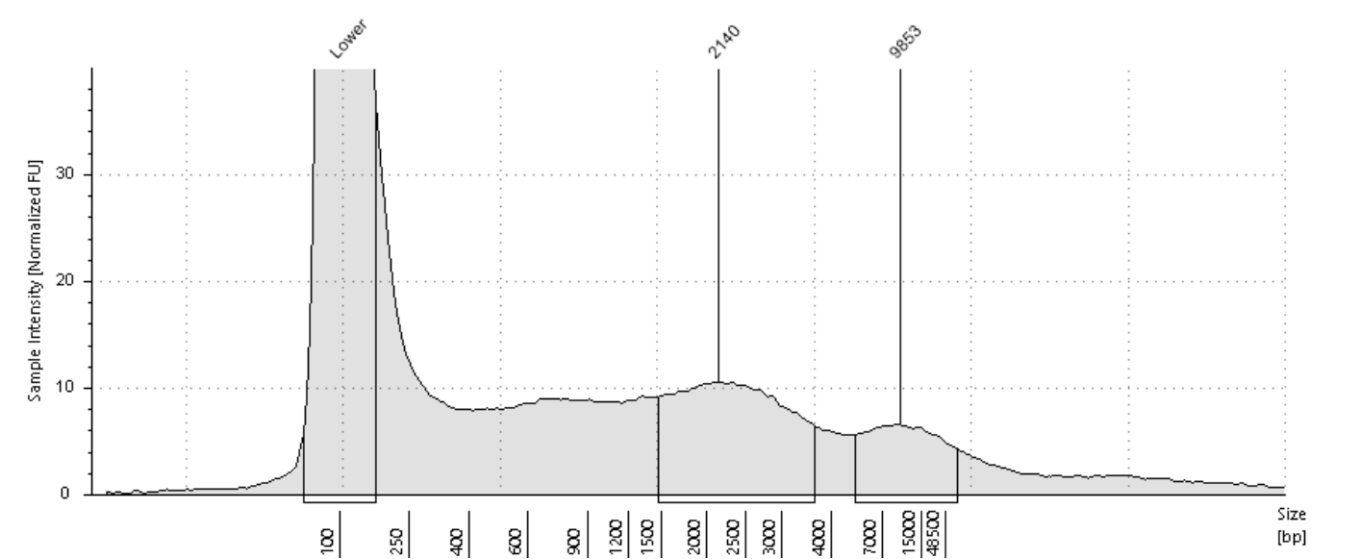

Sample Table

Source	Well	DIN	Conc. [ng/μl]	Sample Description	Alert	Observations
	C1	2.7	3.23	14		Caution! Expired ScreenTape device; Sample concentration outside functional range for DIN and the assay; DIN Edited (Ladder sizing changed)

Peak Table

Size [bp]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	% Integrated Area	From [bp]	To [bp]	Peak Molarity [nmol/l]	Peak Comment
100	8.50	8.50	-	62	163	131	
2140	0.835	-	71.60	1479	3630	0.600	
9853	0.331	-	28.40	5224	>60000	0.0517	