


Filename: 2024-06-17 - 14.13.28.D5000

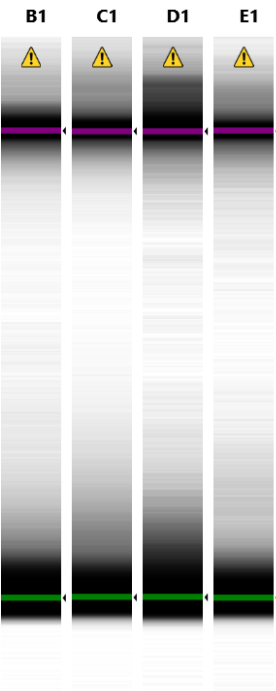


Default image (Contrast 179%)

Sample Info

Well	Conc. [ng/μl]	Sample Description	Alert	Observations
B1		5	⚠	Caution! Expired ScreenTape device
C1		6	⚠	Caution! Expired ScreenTape device
D1		10	⚠	Caution! Expired ScreenTape device
E1		14	⚠	Caution! Expired ScreenTape device

B1: 5

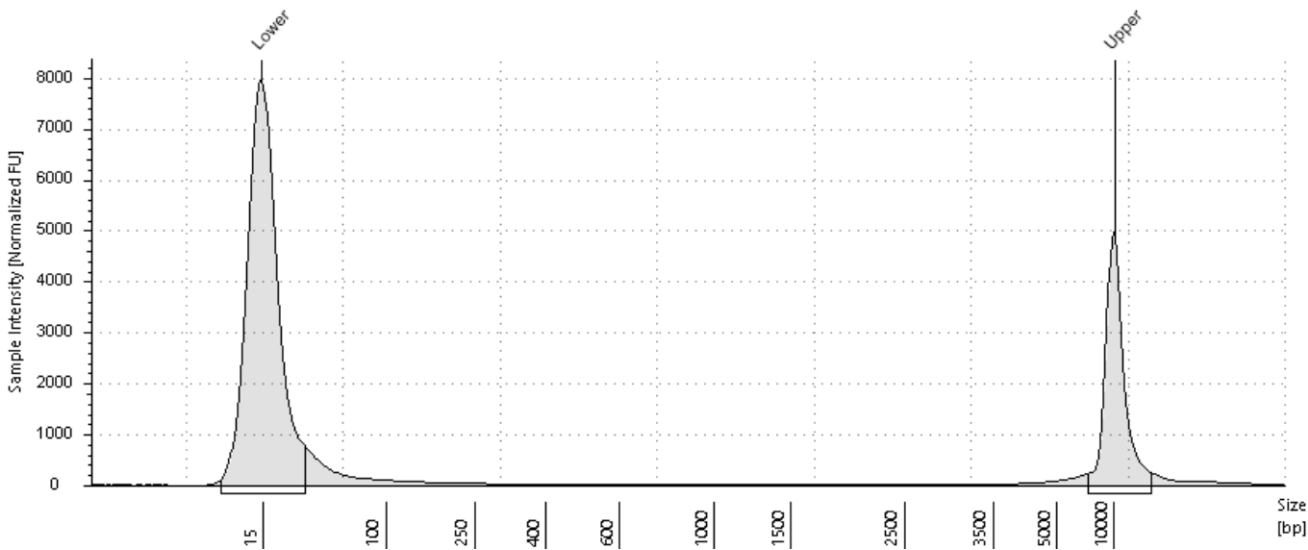


Sample Table

Well	Conc. [ng/μl]	Sample Description	Alert	Observations
B1		5		Caution! Expired ScreenTape device

Peak Table

Size [bp]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
15	8.94	-	917	-		Lower Marker
10000	3.25	3.25	0.500	-		Upper Marker

C1: 6

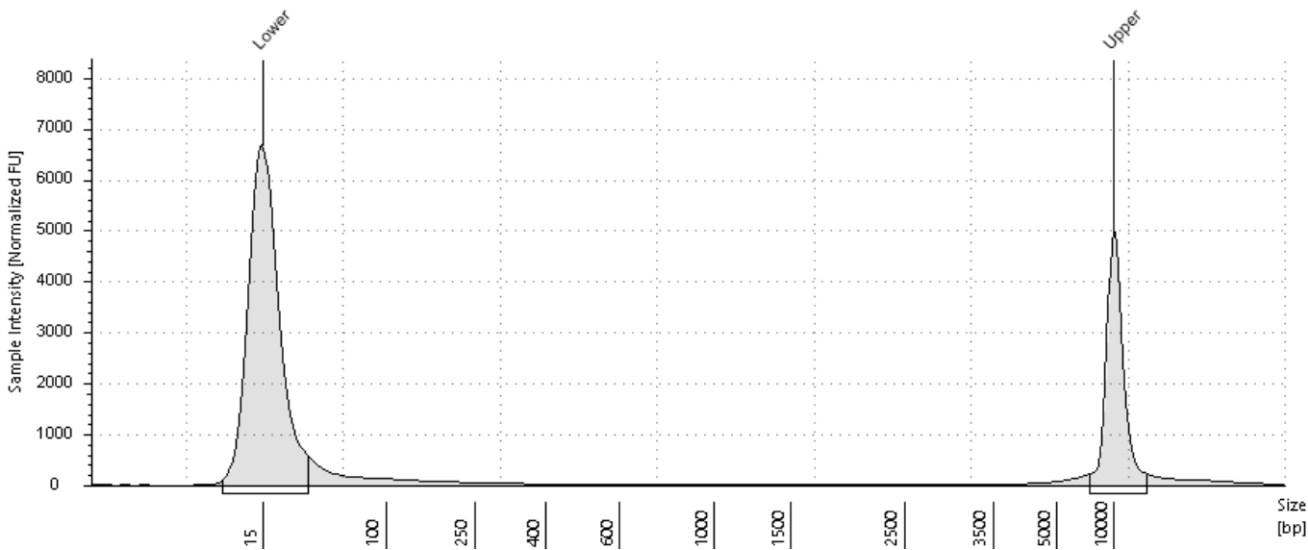


Sample Table

Well	Conc. [ng/μl]	Sample Description	Alert	Observations
C1		6		Caution! Expired ScreenTape device

Peak Table

Size [bp]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
15	8.24	-	845	-		Lower Marker
10000	3.25	3.25	0.500	-		Upper Marker

D1: 10

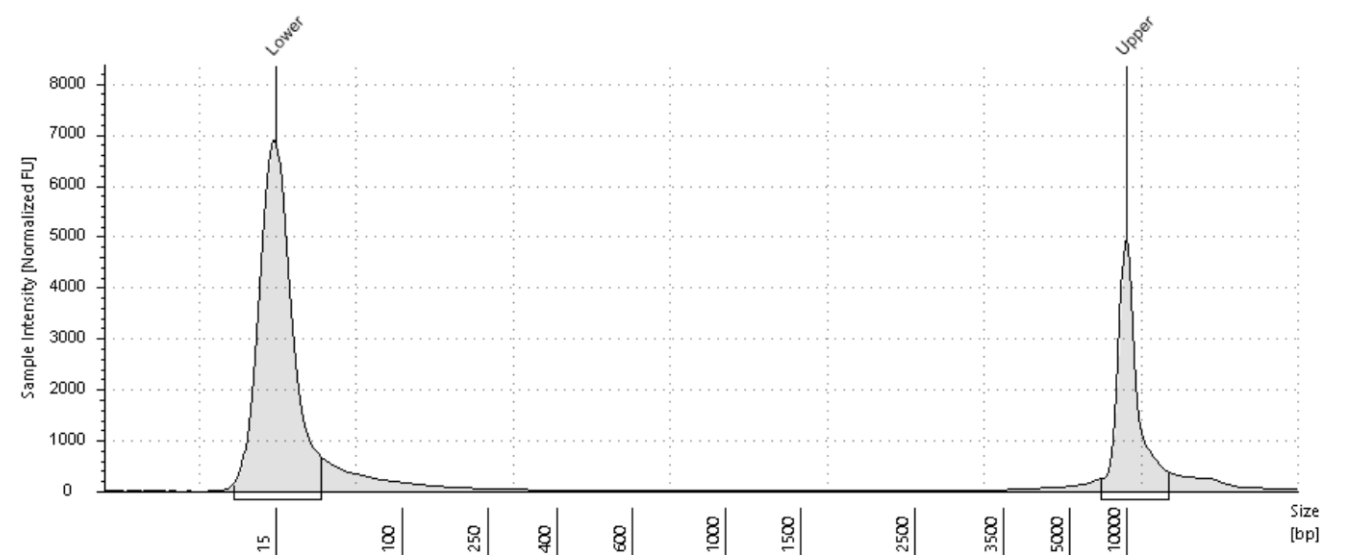


Sample Table

Well	Conc. [ng/μl]	Sample Description	Alert	Observations
D1		10		Caution! Expired ScreenTape device

Peak Table

Size [bp]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
15	8.23	-	844	-		Lower Marker
10000	3.25	3.25	0.500	-		Upper Marker

E1: 14

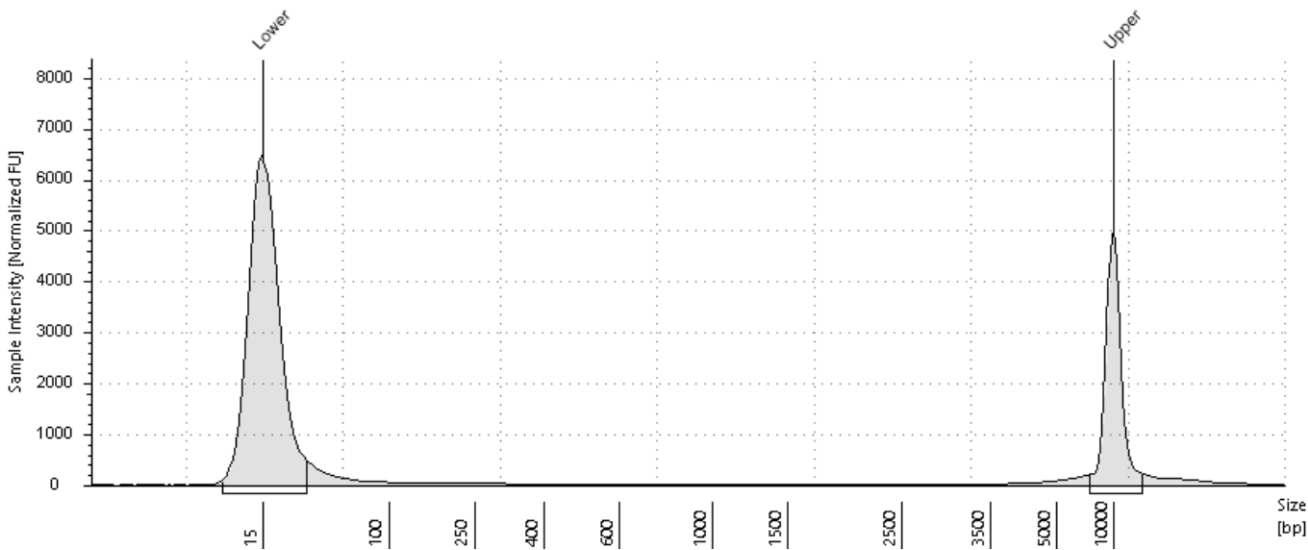

Sample Table

Well	Conc. [ng/μl]	Sample Description	Alert	Observations
E1		14		Caution! Expired ScreenTape device

Peak Table

Size [bp]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
15	9.02	-	925	-		Lower Marker
10000	3.25	3.25	0.500	-		Upper Marker