


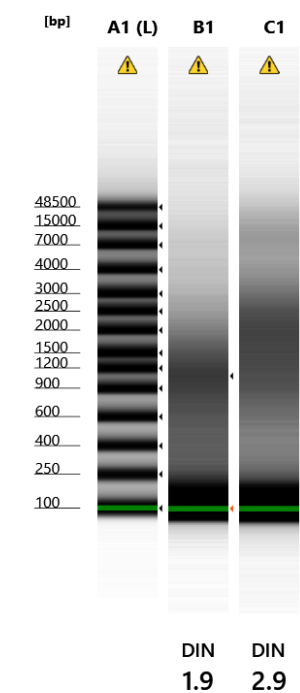


Filename: 2024-12-06 - 10.46.44.gDNA


Sample Info

Source	Well	DIN	Conc. [ng/ul]	Sample Description	Alert	Observations
	A1	-	85.1	Ladder		Caution! Expired ScreenTape device; Ladder
	B1	1.9	3.70	17		Caution! Expired ScreenTape device; Sample concentration outside functional range for DIN and the assay
	C1	2.9	3.18	18		Caution! Expired ScreenTape device; Sample concentration outside functional range for DIN and the assay



Default image (Contrast 100%), Image is Scaled to Sample

A1: Ladder

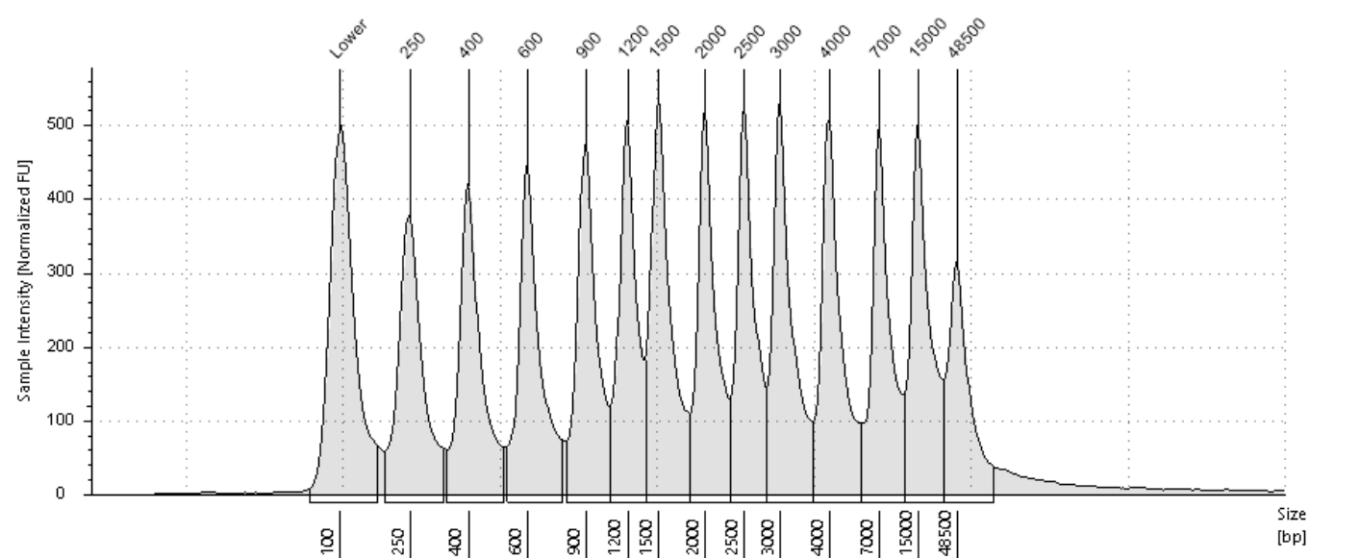


Sample Table

Source	Well	DIN	Conc. [ng/ul]	Sample Description	Alert	Observations
	A1	-	85.1	Ladder		Caution! Expired ScreenTape device; Ladder

Peak Table

Size [bp]	Calibrated Conc. [ng/ul]	Assigned Conc. [ng/ul]	% Integrated Area	From [bp]	To [bp]	Peak Molarity [nmol/l]	Peak Comment
100	8.50	8.50	-	67	164	131	
250	6.21	-	7.38	178	328	38.2	
400	6.25	-	7.43	335	507	24.0	
600	6.56	-	7.80	521	765	16.8	
900	6.41	-	7.61	786	1068	11.0	
1200	6.34	-	7.53	1068	1367	8.13	
1500	7.48	-	8.89	1367	1817	7.67	
2000	6.65	-	7.90	1817	2304	5.12	
2500	6.49	-	7.71	2304	2793	3.99	
3000	7.25	-	8.61	2793	3625	3.72	
4000	6.72	-	7.99	3625	5644	2.59	
7000	6.48	-	7.69	5644	11343	1.42	
15000	6.64	-	7.89	11343	24356	0.681	
48500	4.69	-	5.57	24356	79767	0.149	

B1: 17

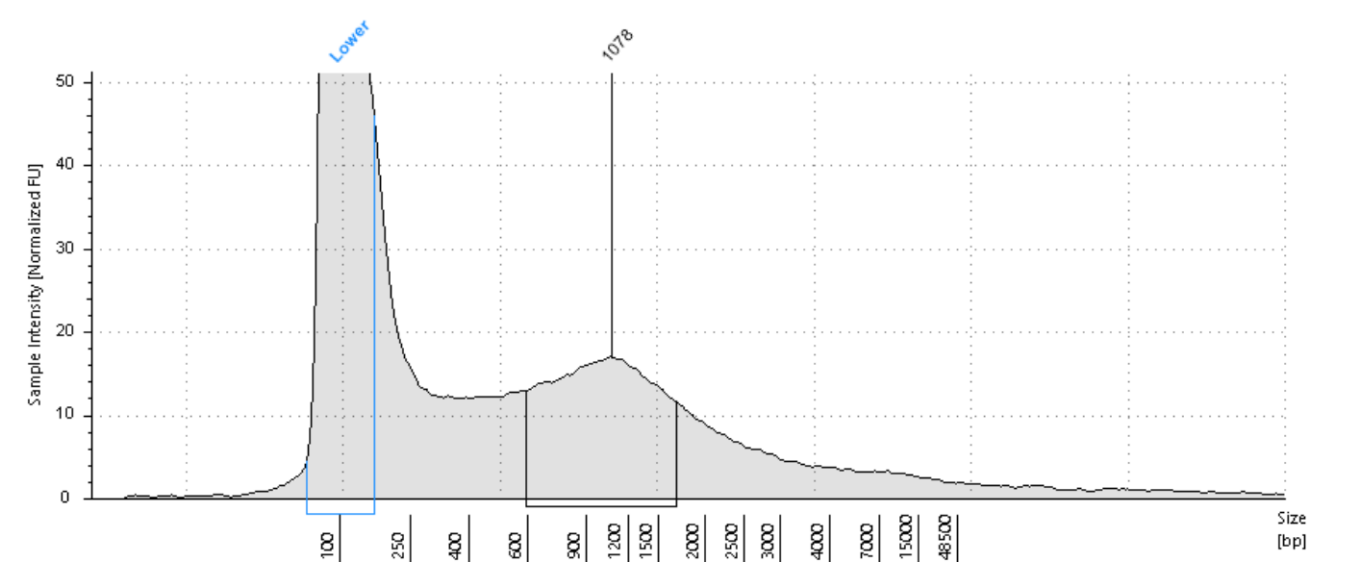


Sample Table

Source	Well	DIN	Conc. [ng/μl]	Sample Description	Alert	Observations
	B1	1.9	3.70	17		Caution! Expired ScreenTape device; Sample concentration outside functional range for DIN and the assay

Peak Table

Size [bp]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	% Integrated Area	From [bp]	To [bp]	Peak Molarity [nmol/l]	Peak Comment
100	8.50	8.50	-	65	157	131	
1078	1.39	-	100.00	592	1685	1.98	

C1: 18

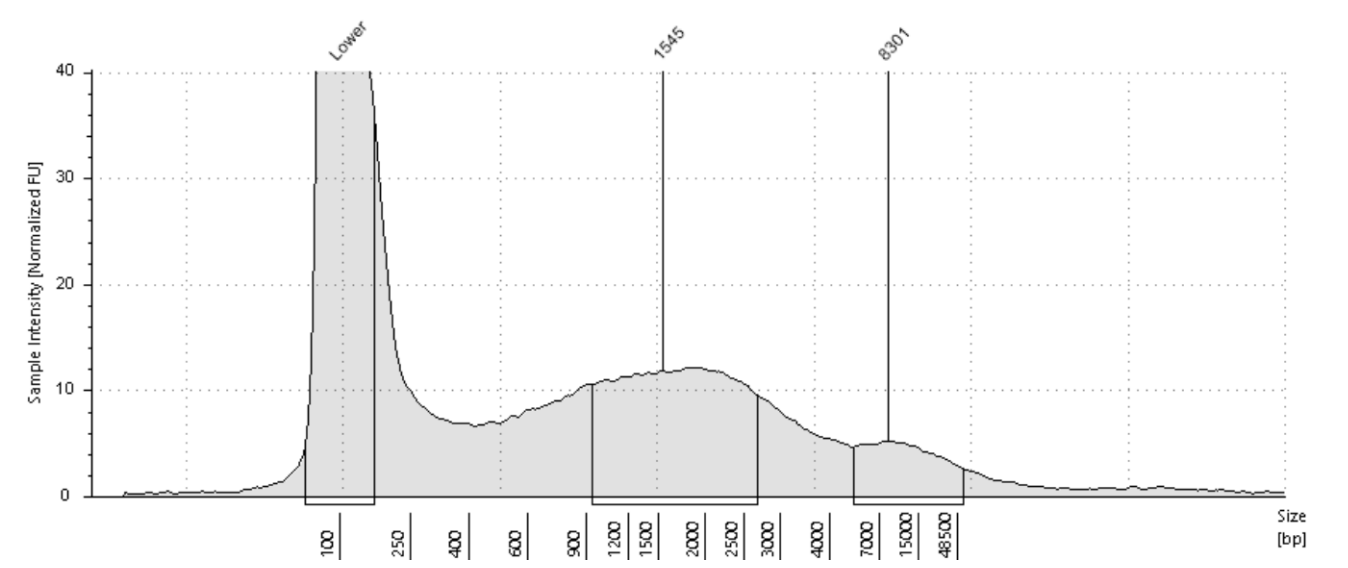

Sample Table

Source	Well	DIN	Conc. [ng/μl]	Sample Description	Alert	Observations
	C1	2.9	3.18	18		Caution! Expired ScreenTape device; Sample concentration outside functional range for DIN and the assay

Peak Table

Size [bp]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	% Integrated Area	From [bp]	To [bp]	Peak Molarity [nmol/l]	Peak Comment
100	8.50	8.50	-	64	157	131	
1545	1.15	-	80.86	939	2674	1.14	
8301	0.272	-	19.14	5232	53784	0.0504	