


Filename: 2025-08-18 - 15.33.41.D5000

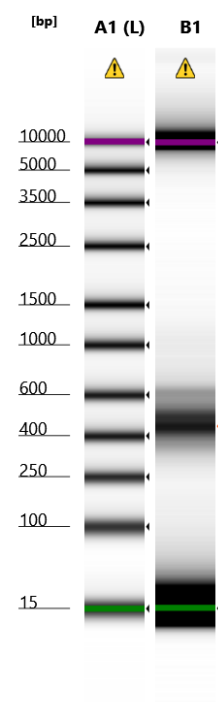


Default image (Contrast 50%), Image is Scaled to Sample

Sample Info

Well	Conc. [ng/μl]	Sample Description	Alert	Observations
A1	49.3	Ladder		Caution! Expired ScreenTape device (used after two weeks of first use); Ladder
B1	1.20	POOL		Caution! Expired ScreenTape device (used after two weeks of first use)

A1: Ladder

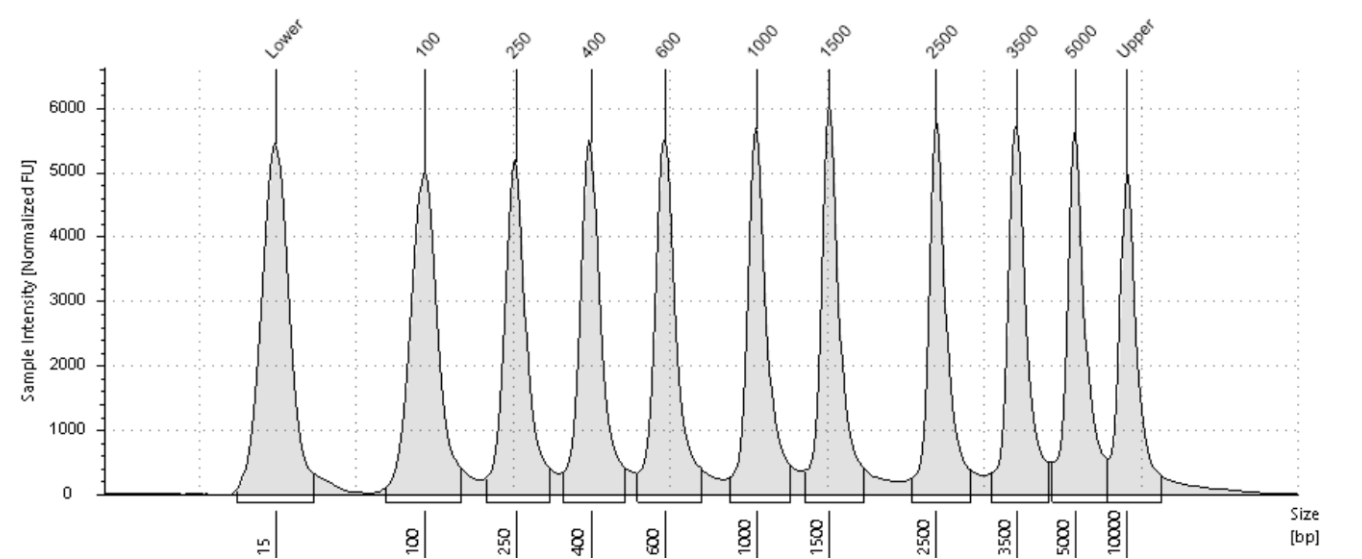


Sample Table

Well	Conc. [ng/μl]	Sample Description	Alert	Observations
A1	49.3	Ladder		Caution! Expired ScreenTape device (used after two weeks of first use); Ladder

Peak Table

Size [bp]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
15	6.67	-	684	-		Lower Marker
100	6.59	-	101	13.35		
250	5.54	-	34.1	11.23		
400	5.58	-	21.5	11.32		
600	5.56	-	14.3	11.28		
1000	5.46	-	8.40	11.08		
1500	5.47	-	5.61	11.08		
2500	5.01	-	3.09	10.17		
3500	5.06	-	2.22	10.26		
5000	5.05	-	1.55	10.24		
10000	3.25	3.25	0.500	-		Upper Marker

B1: POOL

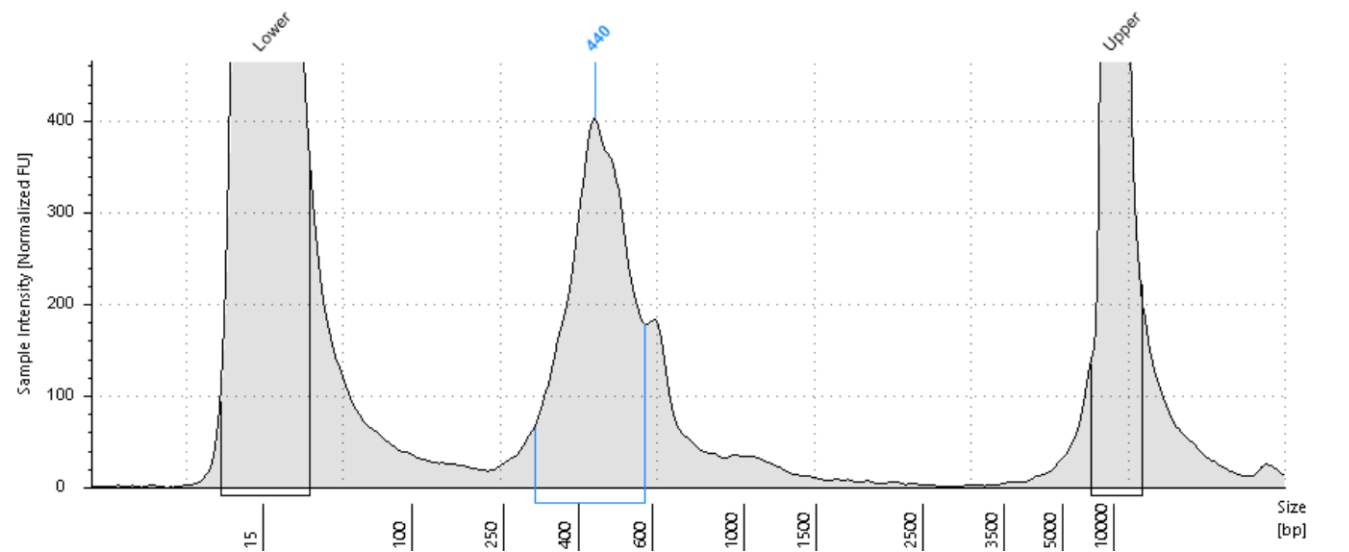

Sample Table

Well	Conc. [ng/μl]	Sample Description	Alert	Observations
B1	1.20	POOL		Caution! Expired ScreenTape device (used after two weeks of first use)

Peak Table

Size [bp]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
15	7.01	-	719	-		Lower Marker
440	1.20	-	4.19	100.00		
10000	3.25	3.25	0.500	-		Upper Marker