



Filename: 2025-08-21 - 11.44.07.gDNA

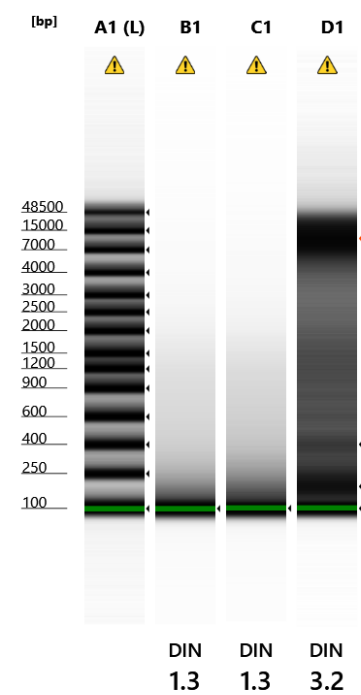

Default image (Contrast 100%)

Sample Info

Source	Well	DIN	Conc. [ng/ul]	Sample Description	Alert	Observations
	A1	-	69.3	Ladder	⚠	Caution! Expired ScreenTape device; Ladder
	B1	1.3	4.09	0819_1	⚠	Caution! Expired ScreenTape device; Sample concentration outside functional range for DIN and the assay
	C1	1.3	4.08	0819_3	⚠	Caution! Expired ScreenTape device; Sample concentration outside functional range for DIN and the assay
	D1	3.2	68.0	JA_E5_417	⚠	Caution! Expired ScreenTape device

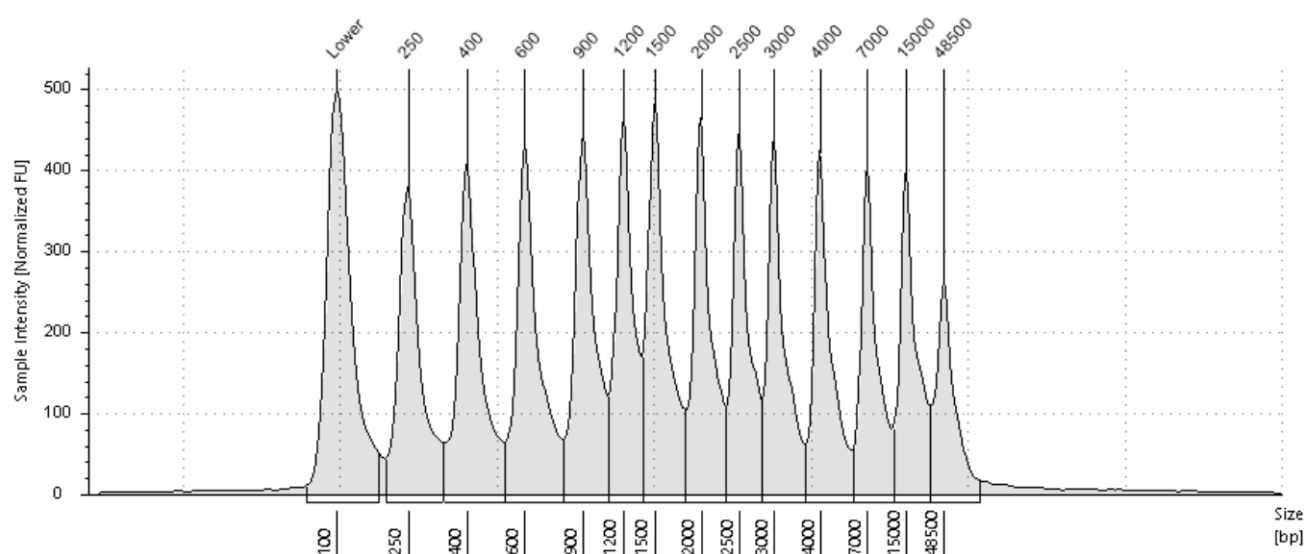
A1: Ladder**Sample Table**

Source	Well	DIN	Conc. [ng/ul]	Sample Description	Alert	Observations
	A1	-	69.3	Ladder	⚠	Caution! Expired ScreenTape device; Ladder

Peak Table

Size [bp]	Calibrated Conc. [ng/ul]	Assigned Conc. [ng/ul]	% Integrated Area	From [bp]	To [bp]	Peak Molarity [nmol/l]	Peak Comment
100	8.50	8.50	-	68	172	131	
250	5.58	-	8.03	187	328	34.3	
400	6.18	-	8.90	331	521	23.8	
600	6.48	-	9.34	521	784	16.6	
900	5.98	-	8.61	784	1080	10.2	
1200	5.66	-	8.15	1080	1380	7.25	
1500	6.30	-	9.08	1380	1812	6.47	
2000	5.68	-	8.18	1812	2315	4.37	
2500	5.08	-	7.32	2315	2817	3.13	
3000	5.19	-	7.48	2817	3654	2.66	
4000	4.86	-	7.00	3654	5966	1.87	
7000	4.45	-	6.42	5966	11635	0.979	
15000	4.62	-	6.66	11635	23761	0.474	
48500	3.36	-	4.83	23761	80804	0.106	

B1: 0819_1

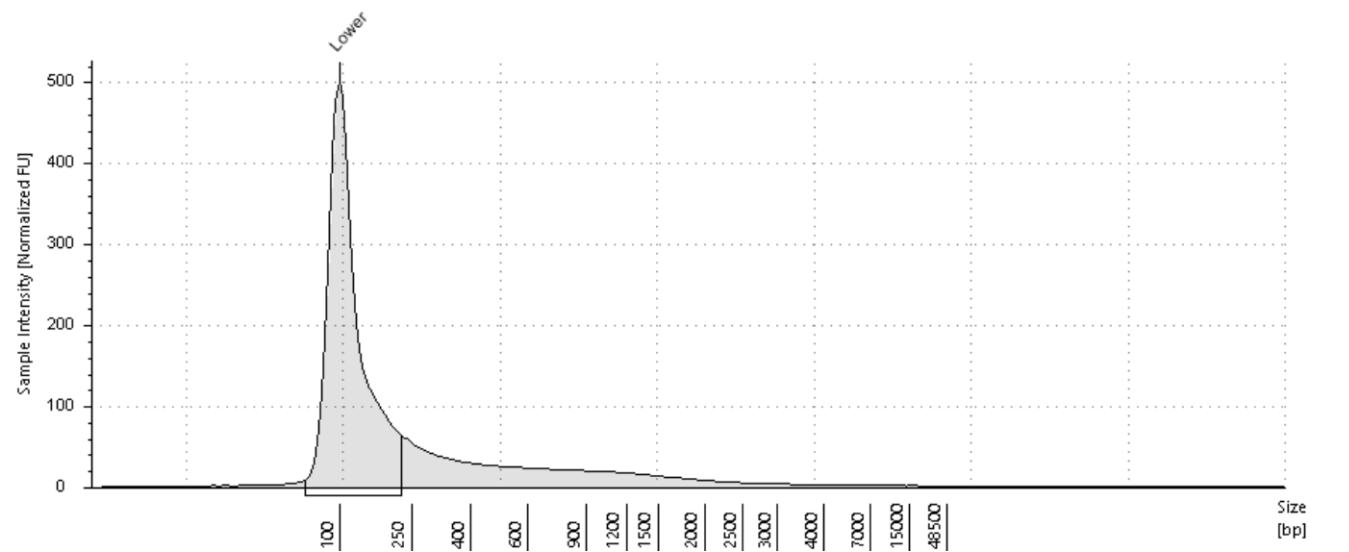


Sample Table

Source	Well	DIN	Conc. [ng/μl]	Sample Description	Alert	Observations
	B1	1.3	4.09	0819_1		Caution! Expired ScreenTape device; Sample concentration outside functional range for DIN and the assay

Peak Table

Size [bp]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	% Integrated Area	From [bp]	To [bp]	Peak Molarity [nmol/l]	Peak Comment
100	8.50	8.50	-	64	219	131	

C1: 0819_3

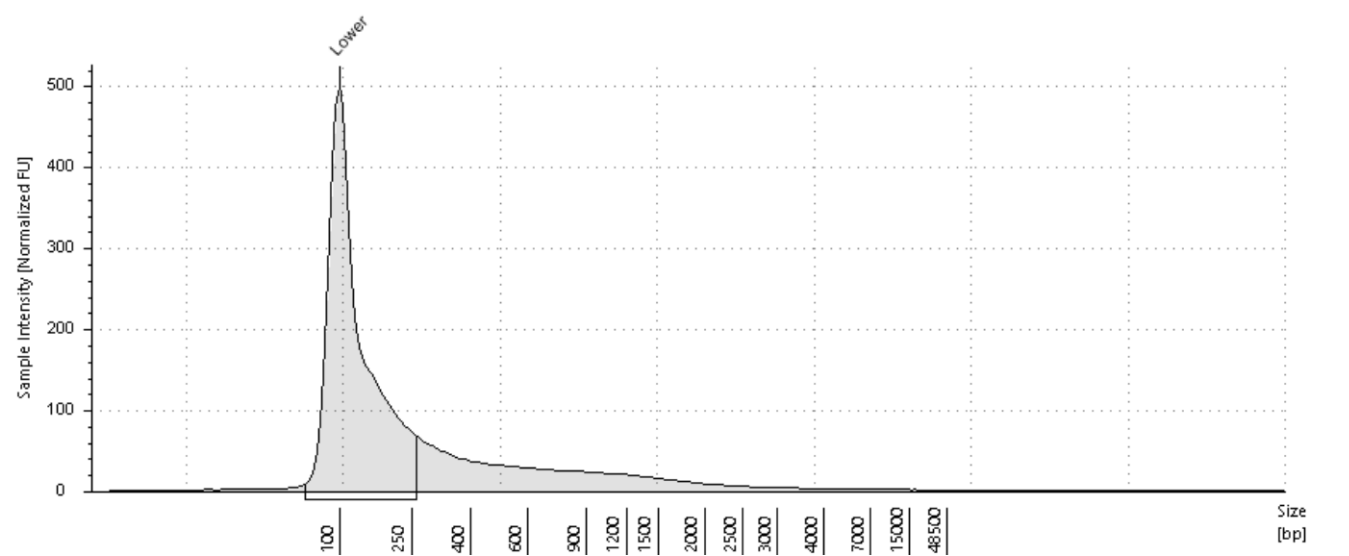


Sample Table

Source	Well	DIN	Conc. [ng/μl]	Sample Description	Alert	Observations
	C1	1.3	4.08	0819_3		Caution! Expired ScreenTape device; Sample concentration outside functional range for DIN and the assay

Peak Table

Size [bp]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	% Integrated Area	From [bp]	To [bp]	Peak Molarity [nmol/l]	Peak Comment
100	8.50	8.50	-	64	258	131	

D1: JA_E5_417

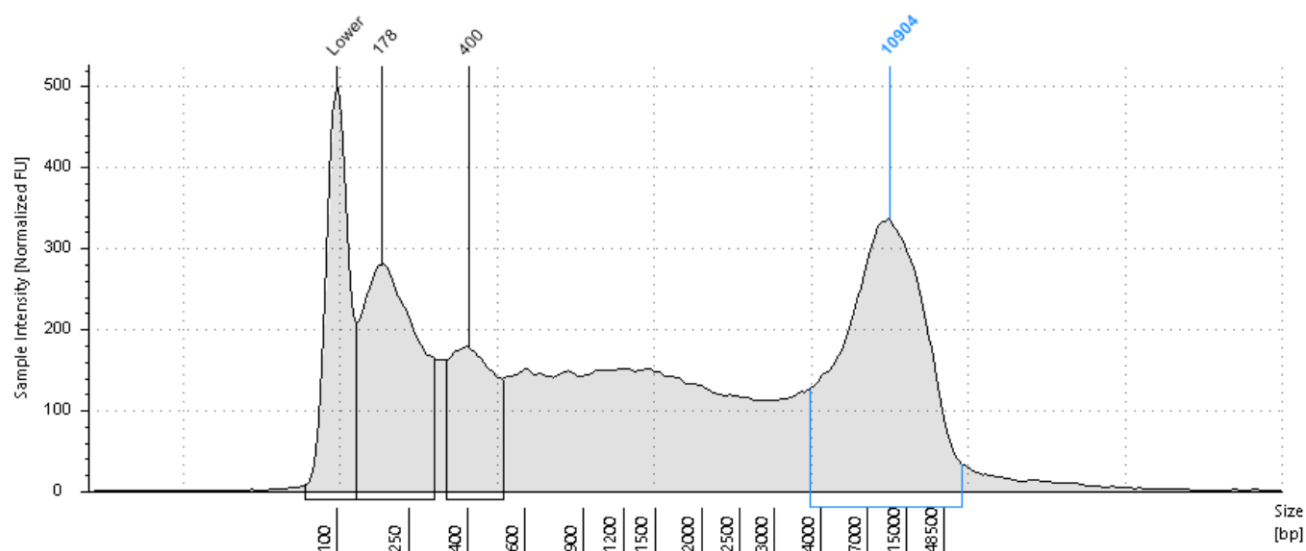

Sample Table

Source	Well	DIN	Conc. [ng/μl]	Sample Description	Alert	Observations
	D1	3.2	68.0	JA_E5_417	⚠	Caution! Expired ScreenTape device

Peak Table

Size [bp]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	% Integrated Area	From [bp]	To [bp]	Peak Molarity [nmol/l]	Peak Comment
100	8.50	8.50	-	67	129	131	
178	11.7	-	28.33	129	305	101	
400	6.21	-	15.04	335	512	23.8	
10904	20.8	-	50.50	3752	>60000	2.94	
-	-	-	-	-	-	-	