


Filename: 2026-06-21 - 13.58.09.HSRNA

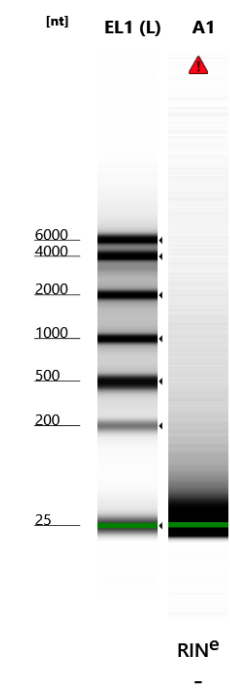


Default image (Contrast 100%), Image is Scaled to Sample

Sample Info

Well	RIN ^e	28S/18S (Area)	Conc. [pg/ul]	Sample Description	Alert	Observations
EL1	-	-	3750	Electronic Ladder		Ladder
A1	-	-	57.6	345_newtape	▲	Sample concentration outside functional range for RIN ^e and the assay

EL1: Electronic Ladder

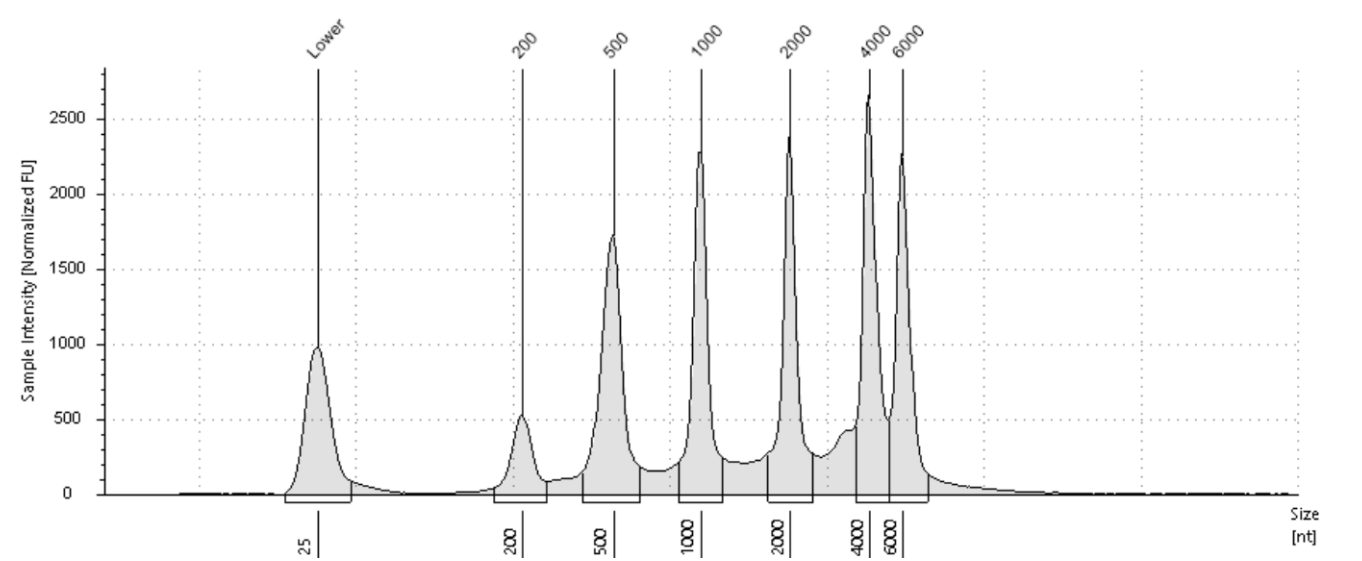


Sample Table

Well	RINe	28S/18S (Area)	Conc. [pg/ul]	Sample Description	Alert	Observations
EL1	-	-	3750	Electronic Ladder		Ladder

Peak Table

Size [nt]	Calibrated Conc. [pg/ul]	Assigned Conc. [pg/ul]	Peak Molarity [pmol/l]	% Integrated Area	Peak Comment	Observations
25	700	700	82400	-		Lower Marker
200	189	-	2770	5.98		
500	638	-	3760	20.25		
1000	557	-	1640	17.66		
2000	580	-	854	18.42		
4000	634	-	466	20.11		
6000	554	-	272	17.58		

A1: 345_newtape

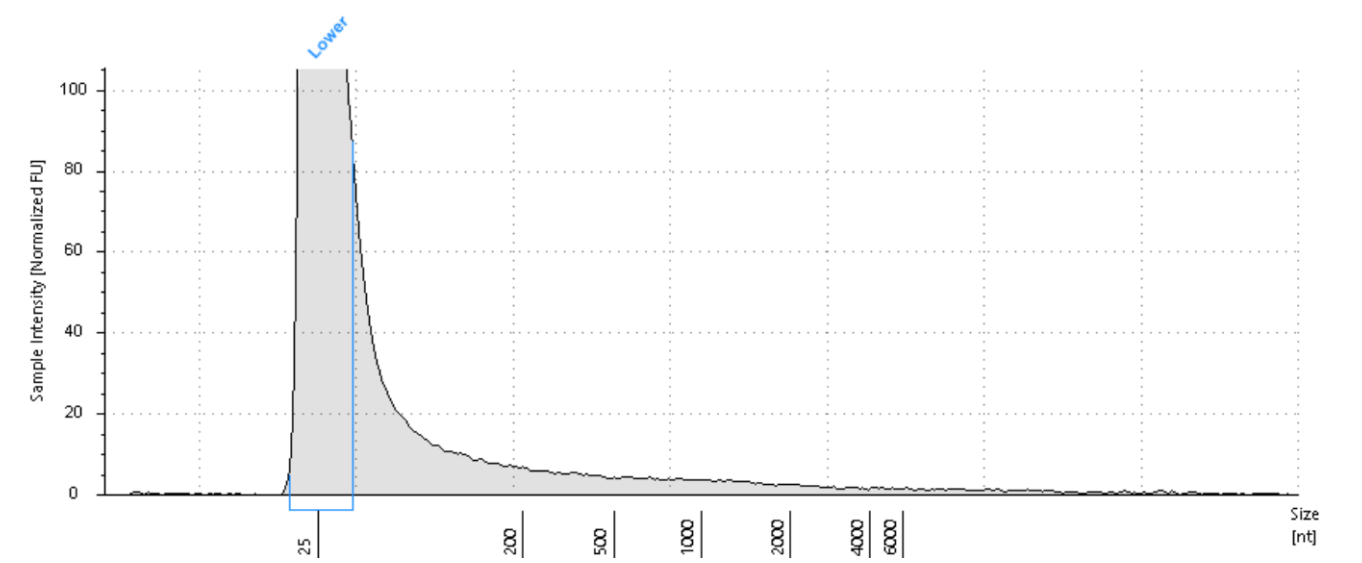


Sample Table

Well	RINe	28S/18S (Area)	Conc. [pg/ul]	Sample Description	Alert	Observations
A1	-	-	57.6	345_newtape		Sample concentration outside functional range for RINe and the assay

Peak Table


Size [nt]	Calibrated Conc. [pg/ul]	Assigned Conc. [pg/ul]	Peak Molarity [pmol/l]	% Integrated Area	Peak Comment	Observations
25	700	700	82400	-		Lower Marker

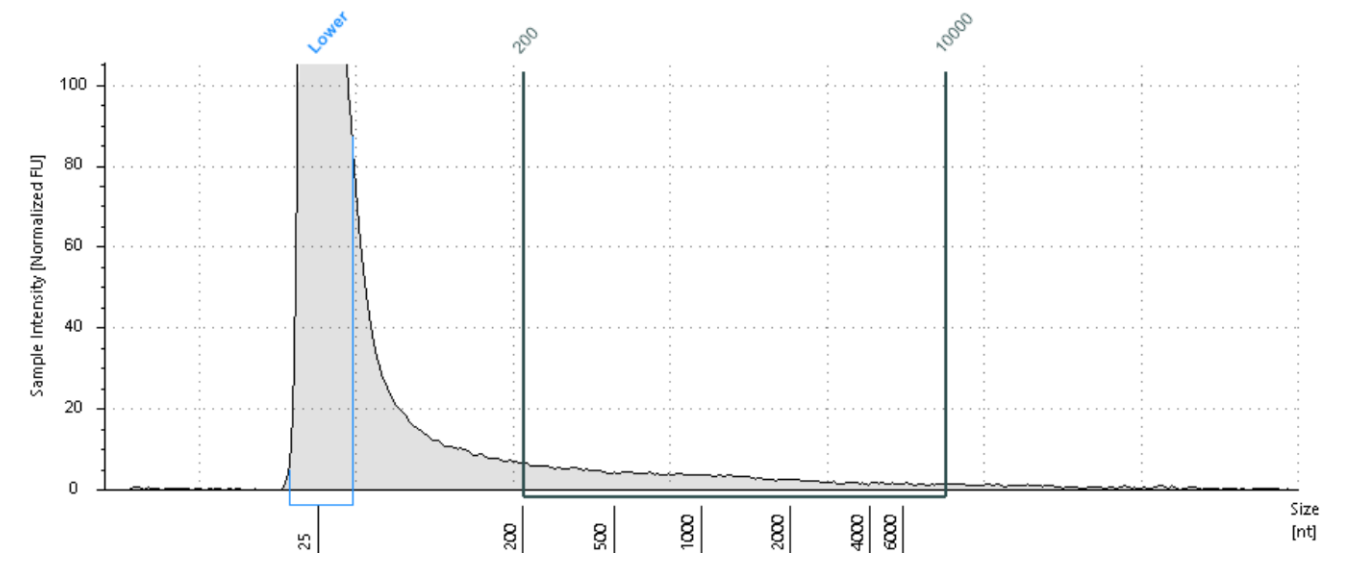

Region Table

From [nt]	To [nt]	Average Size [nt]	Conc. [pg/ul]	Region Molarity [pmol/l]	% of Total	Region Comment	Color
200	10000	3980	14.8	10.9	25.70	dv200	

Profile Comparison

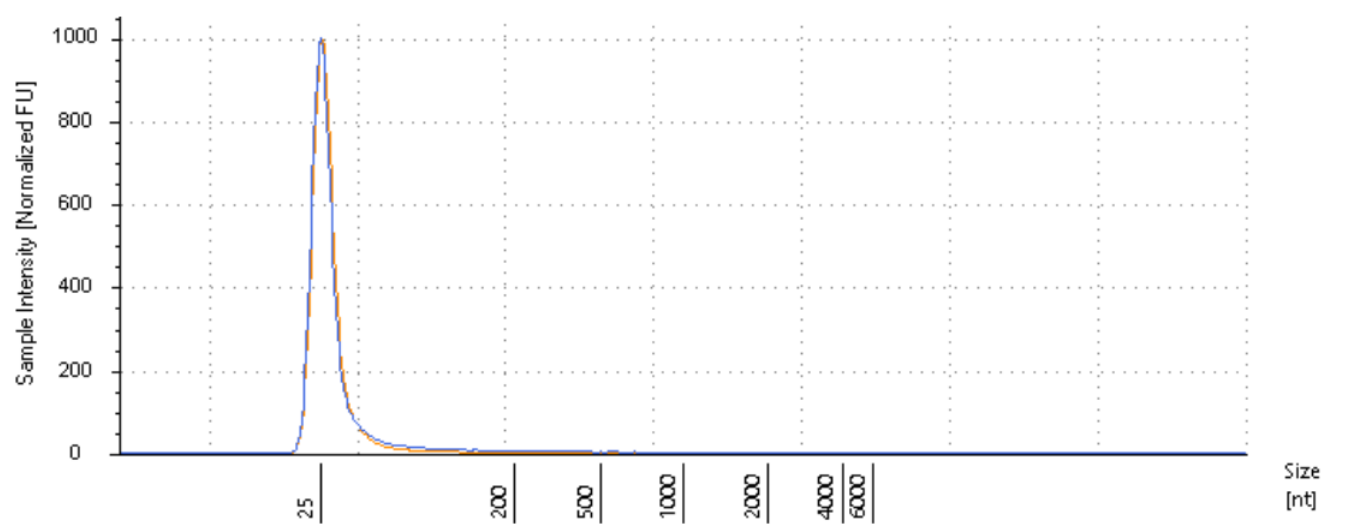

Samples

File	Indicator	Well ID	Comment
File 1		A1	345 newtape
File 2		D1	345

Files used in the Profile Comparison

File	Comments	Filename
File 1		C:\Users\admin\Documents\Agilent\TapeStation Data\2026-06-21\2026-06-21 - 13.58.09.HSRNA
File 2		C:\Users\admin\Documents\Agilent\TapeStation Data\2026-06-21\2026-06-21 - 12.13.23.HSRNA