



Filename: 2026-06-21 - 12.13.23.HSRNA

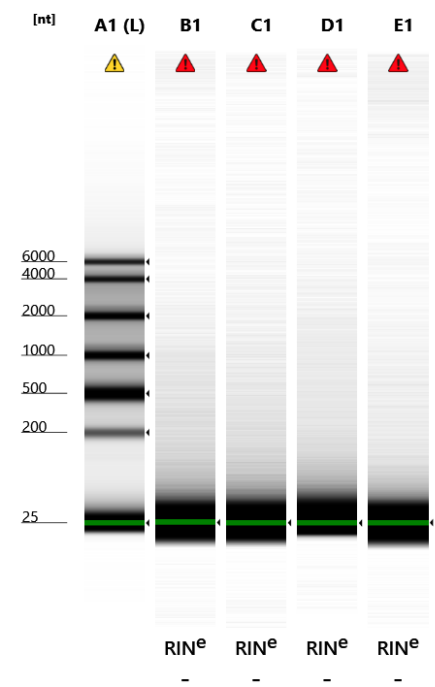

Sample Info

Well	RINe	28S/18S (Area)	Conc. [pg/ul]	Sample Description	Alert	Observations
A1	-	-	738	Ladder		Caution! Expired ScreenTape device (used after two weeks of first use); Ladder
B1	-	-	28.5	370		Caution! Expired ScreenTape device (used after two weeks of first use); Sample concentration outside functional range for RINe and the assay
C1	-	-	24.5	371		Caution! Expired ScreenTape device (used after two weeks of first use); Sample concentration outside functional range for RINe and the assay
D1	-	-	33.9	345		Caution! Expired ScreenTape device (used after two weeks of first use); Sample concentration outside functional range for RINe and the assay
E1	-	-	22.6	346		Caution! Expired ScreenTape device (used after two weeks of first use); Sample concentration outside functional range for RINe and the assay

A1: Ladder

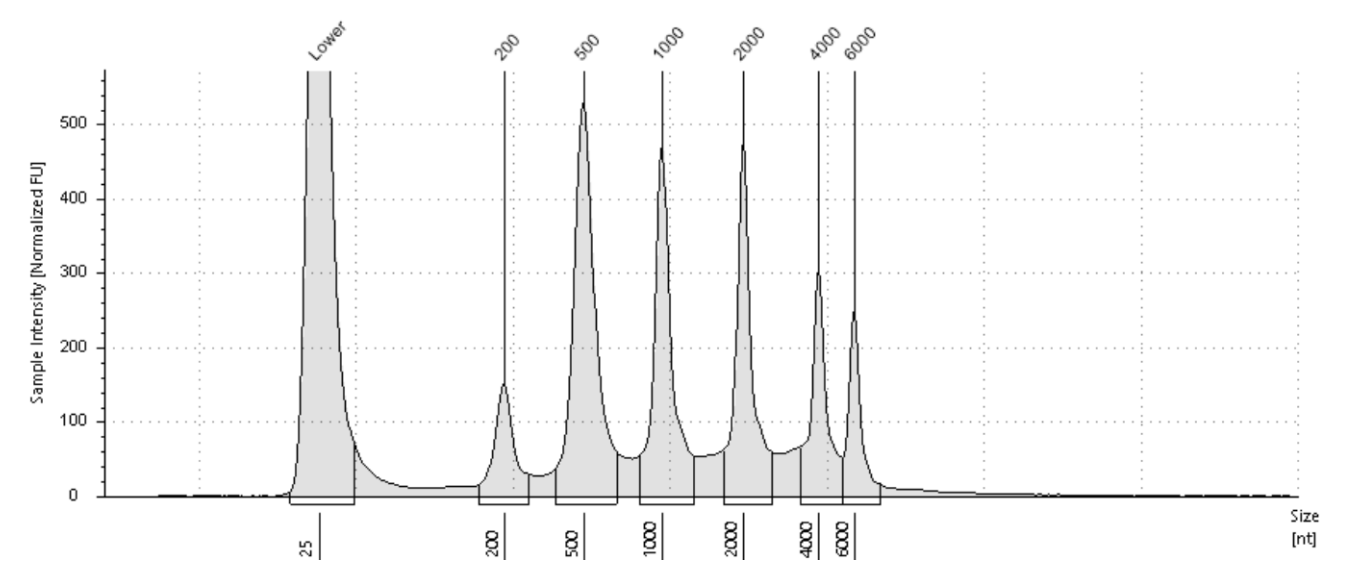


Sample Table

Well	RINe	28S/18S (Area)	Conc. [pg/ul]	Sample Description	Alert	Observations
A1	-	-	738	Ladder		Caution! Expired ScreenTape device (used after two weeks of first use); Ladder

Peak Table


Size [nt]	Calibrated Conc. [pg/ul]	Assigned Conc. [pg/ul]	Peak Molarity [pmol/l]	% Integrated Area	Peak Comment	Observations
25	700	700	82400	-		Lower Marker
200	49.0	-	721	7.88		
500	191	-	1120	30.69		
1000	131	-	385	21.06		
2000	121	-	178	19.44		
4000	78.0	-	57.4	12.53		
6000	52.3	-	25.6	8.40		

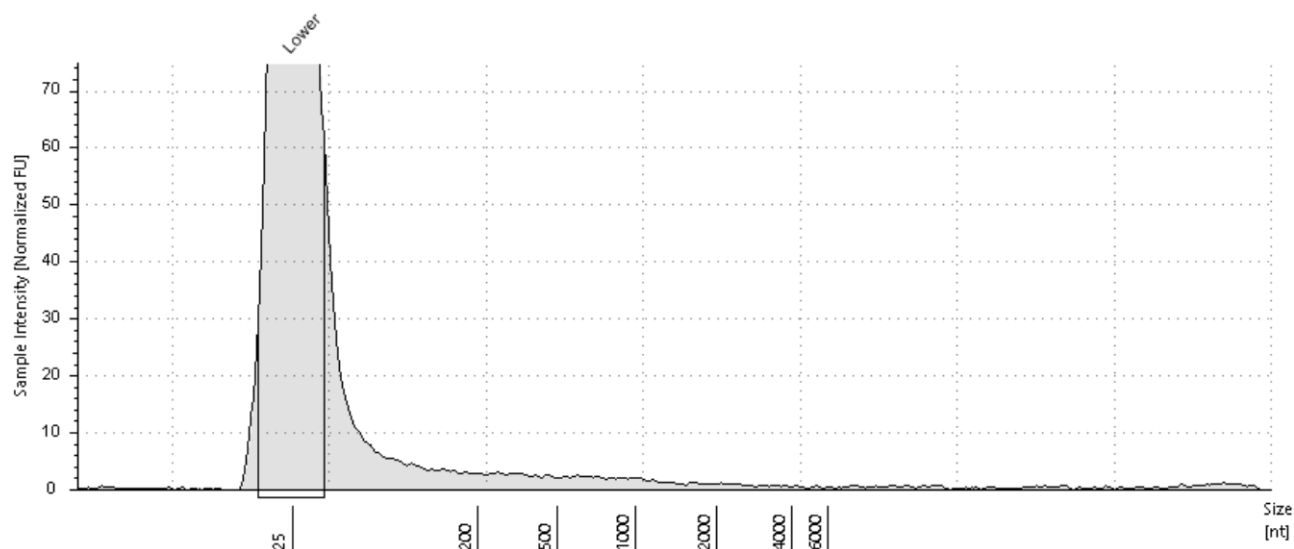B1: 370**Sample Table**

Well	RINe	28S/18S (Area)	Conc. [pg/ul]	Sample Description	Alert	Observations
B1	-	-	28.5	370	▲	Caution! Expired ScreenTape device (used after two weeks of first use); Sample concentration outside functional range for RINe and the assay


Peak Table

Size [nt]	Calibrated Conc. [pg/ul]	Assigned Conc. [pg/ul]	Peak Molarity [pmol/l]	% Integrated Area	Peak Comment	Observations
25	700	700	82400	-		Lower Marker

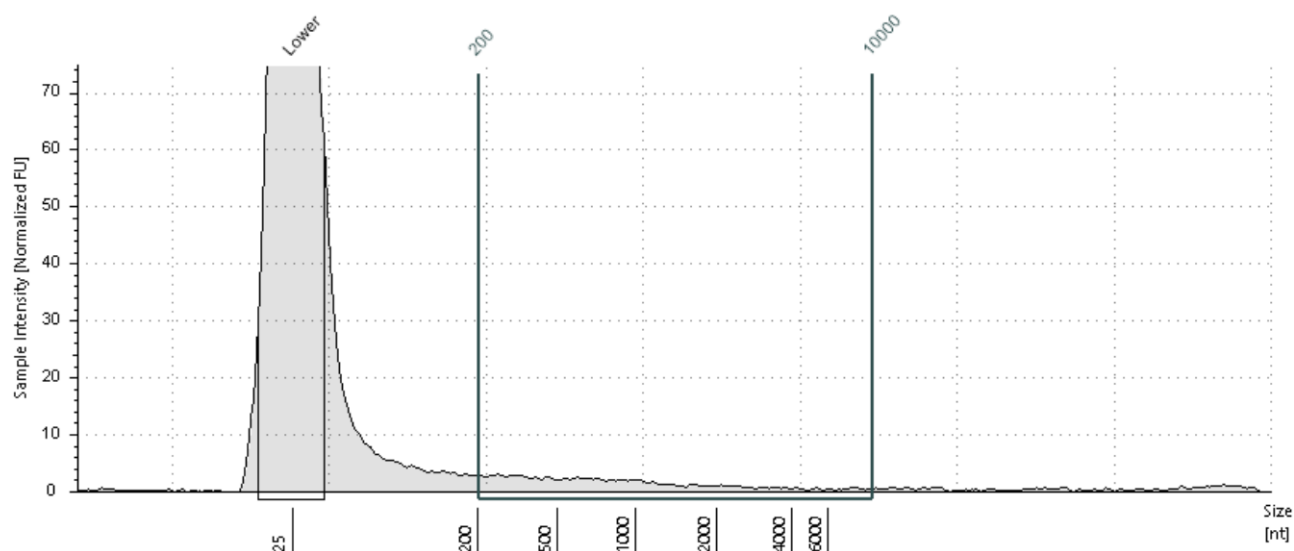**Region Table**

From [nt]	To [nt]	Average Size [nt]	Conc. [pg/ul]	Region Molarity [pmol/l]	% of Total	Region Comment	Color
200	10000	3547	5.40	4.47	18.96	dv200	■

C1: 371

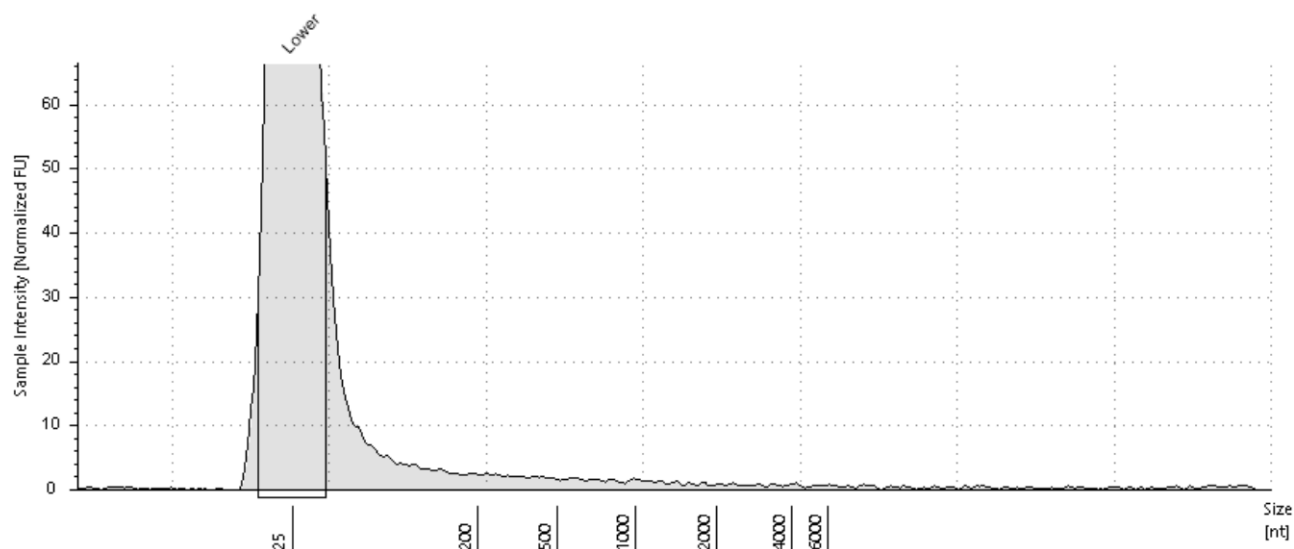


Sample Table

Well	RINe	28S/18S (Area)	Conc. [pg/ul]	Sample Description	Alert	Observations
C1	-	-	24.5	371	▲	Caution! Expired ScreenTape device (used after two weeks of first use); Sample concentration outside functional range for RINe and the assay

Peak Table


Size [nt]	Calibrated Conc. [pg/ul]	Assigned Conc. [pg/ul]	Peak Molarity [pmol/l]	% Integrated Area	Peak Comment	Observations
25	700	700	82400	-		Lower Marker

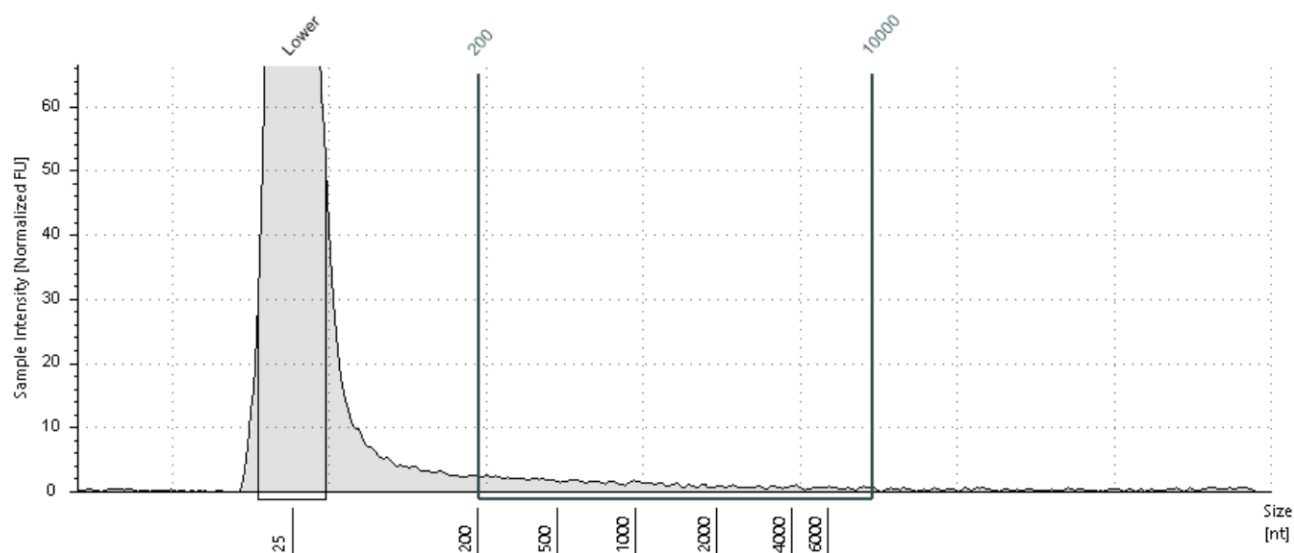

Region Table

From [nt]	To [nt]	Average Size [nt]	Conc. [pg/ul]	Region Molarity [pmol/l]	% of Total	Region Comment	Color
200	10000	4164	4.73	3.34	19.29	dv200	■

D1: 345

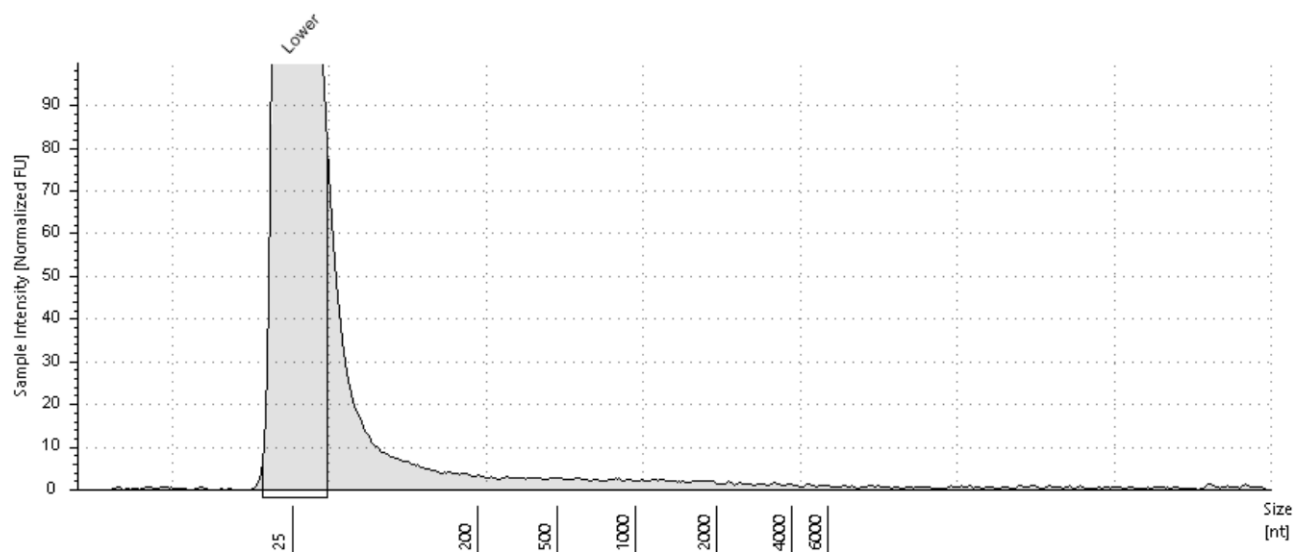


Sample Table

Well	RINe	28S/18S (Area)	Conc. [pg/ul]	Sample Description	Alert	Observations
D1	-	-	33.9	345	▲	Caution! Expired ScreenTape device (used after two weeks of first use); Sample concentration outside functional range for RINe and the assay

Peak Table


Size [nt]	Calibrated Conc. [pg/ul]	Assigned Conc. [pg/ul]	Peak Molarity [pmol/l]	% Integrated Area	Peak Comment	Observations
25	700	700	82400	-		Lower Marker

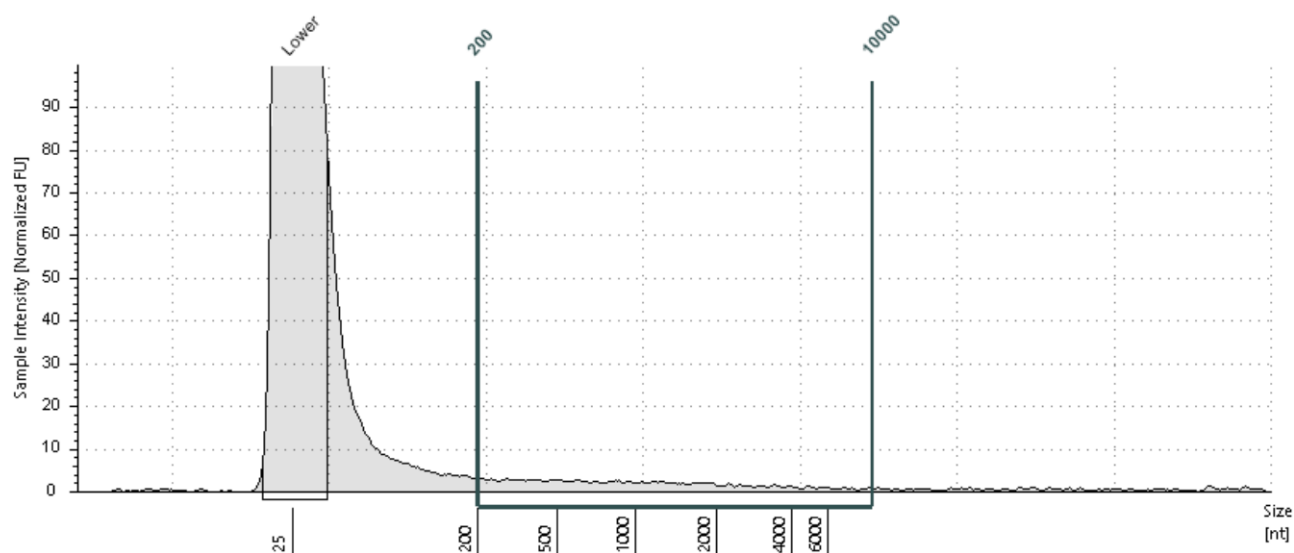

Region Table

From [nt]	To [nt]	Average Size [nt]	Conc. [pg/ul]	Region Molarity [pmol/l]	% of Total	Region Comment	Color
200	10000	3843	6.71	5.14	19.77	dv200	■

E1: 346

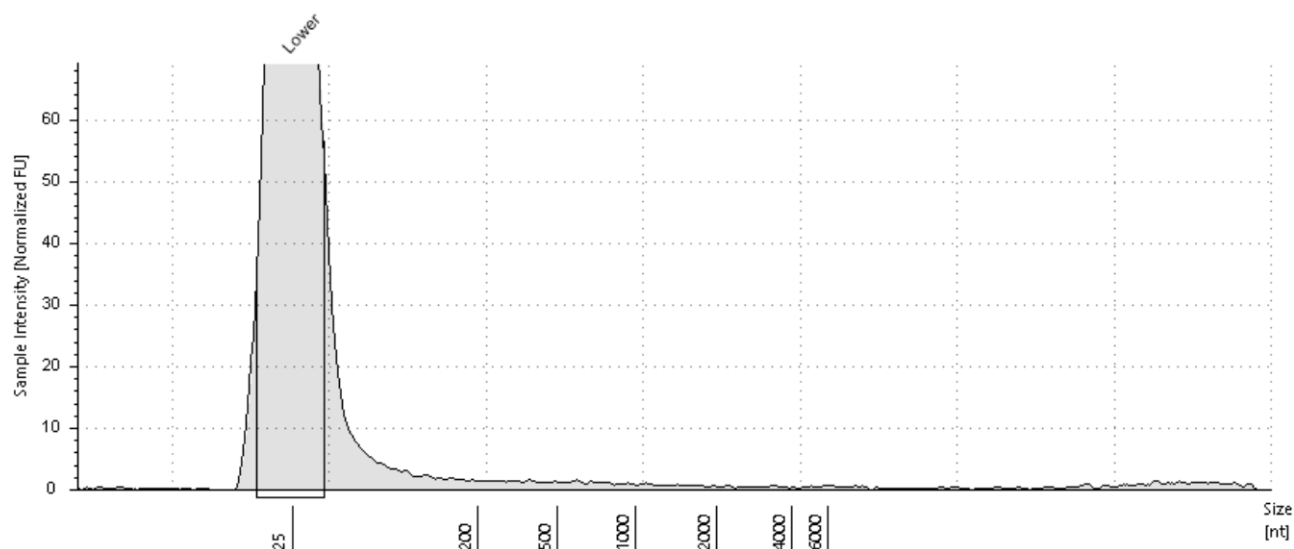


Sample Table

Well	RINe	28S/18S (Area)	Conc. [pg/ul]	Sample Description	Alert	Observations
E1	-	-	22.6	346	▲	Caution! Expired ScreenTape device (used after two weeks of first use); Sample concentration outside functional range for RINe and the assay

Peak Table


Size [nt]	Calibrated Conc. [pg/ul]	Assigned Conc. [pg/ul]	Peak Molarity [pmol/l]	% Integrated Area	Peak Comment	Observations
25	700	700	82400	-		Lower Marker

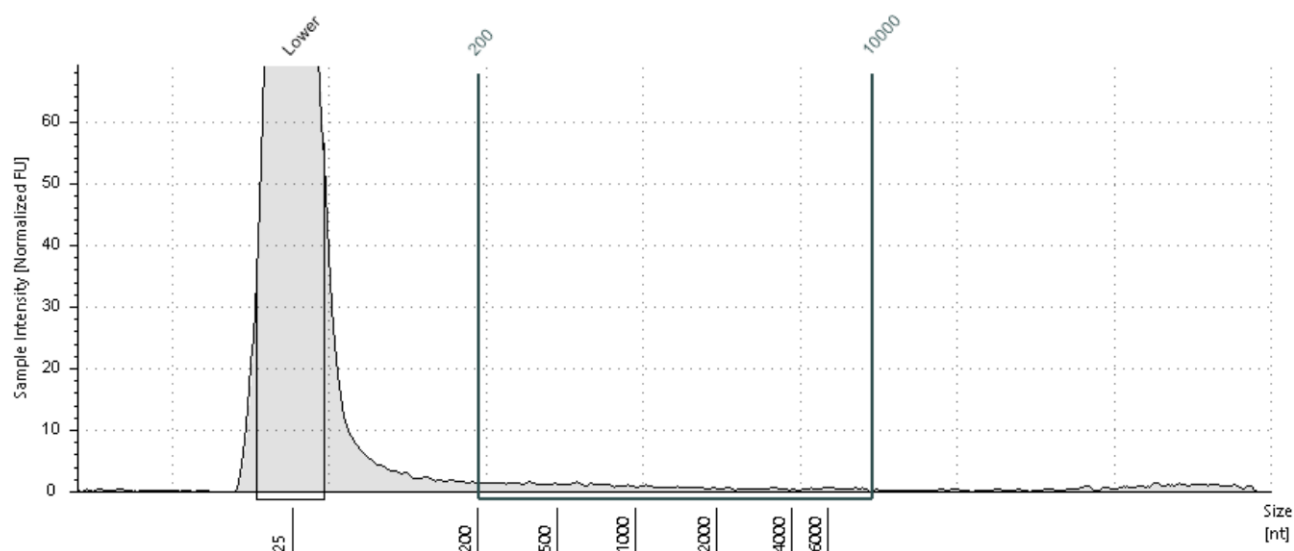

Region Table

From [nt]	To [nt]	Average Size [nt]	Conc. [pg/ul]	Region Molarity [pmol/l]	% of Total	Region Comment	Color
200	10000	4208	2.34	1.64	10.37	dv200	■

Profile Comparison

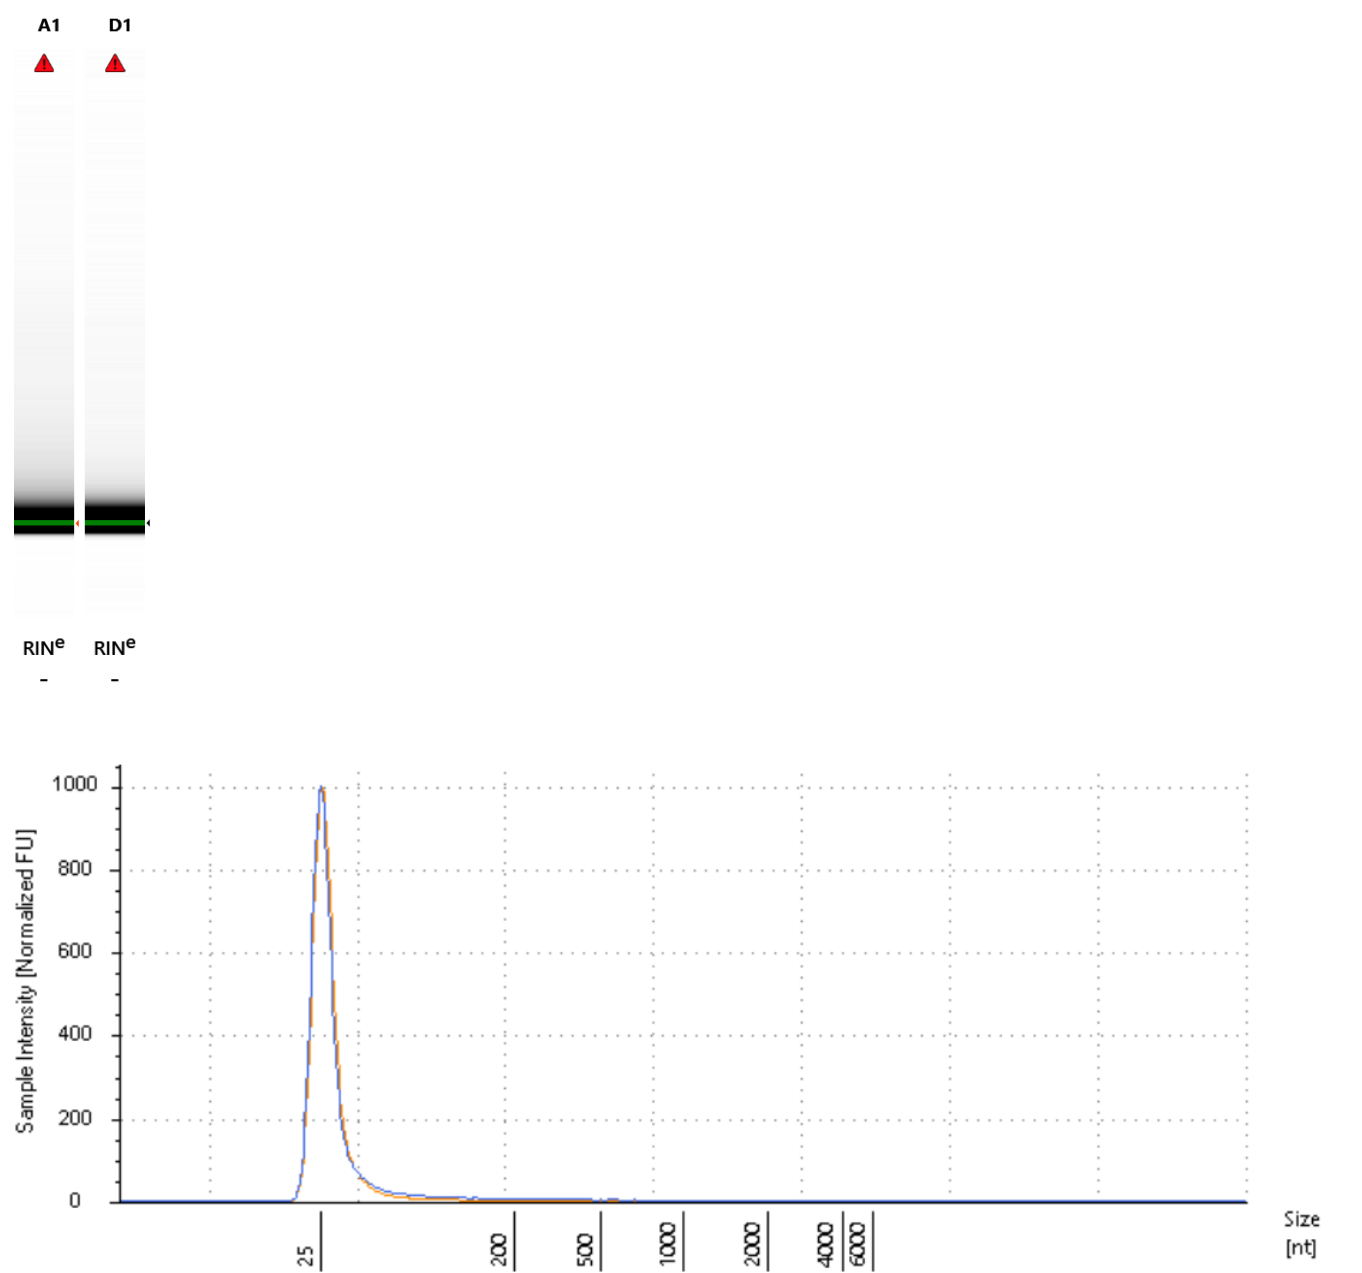

Samples

File	Indicator	Well ID	Comment
File 1		A1	345 newtape
File 2		D1	345

Files used in the Profile Comparison

File	Comments	Filename
File 1		C:\Users\admin\Documents\Agilent\TapeStation Data\2026-06-21\2026-06-21 - 13.58.09.HSRNA
File 2		C:\Users\admin\Documents\Agilent\TapeStation Data\2026-06-21\2026-06-21 - 12.13.23.HSRNA