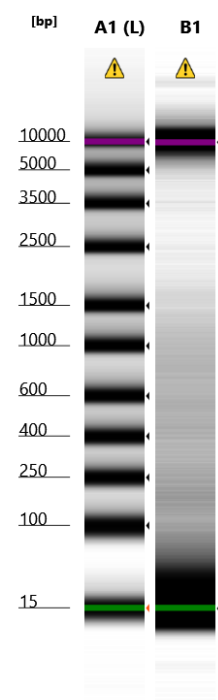


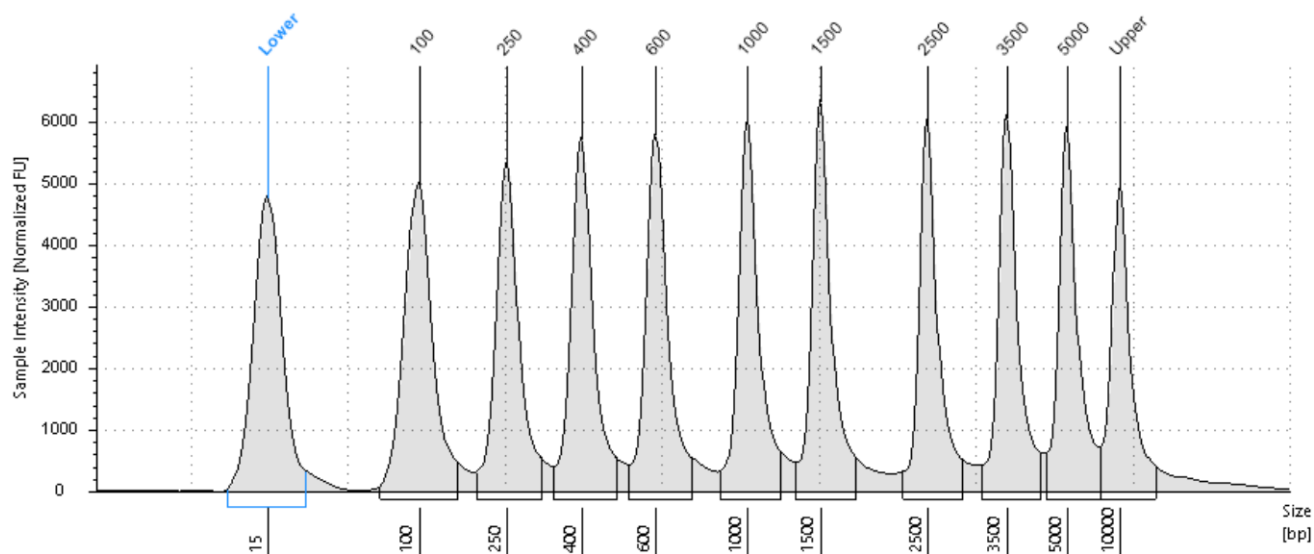
Filename: 2026-06-22 - 09.05.24.D5000



Default image (Contrast 100%), Image is Scaled to Sample

Sample Info

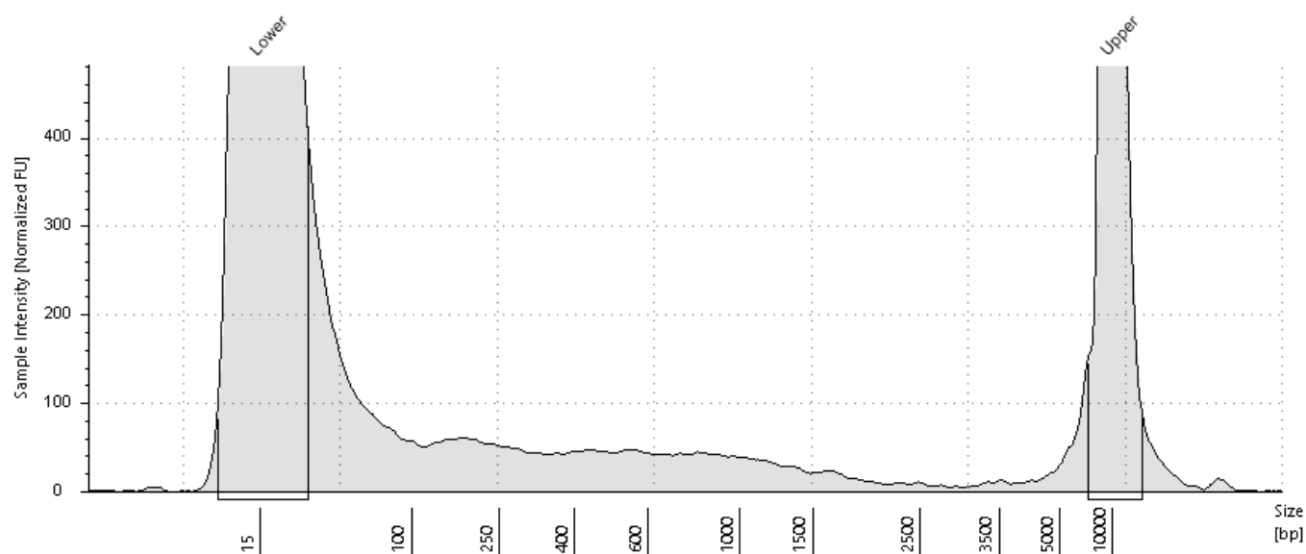
Well	Conc. [ng/μl]	Sample Description	Alert	Observations
A1	53.9	Ladder	⚠	Caution! Expired ScreenTape device; Ladder
B1		345_cDNA	⚠	Caution! Expired ScreenTape device

A1: Ladder**Sample Table**

Well	Conc. [ng/μl]	Sample Description	Alert	Observations
A1	53.9	Ladder		Caution! Expired ScreenTape device; Ladder

Peak Table

Size [bp]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
15	6.04	-	619	-		Lower Marker
100	6.88	-	106	12.77		
250	6.00	-	36.9	11.12		
400	6.14	-	23.6	11.38		
600	6.10	-	15.7	11.32		
1000	6.05	-	9.31	11.22		
1500	6.09	-	6.24	11.29		
2500	5.52	-	3.39	10.23		
3500	5.65	-	2.48	10.47		
5000	5.51	-	1.70	10.22		
10000	3.25	3.25	0.500	-		Upper Marker

B1: 345_cDNA**Sample Table**

Well	Conc. [ng/μl]	Sample Description	Alert	Observations
B1		345_cDNA		Caution! Expired ScreenTape device

Peak Table

Size [bp]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
15	6.41	-	658	-		Lower Marker
10000	3.25	3.25	0.500	-		Upper Marker