



Filename: 2026-06-22 - 17.01.11.D5000

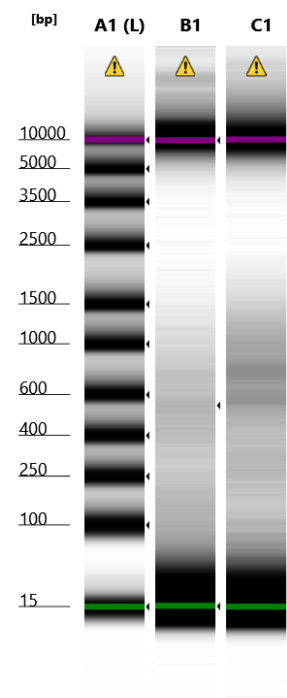

Default image (Contrast 100%), Image is Scaled to Sample

Sample Info

Well	Conc. [ng/μl]	Sample Description	Alert	Observations
A1	66.8	Ladder		Caution! Expired ScreenTape device; Ladder
B1	0.465	362		Caution! Expired ScreenTape device
C1	0.642	363		Caution! Expired ScreenTape device

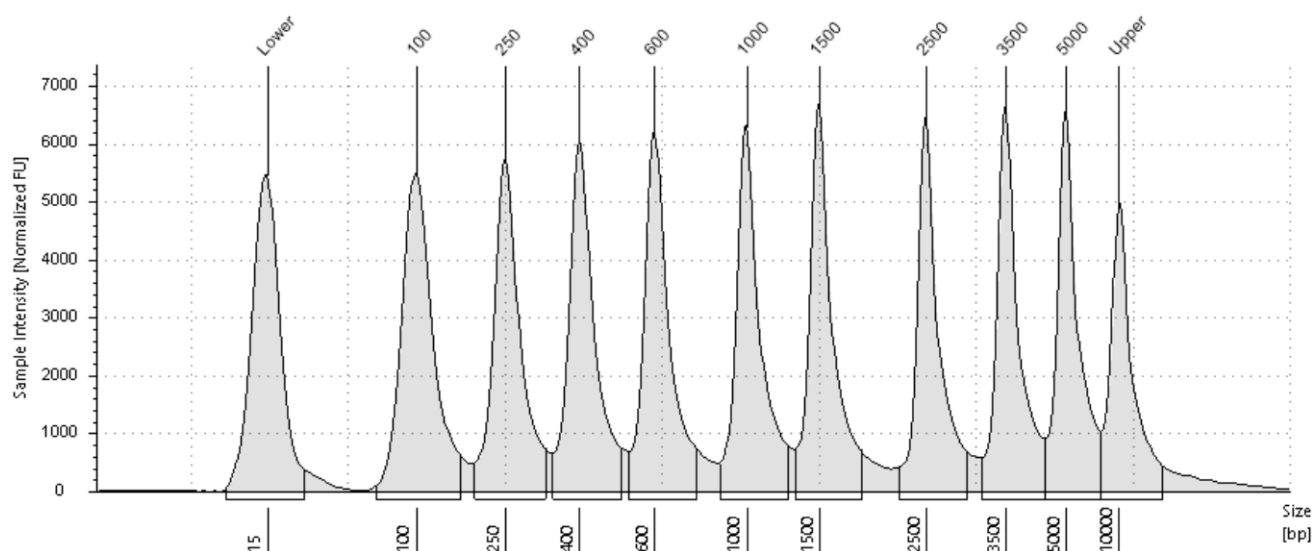
A1: Ladder**Sample Table**

Well	Conc. [ng/μl]	Sample Description	Alert	Observations
A1	66.8	Ladder		Caution! Expired ScreenTape device; Ladder

Peak Table

Size [bp]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
15	6.86	-	703	-		Lower Marker
100	8.44	-	130	12.63		
250	7.51	-	46.2	11.25		
400	7.63	-	29.3	11.42		
600	7.55	-	19.4	11.30		
1000	7.51	-	11.6	11.25		
1500	7.51	-	7.70	11.25		
2500	6.84	-	4.21	10.24		
3500	6.97	-	3.06	10.44		
5000	6.83	-	2.10	10.22		
10000	3.25	3.25	0.500	-		Upper Marker

B1: 362

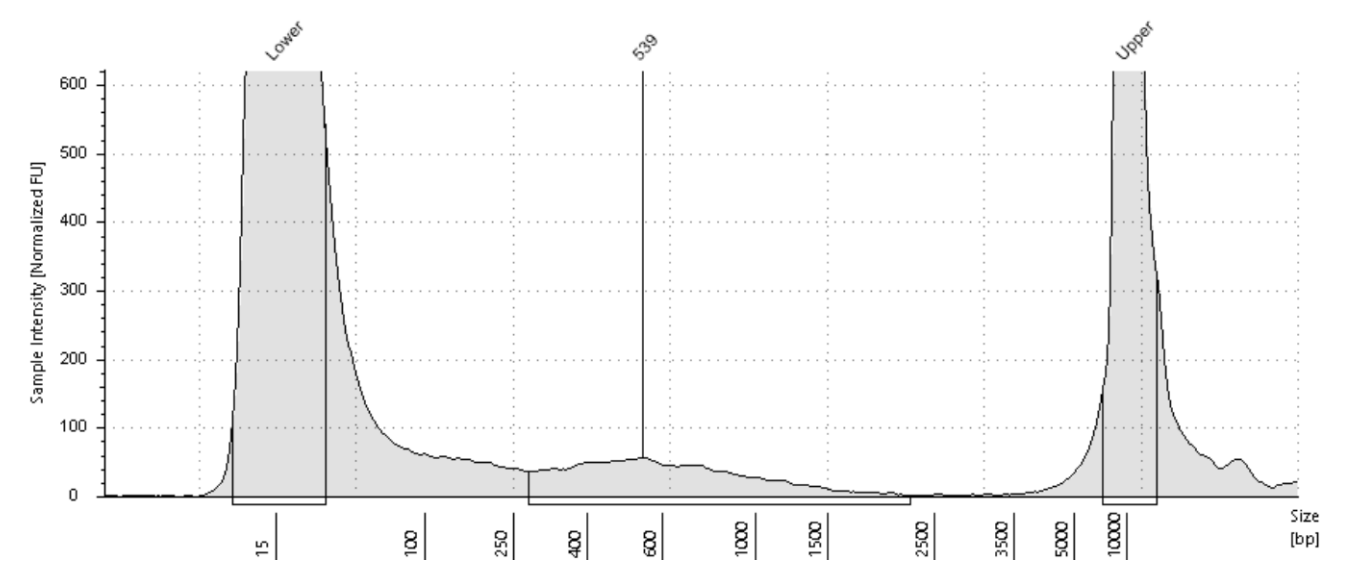


Sample Table

Well	Conc. [ng/μl]	Sample Description	Alert	Observations
B1	0.465	362		Caution! Expired ScreenTape device

Peak Table

Size [bp]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
15	7.69	-	789	-		Lower Marker
539	0.465	-	1.33	100.00		
10000	3.25	3.25	0.500	-		Upper Marker

C1: 363

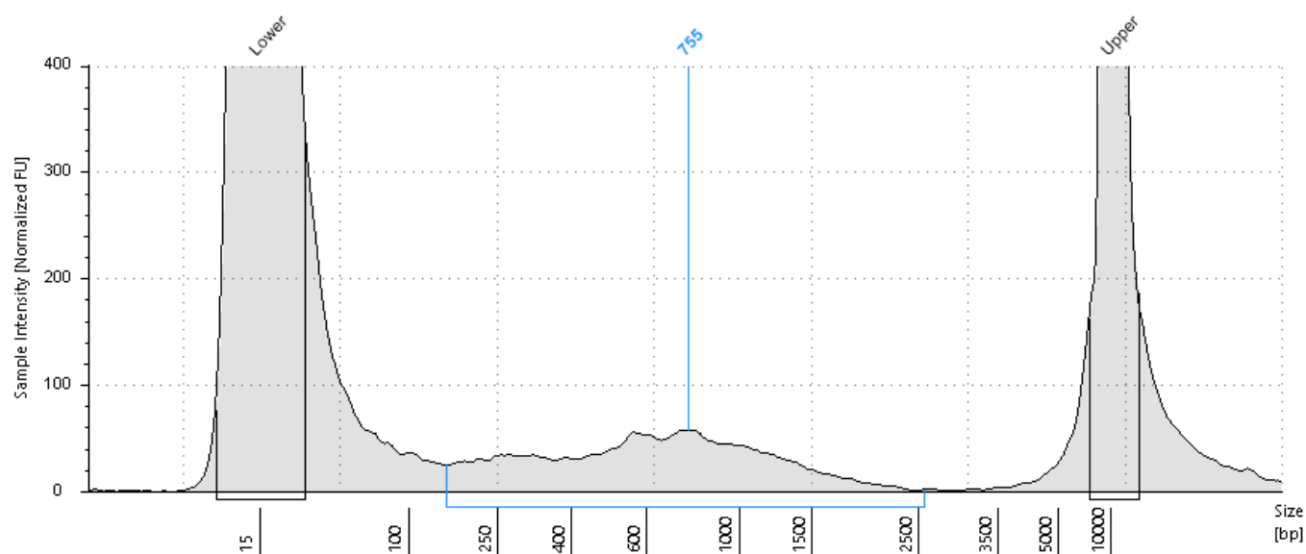



Sample Table

Well	Conc. [ng/μl]	Sample Description	Alert	Observations
C1	0.642	363	⚠	Caution! Expired ScreenTape device

Peak Table

Size [bp]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
15	6.75	-	692	-		Lower Marker
755	0.642	-	1.31	100.00		
10000	3.25	3.25	0.500	-		Upper Marker

Profile Comparison

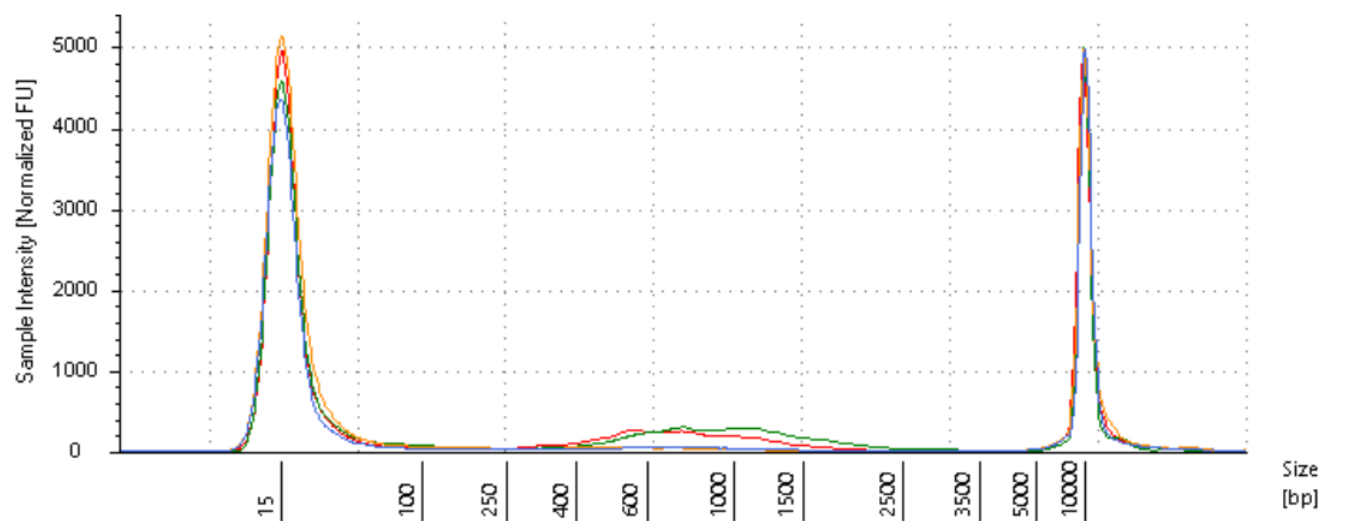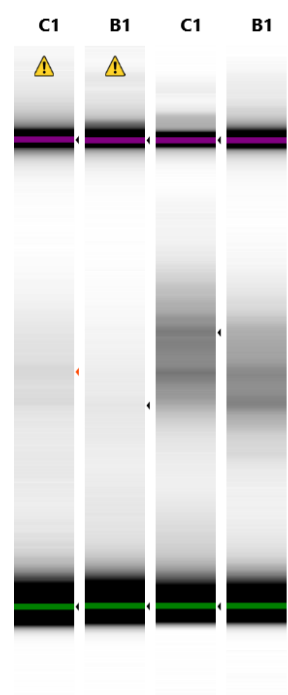

Samples

File	Indicator	Well ID	Comment
File 1		C1	363
File 1		B1	362
File 2		C1	2_34
File 2		B1	1_13

Files used in the Profile Comparison

File	Comments	Filename
File 1		C:\Users\admin\Documents\Agilent\TapeStation Data\2026-06-22\2026-06-22 - 17.01.11.D5000
File 2		C:\Users\admin\Documents\Agilent\TapeStation Data\2026-05-15\2026-05-15 - 12.49.08.D5000