


Filename: 2026-05-08 - 11.58.20.RNA

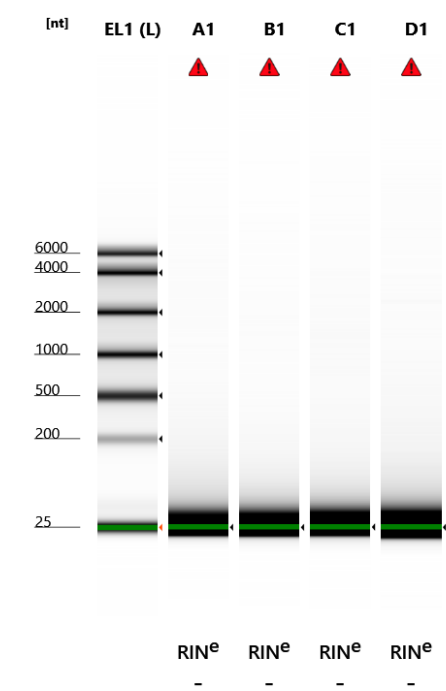


Default image (Contrast 50%), Image is Scaled to Sample

Sample Info

Well	RINe	28S/18S (Area)	Conc. [ng/ul]	Sample Description	Alert	Observations
EL1	-	-	84.9	Electronic Ladder		Ladder
A1	-	-	2.65	21_elution2	▲	Caution! Expired ScreenTape device; Sample concentration outside functional range for RINe and the assay
B1	-	-	2.00	22	▲	Caution! Expired ScreenTape device; Sample concentration outside functional range for RINe and the assay
C1	-	-	2.10	24	▲	Caution! Expired ScreenTape device; Sample concentration outside functional range for RINe and the assay
D1	-	-	1.87	24_elution2	▲	Caution! Expired ScreenTape device; Sample concentration outside functional range for RINe and the assay

EL1: Electronic Ladder

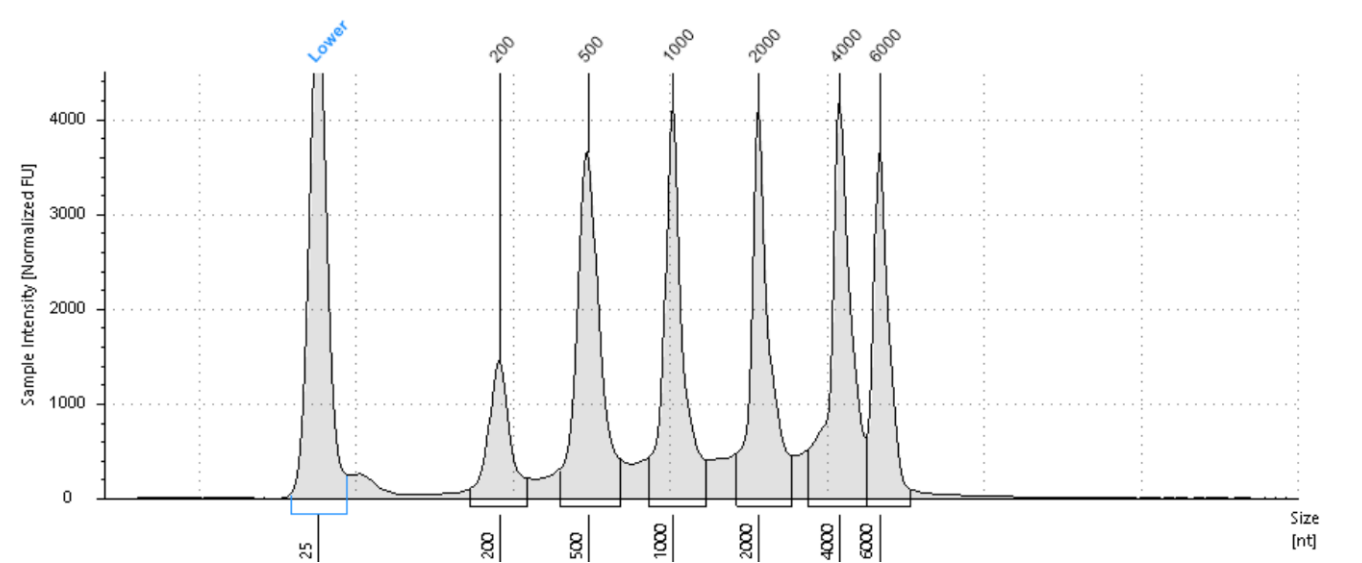


Sample Table

Well	RINe	28S/18S (Area)	Conc. [ng/ul]	Sample Description	Alert	Observations
EL1	-	-	84.9	Electronic Ladder		Ladder

Peak Table

Size [nt]	Calibrated Conc. [ng/ul]	Assigned Conc. [ng/ul]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
25	40.0	40.0	4710	-		Lower Marker
200	5.94	-	87.4	7.80		
500	15.9	-	93.6	20.88		
1000	14.2	-	41.8	18.62		
2000	13.8	-	20.3	18.11		
4000	15.5	-	11.4	20.38		
6000	10.8	-	5.31	14.22		

A1: 21_elution2

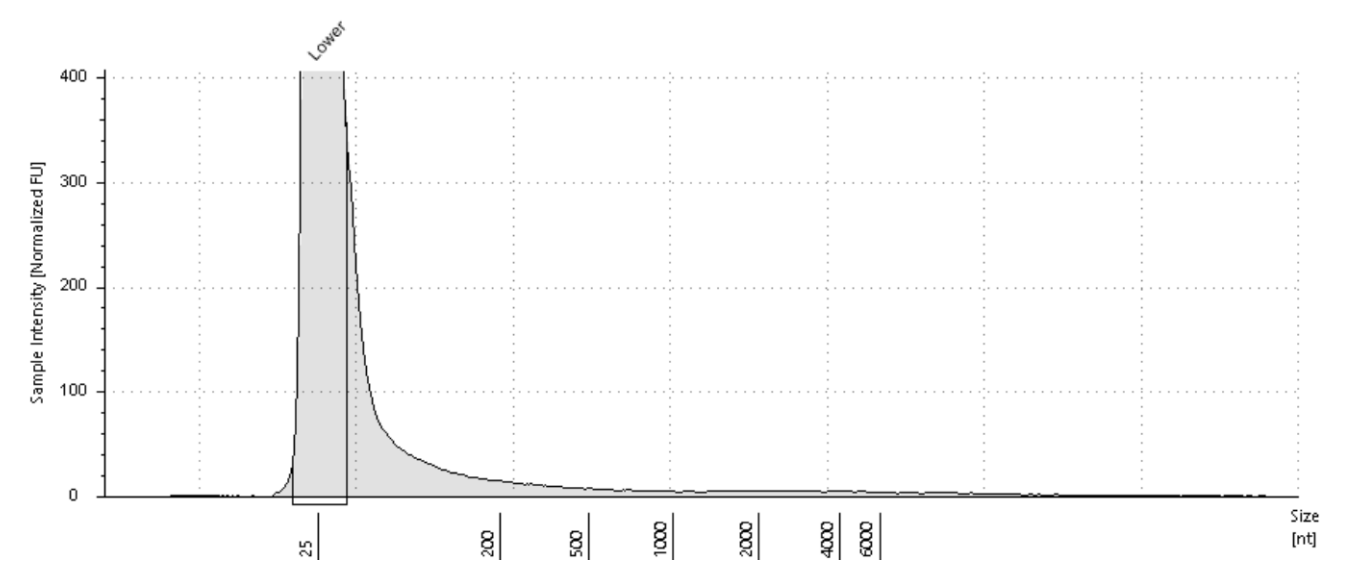


Sample Table

Well	RINe	28S/18S (Area)	Conc. [ng/µl]	Sample Description	Alert	Observations
A1	-	-	2.65	21_elution2		Caution! Expired ScreenTape device; Sample concentration outside functional range for RINe and the assay

Peak Table

Size [nt]	Calibrated Conc. [ng/µl]	Assigned Conc. [ng/µl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
25	40.0	40.0	4710	-		Lower Marker

B1: 22

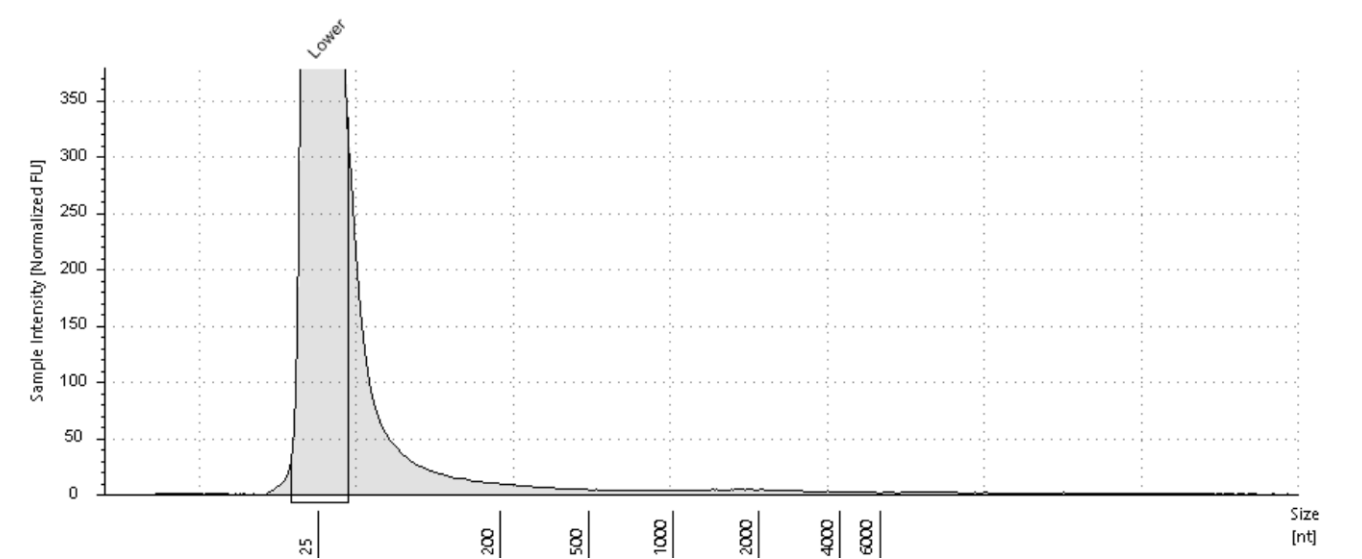


Sample Table

Well	RINe	28S/18S (Area)	Conc. [ng/μl]	Sample Description	Alert	Observations
B1	-	-	2.00	22		Caution! Expired ScreenTape device; Sample concentration outside functional range for RINe and the assay

Peak Table

Size [nt]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
25	40.0	40.0	4710	-		Lower Marker

C1: 24

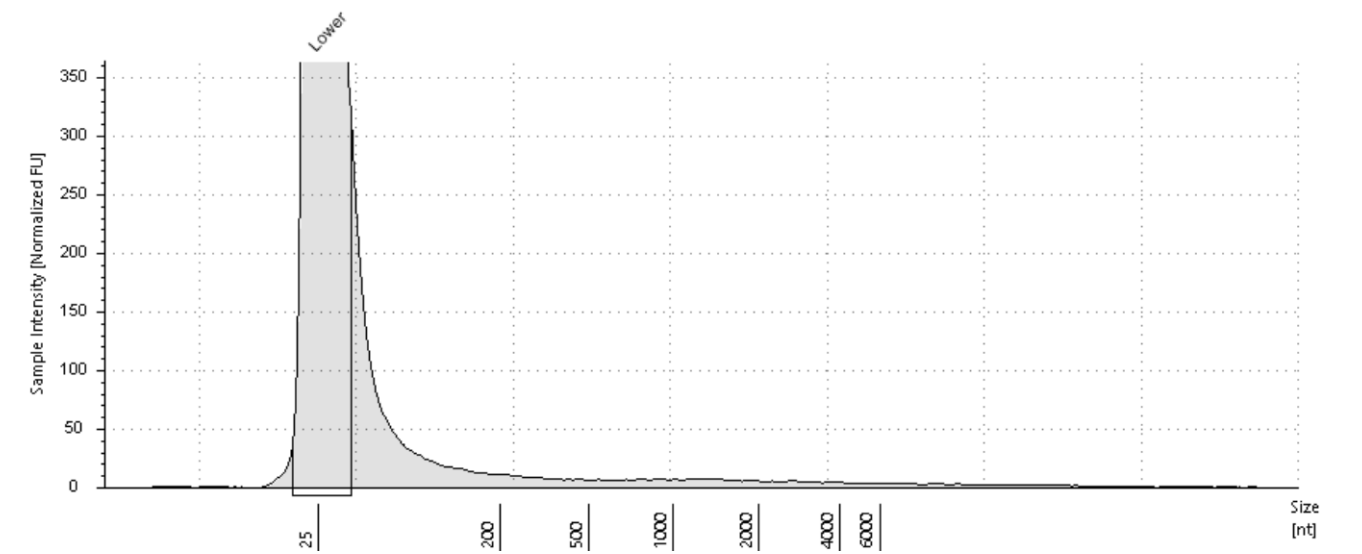


Sample Table

Well	RINe	28S/18S (Area)	Conc. [ng/μl]	Sample Description	Alert	Observations
C1	-	-	2.10	24		Caution! Expired ScreenTape device; Sample concentration outside functional range for RINe and the assay

Peak Table

Size [nt]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
25	40.0	40.0	4710	-		Lower Marker

D1: 24_elution2

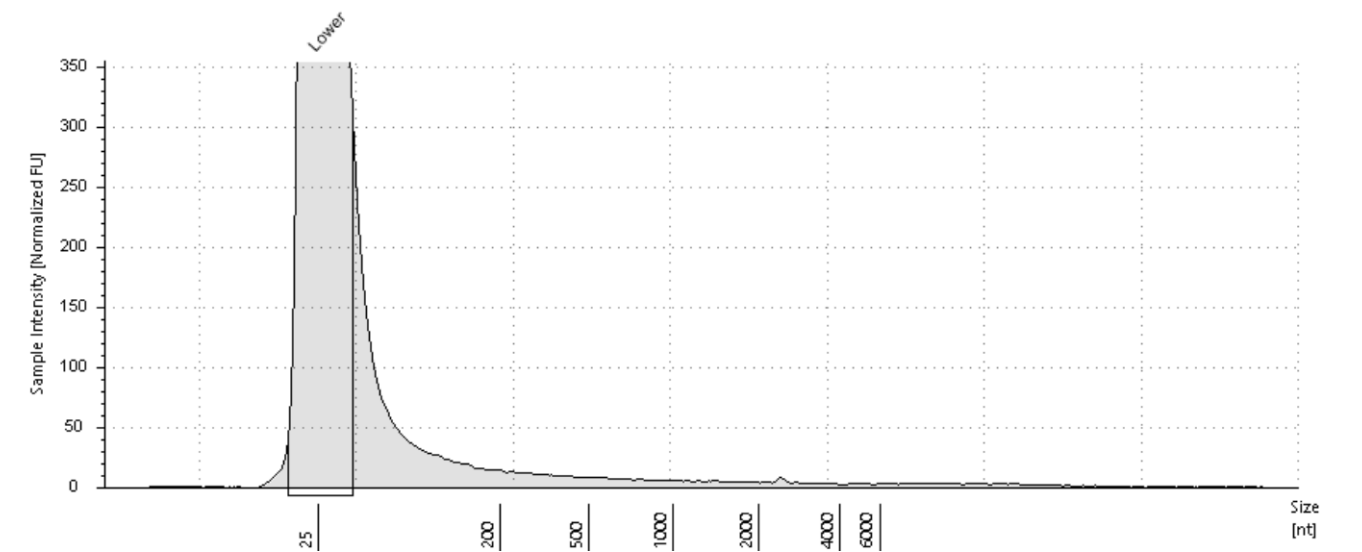

Sample Table

Well	RINe	28S/18S (Area)	Conc. [ng/μl]	Sample Description	Alert	Observations
D1	-	-	1.87	24_elution2		Caution! Expired ScreenTape device; Sample concentration outside functional range for RINe and the assay

Peak Table

Size [nt]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
25	40.0	40.0	4710	-		Lower Marker