


Filename: 2026-05-28 - 09.42.13.HSRNA

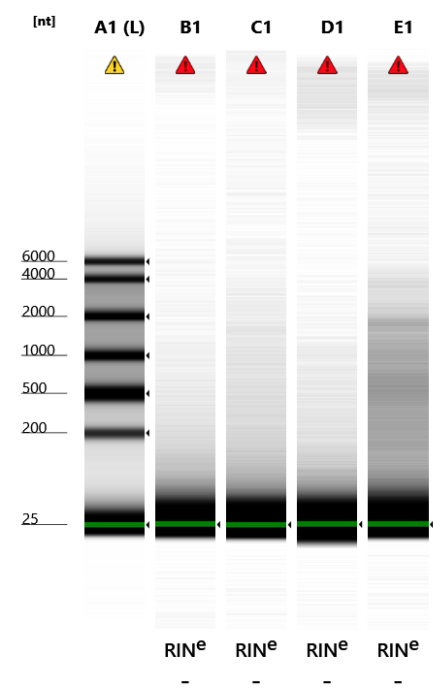


Default image (Contrast 105%), Image is Scaled to Sample

Sample Info

Well	RINe	28S/18S (Area)	Conc. [pg/ul]	Sample Description	Alert	Observations
A1	-	-	595	Ladder		Caution! Expired ScreenTape device (used after two weeks of first use); Ladder
B1	-	-	21.2	101_POR		Caution! Expired ScreenTape device (used after two weeks of first use); Sample concentration outside functional range for RINe and the assay
C1	-	-	31.6	211_POC_OE		Caution! Expired ScreenTape device (used after two weeks of first use); Sample concentration outside functional range for RINe and the assay
D1	-	-	17.5	212_POC_OG		Caution! Expired ScreenTape device (used after two weeks of first use); Sample concentration outside functional range for RINe and the assay
E1	-	-	60.9	214_POC_bulk		Caution! Expired ScreenTape device (used after two weeks of first use); Sample concentration outside functional range for RINe and the assay

A1: Ladder

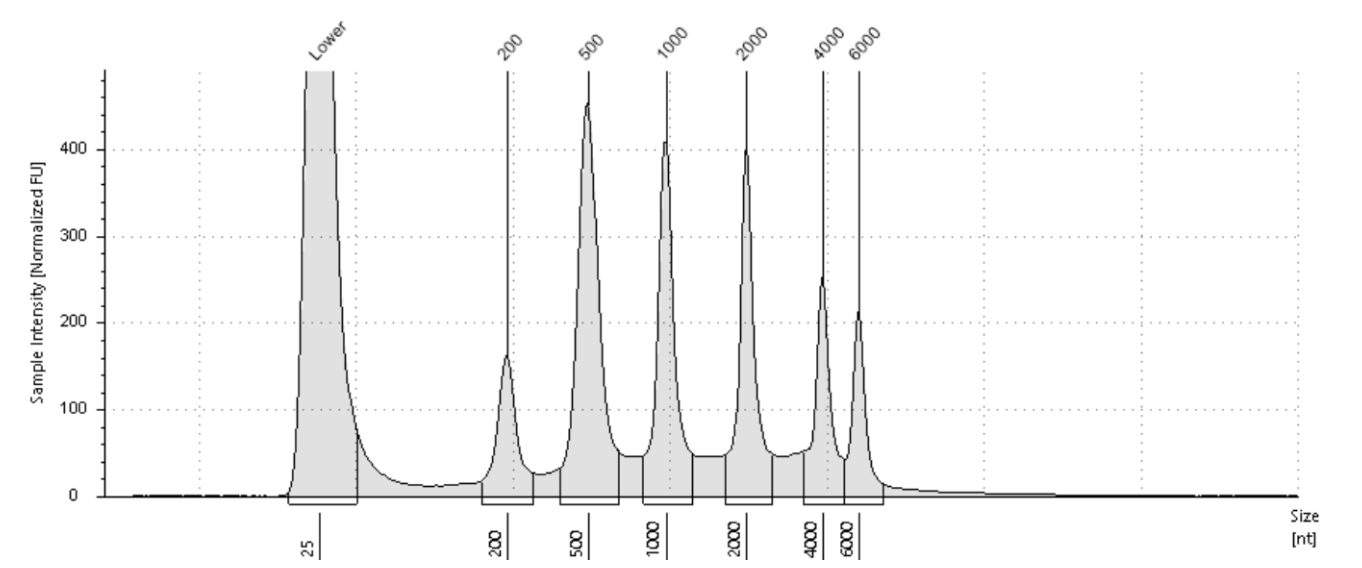


Sample Table

Well	RINe	28S/18S (Area)	Conc. [pg/ul]	Sample Description	Alert	Observations
A1	-	-	595	Ladder		Caution! Expired ScreenTape device (used after two weeks of first use); Ladder

Peak Table

Size [nt]	Calibrated Conc. [pg/ul]	Assigned Conc. [pg/ul]	Peak Molarity [pmol/l]	% Integrated Area	Peak Comment	Observations
25	700	700	82400	-		Lower Marker
200	49.0	-	720	9.92		
500	147	-	865	29.79		
1000	101	-	298	20.52		
2000	92.4	-	136	18.71		
4000	60.1	-	44.2	12.17		
6000	43.9	-	21.5	8.88		

B1: 101_POR

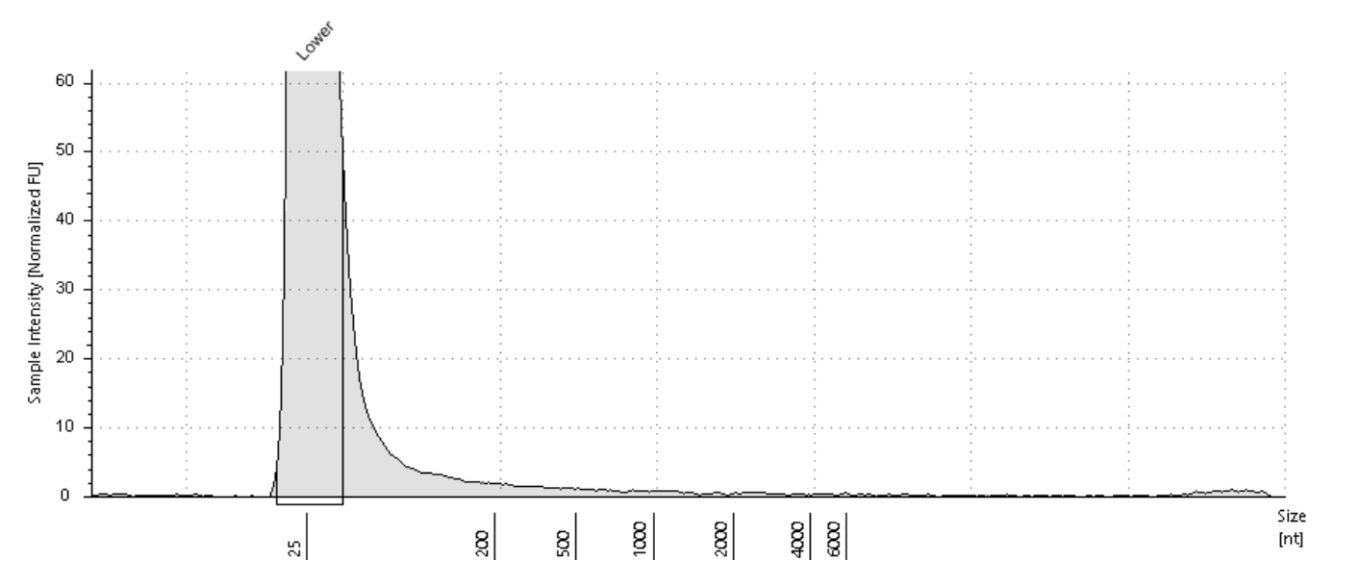


Sample Table

Well	RINe	28S/18S (Area)	Conc. [pg/ul]	Sample Description	Alert	Observations
B1	-	-	21.2	101_POR		Caution! Expired ScreenTape device (used after two weeks of first use); Sample concentration outside functional range for RINe and the assay

Peak Table

Size [nt]	Calibrated Conc. [pg/ul]	Assigned Conc. [pg/ul]	Peak Molarity [pmol/l]	% Integrated Area	Peak Comment	Observations
25	700	700	82400	-		Lower Marker

C1: 211_POC_OE

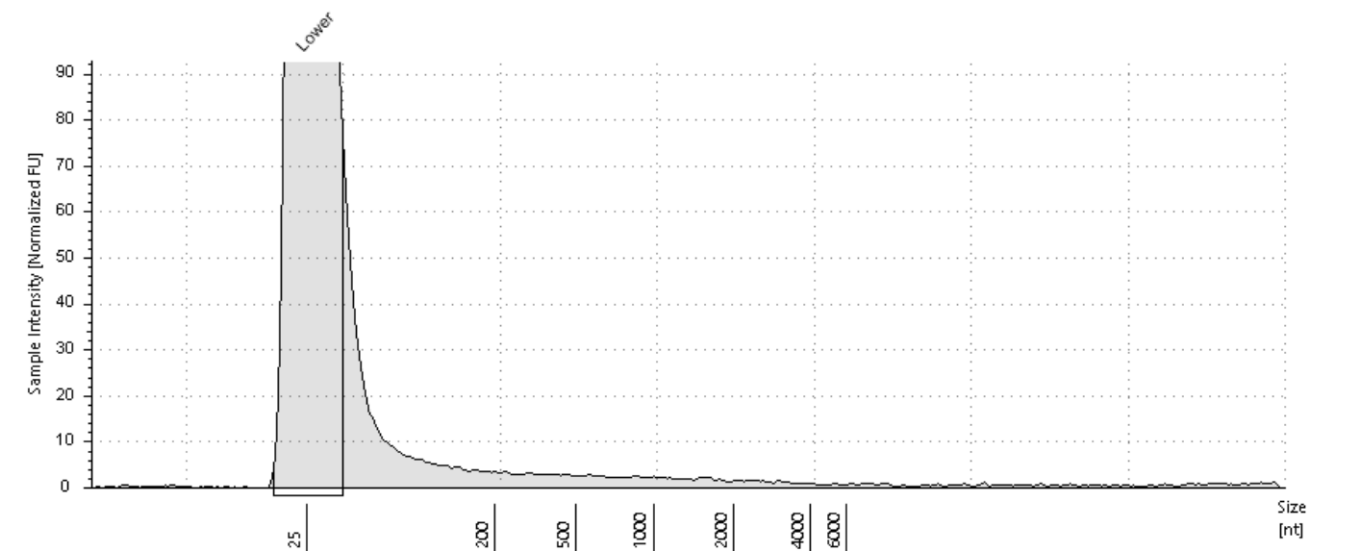


Sample Table

Well	RINe	28S/18S (Area)	Conc. [pg/ul]	Sample Description	Alert	Observations
C1	-	-	31.6	211_POC_OE		Caution! Expired ScreenTape device (used after two weeks of first use); Sample concentration outside functional range for RINe and the assay

Peak Table

Size [nt]	Calibrated Conc. [pg/ul]	Assigned Conc. [pg/ul]	Peak Molarity [pmol/l]	% Integrated Area	Peak Comment	Observations
25	700	700	82400	-		Lower Marker

D1: 212_POC_OG

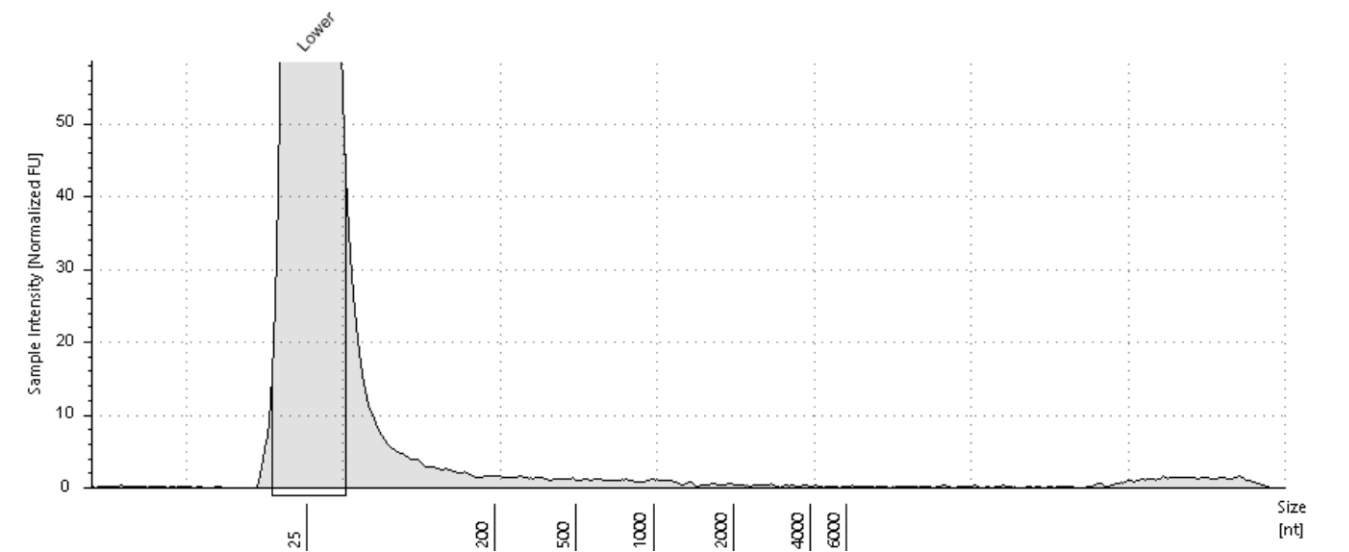


Sample Table

Well	RINe	28S/18S (Area)	Conc. [pg/ul]	Sample Description	Alert	Observations
D1	-	-	17.5	212_POC_OG		Caution! Expired ScreenTape device (used after two weeks of first use); Sample concentration outside functional range for RINe and the assay

Peak Table

Size [nt]	Calibrated Conc. [pg/ul]	Assigned Conc. [pg/ul]	Peak Molarity [pmol/l]	% Integrated Area	Peak Comment	Observations
25	700	700	82400	-		Lower Marker

E1: 214_POC_bulk

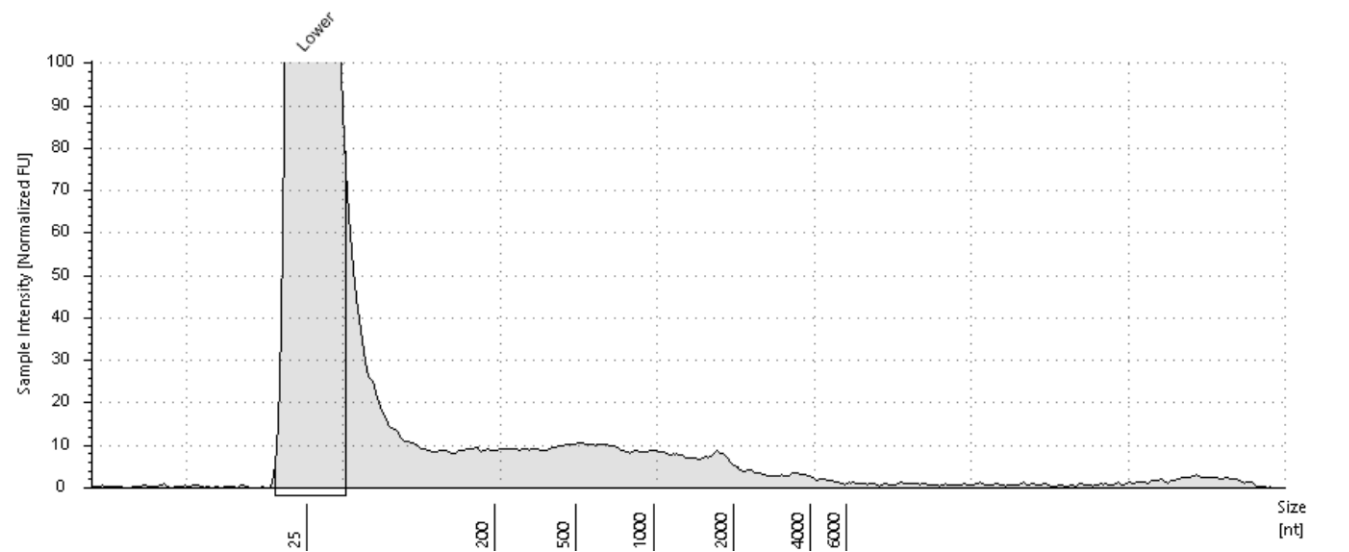

Sample Table

Well	RINe	28S/18S (Area)	Conc. [pg/ul]	Sample Description	Alert	Observations
E1	-	-	60.9	214_POC_bulk		Caution! Expired ScreenTape device (used after two weeks of first use); Sample concentration outside functional range for RINe and the assay

Peak Table

Size [nt]	Calibrated Conc. [pg/ul]	Assigned Conc. [pg/ul]	Peak Molarity [pmol/l]	% Integrated Area	Peak Comment	Observations
25	700	700	82400	-		Lower Marker