


Filename: 2026-05-08 - 11.31.55.HSRNA

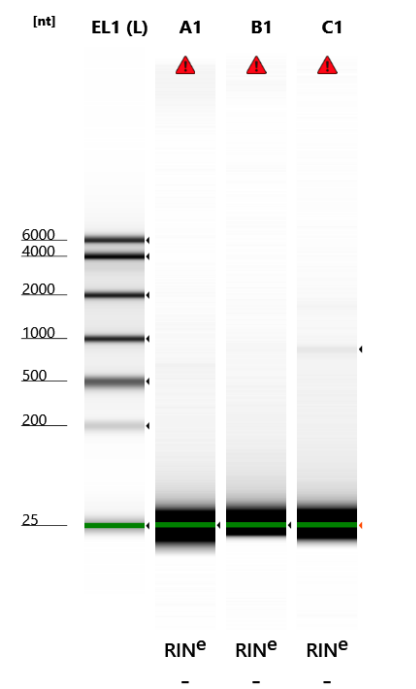


Default image (Contrast 50%), Image is Scaled to Sample

Sample Info

Well	RINe	28S/18S (Area)	Conc. [pg/ul]	Sample Description	Alert	Observations
EL1	-	-	3750	Electronic Ladder		Ladder
A1	-	-	43.5	21	▲	Caution! Expired ScreenTape device (used after two weeks of first use); Sample concentration outside functional range for RINe and the assay
B1	-	-	44.7	22	▲	Caution! Expired ScreenTape device (used after two weeks of first use); Sample concentration outside functional range for RINe and the assay
C1	-	-	38.3	24	▲	Caution! Expired ScreenTape device (used after two weeks of first use); Sample concentration outside functional range for RINe and the assay

EL1: Electronic Ladder

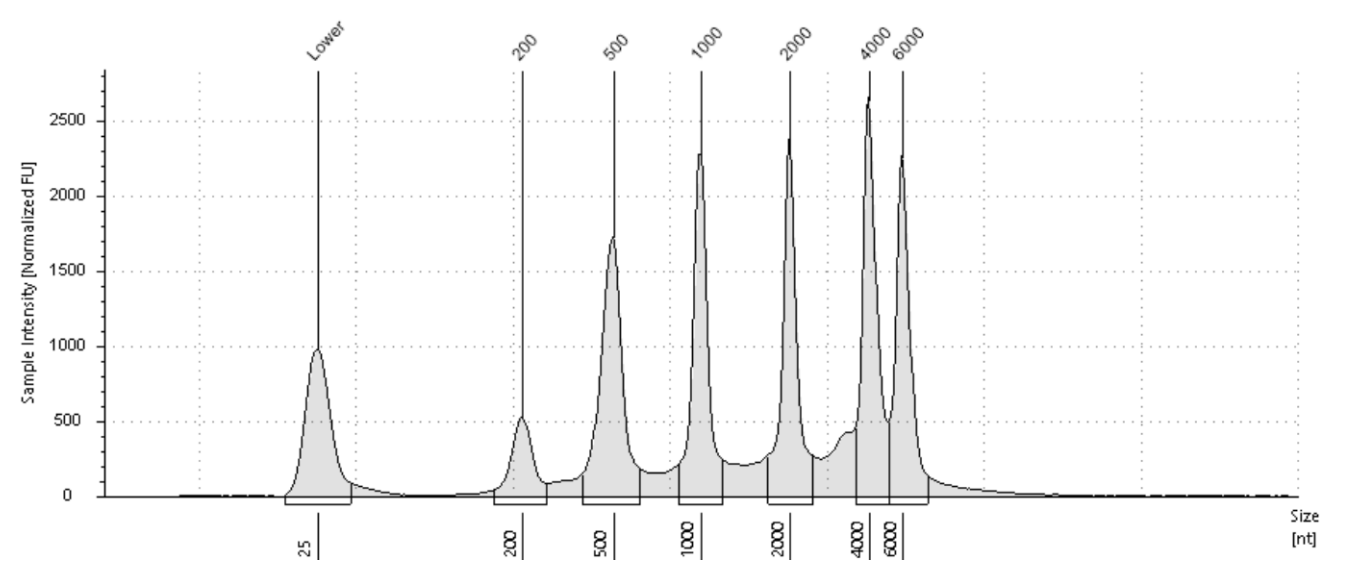


Sample Table

Well	RINe	28S/18S (Area)	Conc. [pg/ul]	Sample Description	Alert	Observations
EL1	-	-	3750	Electronic Ladder		Ladder

Peak Table

Size [nt]	Calibrated Conc. [pg/ul]	Assigned Conc. [pg/ul]	Peak Molarity [pmol/l]	% Integrated Area	Peak Comment	Observations
25	700	700	82400	-		Lower Marker
200	189	-	2770	5.98		
500	638	-	3760	20.25		
1000	557	-	1640	17.66		
2000	580	-	854	18.42		
4000	634	-	466	20.11		
6000	554	-	272	17.58		

A1: 21

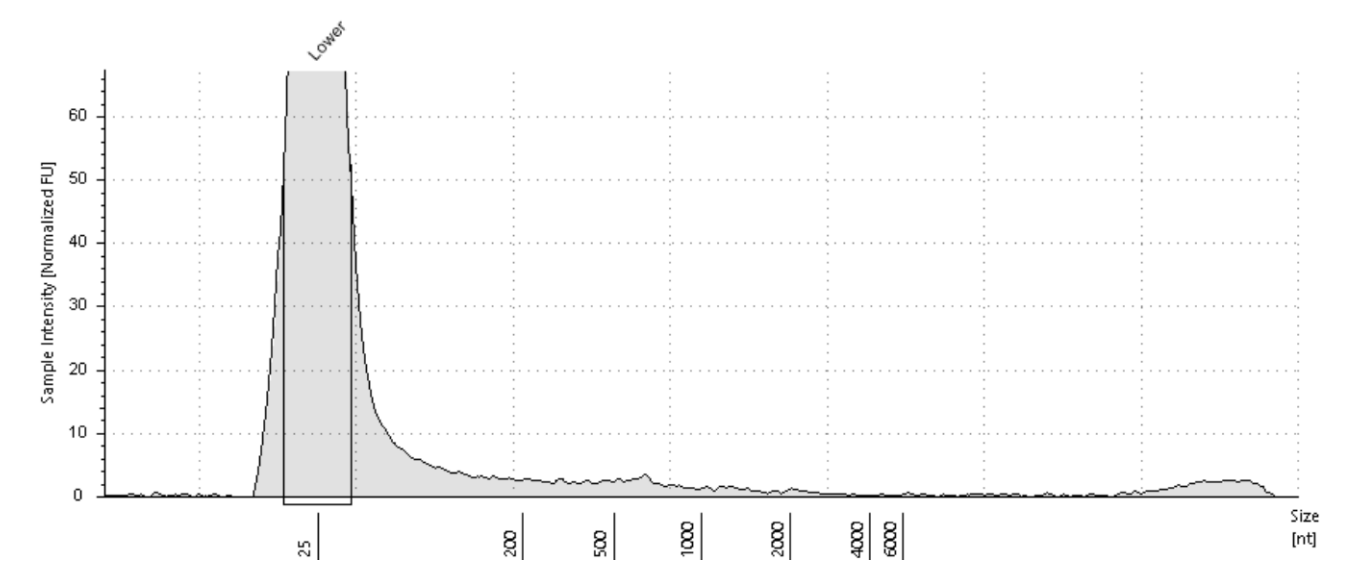


Sample Table

Well	RINe	28S/18S (Area)	Conc. [pg/ul]	Sample Description	Alert	Observations
A1	-	-	43.5	21		Caution! Expired ScreenTape device (used after two weeks of first use); Sample concentration outside functional range for RINe and the assay

Peak Table

Size [nt]	Calibrated Conc. [pg/ul]	Assigned Conc. [pg/ul]	Peak Molarity [pmol/l]	% Integrated Area	Peak Comment	Observations
25	700	700	82400	-		Lower Marker

B1: 22

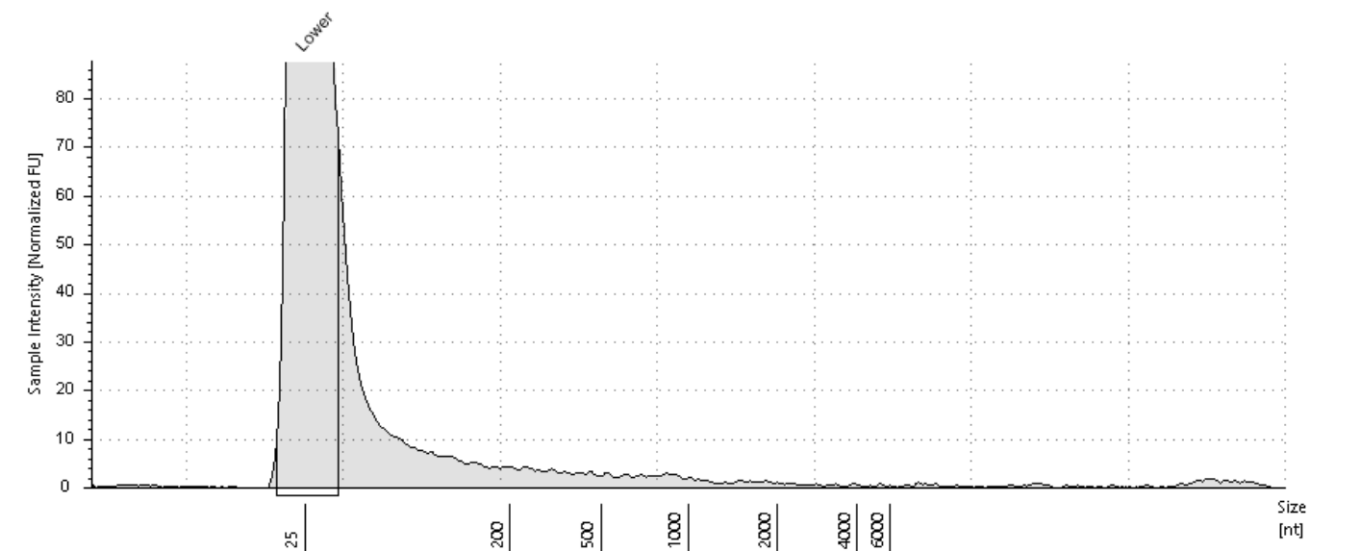


Sample Table

Well	RINe	28S/18S (Area)	Conc. [pg/ul]	Sample Description	Alert	Observations
B1	-	-	44.7	22		Caution! Expired ScreenTape device (used after two weeks of first use); Sample concentration outside functional range for RINe and the assay

Peak Table

Size [nt]	Calibrated Conc. [pg/ul]	Assigned Conc. [pg/ul]	Peak Molarity [pmol/l]	% Integrated Area	Peak Comment	Observations
25	700	700	82400	-		Lower Marker

C1: 24

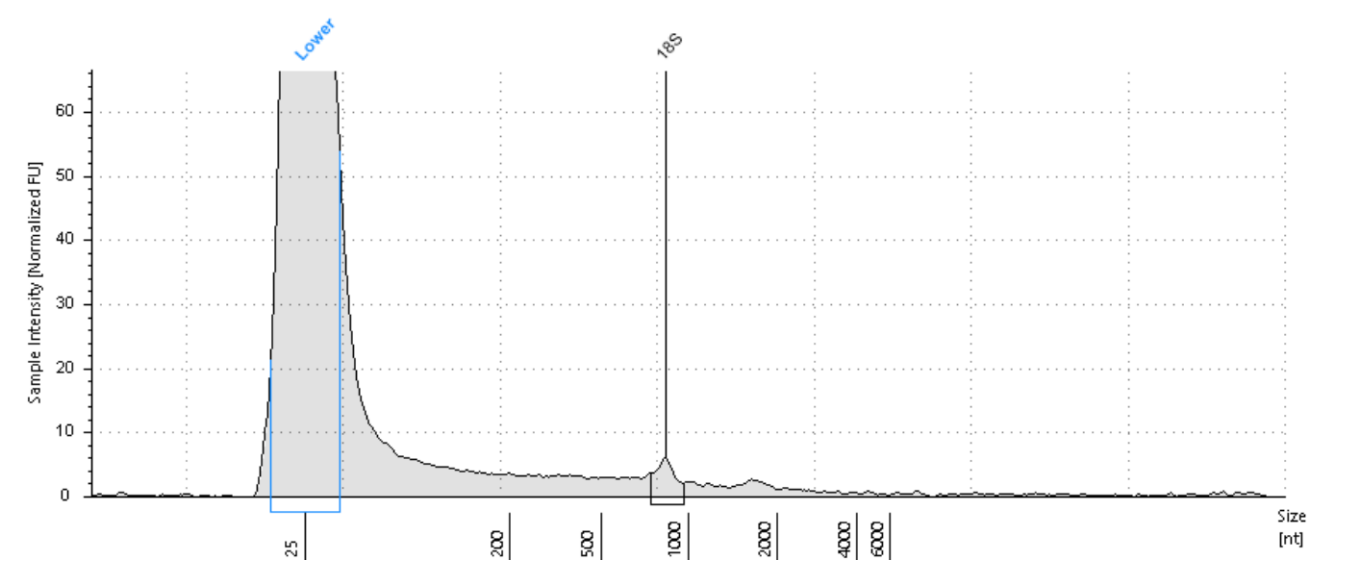

Sample Table

Well	RINe	28S/18S (Area)	Conc. [pg/ul]	Sample Description	Alert	Observations
C1	-	-	38.3	24		Caution! Expired ScreenTape device (used after two weeks of first use); Sample concentration outside functional range for RINe and the assay

Peak Table

Size [nt]	Calibrated Conc. [pg/ul]	Assigned Conc. [pg/ul]	Peak Molarity [pmol/l]	% Integrated Area	Peak Comment	Observations
25	700	700	82400	-		Lower Marker
836	2.21	-	7.79	100.00		18S