


Filename: 2026-05-13 - 11.24.36.HSRNA

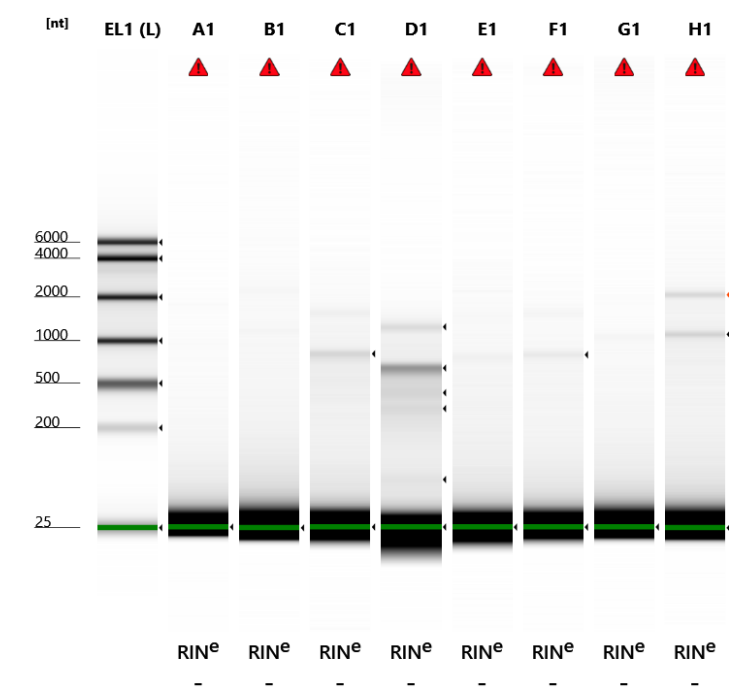


Default image (Contrast 50%), Image is Scaled to Sample

Sample Info

Well	RINe	28S/18S (Area)	Conc. [pg/ul]	Sample Description	Alert	Observations
EL1	-	-	3750	Electronic Ladder		Ladder
A1	-	-	44.6	1	▲	Sample concentration outside functional range for RINe and the assay
B1	-	-	54.9	2	▲	Sample concentration outside functional range for RINe and the assay
C1	-	-	48.1	9	▲	Sample concentration outside functional range for RINe and the assay
D1	-	-	108	13	▲	Markers outside standard running position; Sample concentration outside functional range for RINe and the assay; RINe edited
E1	-	-	46.3	31	▲	Sample concentration outside functional range for RINe and the assay
F1	-	-	46.1	32	▲	Sample concentration outside functional range for RINe and the assay
G1	-	-	48.4	33	▲	Sample concentration outside functional range for RINe and the assay
H1	-	-	65.9	34	▲	Sample concentration outside functional range for RINe and the assay

EL1: Electronic Ladder

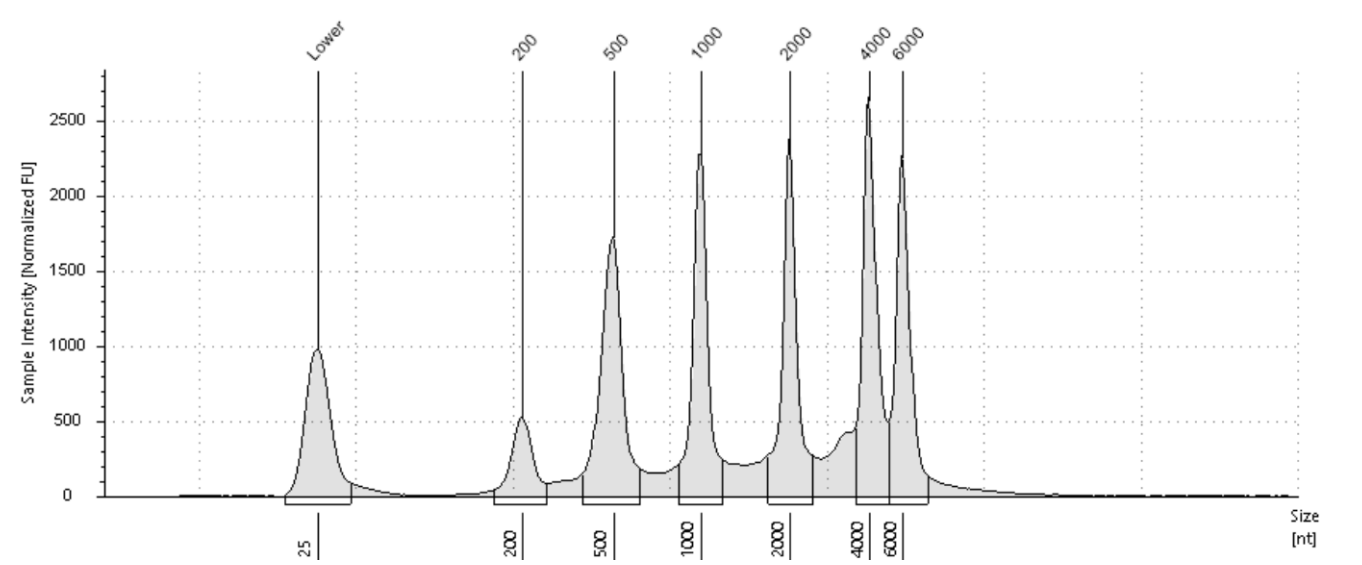


Sample Table

Well	RINe	28S/18S (Area)	Conc. [pg/ul]	Sample Description	Alert	Observations
EL1	-	-	3750	Electronic Ladder		Ladder

Peak Table

Size [nt]	Calibrated Conc. [pg/ul]	Assigned Conc. [pg/ul]	Peak Molarity [pmol/l]	% Integrated Area	Peak Comment	Observations
25	700	700	82400	-		Lower Marker
200	189	-	2770	5.98		
500	638	-	3760	20.25		
1000	557	-	1640	17.66		
2000	580	-	854	18.42		
4000	634	-	466	20.11		
6000	554	-	272	17.58		

A1: 1

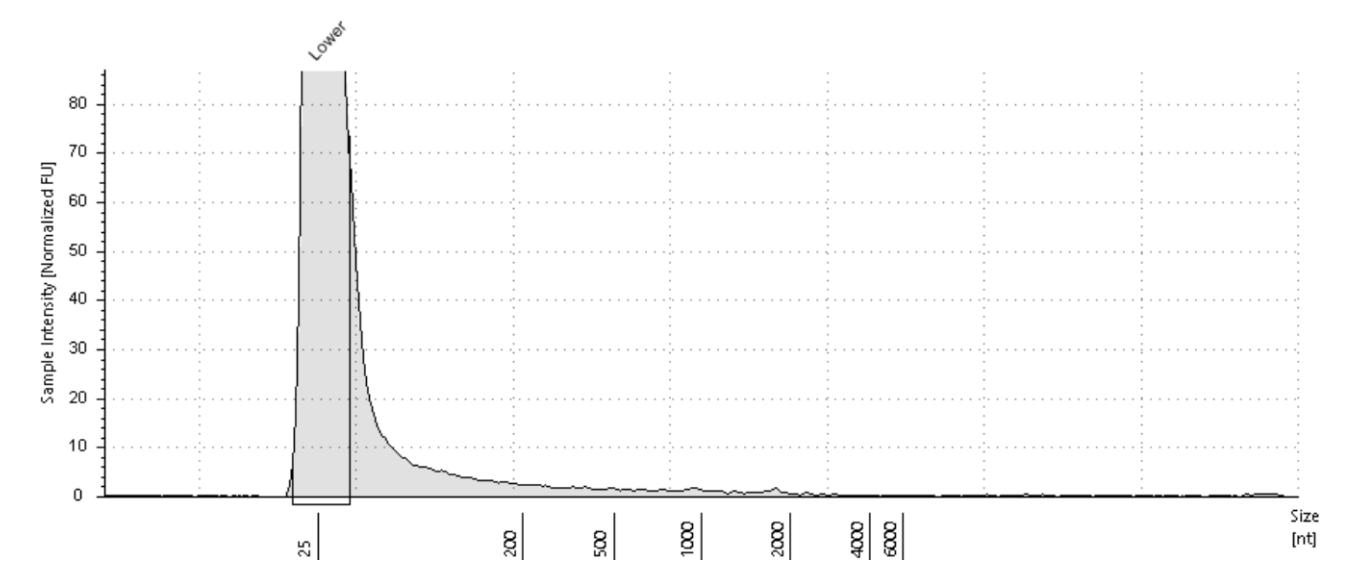


Sample Table

Well	RINe	28S/18S (Area)	Conc. [pg/ul]	Sample Description	Alert	Observations
A1	-	-	44.6	1		Sample concentration outside functional range for RINe and the assay

Peak Table

Size [nt]	Calibrated Conc. [pg/ul]	Assigned Conc. [pg/ul]	Peak Molarity [pmol/l]	% Integrated Area	Peak Comment	Observations
25	700	700	82400	-		Lower Marker

B1: 2

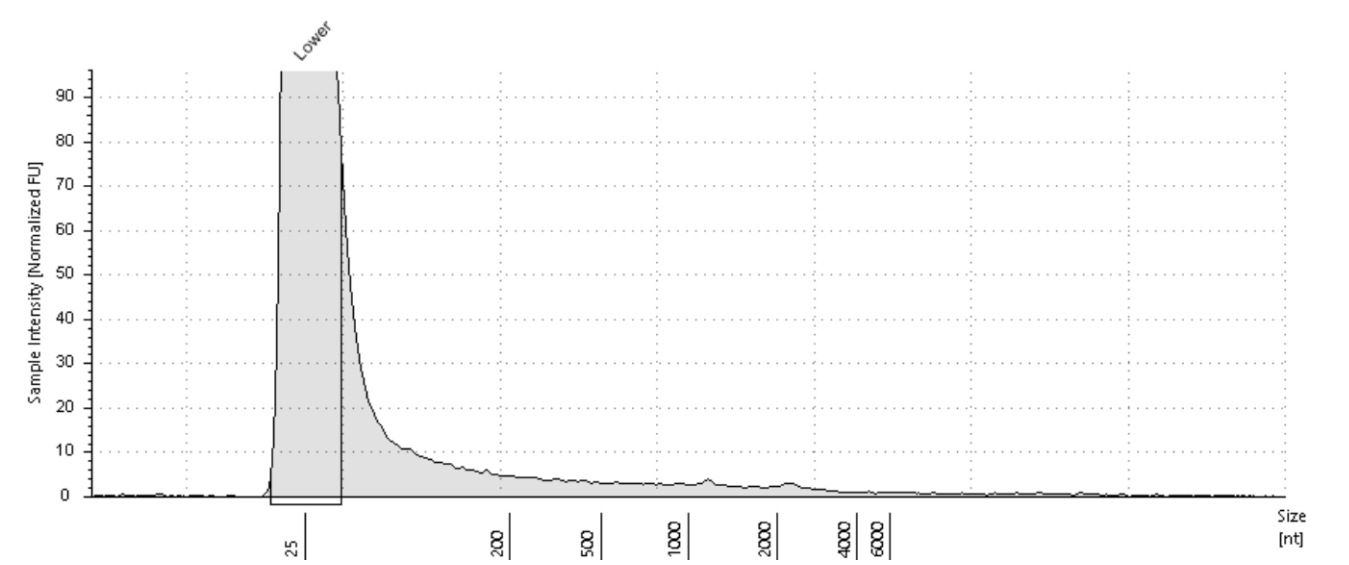


Sample Table

Well	RINe	28S/18S (Area)	Conc. [pg/ul]	Sample Description	Alert	Observations
B1	-	-	54.9	2		Sample concentration outside functional range for RINe and the assay

Peak Table

Size [nt]	Calibrated Conc. [pg/ul]	Assigned Conc. [pg/ul]	Peak Molarity [pmol/l]	% Integrated Area	Peak Comment	Observations
25	700	700	82400	-		Lower Marker

C1: 9

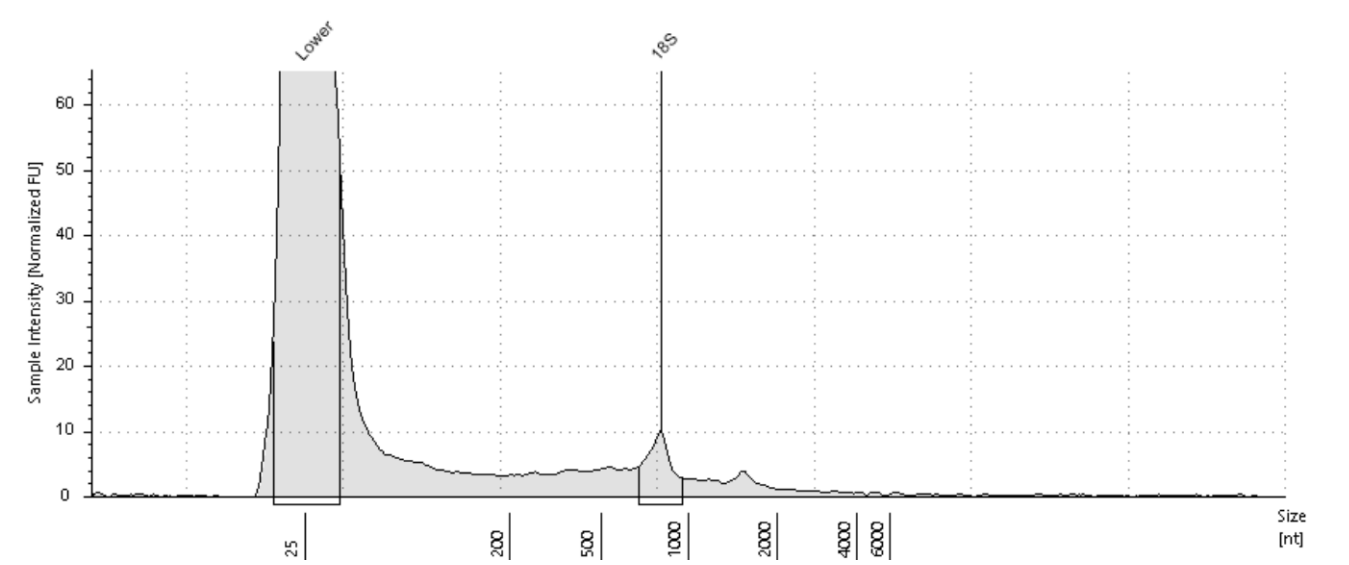


Sample Table

Well	RINe	28S/18S (Area)	Conc. [pg/ul]	Sample Description	Alert	Observations
C1	-	-	48.1	9		Sample concentration outside functional range for RINe and the assay

Peak Table

Size [nt]	Calibrated Conc. [pg/ul]	Assigned Conc. [pg/ul]	Peak Molarity [pmol/l]	% Integrated Area	Peak Comment	Observations
25	700	700	82400	-		Lower Marker
802	5.38	-	19.7	100.00		18S

D1: 13

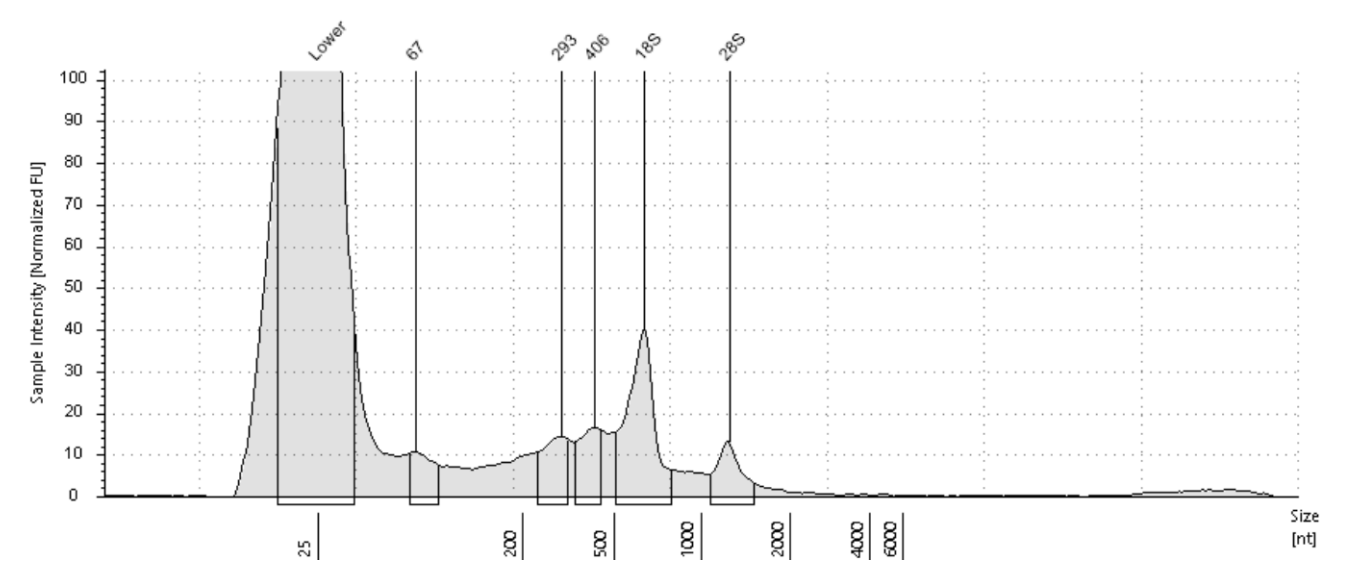


Sample Table

Well	RINe	28S/18S (Area)	Conc. [pg/ul]	Sample Description	Alert	Observations
D1	-	-	108	13		Markers outside standard running position; Sample concentration outside functional range for RINe and the assay; RINe edited

Peak Table

Size [nt]	Calibrated Conc. [pg/ul]	Assigned Conc. [pg/ul]	Peak Molarity [pmol/l]	% Integrated Area	Peak Comment	Observations
25	700	700	82400	-		edited Lower Marker
67	4.76	-	208	10.37		
293	7.06	-	70.8	15.39		
406	6.97	-	50.4	15.18		
634	21.2	-	98.2	46.15		18S edited
1234	5.93	-	14.1	12.91		28S edited

E1: 31

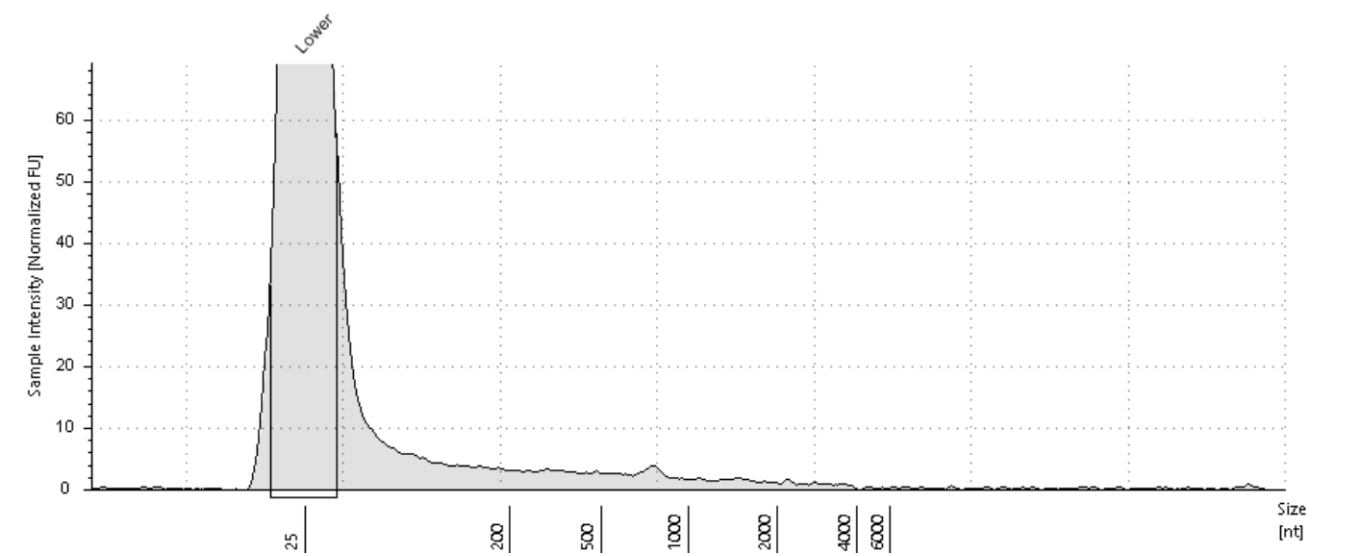


Sample Table

Well	RINe	28S/18S (Area)	Conc. [pg/ul]	Sample Description	Alert	Observations
E1	-	-	46.3	31		Sample concentration outside functional range for RINe and the assay

Peak Table

Size [nt]	Calibrated Conc. [pg/ul]	Assigned Conc. [pg/ul]	Peak Molarity [pmol/l]	% Integrated Area	Peak Comment	Observations
25	700	700	82400	-		Lower Marker

F1: 32

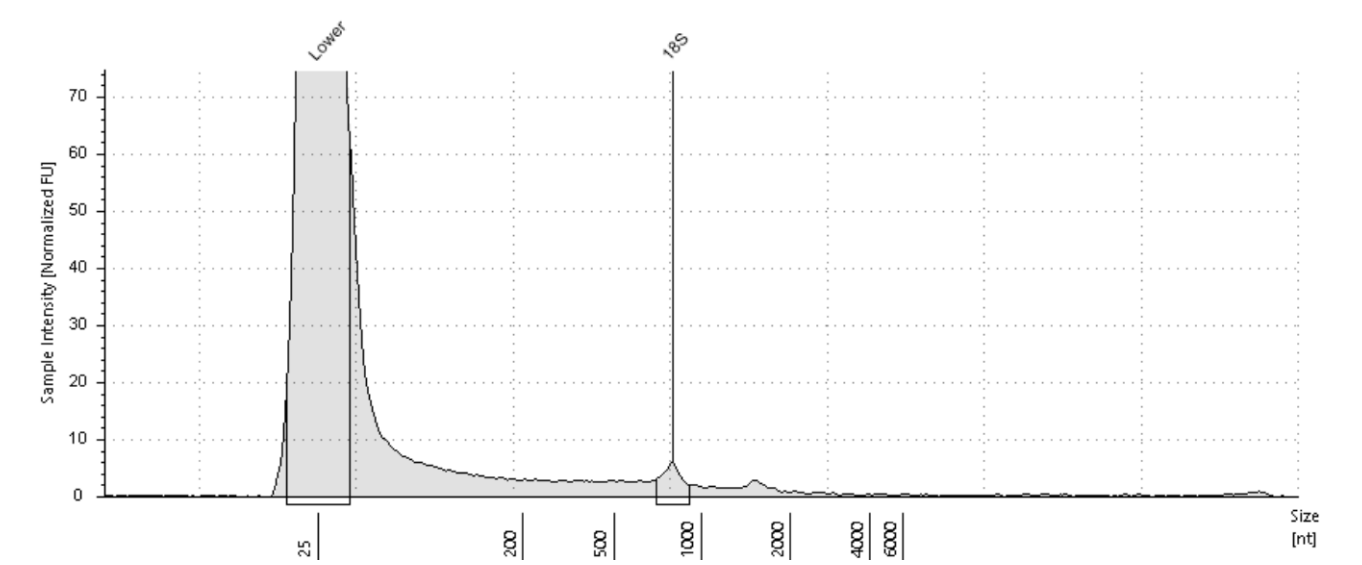


Sample Table

Well	RINe	28S/18S (Area)	Conc. [pg/ul]	Sample Description	Alert	Observations
F1	-	-	46.1	32		Sample concentration outside functional range for RINe and the assay

Peak Table

Size [nt]	Calibrated Conc. [pg/ul]	Assigned Conc. [pg/ul]	Peak Molarity [pmol/l]	% Integrated Area	Peak Comment	Observations
25	700	700	82400	-		Lower Marker
789	2.72	-	10.1	100.00		18S

G1: 33

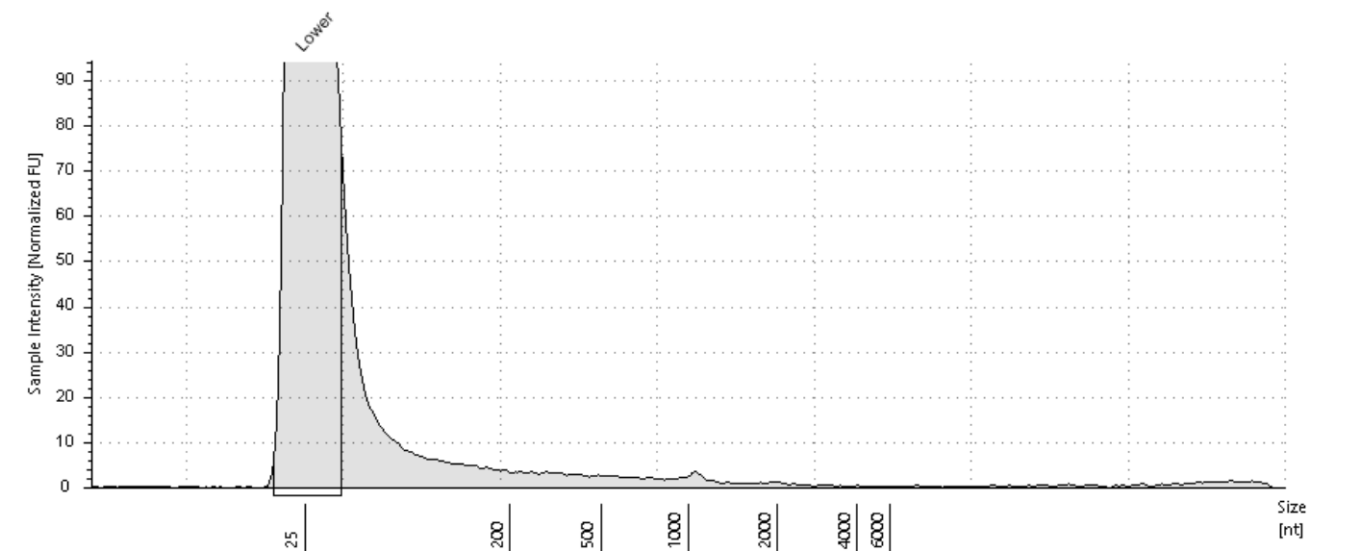


Sample Table

Well	RINe	28S/18S (Area)	Conc. [pg/ul]	Sample Description	Alert	Observations
G1	-	-	48.4	33		Sample concentration outside functional range for RINe and the assay

Peak Table

Size [nt]	Calibrated Conc. [pg/ul]	Assigned Conc. [pg/ul]	Peak Molarity [pmol/l]	% Integrated Area	Peak Comment	Observations
25	700	700	82400	-		Lower Marker

H1: 34

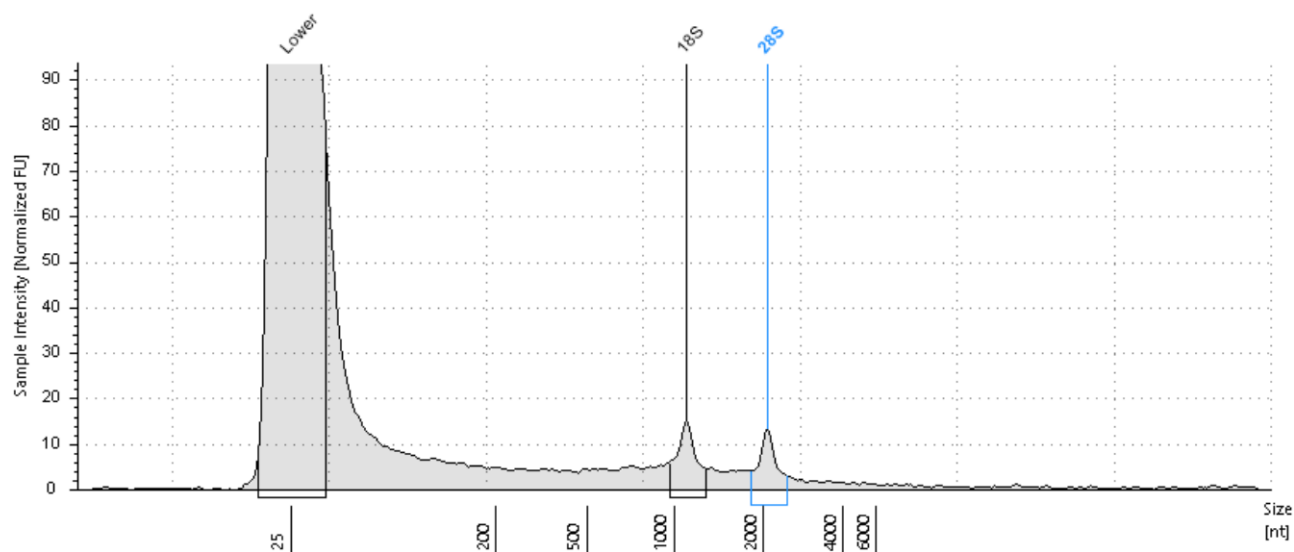

Sample Table

Well	RINe	28S/18S (Area)	Conc. [pg/ul]	Sample Description	Alert	Observations
H1	-	-	65.9	34	▲	Sample concentration outside functional range for RINe and the assay

Peak Table

Size [nt]	Calibrated Conc. [pg/ul]	Assigned Conc. [pg/ul]	Peak Molarity [pmol/l]	% Integrated Area	Peak Comment	Observations
25	700	700	82400	-		Lower Marker
1107	5.49	-	14.6	56.74		18S
2086	4.19	-	5.90	43.26		28S