



Filename: 2026-09-07 - 12.59.18.HSRNA

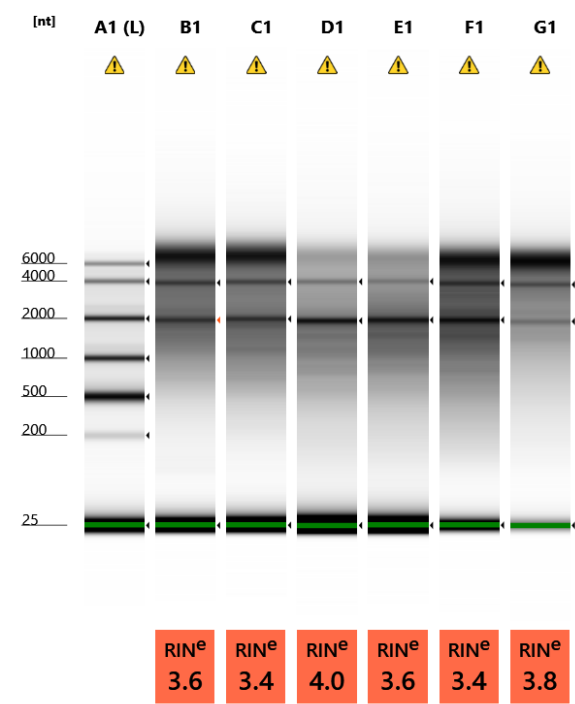

Default image (Contrast 50%), Image is Scaled to Sample

A1: Ladder

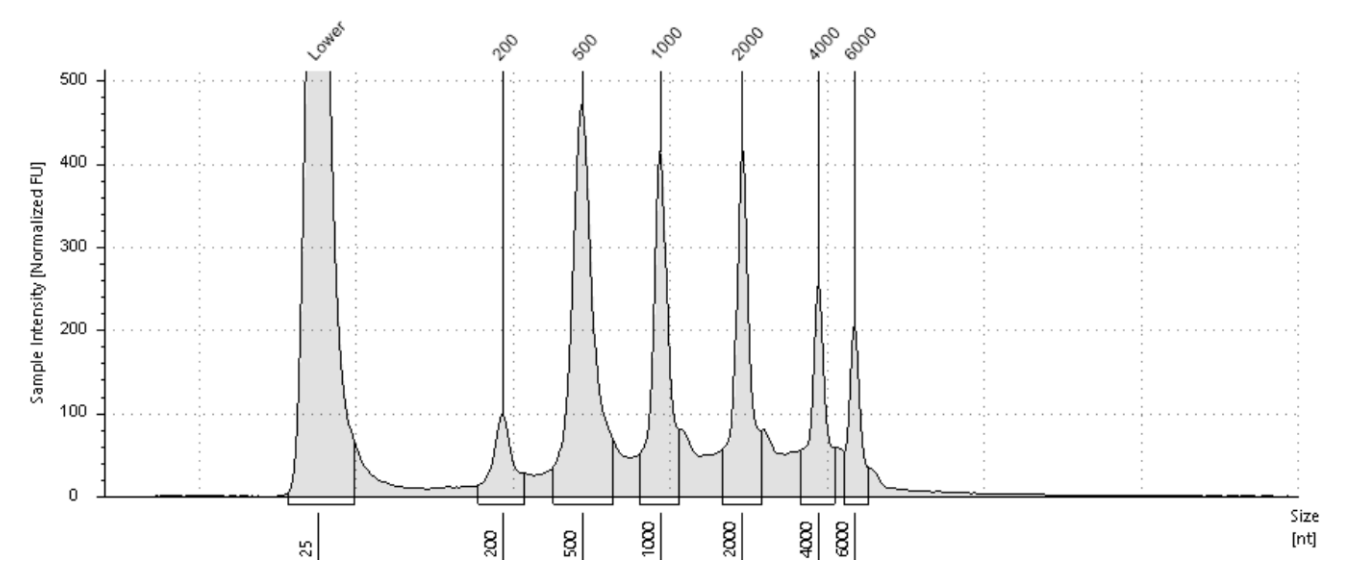


Sample Table

Well	RINe	28S/18S (Area)	Conc. [pg/ul]	Sample Description	Alert	Observations
A1	-	-	632	Ladder		Caution! Expired ScreenTape device (used after two weeks of first use); Ladder

Peak Table

Size [nt]	Calibrated Conc. [pg/ul]	Assigned Conc. [pg/ul]	Peak Molarity [pmol/l]	% Integrated Area	Peak Comment	Observations
25	700	700	82400	-		Lower Marker
200	31.2	-	458	6.38		
500	168	-	986	34.31		
1000	100	-	294	20.48		
2000	94.1	-	138	19.26		
4000	57.7	-	42.4	11.81		
6000	37.9	-	18.6	7.75		

B1: POC_120_C

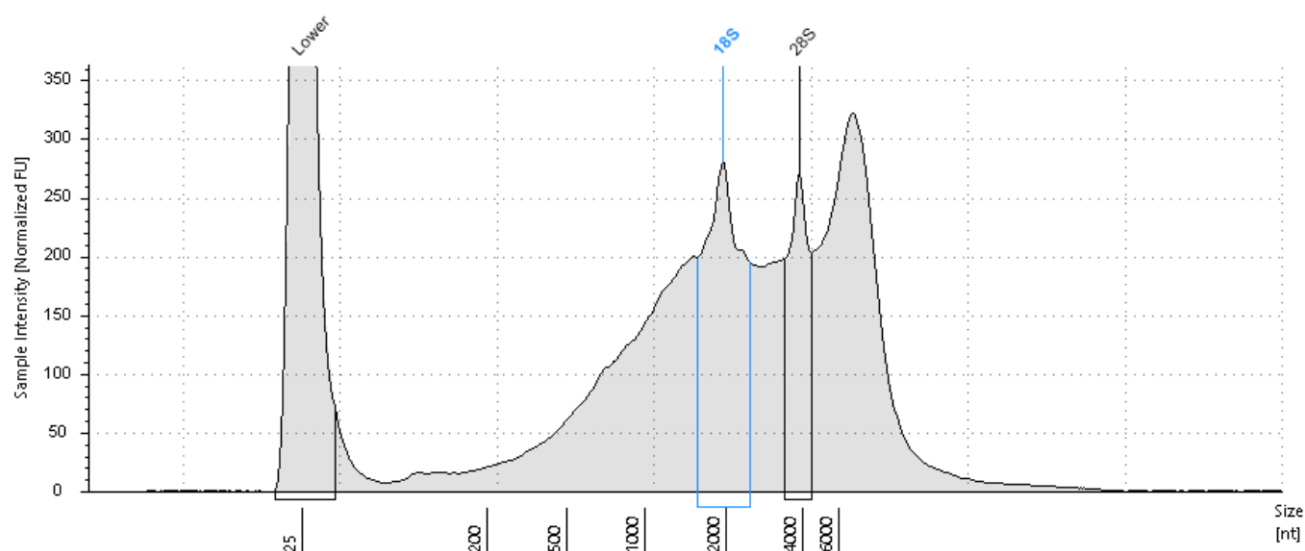


Sample Table

Well	RINe	28S/18S (Area)	Conc. [pg/ul]	Sample Description	Alert	Observations
B1	3.6	0.5	1030	POC_120_C		Caution! Expired ScreenTape device (used after two weeks of first use)

Peak Table


Size [nt]	Calibrated Conc. [pg/ul]	Assigned Conc. [pg/ul]	Peak Molarity [pmol/l]	% Integrated Area	Peak Comment	Observations
25	700	700	82400	-		Lower Marker
1947	179	-	270	64.75		18S
3898	97.4	-	73.5	35.25		28S edited

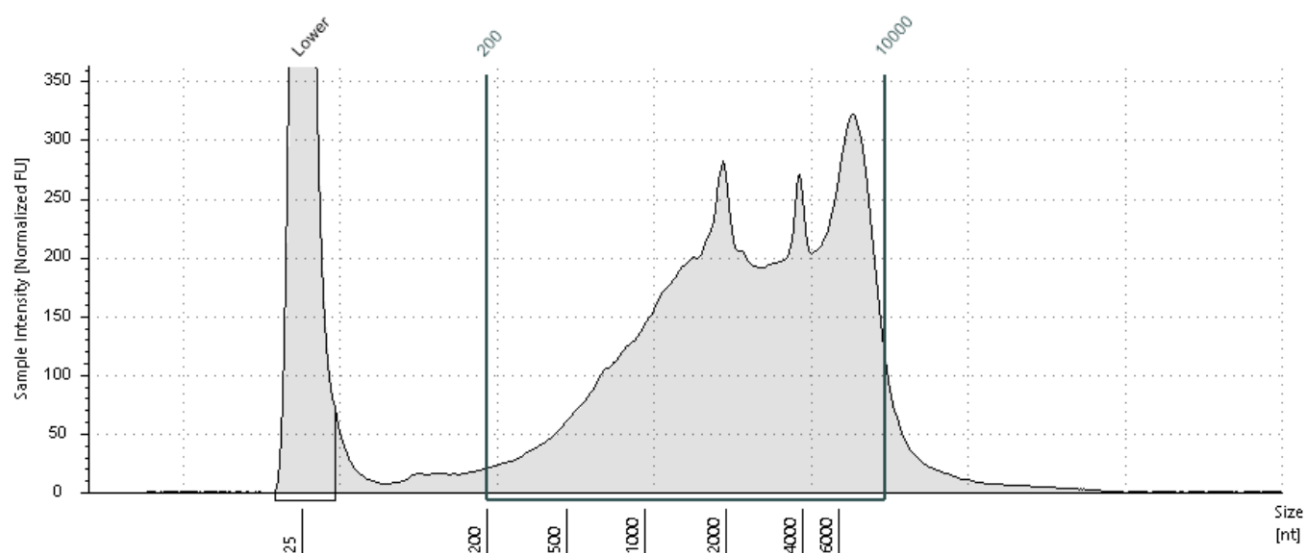

Region Table

From [nt]	To [nt]	Average Size [nt]	Conc. [pg/ul]	Region Molarity [pmol/l]	% of Total	Region Comment	Color
200	10000	5485	940	504	91.54	dv200	

C1: POC_120_H

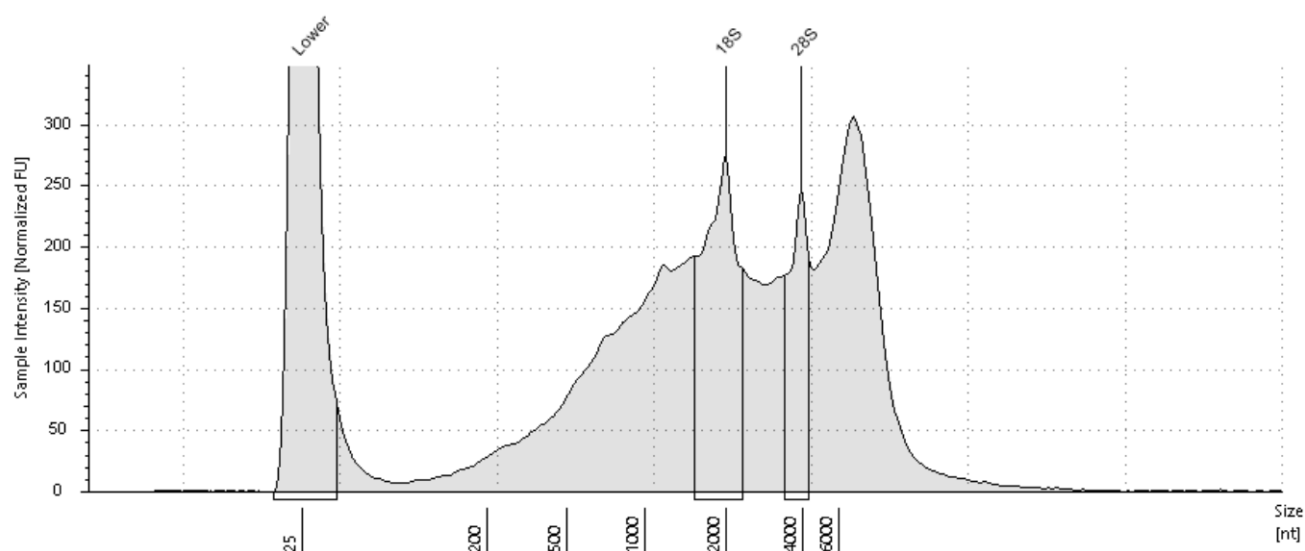


Sample Table

Well	RINe	28S/18S (Area)	Conc. [pg/ul]	Sample Description	Alert	Observations
C1	3.4	0.5	986	POC_120_H		Caution! Expired ScreenTape device (used after two weeks of first use); RNA concentration outside recommended range for RINe

Peak Table

Size [nt]	Calibrated Conc. [pg/ul]	Assigned Conc. [pg/ul]	Peak Molarity [pmol/l]	% Integrated Area	Peak Comment	Observations
25	700	700	82400	-		Lower Marker
1987	157	-	232	66.49		18S
3964	78.9	-	58.5	33.51		28S edited

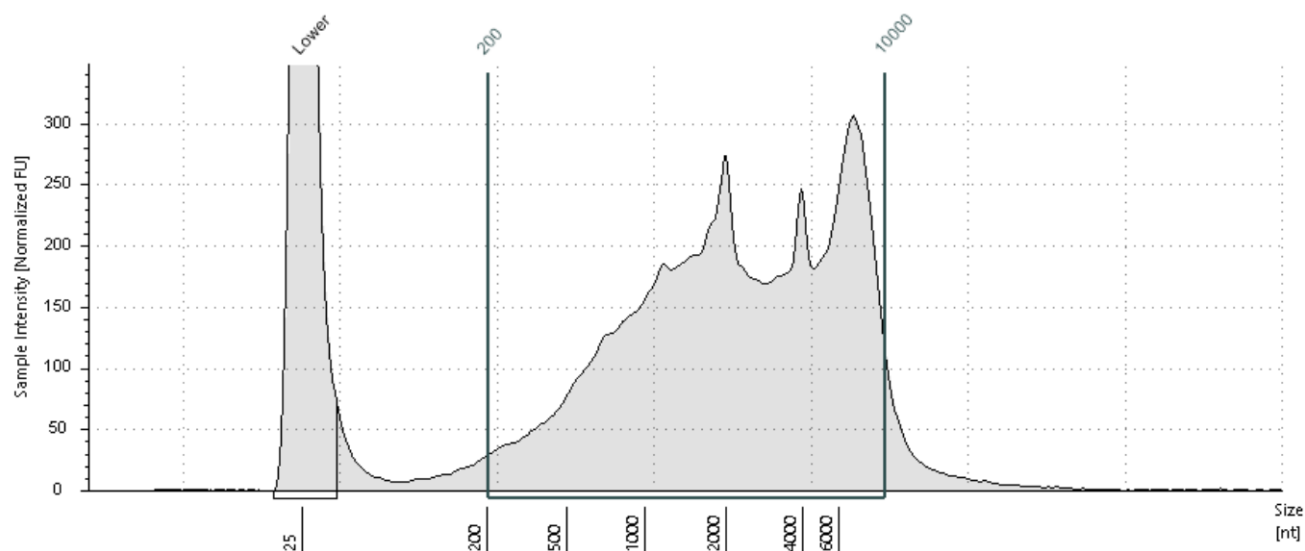


Region Table

From [nt]	To [nt]	Average Size [nt]	Conc. [pg/ul]	Region Molarity [pmol/l]	% of Total	Region Comment	Color
-----------	---------	-------------------	---------------	--------------------------	------------	----------------	-------

200	10000	5497	908	486	92.15	dv200	
-----	-------	------	-----	-----	-------	-------	---

D1: POR_120_C1

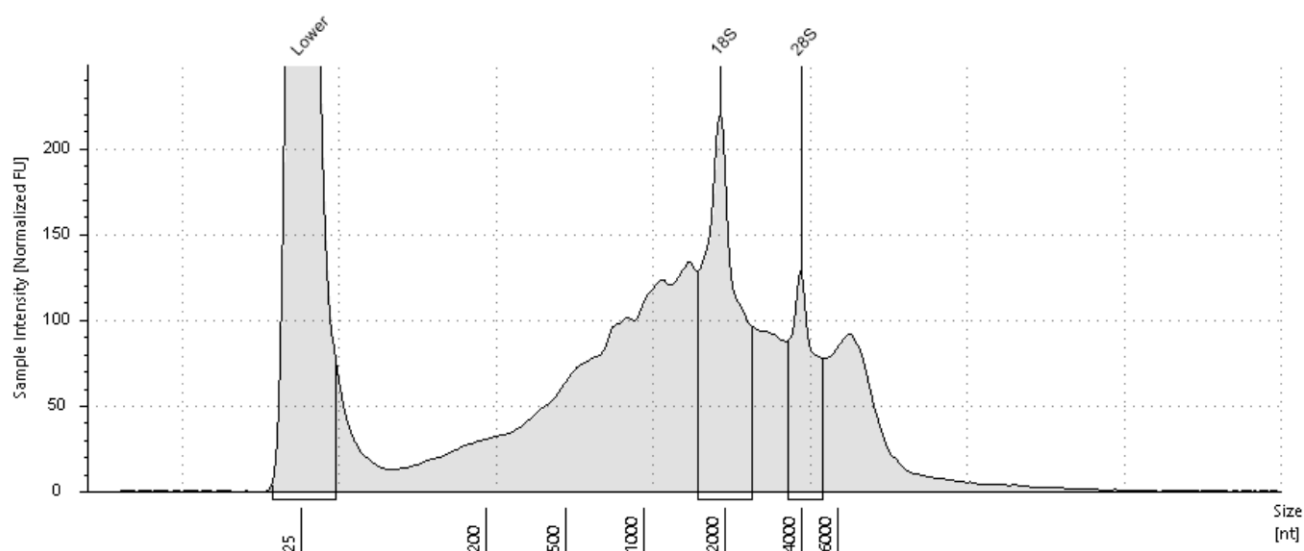


Sample Table

Well	RINe	28S/18S (Area)	Conc. [pg/ul]	Sample Description	Alert	Observations
D1	4.0	0.4	556	POR_120_C1		Caution! Expired ScreenTape device (used after two weeks of first use); RNA concentration outside recommended range for RINe

Peak Table

Size [nt]	Calibrated Conc. [pg/ul]	Assigned Conc. [pg/ul]	Peak Molarity [pmol/l]	% Integrated Area	Peak Comment	Observations
25	700	700	82400	-		Lower Marker
1927	109	-	166	69.57		18S
3987	47.5	-	35.0	30.43		28S

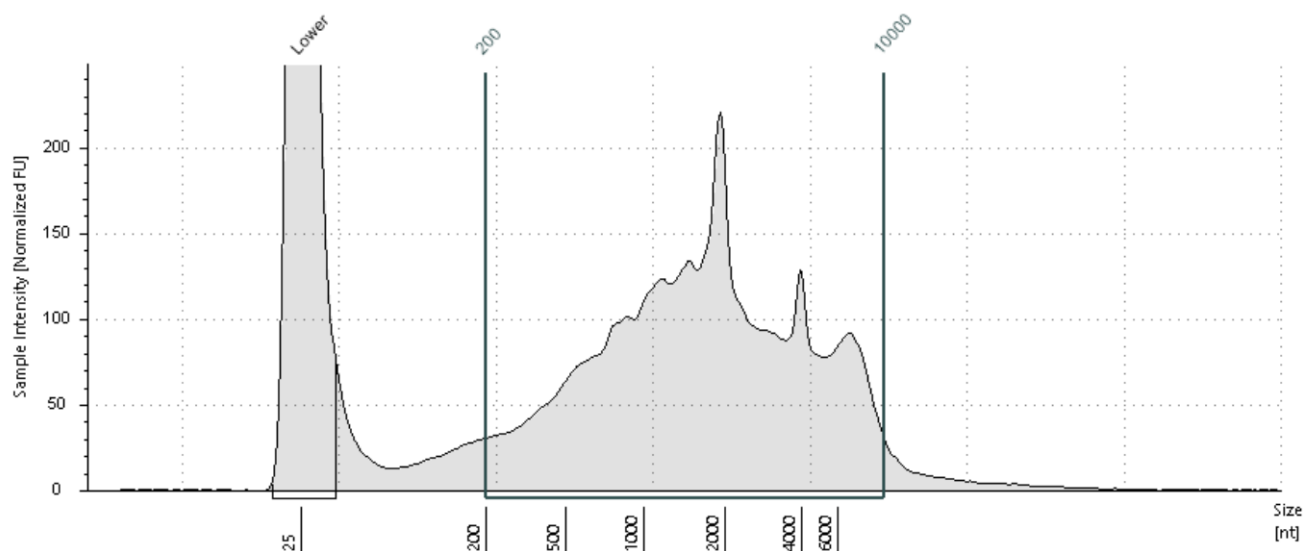


Region Table

From [nt]	To [nt]	Average Size [nt]	Conc. [pg/ul]	Region Molarity [pmol/l]	% of Total	Region Comment	Color
-----------	---------	-------------------	---------------	--------------------------	------------	----------------	-------

200	10000	4543	492	319	88.52	dv200	
-----	-------	------	-----	-----	-------	-------	---

E1: POR_120_C2

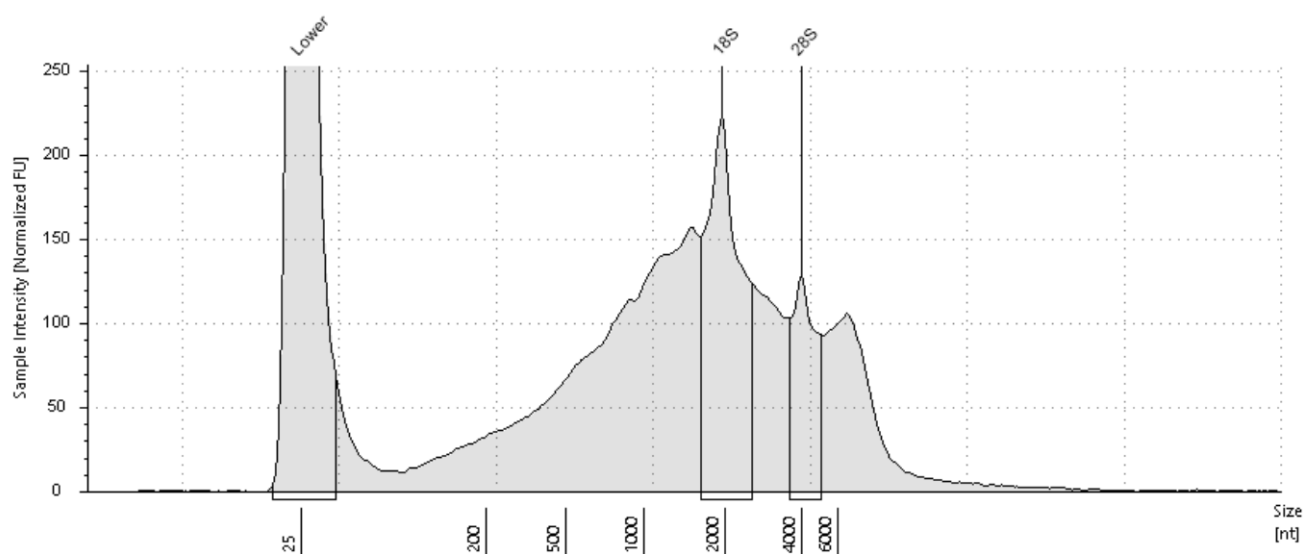


Sample Table

Well	RINe	28S/18S (Area)	Conc. [pg/ul]	Sample Description	Alert	Observations
E1	3.6	0.4	648	POR_120_C2		Caution! Expired ScreenTape device (used after two weeks of first use); RNA concentration outside recommended range for RINe

Peak Table


Size [nt]	Calibrated Conc. [pg/ul]	Assigned Conc. [pg/ul]	Peak Molarity [pmol/l]	% Integrated Area	Peak Comment	Observations
25	700	700	82400	-		Lower Marker
1954	124	-	187	71.21		18S
4006	50.2	-	36.9	28.79		28S

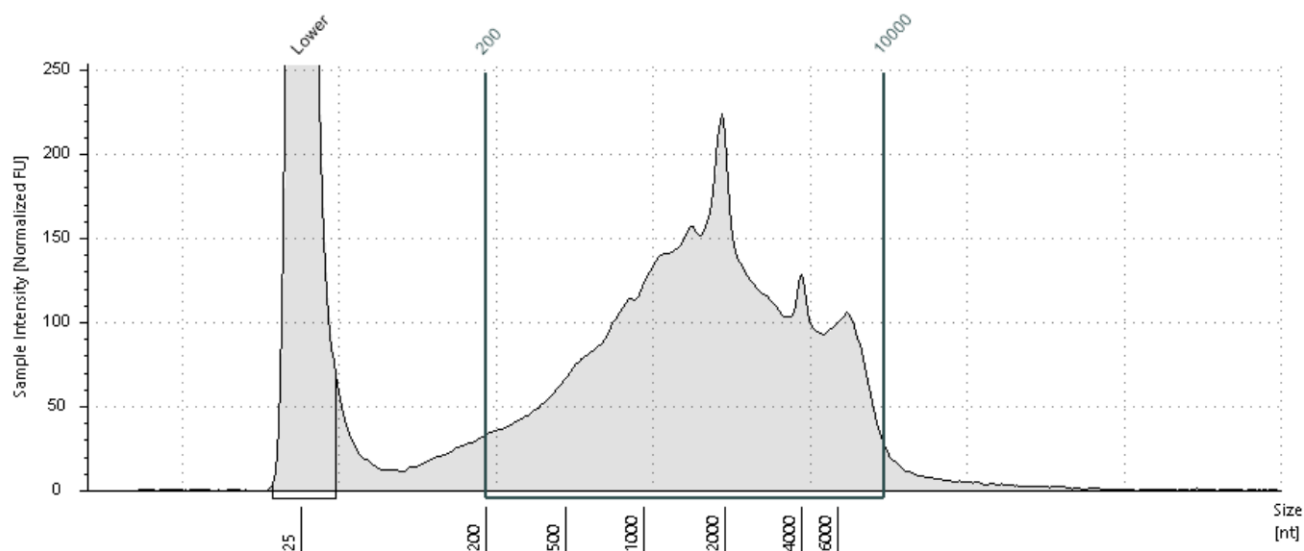

Region Table

From [nt]	To [nt]	Average Size [nt]	Conc. [pg/ul]	Region Molarity [pmol/l]	% of Total	Region Comment	Color
-----------	---------	-------------------	---------------	--------------------------	------------	----------------	-------


200	10000	4450	585	386	90.28	dv200	
-----	-------	------	-----	-----	-------	-------	---

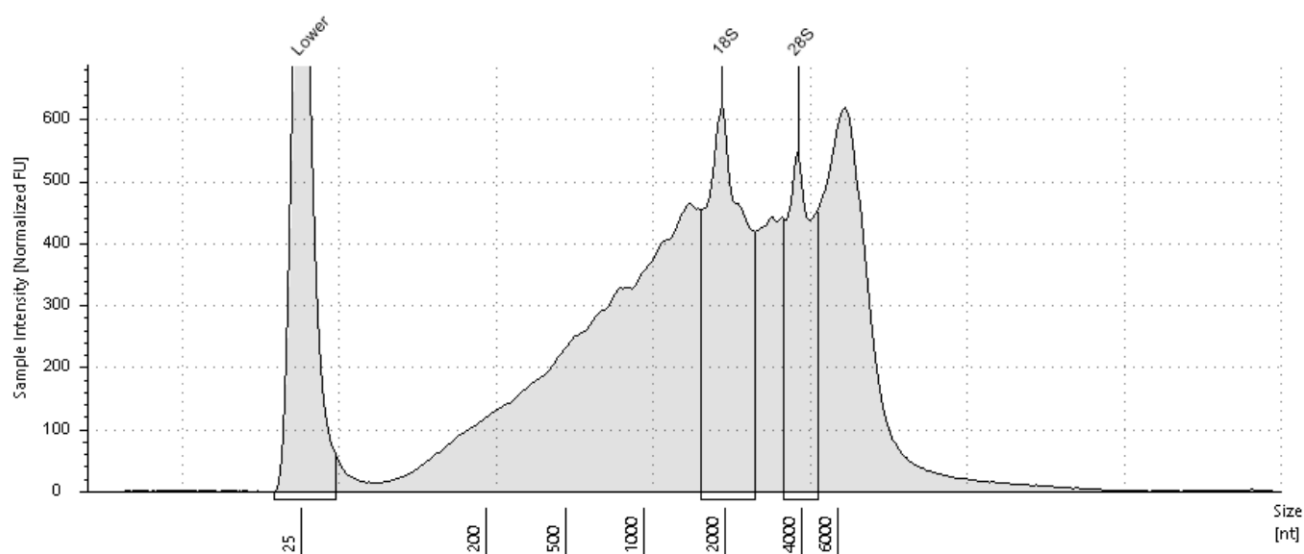F1: MON_120_C**Sample Table**

Well	RINe	28S/18S (Area)	Conc. [pg/ul]	Sample Description	Alert	Observations
F1	3.4	0.6	2410	MON_120_C	⚠	Caution! Expired ScreenTape device (used after two weeks of first use)


Peak Table

Size [nt]	Calibrated Conc. [pg/ul]	Assigned Conc. [pg/ul]	Peak Molarity [pmol/l]	% Integrated Area	Peak Comment	Observations
25	700	700	82400	-		Lower Marker
1949	414	-	626	61.73		18S
3873	257	-	195	38.27		28S edited

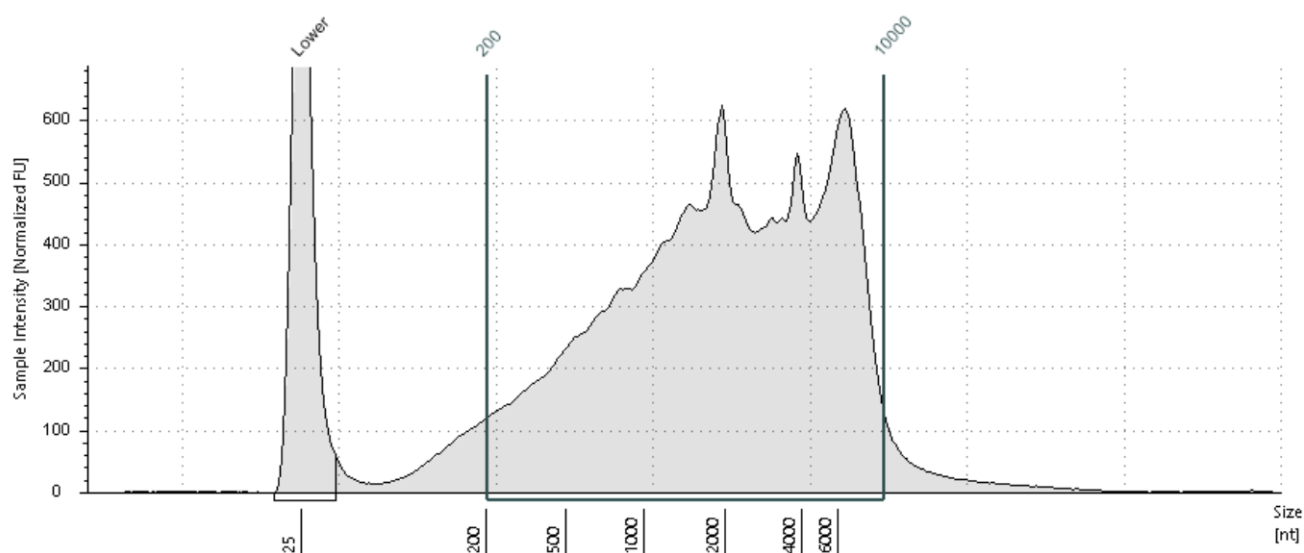**Region Table**

From [nt]	To [nt]	Average Size [nt]	Conc. [pg/ul]	Region Molarity [pmol/l]	% of Total	Region Comment	Color
200	10000	4972	2220	1310	92.33	dv200	■

G1: MON_120_H

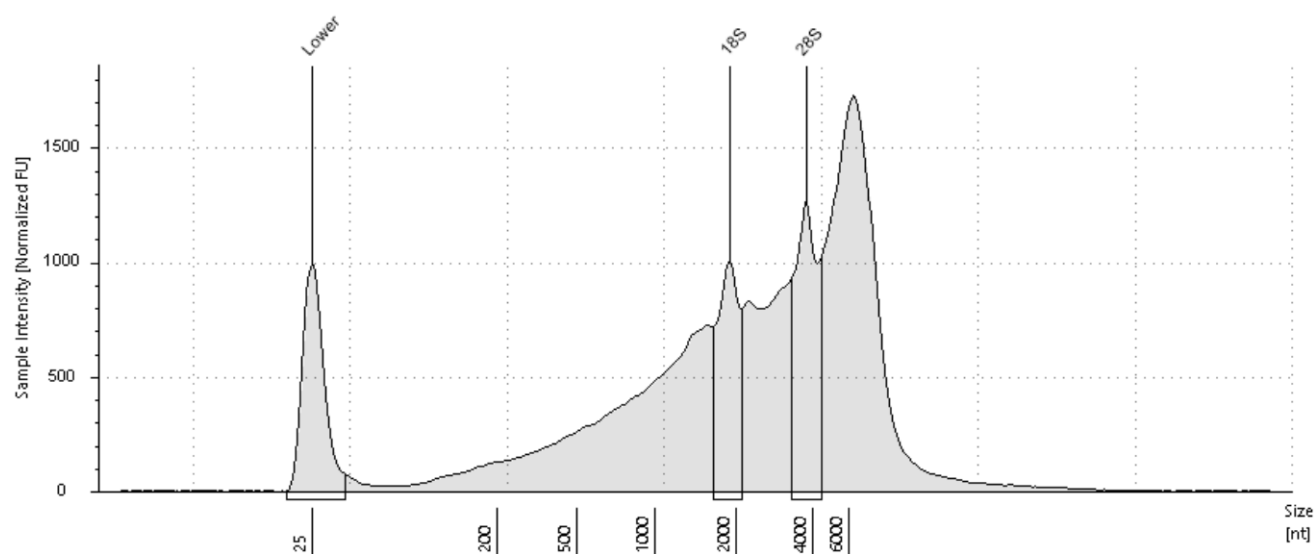


Sample Table

Well	RINe	28S/18S (Area)	Conc. [pg/ul]	Sample Description	Alert	Observations
G1	3.8	1.3	4250	MON_120_H	⚠	Caution! Expired ScreenTape device (used after two weeks of first use)

Peak Table

Size [nt]	Calibrated Conc. [pg/ul]	Assigned Conc. [pg/ul]	Peak Molarity [pmol/l]	% Integrated Area	Peak Comment	Observations
25	700	700	82400	-		Lower Marker
1907	380	-	586	43.32		18S
3780	497	-	387	56.68		28S edited

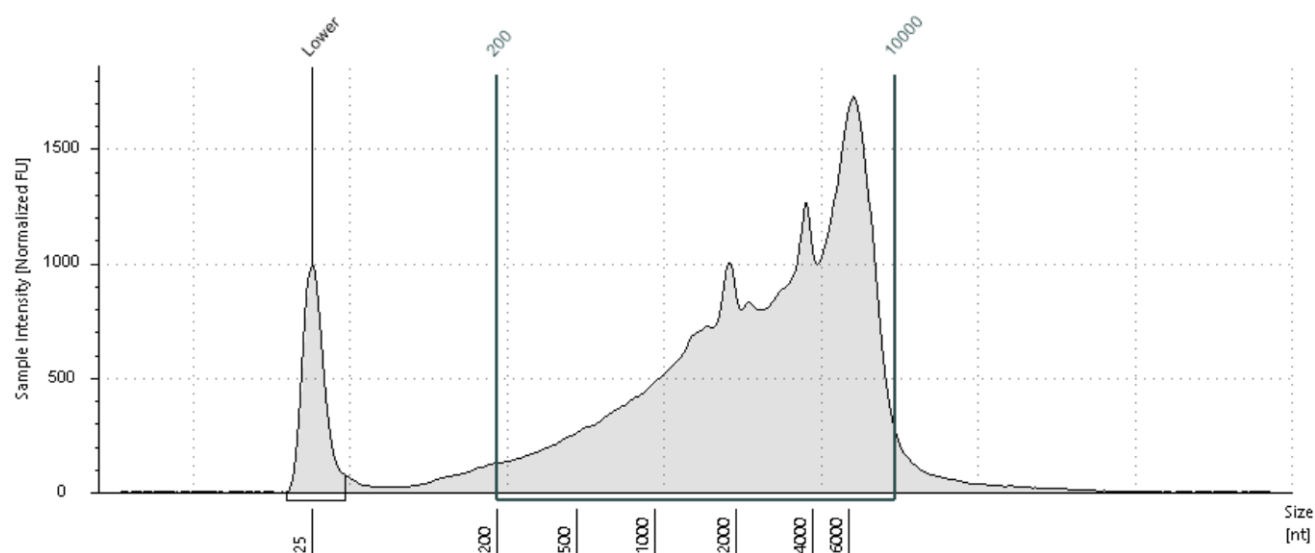

Region Table

From [nt]	To [nt]	Average Size [nt]	Conc. [pg/ul]	Region Molarity [pmol/l]	% of Total	Region Comment	Color
200	10000	5367	3980	2180	93.56	dv200	■

Sample Info

Well	RINe	28S/18S (Area)	Conc. [pg/ul]	Sample Description	Alert	Observations
A1	-	-	632	Ladder		Caution! Expired ScreenTape device (used after two weeks of first use); Ladder
B1	3.6	0.5	1030	POC_120_C		Caution! Expired ScreenTape device (used after two weeks of first use)
C1	3.4	0.5	986	POC_120_H		Caution! Expired ScreenTape device (used after two weeks of first use); RNA concentration outside recommended range for RINe
D1	4.0	0.4	556	POR_120_C1		Caution! Expired ScreenTape device (used after two weeks of first use); RNA concentration outside recommended range for RINe
E1	3.6	0.4	648	POR_120_C2		Caution! Expired ScreenTape device (used after two weeks of first use); RNA concentration outside recommended range for RINe
F1	3.4	0.6	2410	MON_120_C		Caution! Expired ScreenTape device (used after two weeks of first use)
G1	3.8	1.3	4250	MON_120_H		Caution! Expired ScreenTape device (used after two weeks of first use)