



REVIEW MODE

Single

Group

Loaded group

m8f

BASIC DISPLAY

Contour

Mask

CONTOUR STYLE

PRESETS

Brightfield
normal
cells

Brightfield
small cells

Phase
contrast

Phase
contrast 2

Apply to group

Auto detect microscope

Parameter controls

BASIC ANALYSIS

Variance radius

15

Threshold offset

-28

Min component (px)

55000

Ignore tiny islands

Low

Microscope mode

Phase contrast

Brightfield

Scratch orientation

Horizontal scratch

ADVANCED GEOMETRY

FOV cutoff

36

Fine rotation (deg)

0

Show angle ruler

☐ Auto crop FOV

Cuts the non-black microscope field before analysis; rectangular crops are allowed.

☐ Apply current crop ratio to group

Uses the same relative rectangle for each image in group review.

Adjust crop

Apply crop

Reset crop

VIEW

MANUAL CORRECTION

METRICS

EXPORT


m8f_24h_002.png

1800×1800 px horizontal scratch → 90deg variance radius

Overlay review canvas



0 deg

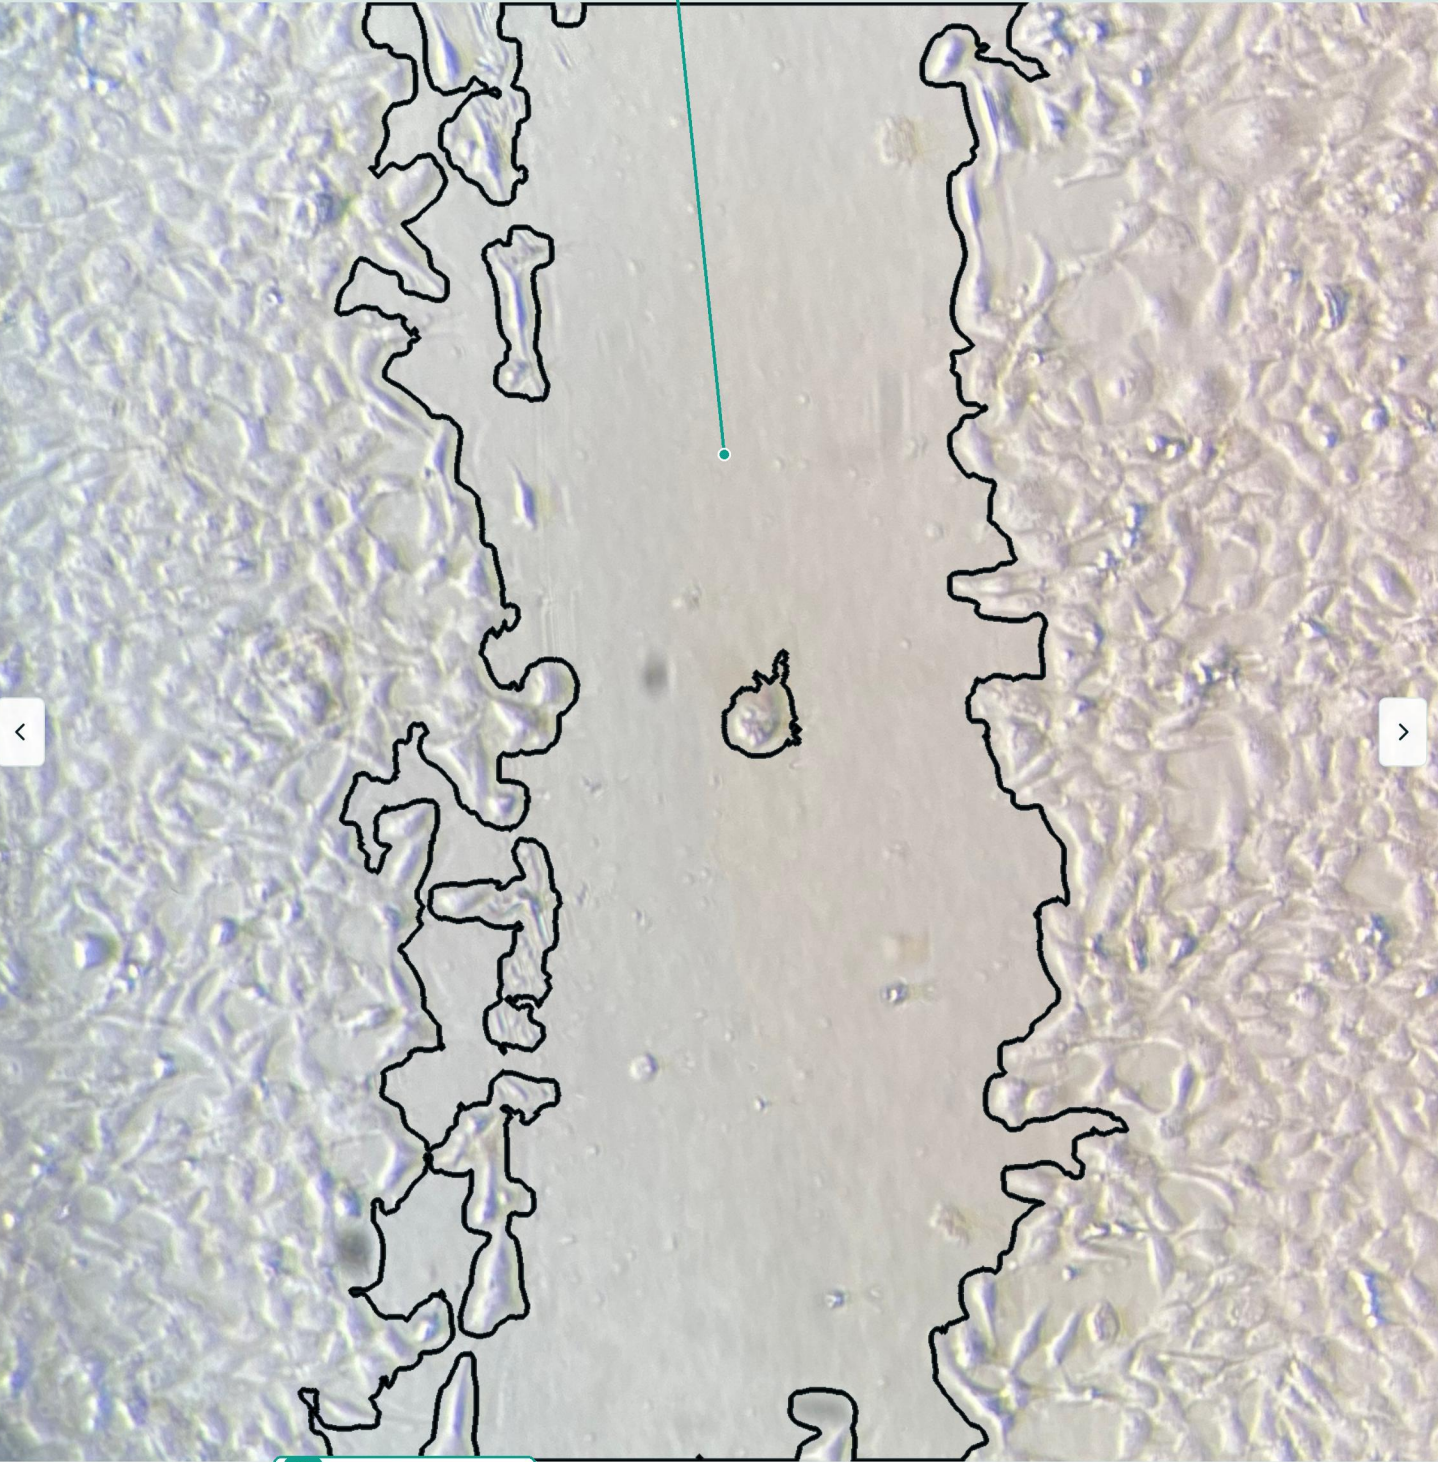

QC and metric cards

SERIES QC

100/100

crop/FOV looks consistent

LATEST AREA CLOSURE

62,7%

t0 to undefined

LATEST WIDTH CLOSURE

55,1%

t0 to undefined

AREA-WIDTH PEARSON R2

0,997

Pearson correlation squared; metrics track together

RECOMMENDED


area and width

area and width can be interpreted together

m8f_0h_001.png

Local / m8f

0h

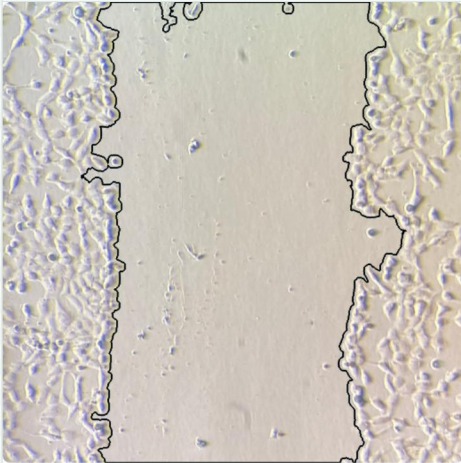


CM area 1.745.326 px
Area % 53,87%
CM width 980,5 px
Valid rows 100%
Image QC 97/100
GT closure n/a

m8f_24h_002.png

Local / m8f

24h

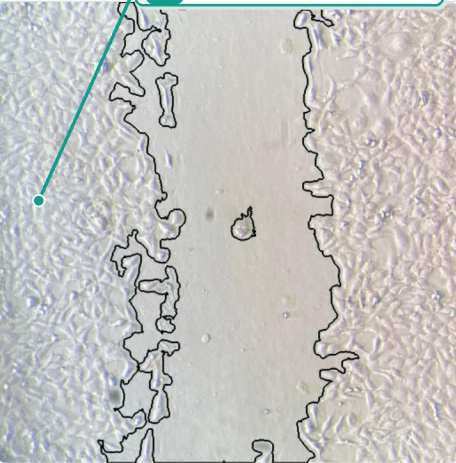


CM area 1.170.683 px
Area % 36,13%
CM width 721,1 px
Valid rows 100%
Image QC 97/100
GT closure n/a

m8f_48h_003.png

Local / m8f

48h

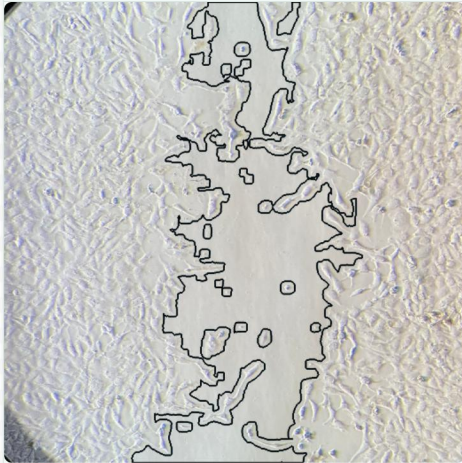

CM area 651.852 px
Area % 20,13%
CM width 440,1 px
Valid rows 100%
Image QC 100/100
GT closure n/a