FREEBOARD TECHNOLOGY

Calibration Report

Y521-A_YL0921234567_20261022-175859

Calibration written to sensor and read back

Verification: 2 of 2 passed

Sensor and session

Model	**Y521-A**	Calibration started	**Oct 22, 2026, 05:58:48 PM UTC**
Serial number	**YL0921234567**	Calibration completed	**Oct 22, 2026, 05:58:53 PM UTC**
Hardware / software	**1.1 / 1.2**	Report generated	**Oct 22, 2026, 05:58:59 PM UTC**
Modbus address	**1**	Operator	**Z. Tester**
Baud rate	**9600**	Tool	**Freeboard Sensor Utility 1.3.0**

Method and conditions

Method	**Two-point, adjusts K and B**
Standards	**1.4083, 12.852 mS/cm**
Settling criterion	**spread of last 10 readings within 0.5% of the mean (minimum 0.002 mS/cm)**
Capture	**average of the last 10 readings, read every 0.15 s**

Calibration coefficients

Group	Parameter	Before	After
User calibration (K, B)	K	1	**1.046009**
User calibration (K, B)	B	0	**-0.01429947**
Temperature calibration	TK	1	1
Temperature calibration	TB	0	0

Calibration points (mS/cm)

Point	Standard	Mean	SD	Range	n	Temp °C	Time	Stable
1	1.4083	1.36	0.0015	1.358 to 1.362	10	21.3	0:03	Yes
2	12.852	12.3	0.0014	12.298 to 12.302	10	21.3	0:03	Yes

Verification (mS/cm)

Pass when within ±1% or ±0.01 mS/cm, whichever is larger.

Standard	Measured	SD	Error	Allowed	Temp °C	Result
1.4083	1.4079	0.0014	-0.000444 (-0.032%)	±0.0141	21.3	**Pass**
12.852	12.852	0.0015	-0.000104 (-0.00081%)	±0.129	21.3	**Pass**

Data file SHA-256: f5bb8245a94e5409cbd6e7ebd756112c09a540c178ee70fec3a84d5114165f18

FREEBOARD TECHNOLOGY

Calibration Report

Y521-A_YL0921234567_20261022-175859

Settling (mS/cm)

Line: reading while in each standard. Shaded: readings averaged for the capture. Dashed: standard value.

Point 1: 1.4083 mS/cm

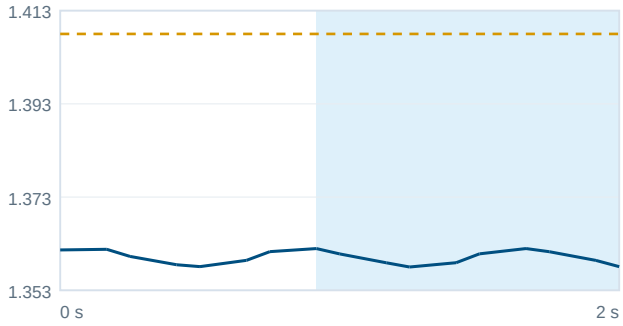

Point 2: 12.852 mS/cm

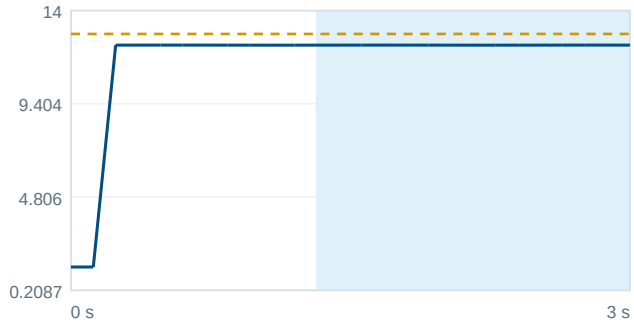

Notes

Bench calibration. Standards opened 10/20 - fresh "KCl" lot.

Sign-off

Calibrated by (Z. Tester)	Date	Reviewed by	Date

Data file SHA-256: f5bb8245a94e5409cbd6e7ebd756112c09a540c178ee70fec3a84d5114165f18