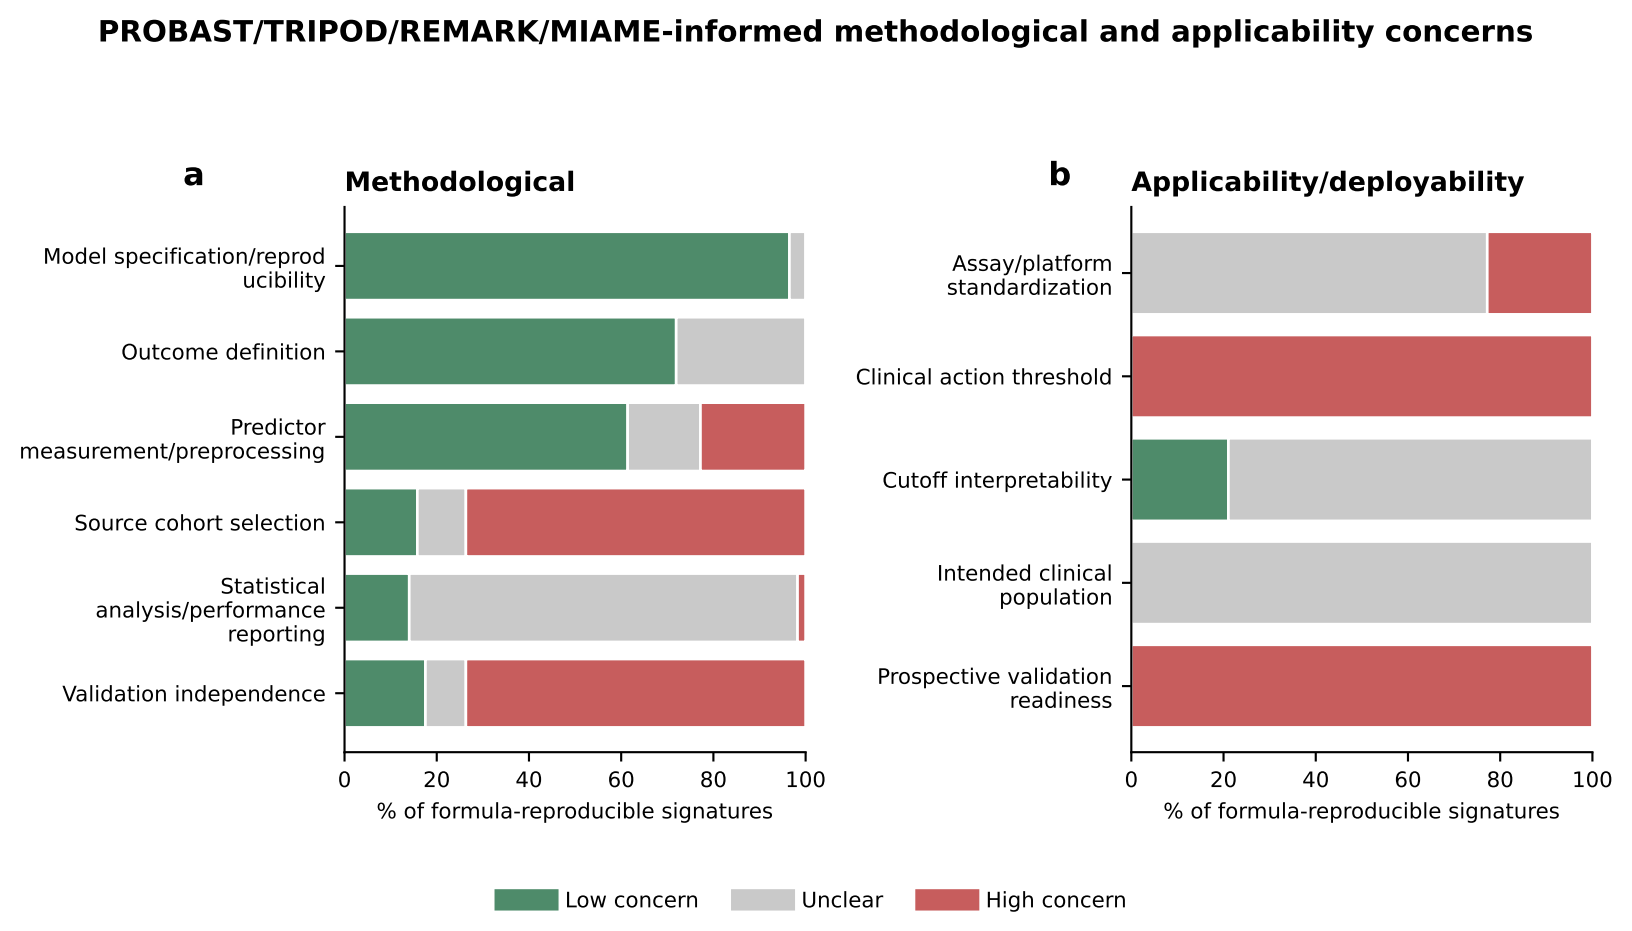
PROBAST/TRIPOD/REMARK/MIAME-informed methodological and applicability concerns
a
Methodological
Model specification/reproducibility
Outcome definition
Predictor measurement/preprocessing
Source cohort selection
Statistical analysis/performance reporting
Validation independence
0
20
40
60
80
100
% of formula-reproducible signatures
b
Applicability/deployability
Assay/platform standardization
Clinical action threshold
Cutoff interpretability
Intended clinical population
Prospective validation readiness
0
20
40
60
80
100
% of formula-reproducible signatures
Low concern
Unclear
High concern