Independent inversion of 180N and 280N DIC data

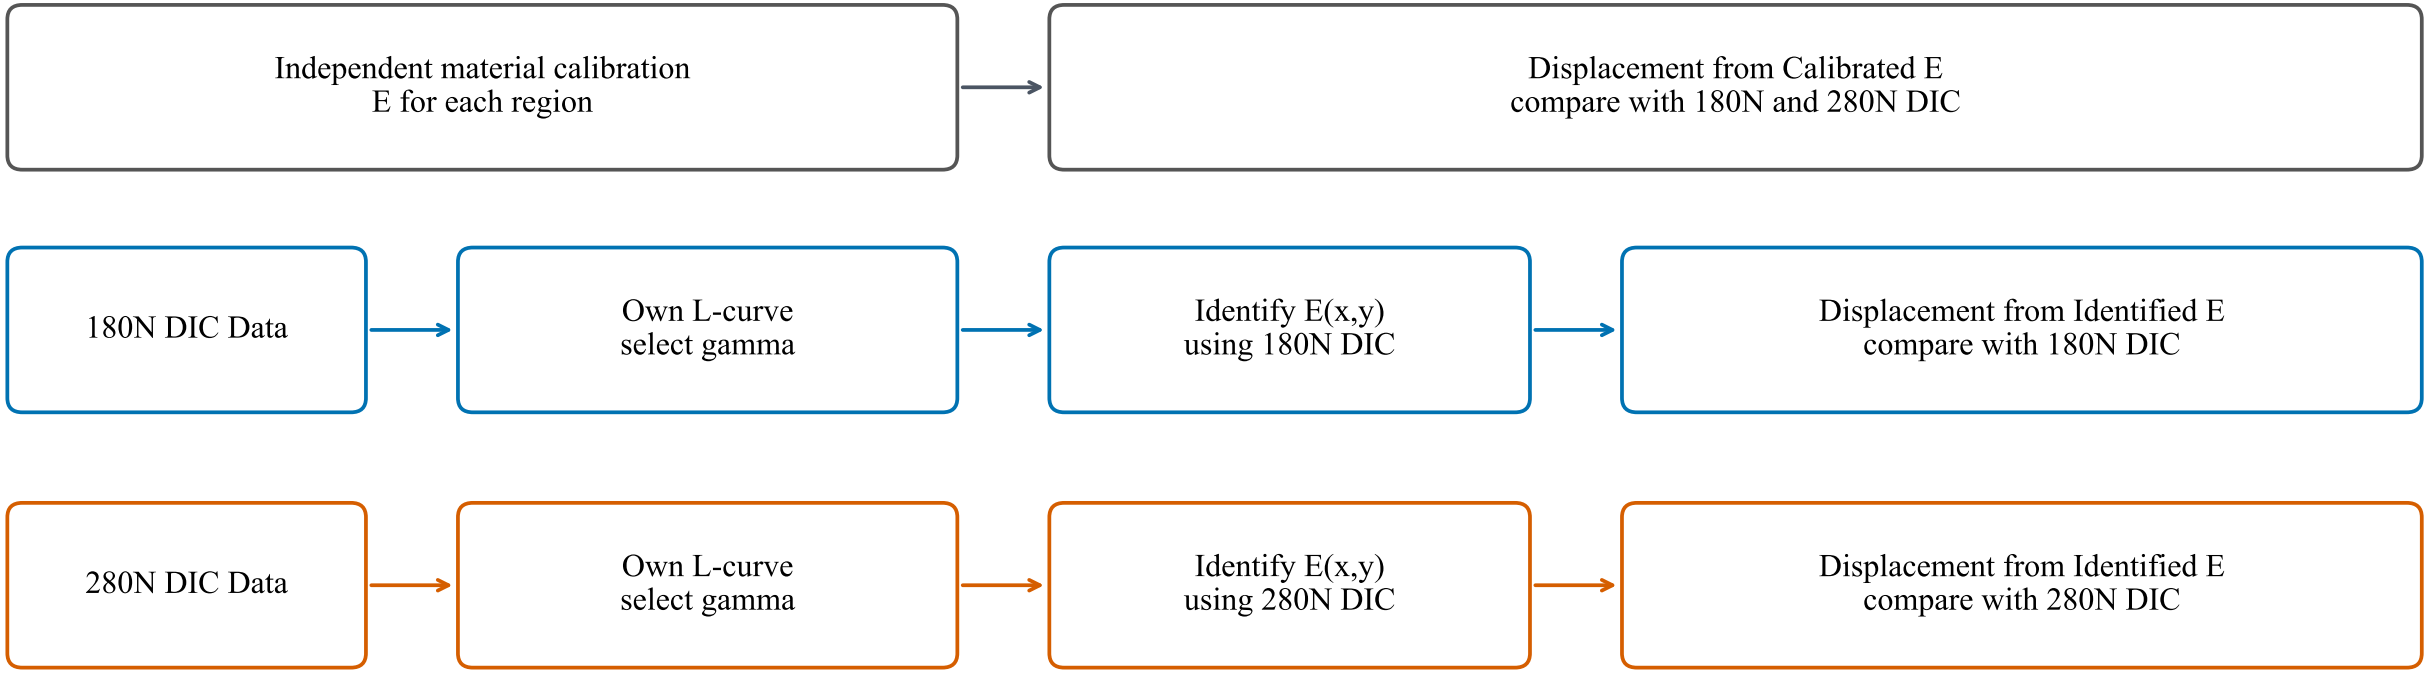

Repeat independently on both meshes: coarse 121 x 19; fine 367 x 64.
Same 23,920 DIC points. Calibration is used for forward comparison and evaluation.