

Spectral Test for RS-S3-0614-207

Detector Serial Number: **19F0000T**

PMT Serial Number **TH5194**

Technician: **EP**


Date: **6/12/2019**

Temperature: **175**


Unit Result: **PASS**

Criteria	Ambient Temperature (25°C)			Result	Elevated Temperature (175°C)			Result
	Data	Spec			Data	Spec		
Cs-137 Peak Channel	209	210 ± 10		PASS	211	210 ± 10		PASS
Pulse Width Resolution (FWHM)	8.68%	13.00% MAX		PASS	11.02%	16.00% MAX		PASS
Voltage	-1338 V	-1700 - 1700		PASS	-1504 V	-1700 - 1700		PASS
Cs-137 Window (600-720 keV)	99.03 cps	100 ± 20% cps		PASS	94.13 cps	100 ± 20% cps		PASS
Thermal Noise Edge						40 keV		PASS

Ambient Temperature Spectrum

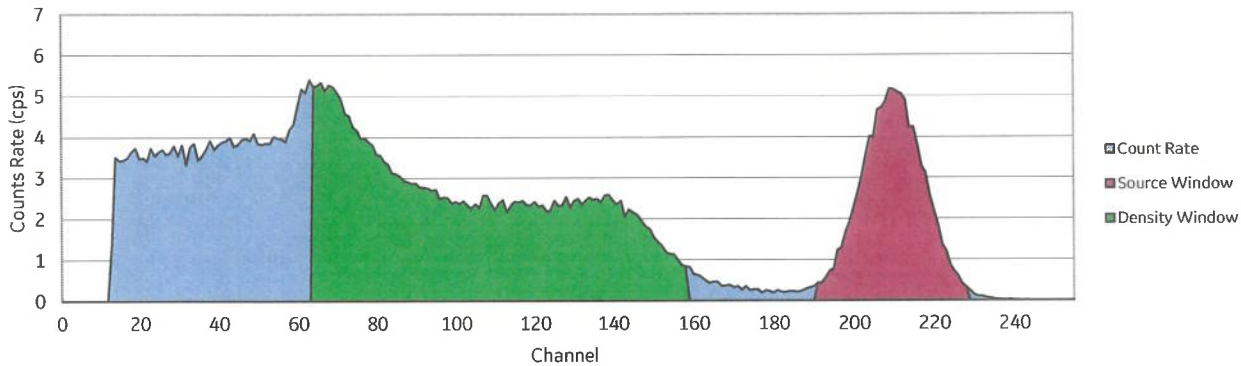

Elevated Temperature Spectrum

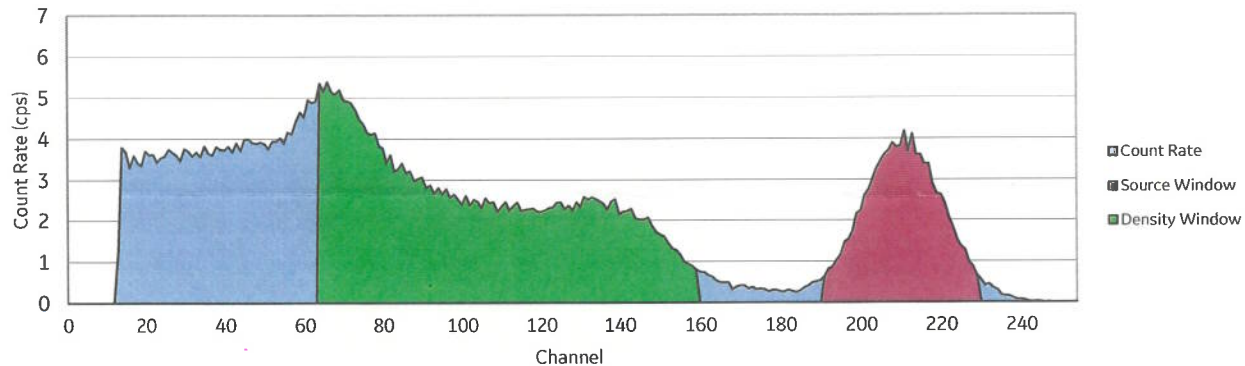



Serial#	Model #	Date	Operator	Axis	Temper ature	Static-Pre	Vibe. Time	Static- Post	Ct rt Base	Ct rt Measured	Ct rt Post	Parameter	Algorithm	Statistic1	Limit	PASS/FAIL
19F0000T	S3-0614-207	6/13/2019	GTN	X	25c	900	900	90	672.51	672.15	669.27	10.00	count	0.36	10.00	PASS
19F0000T	S3-0614-207	6/13/2019	GTN	Y	25c	900	900	90	672.74	672.87	674.24	10.00	count	0.13	10.00	PASS
19F0000T	S3-0614-207	6/13/2019	MES	Z	25c	900	900	90	672.55	674.55	671.47	10.00	count	1.99	10.00	PASS



Eckert & Ziegler

Isotope Products

24937 Avenue Tibbitts
Valencia, California 91355

Tel 661•309•1010

Fax 661•257•8303

NOMINAL SOURCE CERTIFICATE

Customer: Baker Hughes a GE Company
Purchase Order No.: 5051121444

Model No.: 3888

Catalog No.: CS738880230N

Capsule Type: A3888

Active Diameter: 0.25" (6.35 mm)

Cover: Stainless Steel

Backing: Stainless Steel

Certificate Date: 2018-07-20

Quantity: 10

SS&DR No.: CA0406S106S

ISO/ANSI Classification: ISO/99/C22212

Special Form No.: None

Nuclide Half Life: 30.17 ± 0.16 years

Recommended Working Life: 5 years

Nuclide	Source No.	Activity	Radiation Output	Reference Date
Cs-137	Q7-245	230 nCi (8510 Bq)	Not Applicable	2018-08-01
Cs-137	Q7-247	230 nCi (8510 Bq)	Not Applicable	2018-08-01
Cs-137	Q7-248	230 nCi (8510 Bq)	Not Applicable	2018-08-01
Cs-137	Q7-249	230 nCi (8510 Bq)	Not Applicable	2018-08-01
Cs-137	Q7-250	230 nCi (8510 Bq)	Not Applicable	2018-08-01
Cs-137	Q7-726	230 nCi (8510 Bq)	Not Applicable	2018-08-01
Cs-137	Q7-809	230 nCi (8510 Bq)	Not Applicable	2018-08-01
Cs-137	Q7-810	230 nCi (8510 Bq)	Not Applicable	2018-08-01
Cs-137	Q7-811	230 nCi (8510 Bq)	Not Applicable	2018-08-01
Cs-137	Q7-812	230 nCi (8510 Bq)	Not Applicable	2018-08-01

Impurities: Cs-134 = 0.0192% on Reference Date.

Leak Test Information is on Reverse Side:

Remarks:

- This document uses the numerical convention where 1.000 = 1 and 1,000 = 10³.
- This document uses the date convention YYYY-MM-DD in accordance with ISO 8601.
- Nuclear data were taken from IAEA-TECDOC-619, 1991.
- GE Part Number: SP-553-003

Matthew Dy
Name

[Signature]
Signature

2018-07-20
Date

Notebook Page: 1963-88

ISO 9001 CERTIFIED

Medical Imaging Laboratory
24937 Avenue Tibbitts Valencia, California 91355

Industrial Gauging Laboratory
1800 North Keystone Street Burbank, California 91504



Reuter-Stokes

Detector Certification of Radioactive Material

8499 Darrow Rd.
Twinsburg, OH 44087

Date: 6/17/2019

RS Model Number: RS-S3-0614-207 Rev. G

Customer Model Number: 101301007 Rev. E

RS Serial Number: 19F0000T

Source Serial Number: Q7-726

Source Capsule Type: A3888

Radioactive Material: Cs-137

Detector Nominal Activity: 8.5 kBq
230 nCi