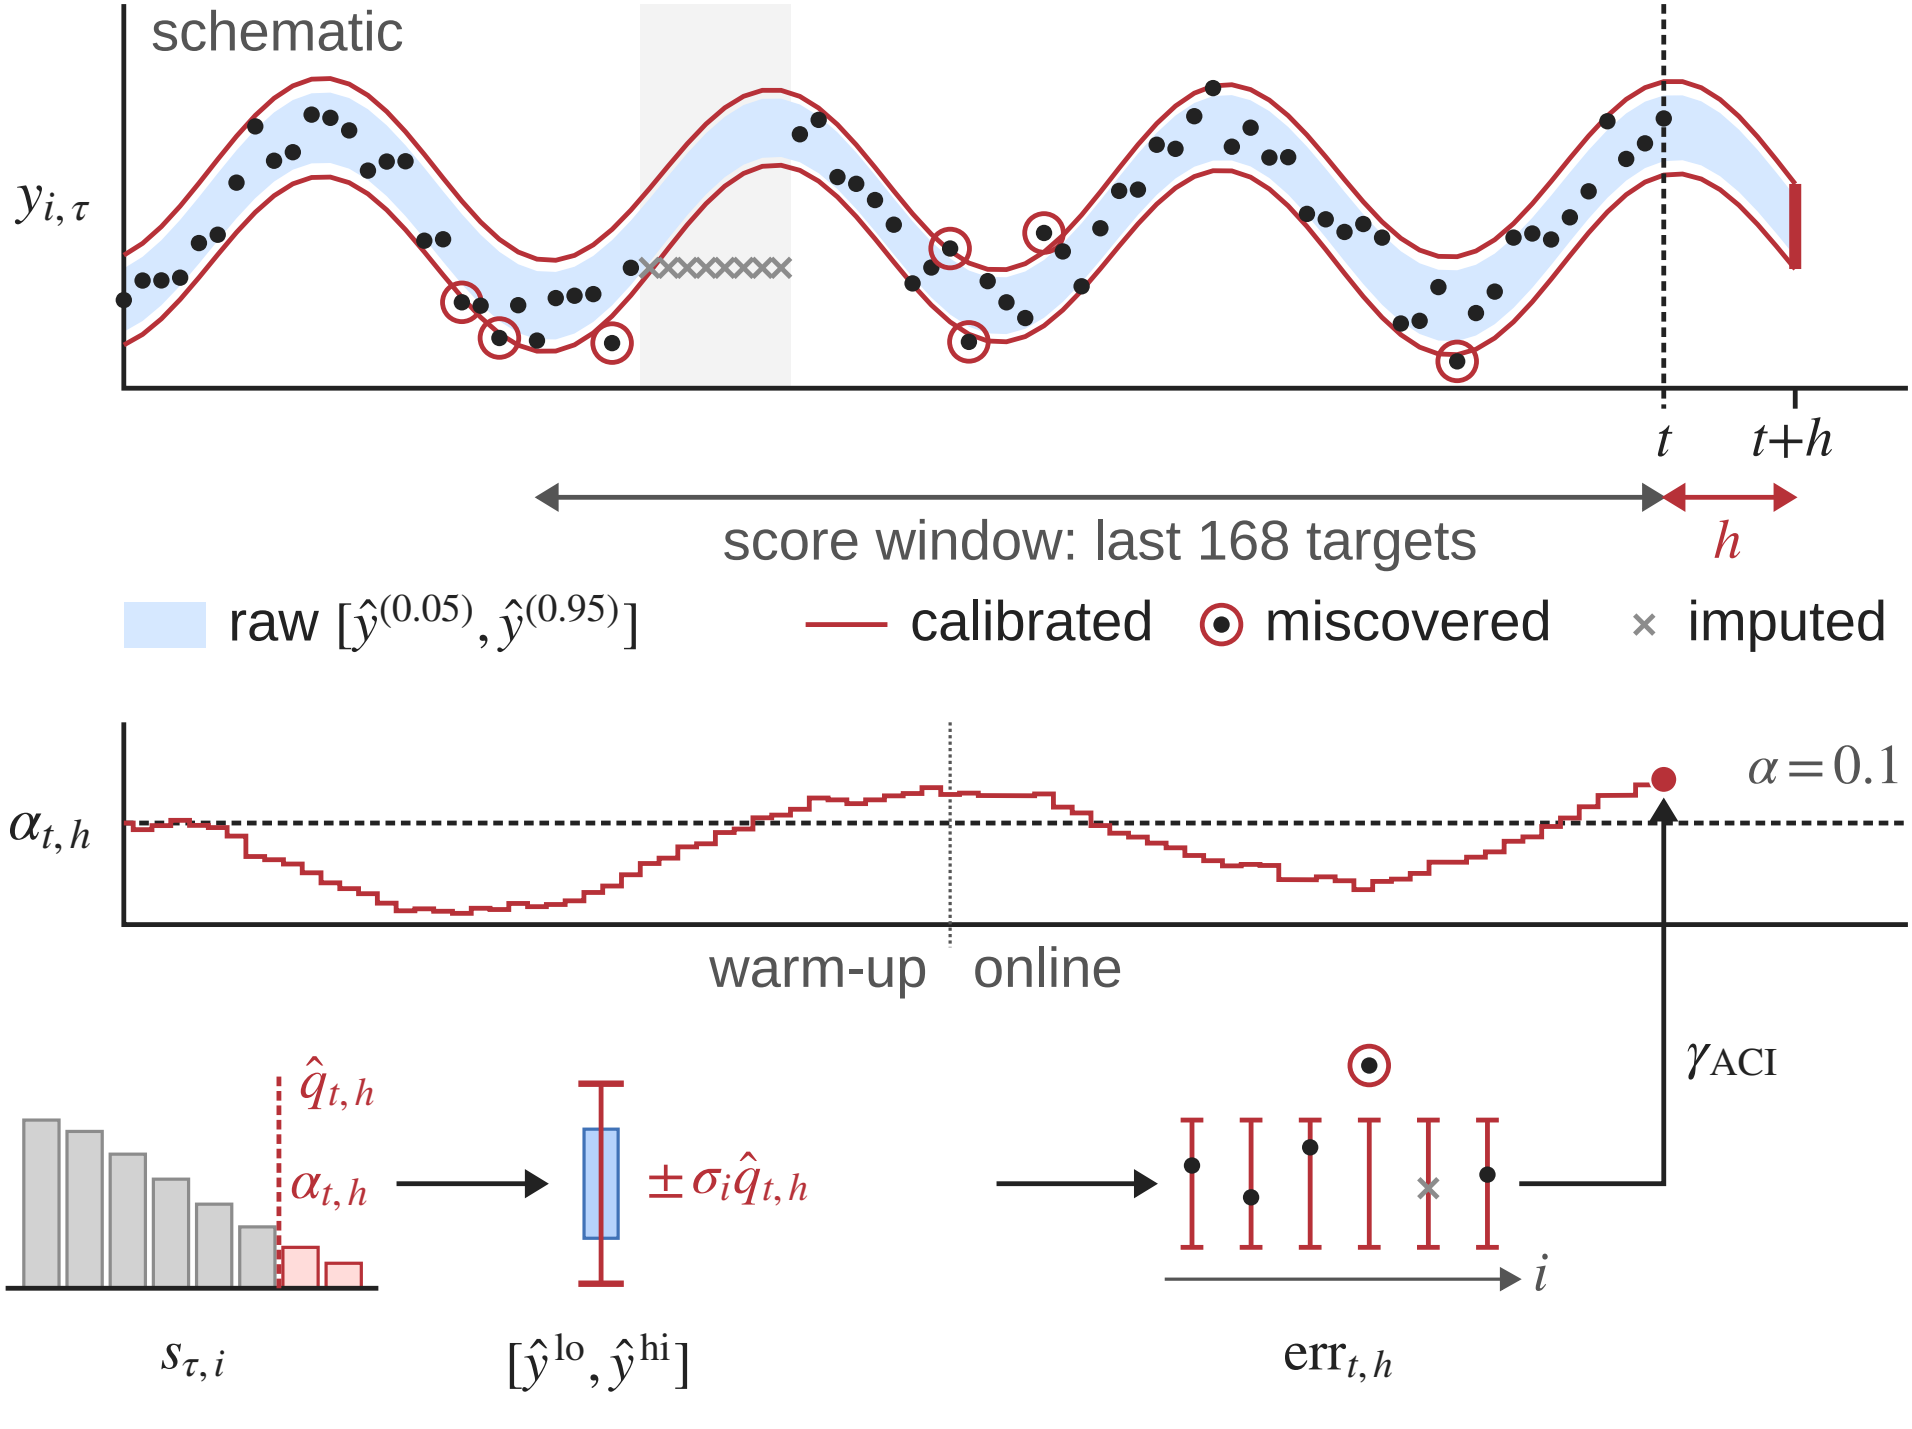# Online calibration of the 90% interval