CLM-B type

Pulse magnetic therapeutic instrument

To make use of a Book

Langfang Haomai medical instrument limited company
Address: Langfang City, Kyushu town Guangyang District Mining Road No. 9
Medical equipment production enterprise license number: 20150011
"Medical device registration certificate" Number: 20152260081
"Product technical requirements" Number: 20152260081
Tel: 0316-2291268 0316-8095912 18831612498
Zip code: 065000
Revision date: December 20, 2014
Production date: see the label of therapeutic instrument
Duration of use: 5 years

Dear user:

hello！ You are welcome to choose medical apparatus Co., Ltd in Langfang City, heroic, in order to ensure you the proper use of this product, give full play to its due role, please before use with reading instructions in the content. If you do not do, please contact the company, you can also consult the professional doctor.

Service Tel: 18831612498 0316-8095912

Thank you for your cooperation!

summary：

CLM type pulse magnetic therapeutic apparatus is composed of a host machine and a treatment head, and the B type is a square and round shaped two groups of therapeutic heads.

The composition and structure of product [diagram]

CLM-B type pulse magnetic therapy instrument front panel

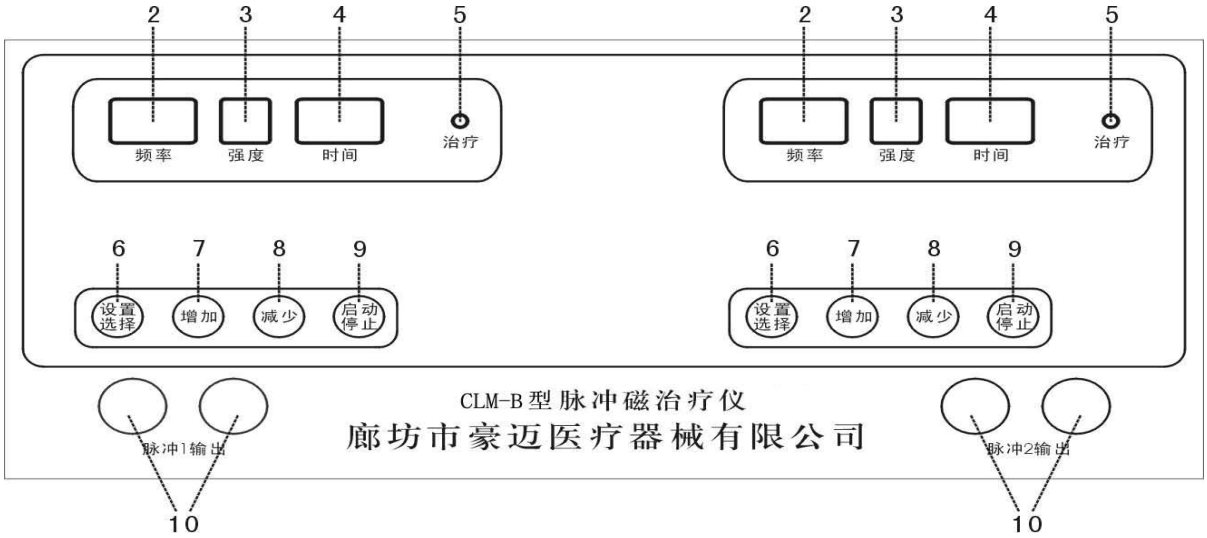

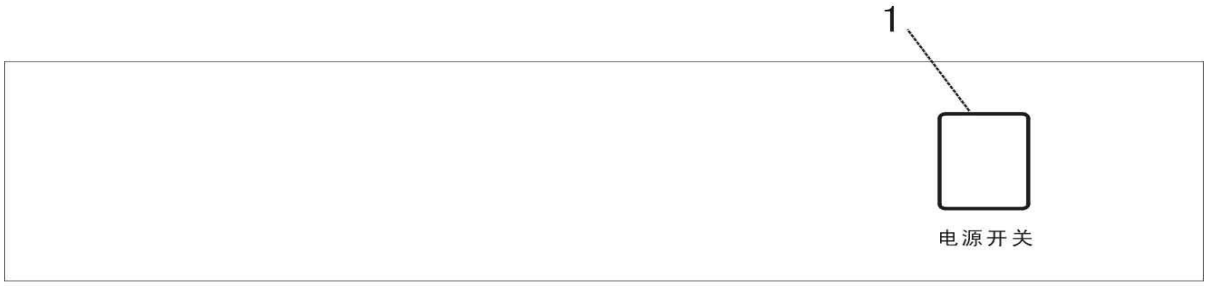

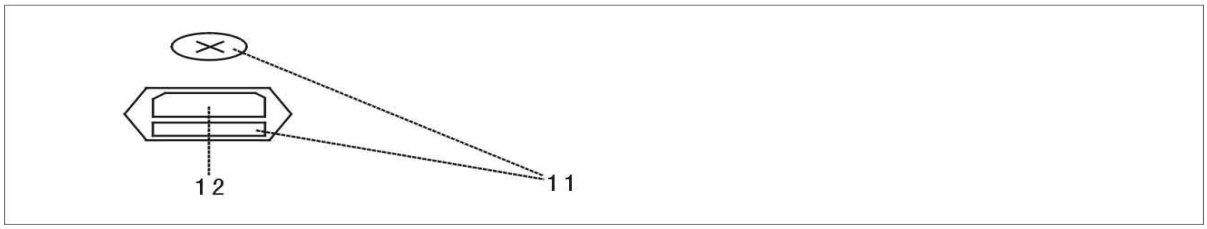

CLM-B type pulse magnetic therapeutic instrument rear panel

1, power switch 2, treatment frequency 3, treatment intensity 4, treatment time 5, treatment indicator 6, set the choice 7, an increase of 8, 9 reduction, start stop 10, treatment output 11, 12, the power supply socket.

[main function]

Antiphlogistic detumescence and analgesic antispasmodic, promote local blood circulation, adjust nerve system function.

[scope]

Neck and back pain, soft tissue contusion caused by osteoarthritis.

[Methods] operation

1, the host (instrument panel) power line plug socket AC 220V power supply power; the power switch is turned on,

The intensity of flashing lights, press the button to select the increase and reduce the intensity of treatment (1, 2 of the output of the magnetic pulse is divided into 5 grades);

2, according to the set time to select the key indicator light flashes, according to the increase or decrease select treatment time (199 minutes);

3, according to the set selection key to frequency flashing lights, according to the increase or decrease select treatment frequency;

4, according to the disease and the treatment site, treatment parameters and head are arranged in parallel or opposed;

5, press the start / stop button, indicator light treatment (5), the start of treatment and the countdown time when the buzzer alarm, turn off the

power switch and the end of treatment;

6, treatment frequency and duration: 1 times a day, each time for 25 minutes, 15~20 days for a course of treatment, treatment interval of 1 weeks, years of feasible 4~5 courses.

[note]

1, the instrument must be well grounded; replacing fuses unplug the power plug;

Not wearing clothes for thick 2, treatment;

3, after boot, do not plug head connection instrument plug;

4 instruments, 1 hours of continuous work to stop off 10 minutes (as appropriate), in order to avoid overheating caused by scald head;

5, the instrument has high pressure, maintenance must be carried out by professional personnel;

6 and before treatment should be removed who is afraid of magnetization of the items (such as a magnetic stripe card, watch, mobile phone and so on), please properly put to far away from the magnetic fields; ferromagnetic objects close to the magnetic field will influence the magnetic field distribution;

7 non circular head overlapped under energized, and beware of falling head injured body;

8, should not be forced to pull the folding line output, to prevent damage;

9, can not be used with high frequency treatment equipment with a power

outlet, to avoid interference;

10, please use under the guidance of the doctor; read the instructions before use;

11, the treatment can not be placed in the heart of the inductor area around the heart, heart disease patients disabled;

12, in the use of any discomfort, should immediately stop the treatment.

[taboo]

Serious heart, liver, kidney disease patients, bleeding or bleeding tendency, pregnant women, pacemaker carriers, cancer, white blood cells, local metal foreign body.

[key technical indicators]

1, pulse frequency

Pulse magnetic output 1, 2 frequency is the same, each file is 20 times /min, 30 times /min, 40 times /min, 50 times /min, 60 times /min, 70 times /min, 80 times /min error is + 5%;

2, the magnetic induction intensity (mT)

Output 1:	output 2:
First file ≥20mT	First file ≥20mT
Second file ≥60mT	Second file ≥40mT
Third file ≥100mT	Third file ≥60mT
Fifth file ≥150mT	Fifth file ≥80mT
Fifth file ≥200mT	Fifth file ≥100mT

3, the use of environmental temperature: 5 DEG --40 DEG relative humidity is less than 85%

4, power: 220V + 22 50Hz V + 1 Hz

5, power: less than 1500VA

6, host size: 400 x 300 x 120 (mm)

7, security type: B application, part

8, fuse: F with 5 * 20 * 2 20A

〈Trouble analysis and elimination〉

Fault analysis of reason of troubleshooting notes

No display of poor contact socket after boot

The breakdown of insurance

Power line access check socket

Replacement policy

Replace the power cord

Normal but no output head socket contact

The treatment head output line check socket is strong

Check the output line

On or near the insurance treatment equipment room placed high frequency breakdown

If you still can not rule out the trouble, please contact the warranty card on the contact method and manufacturers must not open the host, so as not to damage other parts

[maintenance and maintenance]

1, the instrument should pay attention to prevent dust, the instrument is not used for a long time, should be checked once a year.

2, the instrument warranty period of one year.

3, without the company's authorization, the user do not arbitrarily.

[standard configuration list]

1, the treatment of a host machine.

2, a power cord.

3, round treatment head 2; square treatment head 2.

Transport and storage

1, transport, packaging good therapeutic apparatus in the transport process should handle with care available general transport, shockproof, moisture-proof, anti pressure.

2, storage: Packaging good therapeutic apparatus in the temperature of -20 DEG C to + 55 DEG C, relative humidity is less than or equal to 90%, no corrosive vapour ventilation environment storage.

[instrument, instruction manual sign]

⚠- the output jack, attention to safety.

- type B application section.