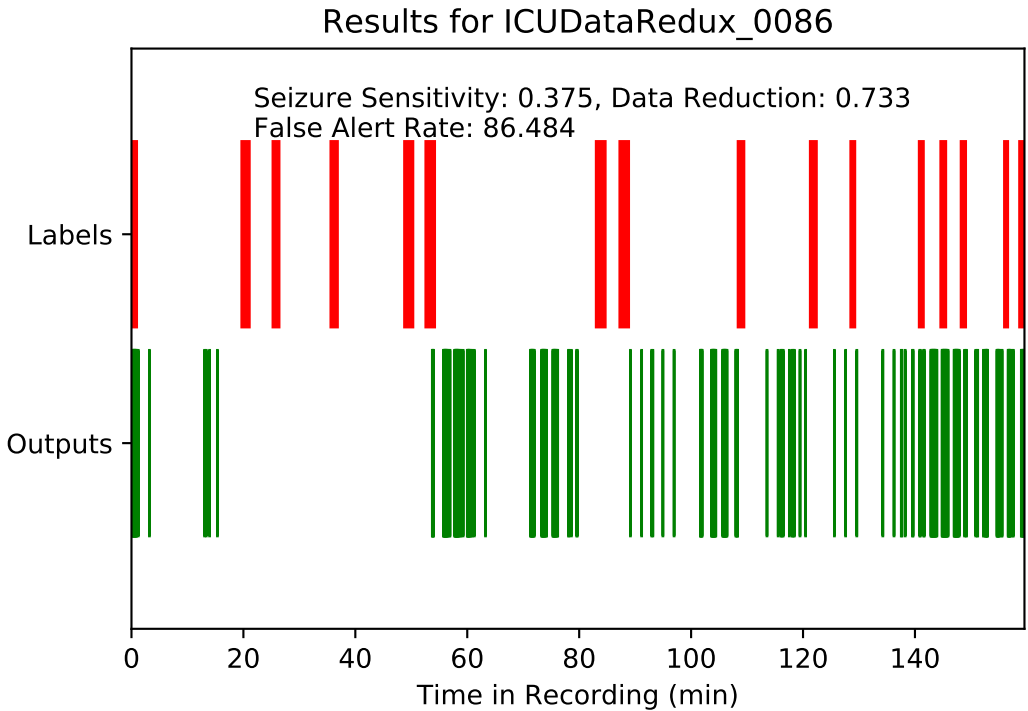
Results for ICUDataRedux_0086
Seizure Sensitivity: 0.375, Data Reduction: 0.733
False Alert Rate: 86.484
Labels
Outputs
0
20
40
60
80
100
120
140
Time in Recording (min)