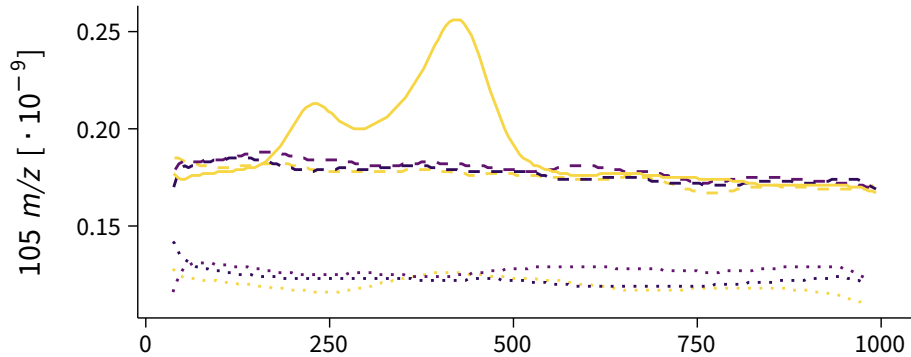
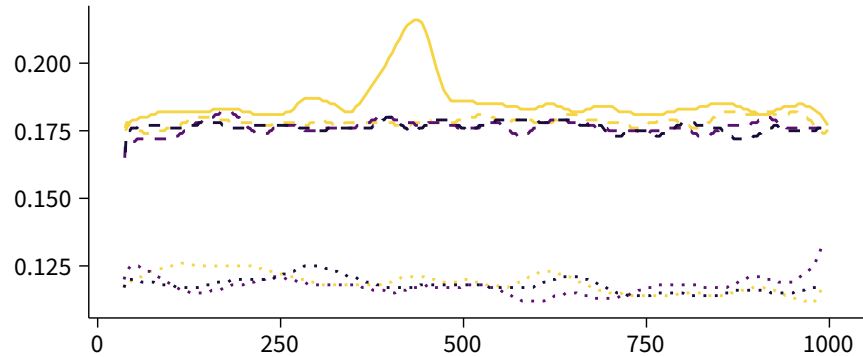



**With internal standard****Without internal standard****PET content [ $\text{g kg}^{-1}$ ]****Type**

..... Clean run after

- - Oxalate after

— Sample